

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
 Data File : BP010124.D
 Acq On : 27 Apr 2022 18:01
 Operator : CG/JU
 Sample : PB144421BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK421

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	44	48	58	rVB	56269	81070	1.78%	0.164%
2	3.781	115	118	139	rBV	599569	1020589	22.40%	2.059%
3	4.117	172	175	181	rVB	14230	19189	0.42%	0.039%
4	7.099	674	682	696	rBV	854832	1374004	30.15%	2.772%
5	7.264	704	710	723	rVB	706400	1120233	24.58%	2.260%
6	7.469	738	745	759	rBV	896512	1420899	31.18%	2.866%
7	7.940	818	825	840	rBV	763906	1244277	27.31%	2.510%
8	8.646	935	945	959	rBV	1105189	1814586	39.82%	3.660%
9	9.099	1013	1022	1035	rBV	895070	1492324	32.75%	3.010%
10	9.822	1137	1145	1159	rBV	738831	1252518	27.49%	2.527%
11	10.363	1229	1237	1255	rBV	1015956	1797638	39.45%	3.626%
12	10.746	1294	1302	1314	rBV	1087201	1848751	40.57%	3.729%
13	10.875	1317	1324	1345	rBV	953614	1832362	40.21%	3.696%
14	12.334	1566	1572	1583	rBV2	17914	36717	0.81%	0.074%
15	12.546	1605	1608	1616	rBV7	2951	4767	0.10%	0.010%
16	12.946	1672	1676	1680	rVB6	3085	5149	0.11%	0.010%
17	13.551	1775	1779	1783	rVB6	2894	4669	0.10%	0.009%
18	13.863	1825	1832	1835	rBV8	3710	7301	0.16%	0.015%
19	13.981	1843	1852	1864	rBV	1943064	2803463	61.52%	5.655%
20	14.069	1865	1867	1880	rVB10	6303	16116	0.35%	0.033%
21	14.269	1893	1901	1917	rBV	2121623	3209108	70.42%	6.474%
22	14.575	1945	1953	1967	rBV	1690651	2506527	55.00%	5.056%
23	14.763	1977	1985	2005	rBV	570223	1123619	24.66%	2.267%
24	15.210	2058	2061	2069	rVB10	3415	7674	0.17%	0.015%
25	15.569	2114	2122	2135	rBV	2687098	3997045	87.71%	8.063%
26	15.687	2135	2142	2158	rVV	771477	1167084	25.61%	2.354%
27	15.810	2158	2163	2170	rVB2	33272	53641	1.18%	0.108%
28	16.351	2251	2255	2262	rVB3	9908	14609	0.32%	0.029%
29	17.004	2362	2366	2372	rVB8	6073	11183	0.25%	0.023%
30	17.122	2381	2386	2387	rBV3	3683	4799	0.11%	0.010%
31	17.328	2414	2421	2431	rBV	1894708	2827750	62.05%	5.704%
32	17.428	2431	2438	2459	rVB	2811399	4228001	92.78%	8.529%
33	18.816	2671	2674	2676	rBV4	3929	4559	0.10%	0.009%
34	19.239	2741	2746	2751	rBV2	33889	51012	1.12%	0.103%
35	19.310	2753	2758	2762	rBV	33057	48247	1.06%	0.097%
36	19.663	2811	2818	2835	rBV	3219750	4556913	100.00%	9.192%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010124.D
Acq On : 27 Apr 2022 18:01
Operator : CG/JU
Sample : PB144421BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	21.416	3110	3116	3131	rBV	1496473	2252723	49.44%	4.544%
38	23.716	3500	3507	3515	rBV2	1300736	2611629	57.31%	5.268%
39	23.874	3527	3534	3546	rVB2	756685	1700005	37.31%	3.429%




Sum of corrected areas: 49572750

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010124.D
Acq On : 27 Apr 2022 18:01
Operator : CG/JU
Sample : PB144421BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

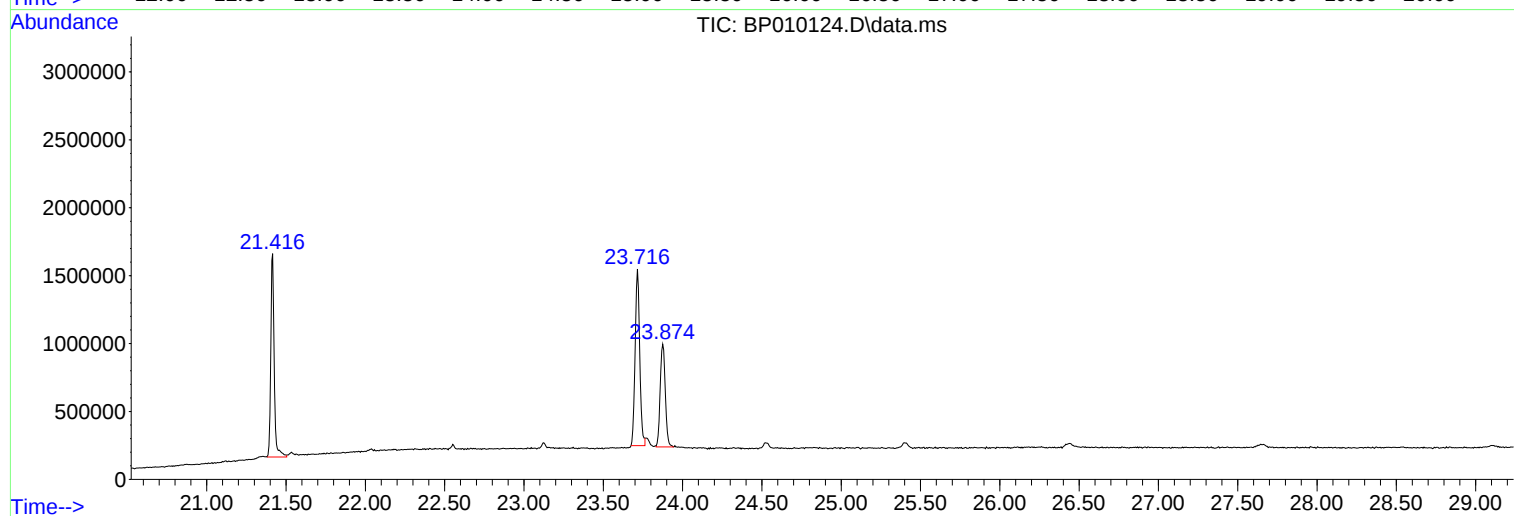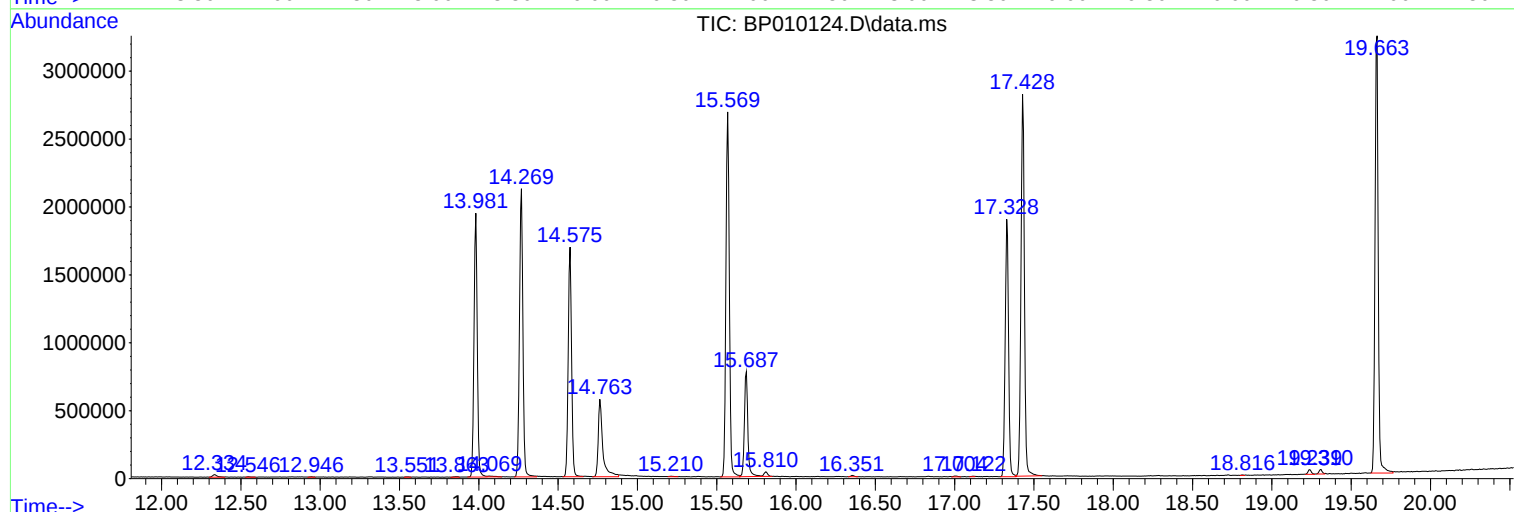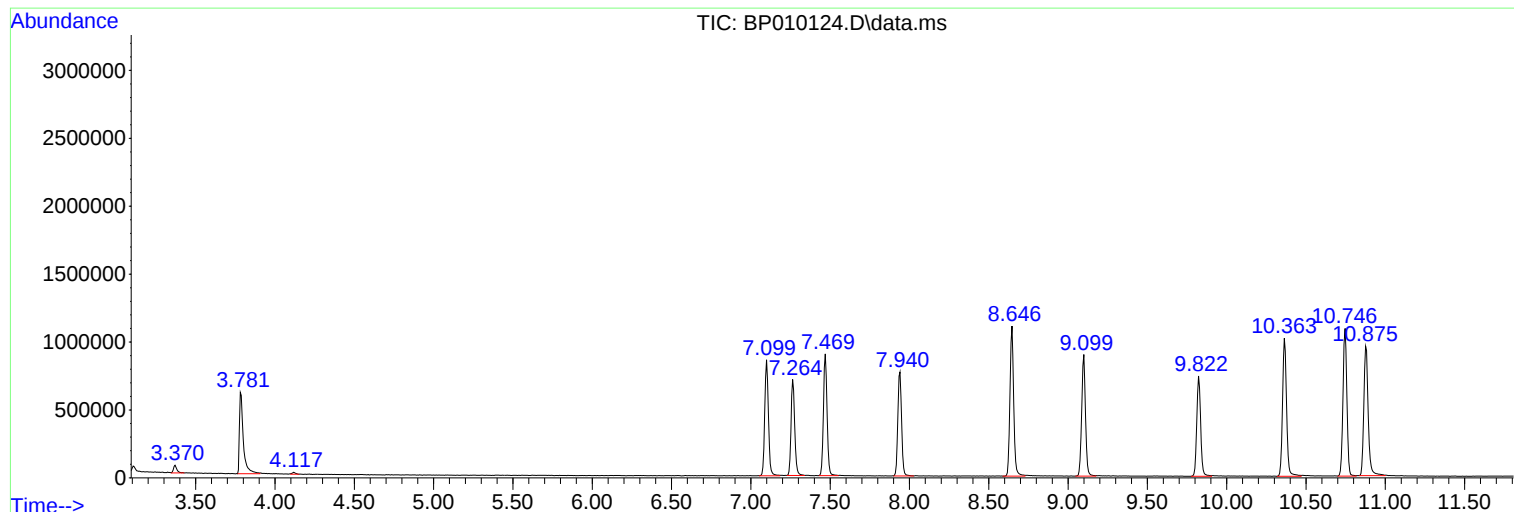

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010124.D
Acq On : 27 Apr 2022 18:01
Operator : CG/JU
Sample : PB144421BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042722\
Data File : BP010124.D
Acq On : 27 Apr 2022 18:01
Operator : CG/JU
Sample : PB144421BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
