
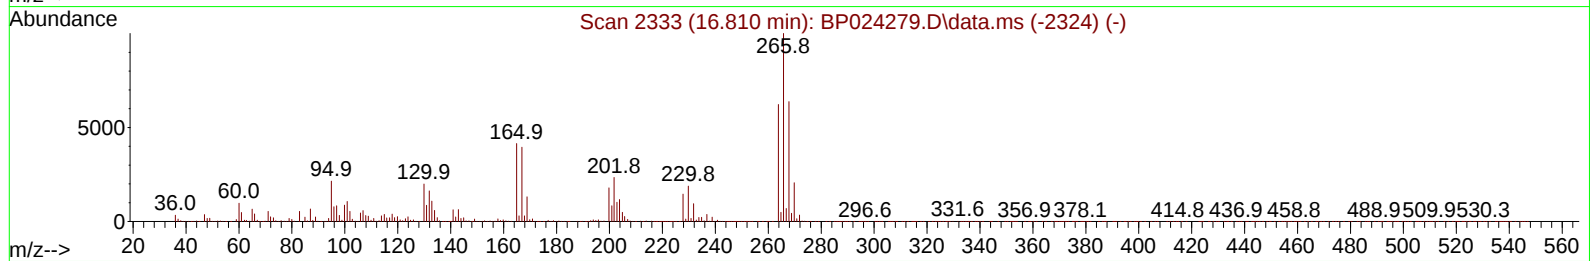
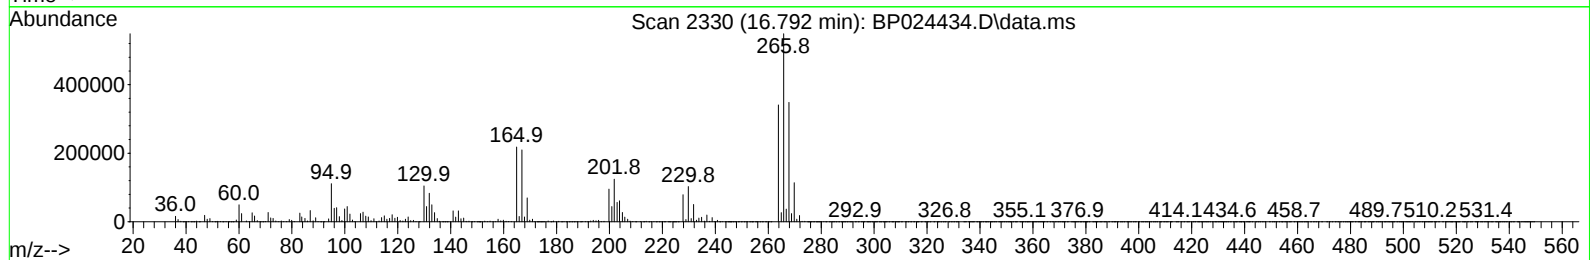


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042825\
Data File : BP024434.D
Acq On : 28 Apr 2025 12:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 14:02:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

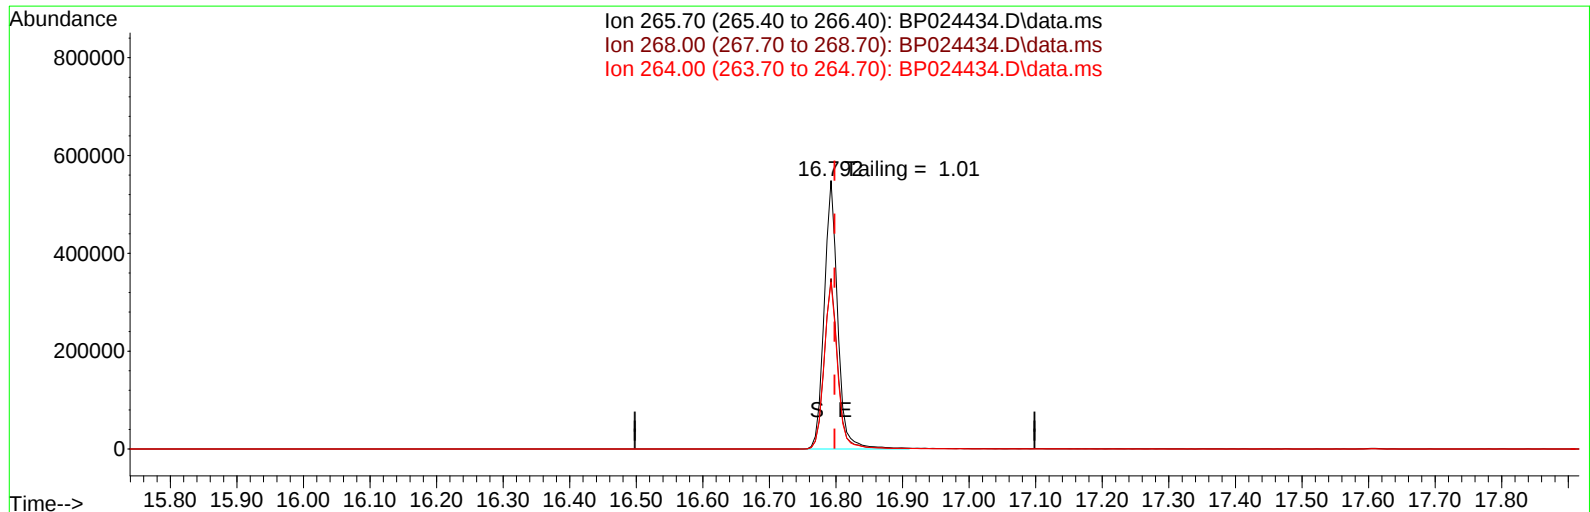

TIC: BP024434.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.006) 264266.31 ng

response 776280

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.49
264.00	62.20	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042825\
Data File : BP024434.D
Acq On : 28 Apr 2025 12:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 14:02:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

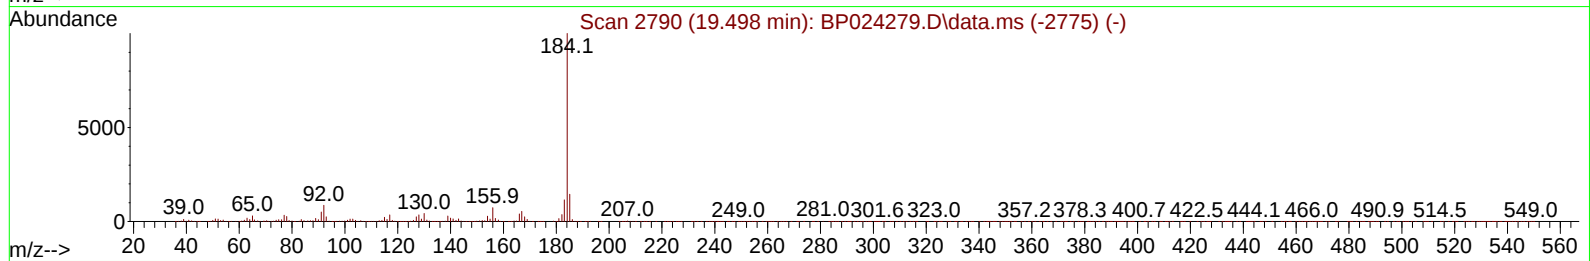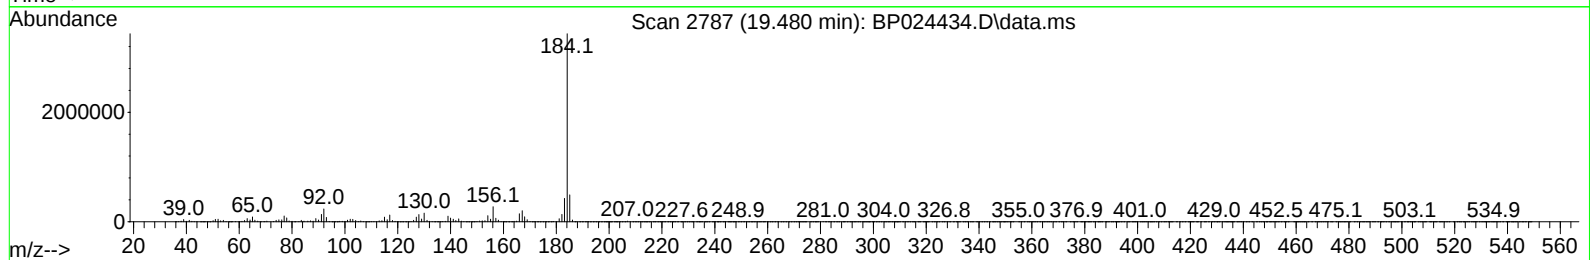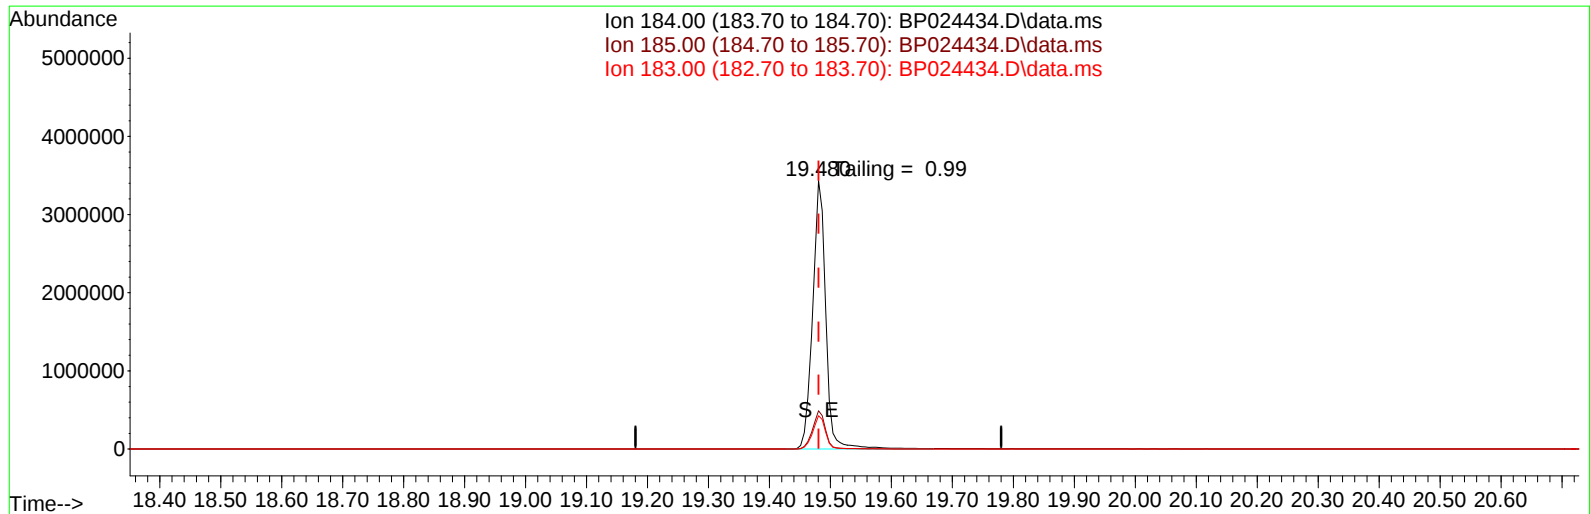

TIC: BP024434.D\data.ms

(77) Benzidine**19.480min (+ 0.000) 246689.07 ng****response 5178300**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.27
183.00	11.50	12.41
0.00	0.00	0.00