




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010155.D
 Acq On : 29 Apr 2022 17:16
 Operator : CG/JU
 Sample : N2587-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

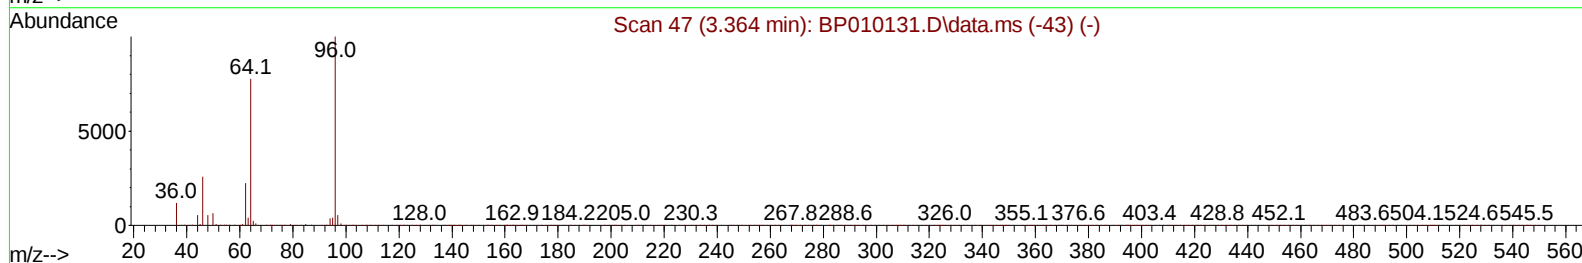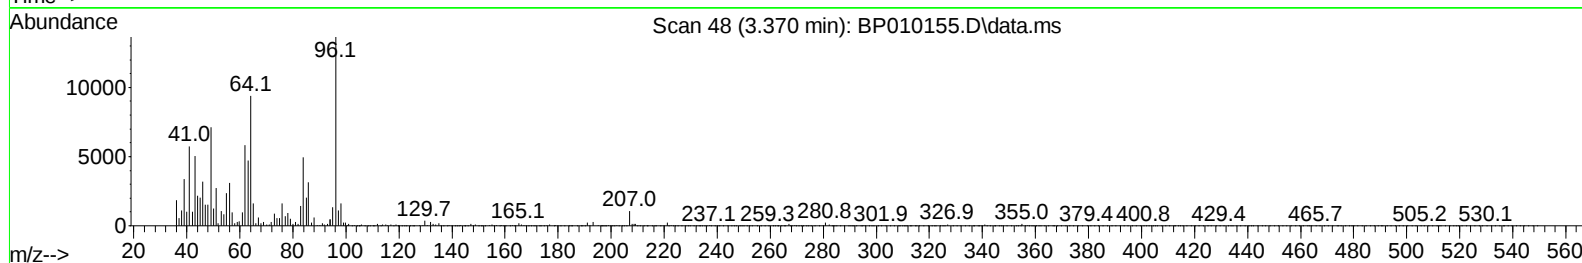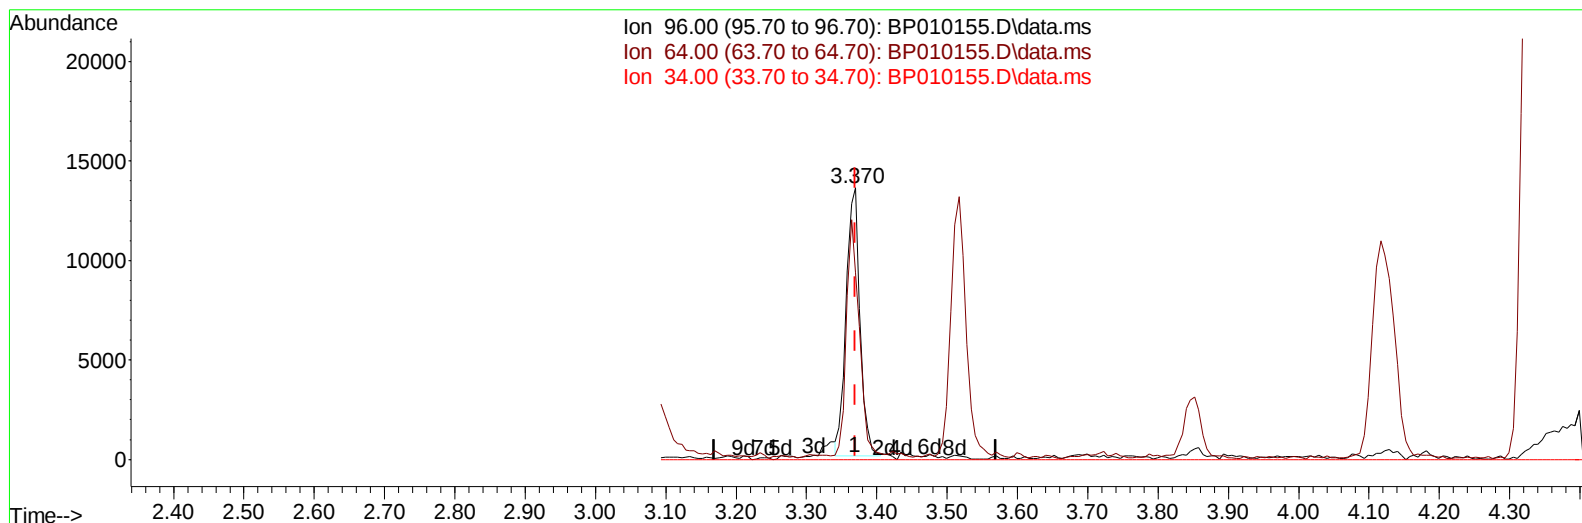

TIC: BP010155.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.370min (+ 0.001) 5.84 ng/uL m

response 18605

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	68.81#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010155.D
 Acq On : 29 Apr 2022 17:16
 Operator : CG/JU
 Sample : N2587-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

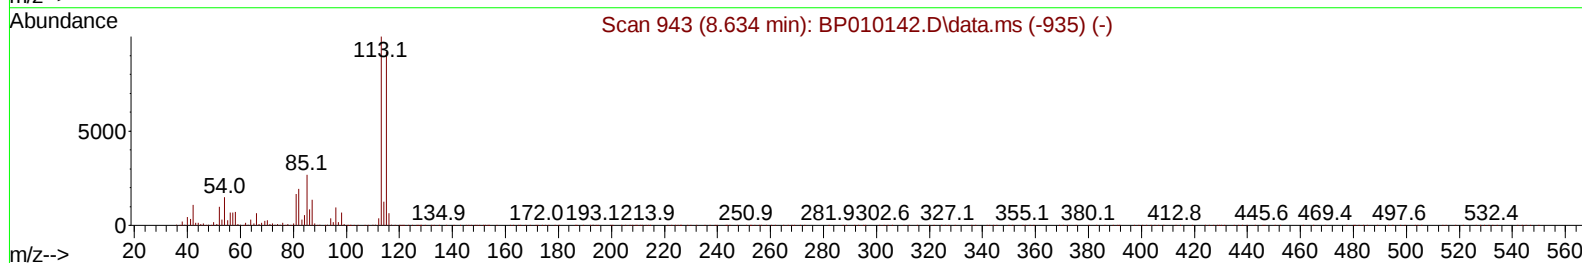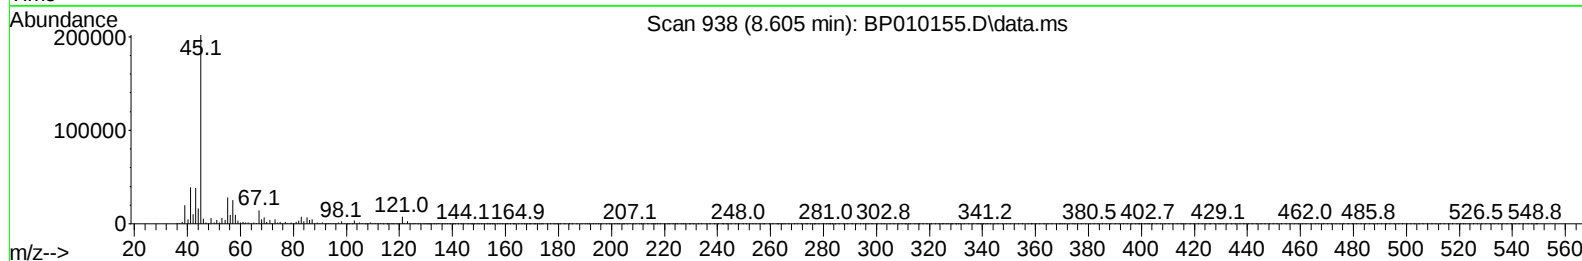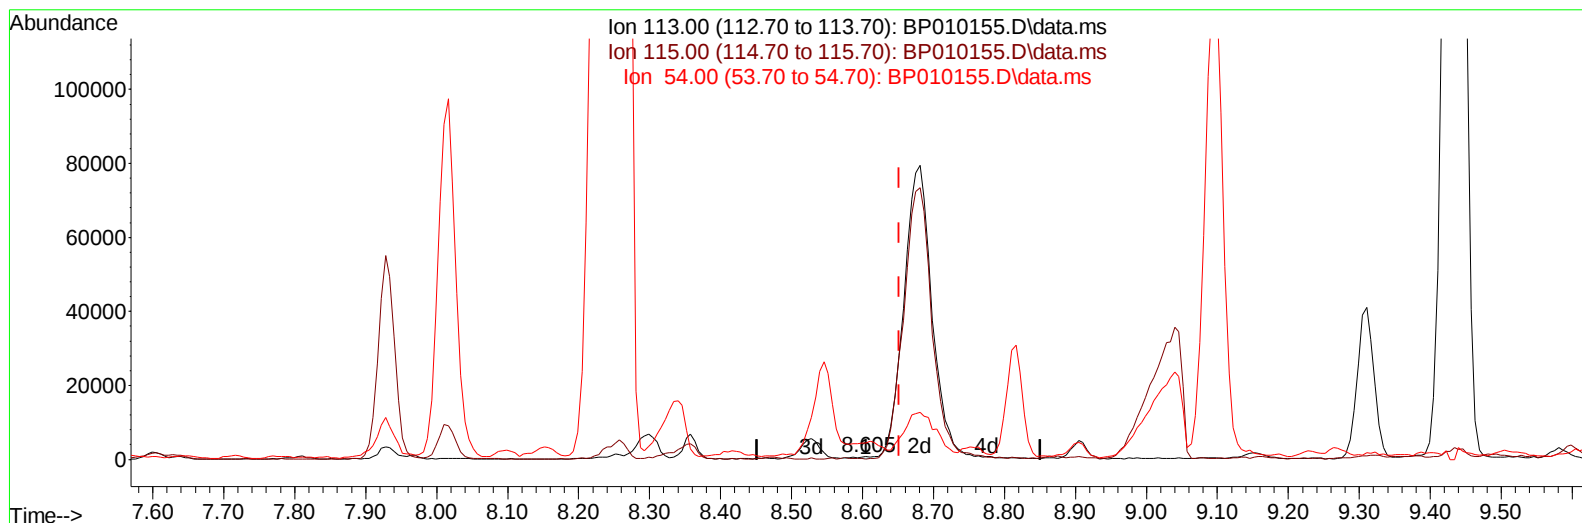

TIC: BP010155.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.605min (-0.047) 0.11 ng/u1

response 1117

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	106.70	25.03#
54.00	4.50	587.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010155.D
Acq On : 29 Apr 2022 17:16
Operator : CG/JU
Sample : N2587-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

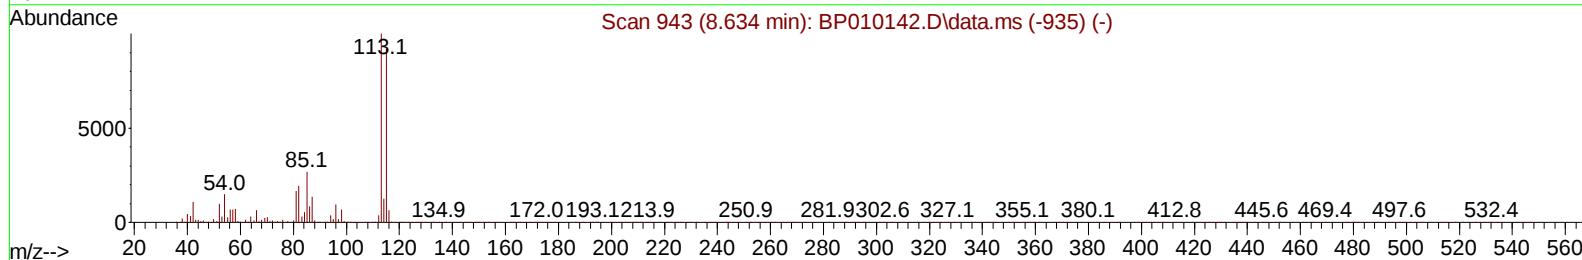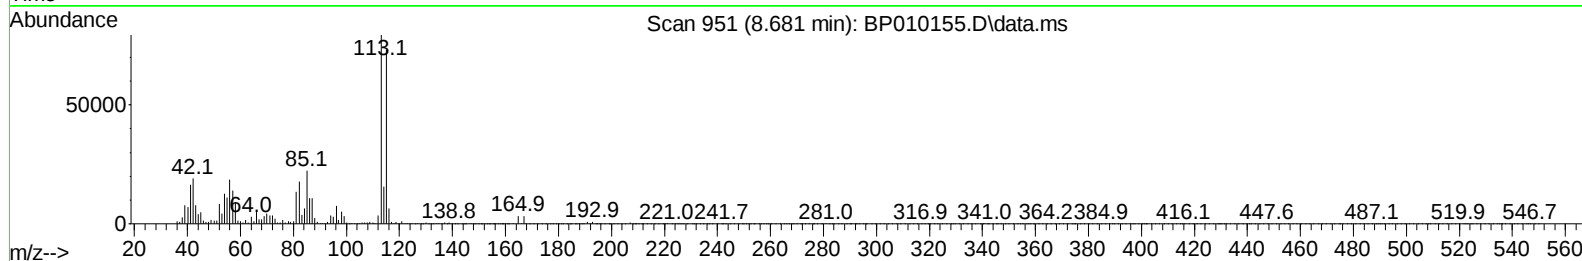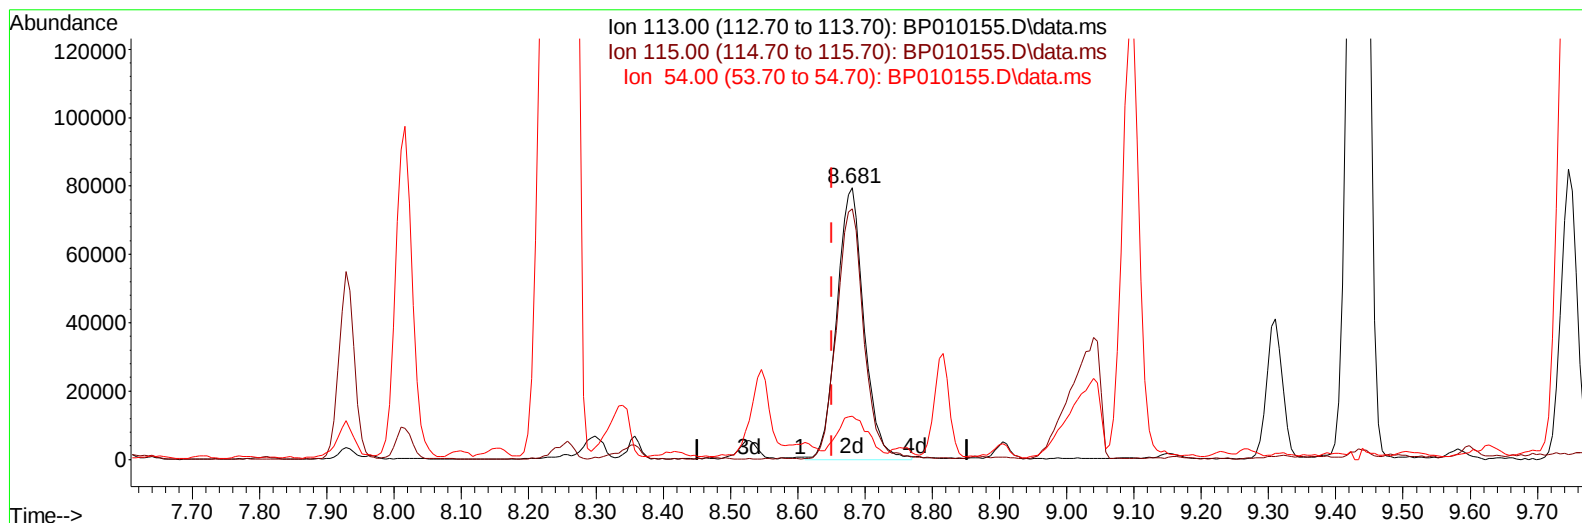

TIC: BP010155.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.681min (+ 0.030) 21.16 ng/ul m

response 221675

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	106.70	92.38
54.00	4.50	16.01#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010155.D
 Acq On : 29 Apr 2022 17:16
 Operator : CG/JU
 Sample : N2587-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

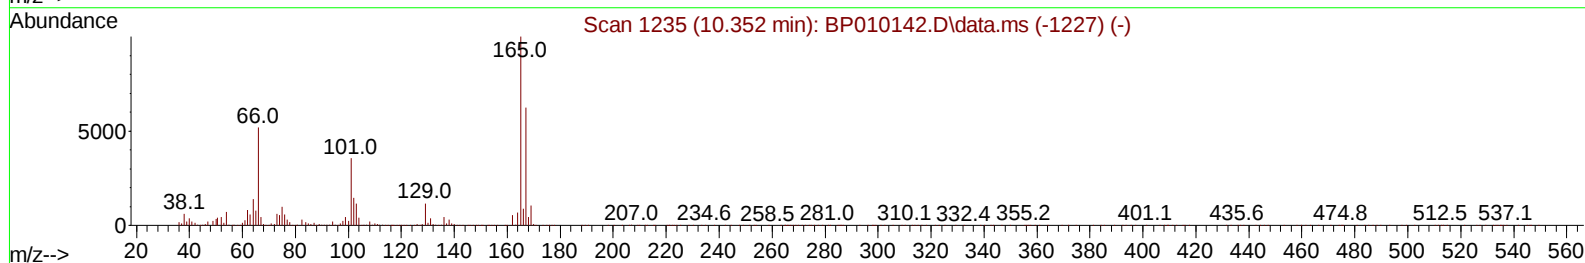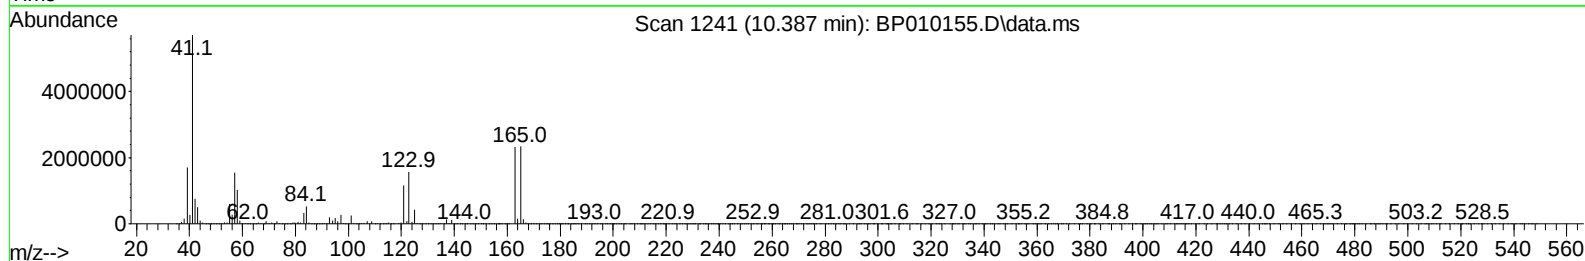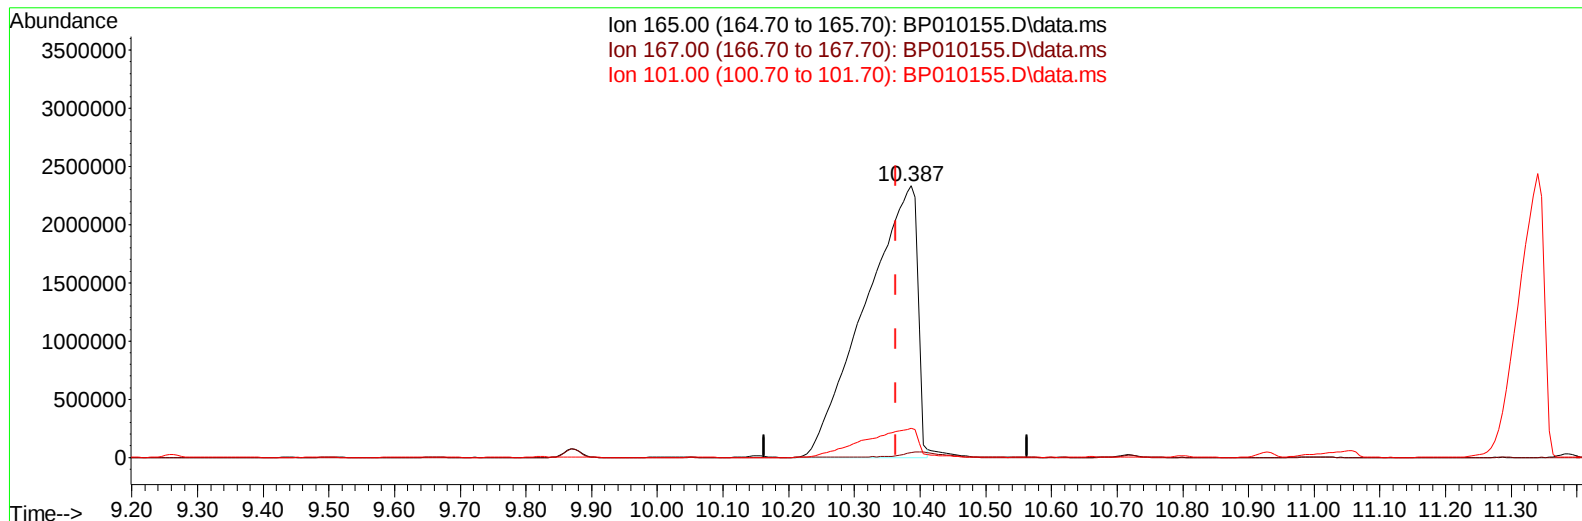

TIC: BP010155.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.387min (+ 0.024) 1369.34 ng/u1

response 12813255

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	1.91#
101.00	49.80	10.66#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010155.D
Acq On : 29 Apr 2022 17:16
Operator : CG/JU
Sample : N2587-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

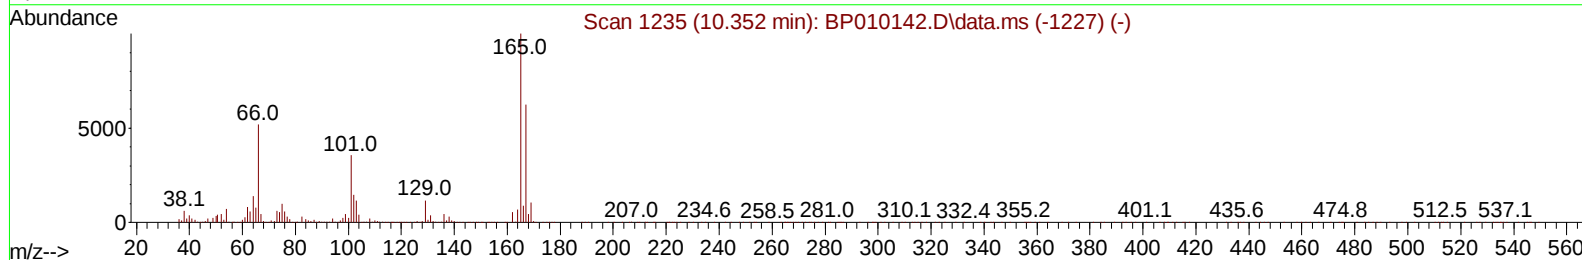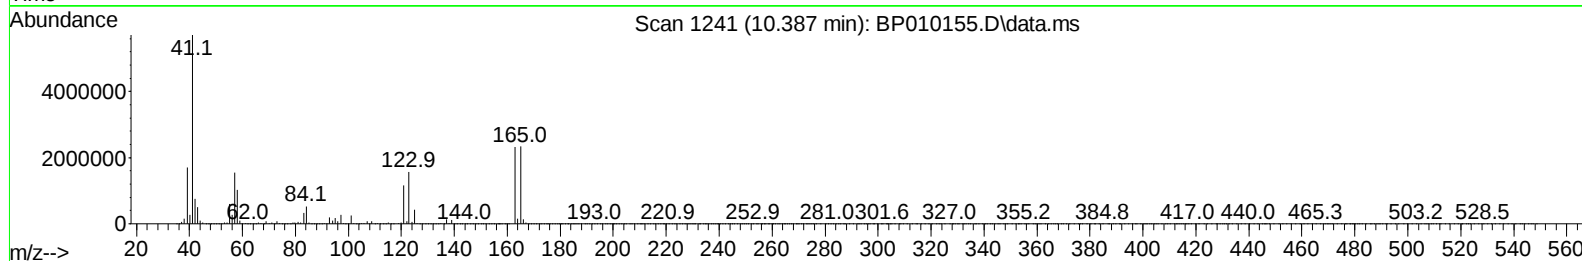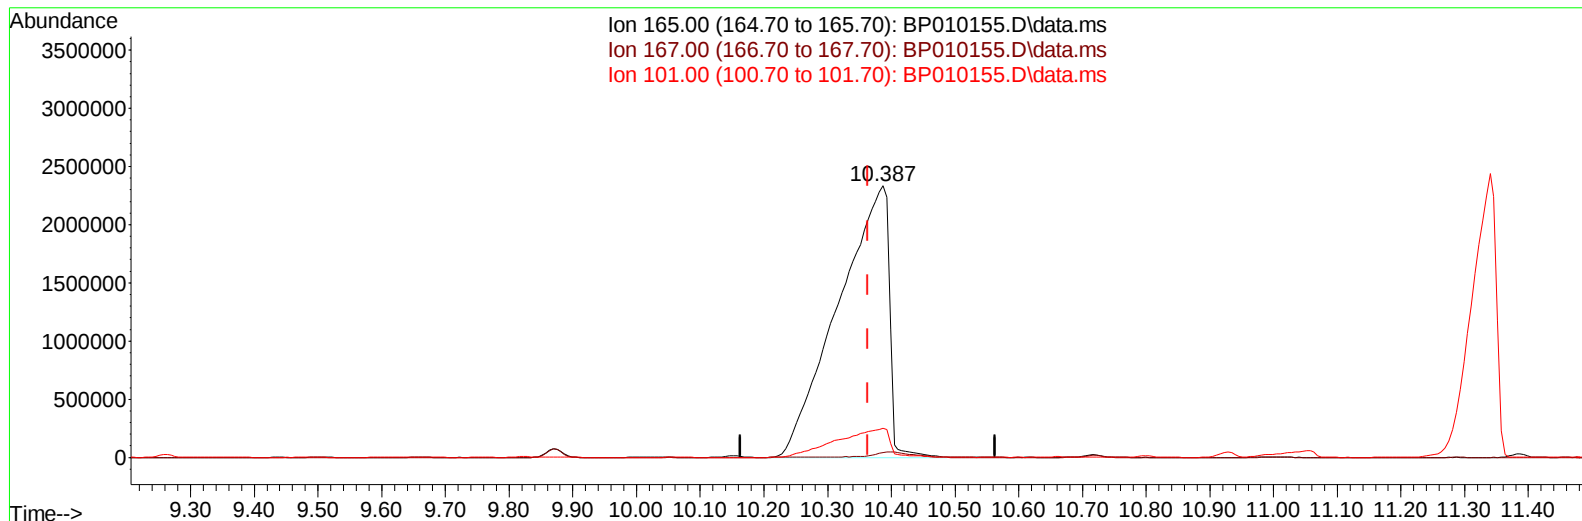

TIC: BP010155.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.387min (+ 0.024) 1383.31 ng/ul m

response 12943988

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	1.91#
101.00	49.80	10.66#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010155.D
Acq On : 29 Apr 2022 17:16
Operator : CG/JU
Sample : N2587-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

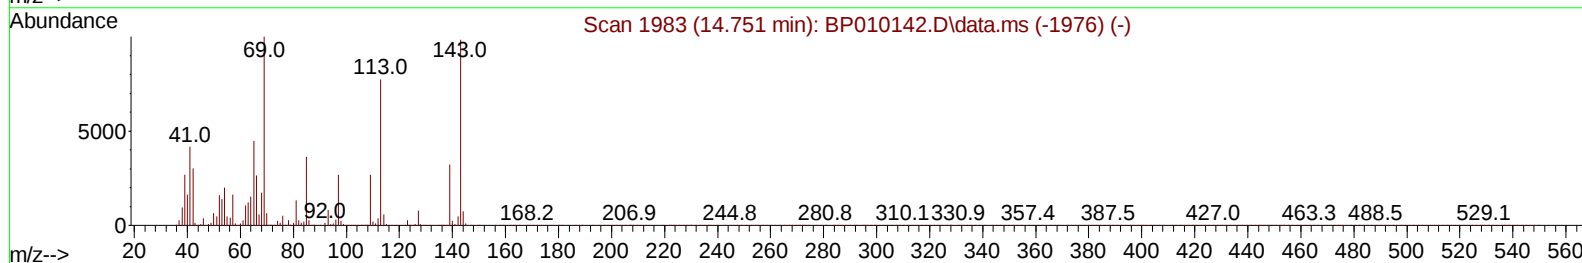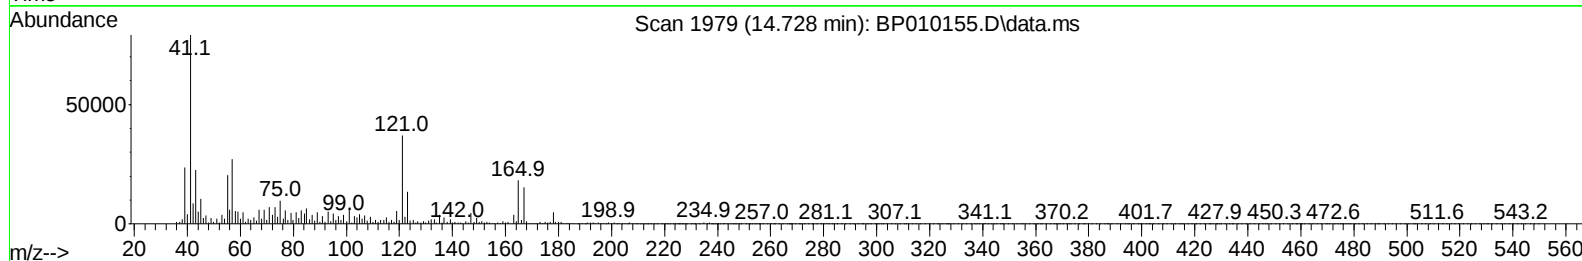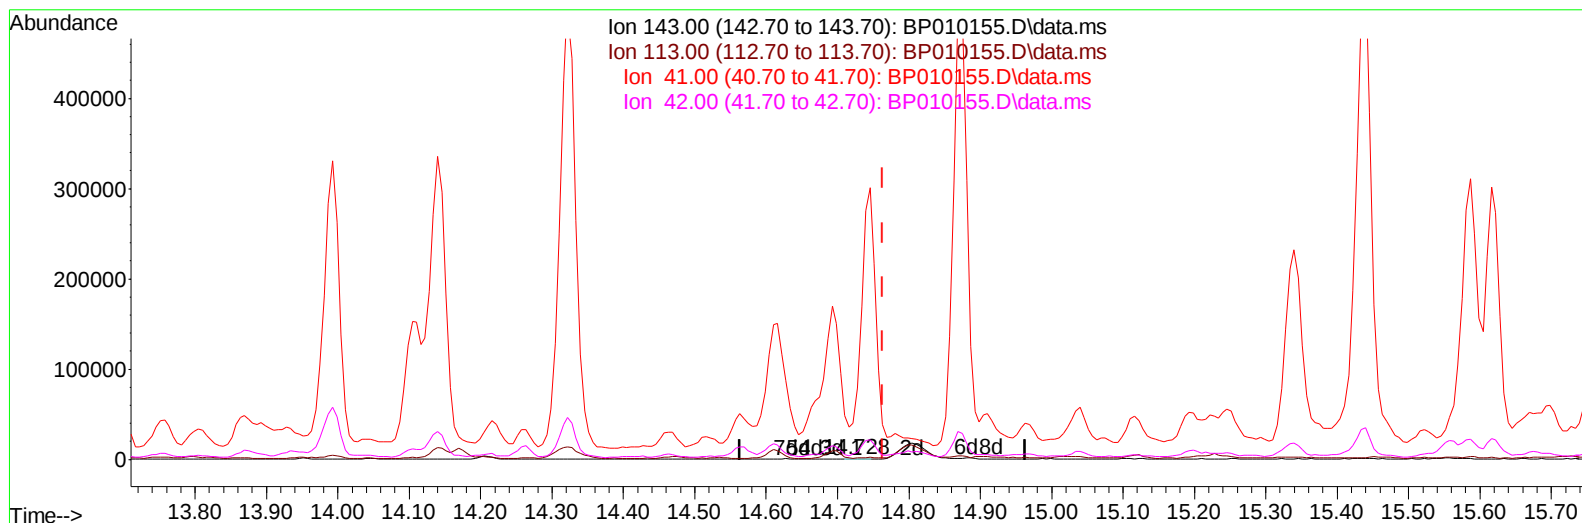

TIC: BP010155.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (-0.035) 0.08 ng/u1

response 409

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	281.71#
41.00	23.20	13284.56#
42.00	18.00	1437.58#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010155.D
Acq On : 29 Apr 2022 17:16
Operator : CG/JU
Sample : N2587-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

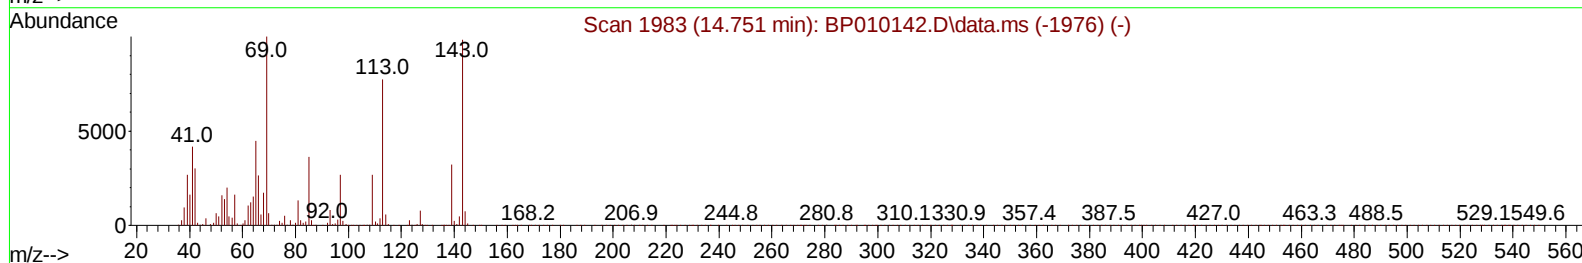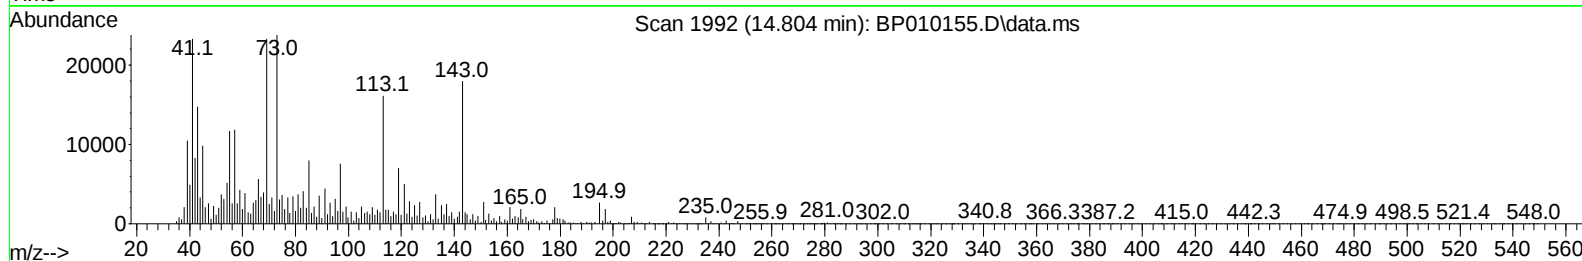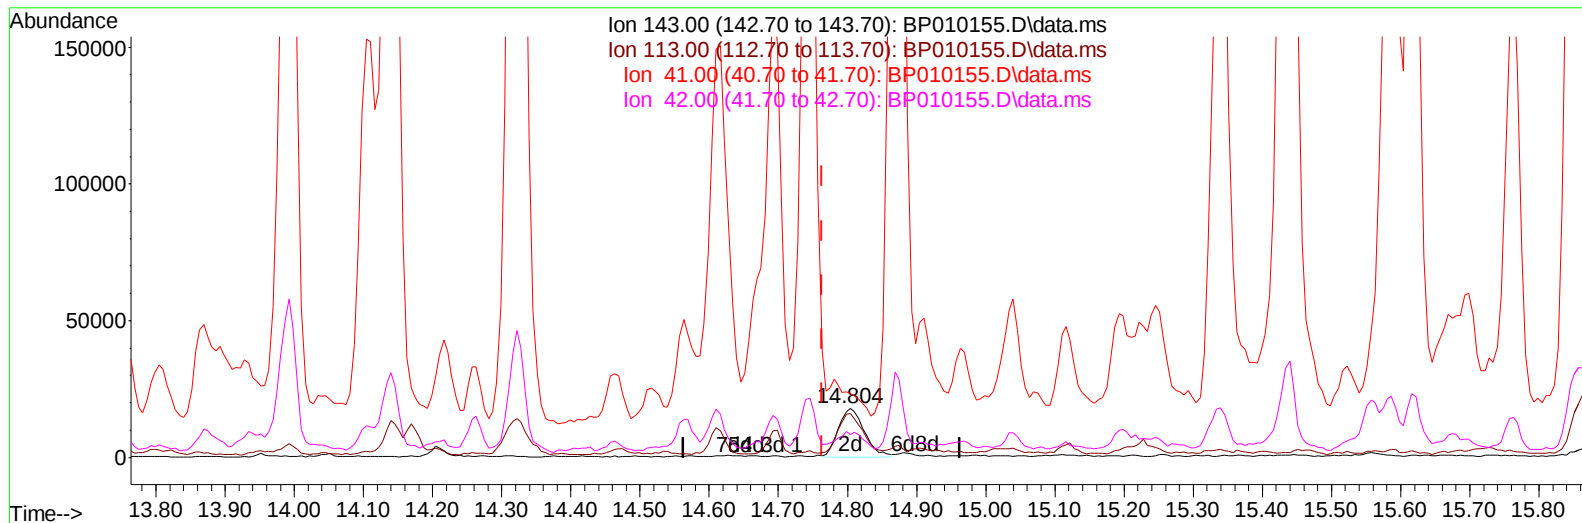

TIC: BP010155.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (+ 0.041) 9.15 ng/ul m

response 46607

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	89.88#
41.00	23.20	129.80#
42.00	18.00	46.48#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010155.D
 Acq On : 29 Apr 2022 17:16
 Operator : CG/JU
 Sample : N2587-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXET5

Manual IntegrationsAPPROVED

Quant Time: Apr 30 00:31:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 21 14:49:38 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/02/2022
 Supervised By :Yogesh Patel 05/05/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	139021	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.746	136	553357	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.569	164	355629	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.316	188	725524	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.398	240	712458	20.000	ng/ul	#-0.01
88) Perylene-d12	23.845	264	699864	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.370	96	18605m	5.836	ng/uL	0.00
4) Pyridine-d5	3.805	84	110241	12.292	ng/ul	0.02
7) Phenol-d5	7.122	99	117013	9.254	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.263	67	269919	35.573	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	277864	29.671	ng/ul	0.00
15) 4-Methylphenol-d8	8.681	113	221675m	21.158	ng/ul	0.03
21) Nitrobenzene-d5	9.099	128	166378	37.804	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	182506	37.970	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	12943988m	1383.312	ng/ul	0.02
31) 4-Chloroaniline-d4	10.910	131	326340	24.323	ng/ul	0.03
46) Dimethylphthalate-d6	13.987	166	998403	36.090	ng/ul	0.00
49) Acenaphthylene-d8	14.263	160	1197716	35.773	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	46607m	9.151	ng/ul	0.04
60) Fluorene-d10	15.557	176	882369	37.079	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200	179466	39.120	ng/ul	0.00
73) Anthracene-d10	17.416	188	1350775	38.483	ng/ul	0.00
81) Pyrene-d10	19.645	212	1569194	38.729	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.692	264	1446693	39.429	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010155.D
Acq On : 29 Apr 2022 17:16
Operator : CG/JU
Sample : N2587-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXET5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/02/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: Apr 30 00:31:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 21 14:49:38 2022
Response via : Initial Calibration

