

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010145.D
 Acq On : 29 Apr 2022 11:41
 Operator : CG/JU
 Sample : N2587-14
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXES9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	43	47	54	rVB	33148	44451	1.18%	0.132%
2	3.793	118	120	130	rBV	33739	60287	1.60%	0.178%
3	4.111	170	174	178	rBV3	11480	15594	0.42%	0.046%
4	4.475	232	236	238	rVB3	4464	4599	0.12%	0.014%
5	5.463	400	404	410	rBV6	2736	5370	0.14%	0.016%
6	5.969	486	490	495	rVB7	2918	5345	0.14%	0.016%
7	6.934	650	654	656	rBV4	3447	3945	0.11%	0.012%
8	7.093	672	681	694	rBV2	113518	232846	6.20%	0.689%
9	7.257	702	709	722	rBV	457918	765677	20.38%	2.267%
10	7.457	736	743	752	rBV	467643	754974	20.10%	2.235%
11	7.928	816	823	830	rBV	520530	841320	22.39%	2.491%
12	8.004	833	836	840	rVB5	6222	8390	0.22%	0.025%
13	8.169	860	864	866	rBV4	4206	5900	0.16%	0.017%
14	8.634	934	943	957	rBV2	333152	572100	15.23%	1.694%
15	8.834	974	977	981	rVB4	3117	5578	0.15%	0.017%
16	9.087	1011	1020	1032	rBV	581696	989347	26.33%	2.929%
17	9.257	1043	1049	1055	rBV5	17808	29565	0.79%	0.088%
18	9.540	1090	1097	1101	rBV	36178	58598	1.56%	0.173%
19	9.746	1126	1132	1135	rBV6	2646	5354	0.14%	0.016%
20	9.810	1135	1143	1152	rBV	448167	781343	20.80%	2.313%
21	10.240	1212	1216	1222	rVB7	4714	7630	0.20%	0.023%
22	10.351	1228	1235	1249	rBV	599699	1064789	28.34%	3.152%
23	10.734	1290	1300	1311	rBV	675686	1156842	30.79%	3.425%
24	10.869	1316	1323	1338	rBV	414019	820604	21.84%	2.430%
25	11.281	1390	1393	1399	rVB8	2323	3968	0.11%	0.012%
26	11.545	1432	1438	1441	rBV8	4073	7861	0.21%	0.023%
27	12.034	1516	1521	1526	rVB5	5470	9691	0.26%	0.029%
28	12.169	1538	1544	1550	rVB5	7633	13023	0.35%	0.039%
29	12.328	1565	1571	1580	rBV4	12215	24756	0.66%	0.073%
30	12.434	1584	1589	1594	rVB9	2699	6427	0.17%	0.019%
31	12.810	1647	1653	1655	rBV7	3011	5400	0.14%	0.016%
32	12.939	1671	1675	1679	rVV7	3039	4415	0.12%	0.013%
33	12.981	1679	1682	1687	rVB7	3695	5947	0.16%	0.018%
34	13.116	1701	1705	1707	rBV5	3847	4984	0.13%	0.015%
35	13.181	1711	1716	1719	rBV7	3284	4833	0.13%	0.014%
36	13.398	1748	1753	1760	rBV	15477	23172	0.62%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010145.D
 Acq On : 29 Apr 2022 11:41
 Operator : CG/JU
 Sample : N2587-14
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXES9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	13.492	1763	1769	1774	rVV5	18460	31284	0.83%	0.093%
38	13.528	1774	1775	1781	rVB4	3576	5799	0.15%	0.017%
39	13.969	1844	1850	1862	rBV	1307703	1864723	49.63%	5.521%
40	14.092	1869	1871	1877	rVB6	3102	4803	0.13%	0.014%
41	14.257	1892	1899	1912	rVB	1383613	2054219	54.68%	6.082%
42	14.469	1929	1935	1941	rBV3	7214	11599	0.31%	0.034%
43	14.563	1944	1951	1963	rBV	995550	1479808	39.39%	4.381%
44	14.757	1978	1984	1999	rBV	63936	147427	3.92%	0.436%
45	14.981	2018	2022	2026	rBV6	3850	6950	0.18%	0.021%
46	15.198	2053	2059	2060	rBV6	2766	4209	0.11%	0.012%
47	15.245	2064	2067	2073	rVB6	6425	11411	0.30%	0.034%
48	15.369	2083	2088	2094	rBV3	9717	18095	0.48%	0.054%
49	15.422	2094	2097	2102	rVB5	7894	10947	0.29%	0.032%
50	15.557	2112	2120	2134	rBV	1820916	2724276	72.51%	8.066%
51	15.675	2134	2140	2150	rBV	703085	1007074	26.81%	2.982%
52	15.798	2157	2161	2171	rVB2	23216	41853	1.11%	0.124%
53	15.928	2180	2183	2188	rVB7	3996	5917	0.16%	0.018%
54	16.133	2213	2218	2222	rVB8	3480	5011	0.13%	0.015%
55	16.286	2240	2244	2249	rVV7	7211	12476	0.33%	0.037%
56	16.345	2251	2254	2260	rVB7	9232	13700	0.36%	0.041%
57	16.992	2358	2364	2371	rBV7	5193	11532	0.31%	0.034%
58	17.086	2376	2380	2386	rBV8	6789	14054	0.37%	0.042%
59	17.316	2412	2419	2428	rBV	1180753	1683514	44.81%	4.984%
60	17.416	2429	2436	2451	rVV	2302956	3252667	86.58%	9.630%
61	17.822	2502	2505	2509	rBV6	4713	7402	0.20%	0.022%
62	17.986	2529	2533	2537	rVB7	7679	13821	0.37%	0.041%
63	18.145	2557	2560	2564	rBV6	13282	19176	0.51%	0.057%
64	18.198	2565	2569	2576	rVV2	62325	100758	2.68%	0.298%
65	18.275	2580	2582	2586	rVB4	10184	11409	0.30%	0.034%
66	18.445	2608	2611	2614	rVB5	12320	12919	0.34%	0.038%
67	19.227	2739	2744	2751	rBV3	28754	46923	1.25%	0.139%
68	19.292	2751	2755	2759	rBV	30370	46598	1.24%	0.138%
69	19.433	2776	2779	2785	rBV8	11949	19442	0.52%	0.058%
70	19.645	2809	2815	2832	rBV	2692582	3757018	100.00%	11.123%
71	21.104	3059	3063	3068	rBV2	188808	241417	6.43%	0.715%
72	21.398	3108	3113	3121	rBV	1226232	1678754	44.68%	4.970%
73	23.692	3496	3503	3511	rBV2	1678475	3363682	89.53%	9.959%
74	23.851	3524	3530	3542	rVB2	790600	1678516	44.68%	4.970%

Sum of corrected areas: 33776108

Instrument :
BNA_P
ClientSampleId :
EXES9

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010145.D
Acq On : 29 Apr 2022 11:41
Operator : CG/JU
Sample : N2587-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXES9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetoxy hexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.104	2.88 ng/ul	241417	Chrysene-d12	21.398

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
2			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
3			1-Heneicosyl formate	340	C22H44O2	077899-03-7	94
4			1-Heneicosanol	312	C21H44O	015594-90-8	94
5			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94

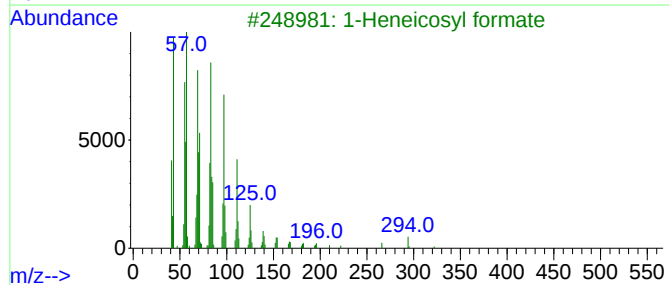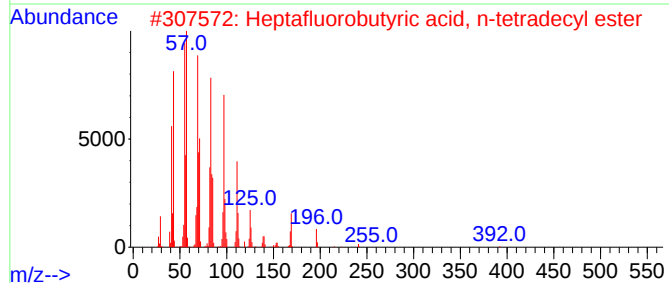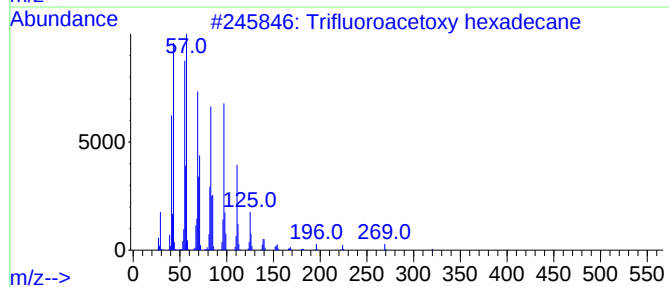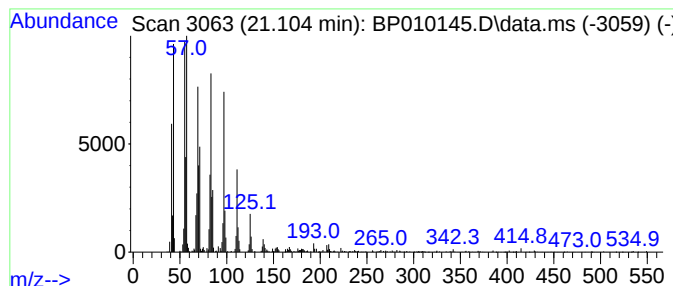

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010145.D
Acq On : 29 Apr 2022 11:41
Operator : CG/JU
Sample : N2587-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXES9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetox...	21.104	2.9	ng/ul	241417	5	21.398	1678750	20.0