

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
 Data File : BP010158.D
 Acq On : 29 Apr 2022 18:57
 Operator : CG/JU
 Sample : PB144448BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	43	46	56	rVB	48803	63577	2.00%	0.178%
2	3.775	114	117	139	rBV	524232	805535	25.31%	2.258%
3	4.105	169	173	180	rVB2	11124	19444	0.61%	0.055%
4	5.358	385	386	390	rBV4	2156	3272	0.10%	0.009%
5	7.087	674	680	697	rBV	616197	1024169	32.18%	2.871%
6	7.252	701	708	726	rVB	523640	838690	26.35%	2.351%
7	7.458	735	743	759	rBV	673490	1084085	34.06%	3.039%
8	7.922	816	822	834	rVB	530091	875068	27.49%	2.453%
9	8.187	863	867	870	rBV5	2146	3429	0.11%	0.010%
10	8.634	935	943	959	rBV	783171	1308434	41.11%	3.668%
11	9.087	1012	1020	1031	rBV	621679	1074449	33.76%	3.012%
12	9.810	1135	1143	1157	rBV	522002	904958	28.43%	2.537%
13	10.351	1227	1235	1254	rBV	718962	1279881	40.21%	3.588%
14	10.728	1290	1299	1312	rBV	708150	1234437	38.78%	3.461%
15	10.863	1315	1322	1337	rBV	683039	1283515	40.33%	3.598%
16	11.381	1405	1410	1415	rVB9	1821	3559	0.11%	0.010%
17	12.328	1562	1571	1581	rBV5	11399	29425	0.92%	0.082%
18	13.969	1843	1850	1862	rBV	1293740	1882627	59.15%	5.278%
19	14.251	1890	1898	1912	rBV	1484674	2196466	69.01%	6.158%
20	14.369	1916	1918	1923	rVB5	2176	3268	0.10%	0.009%
21	14.557	1944	1950	1966	rVB	1037694	1556160	48.89%	4.363%
22	14.757	1977	1984	2008	rBV	356938	817076	25.67%	2.291%
23	15.369	2084	2088	2093	rVB8	3419	6237	0.20%	0.017%
24	15.551	2112	2119	2134	rVV	1859274	2730243	85.78%	7.654%
25	15.669	2134	2139	2152	rVV	543491	809583	25.44%	2.270%
26	15.792	2155	2160	2166	rVB	22967	39707	1.25%	0.111%
27	16.010	2195	2197	2202	rBV6	2153	3436	0.11%	0.010%
28	16.339	2248	2253	2259	rVB9	8579	14348	0.45%	0.040%
29	16.992	2361	2364	2369	rVB7	4147	5343	0.17%	0.015%
30	17.310	2411	2418	2428	rBV	1150145	1759494	55.28%	4.933%
31	17.410	2429	2435	2453	rVB	1932888	2837026	89.14%	7.954%
32	18.251	2576	2578	2584	rBV6	3625	8277	0.26%	0.023%
33	18.916	2687	2691	2694	rBV6	5181	8312	0.26%	0.023%
34	19.222	2739	2743	2750	rVB3	24697	38980	1.22%	0.109%
35	19.292	2750	2755	2760	rBV	26563	44491	1.40%	0.125%
36	19.645	2808	2815	2827	rBV	2194141	3182832	100.00%	8.923%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010158.D
Acq On : 29 Apr 2022 18:57
Operator : CG/JU
Sample : PB144448BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

37	21.398	3108	3113	3128	rBV	1106544	1649069	51.81%	4.623%
38	23.686	3495	3502	3509	rBV2	1313371	2663440	83.68%	7.467%
39	23.845	3522	3529	3539	rVB2	721769	1577476	49.56%	4.422%




Sum of corrected areas: 35669818

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010158.D
Acq On : 29 Apr 2022 18:57
Operator : CG/JU
Sample : PB144448BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

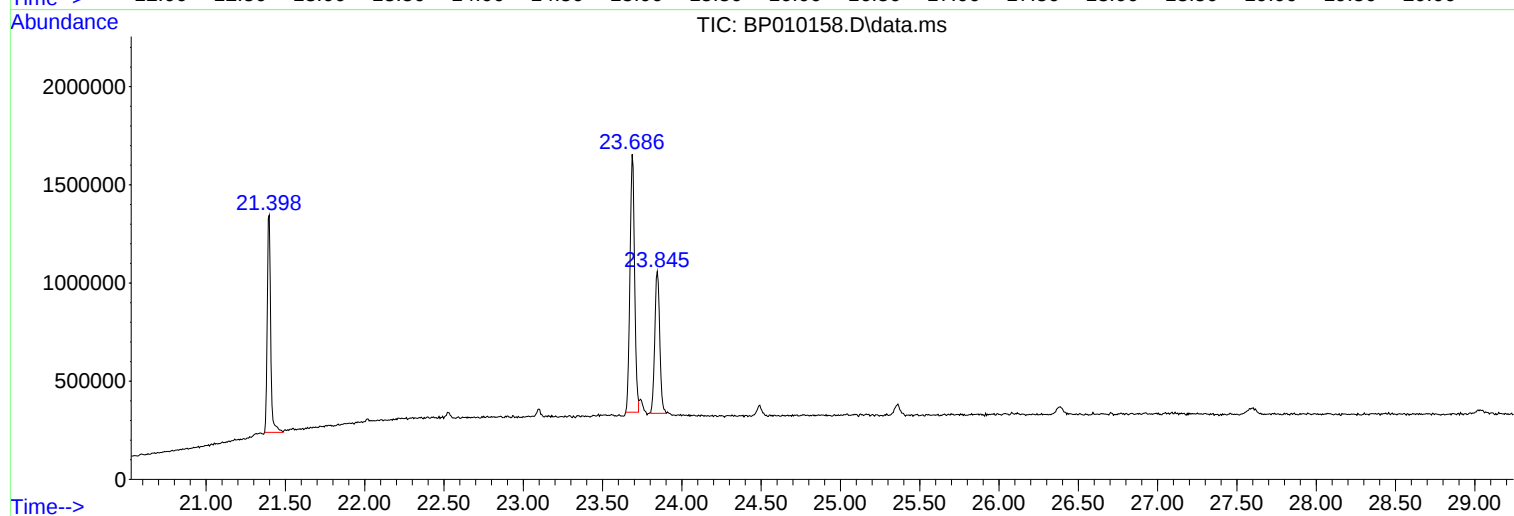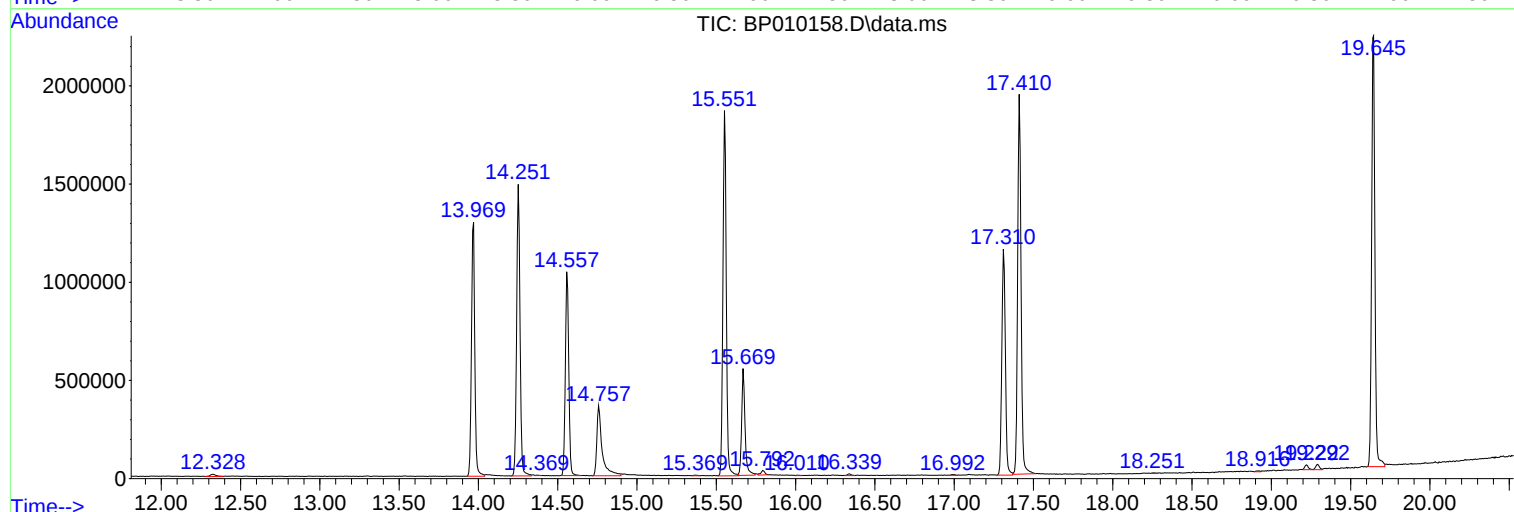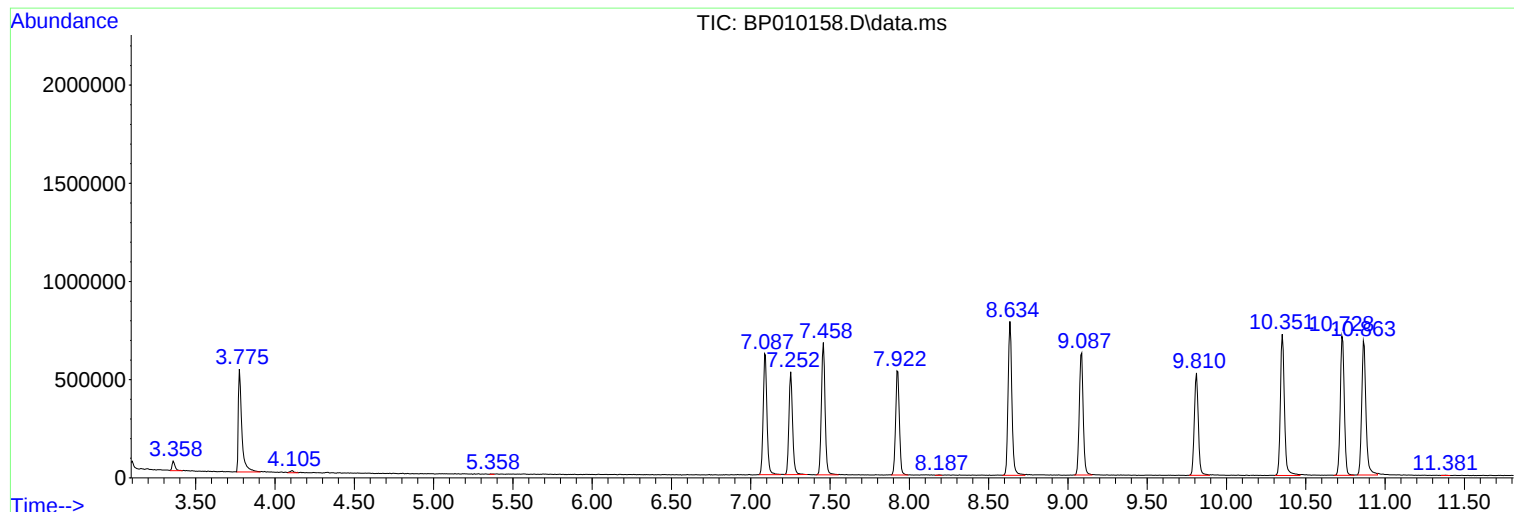

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010158.D
Acq On : 29 Apr 2022 18:57
Operator : CG/JU
Sample : PB144448BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042922\
Data File : BP010158.D
Acq On : 29 Apr 2022 18:57
Operator : CG/JU
Sample : PB144448BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc