
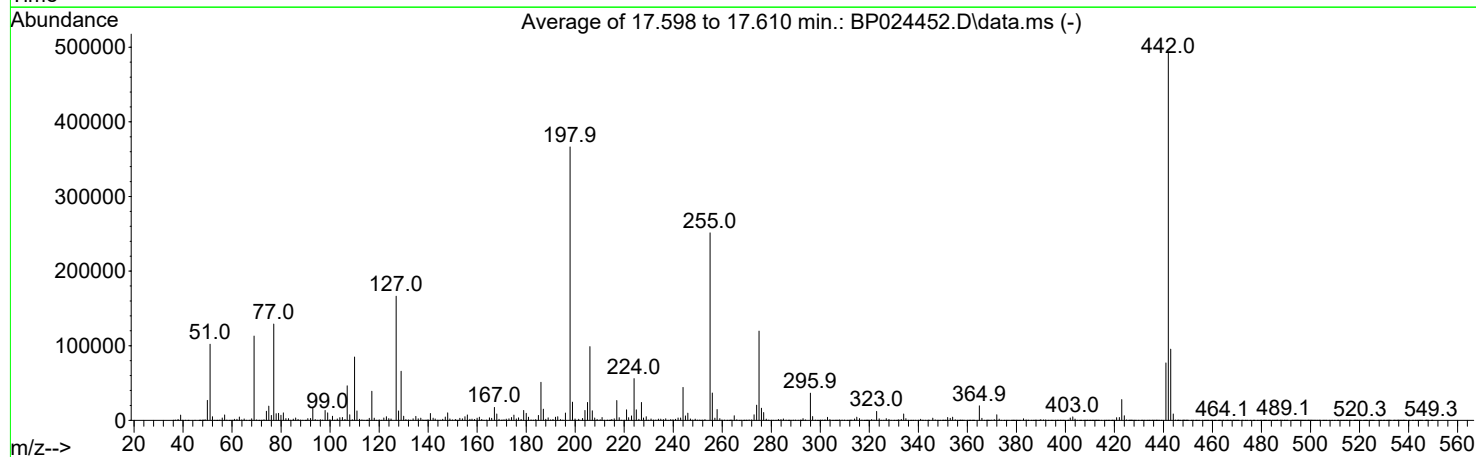


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042925\
Data File : BP024452.D
Acq On : 29 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

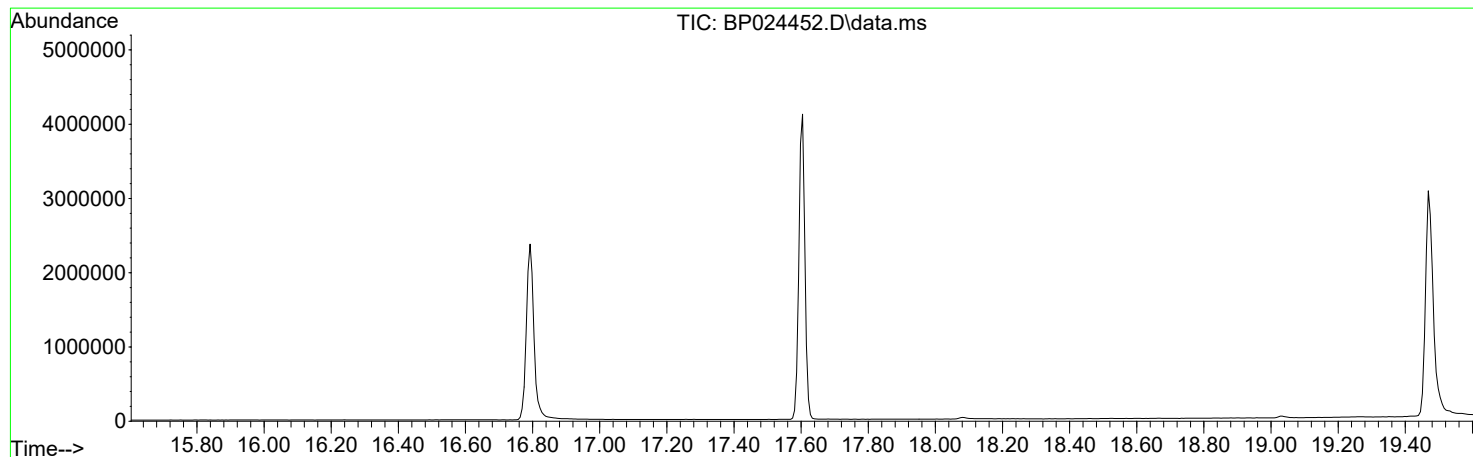

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	102005	PASS
68	69	0.00	2	1.8	2061	PASS
69	198	0.00	100	30.9	113075	PASS
70	69	0.00	2	0.6	622	PASS
127	198	10	80	45.4	166343	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	366336	PASS
199	198	5	9	6.7	24458	PASS
275	198	10	60	32.6	119571	PASS
365	198	1	100	5.3	19574	PASS
441	198	0.01	100	21.0	76973	PASS
442	442	100	100	100.0	492926	PASS
443	442	15	24	19.3	95350	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
4/29/2025	BNA_P	<u>BP024452.D</u>
Compound Name	Response	Retention Time
DDT	1218073	20.763
DDD	47325	20.304
DDE	3100	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
50425	1268498	3.98

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042925\
Data File : BP024452.D
Acq On : 29 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:27:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

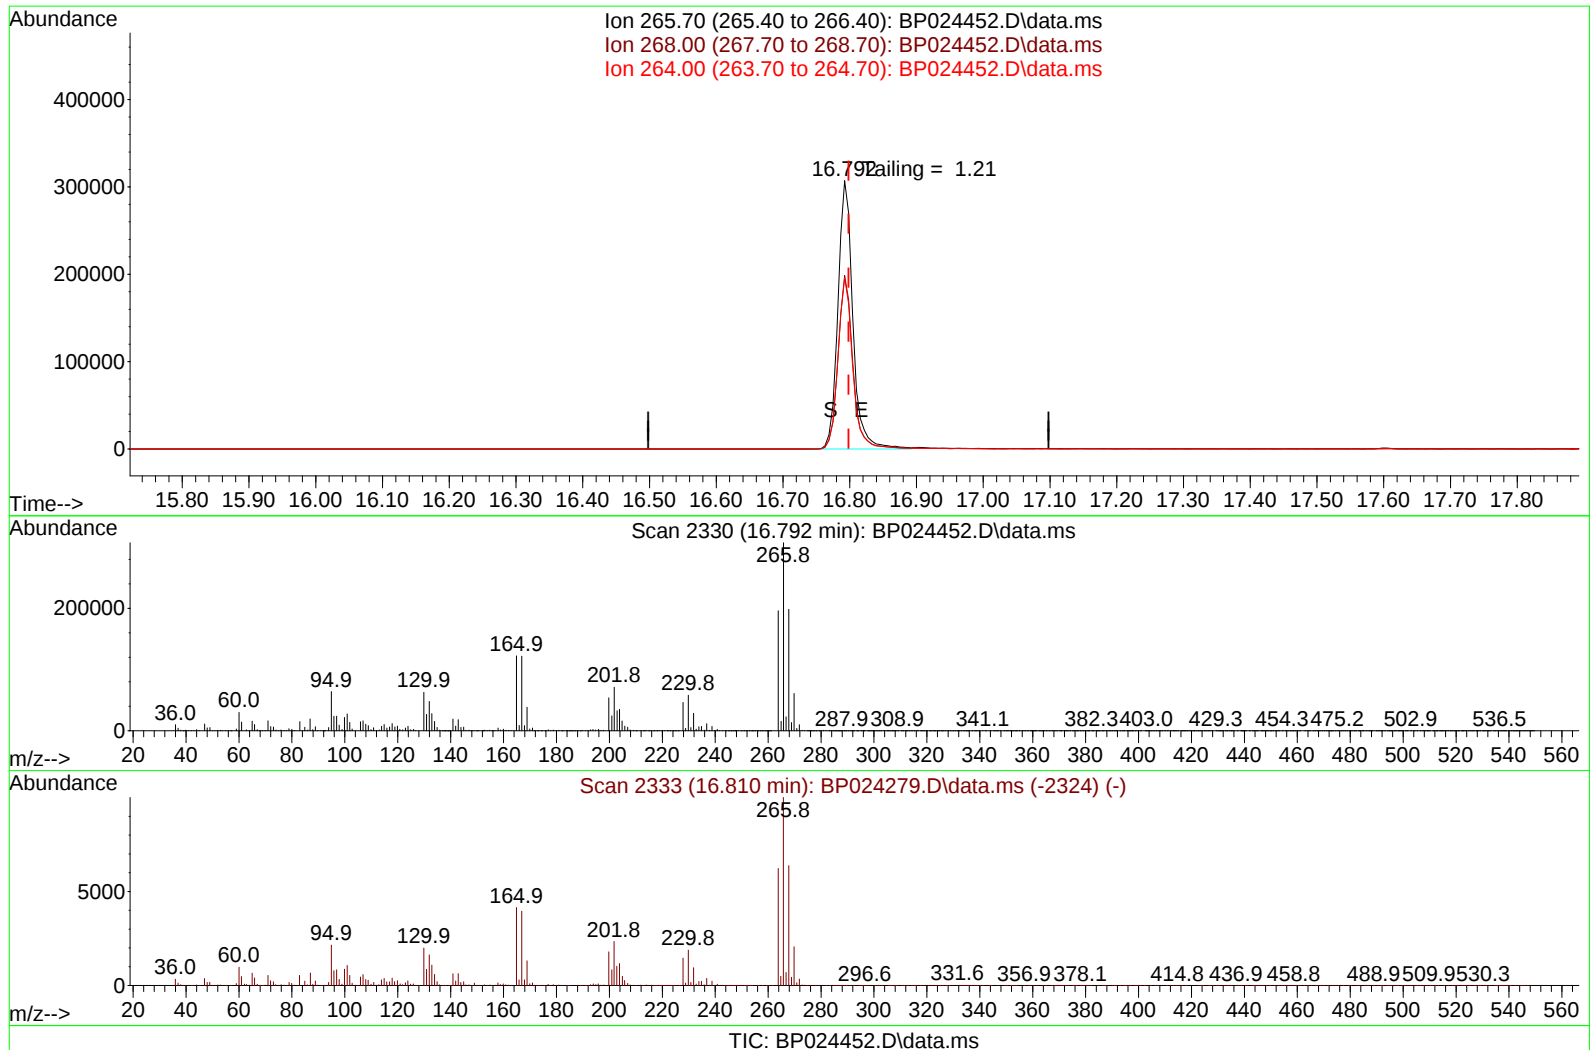

(70) Pentachlorophenol (C)

16.792min (-0.006) 256843.27 ng




response 479697

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.63
264.00	62.20	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP042925\
Data File : BP024452.D
Acq On : 29 Apr 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:27:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

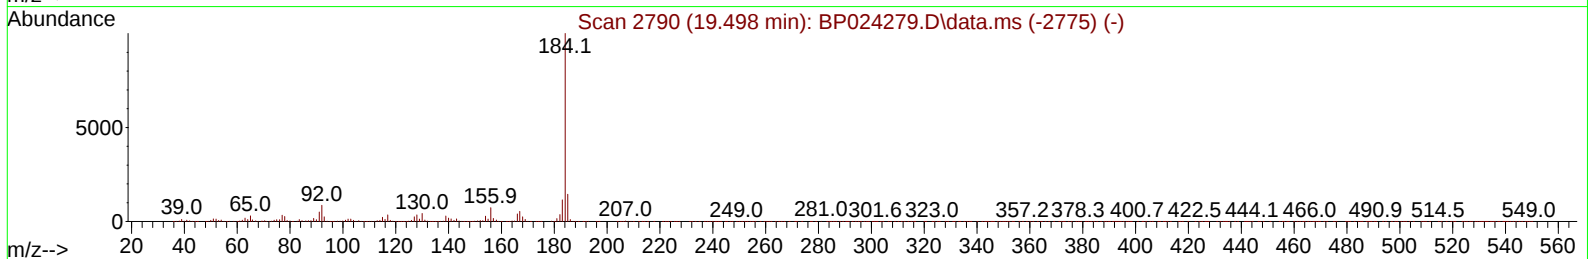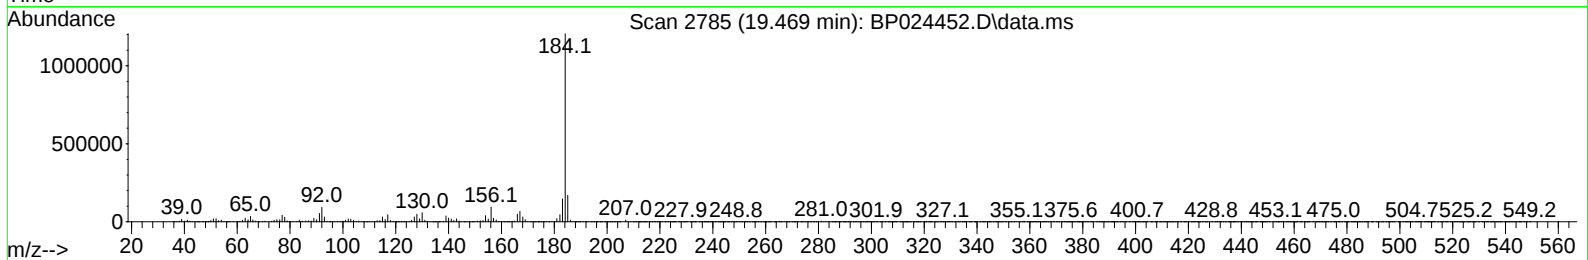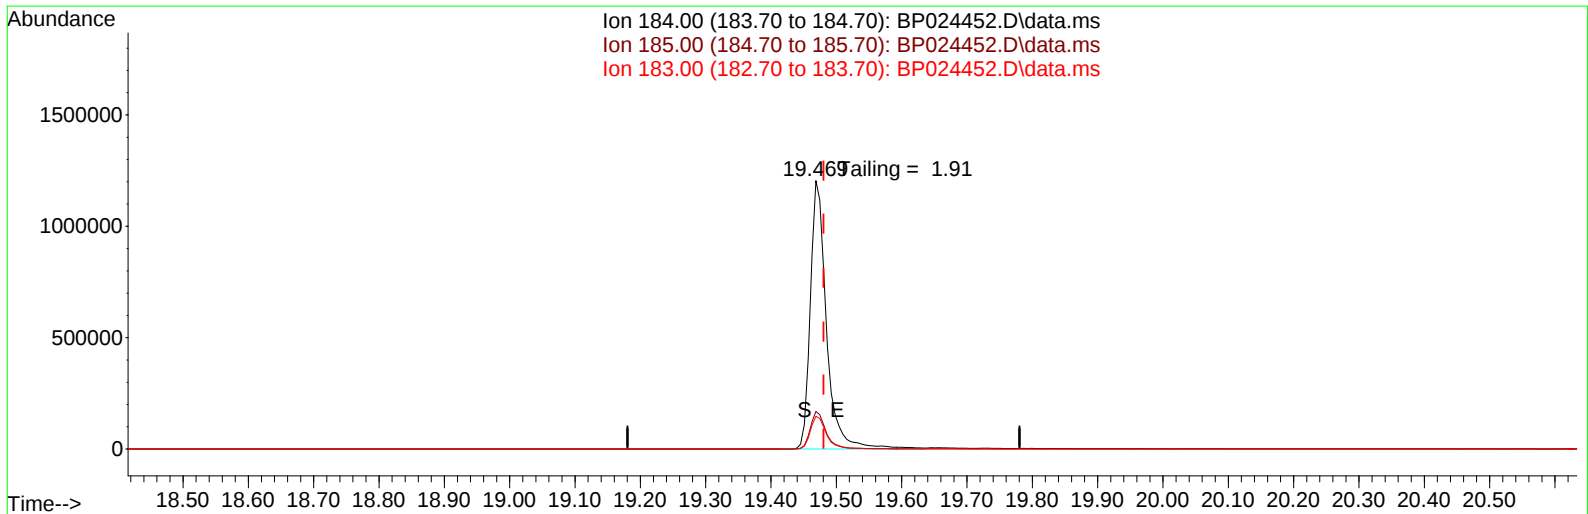

TIC: BP024452.D\data.ms

(77) Benzidine

19.469min (-0.012) 126073.39 ng

response 2077513

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.04
183.00	11.50	12.15
0.00	0.00	0.00