
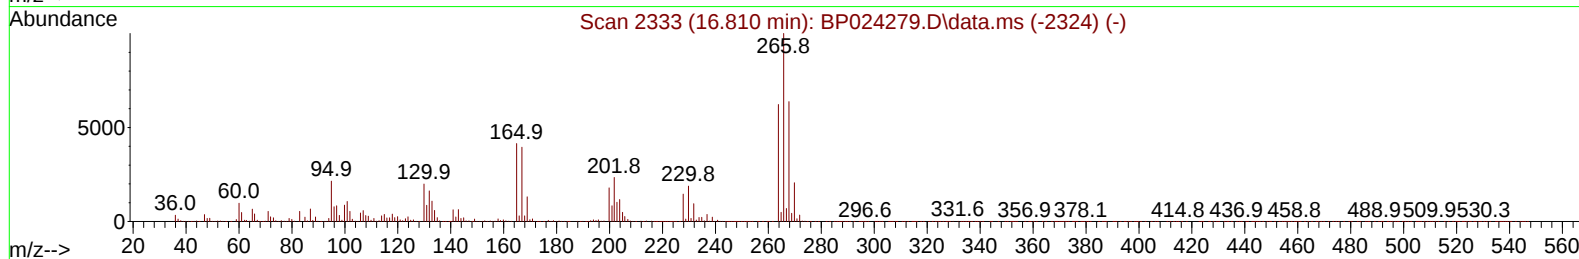
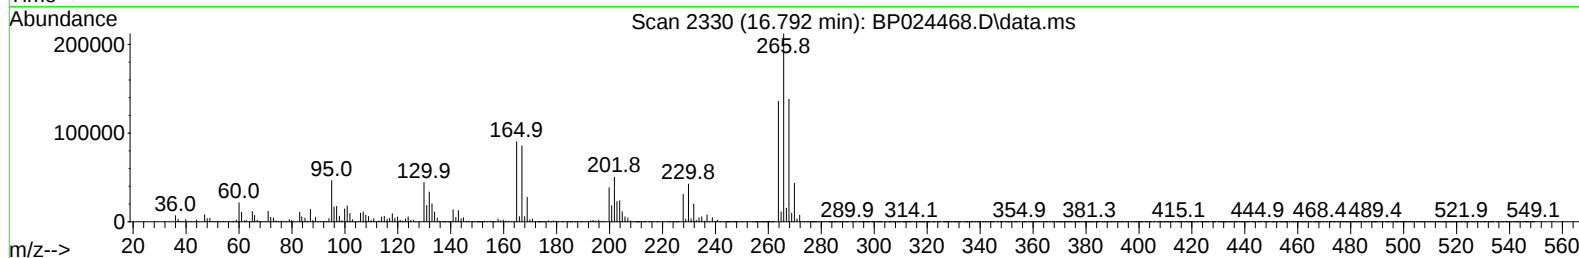


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043025\
Data File : BP024468.D
Acq On : 30 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 11:50:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

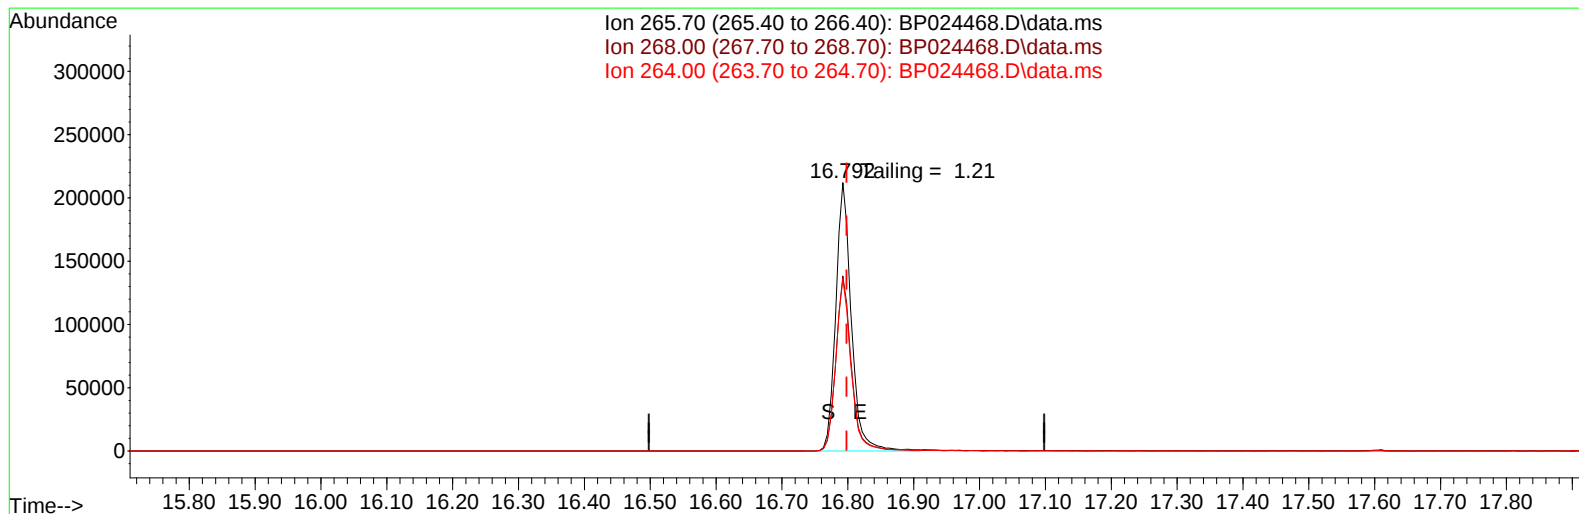

TIC: BP024468.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.006) 14308.85 ng

response 348711

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.21
264.00	62.20	63.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043025\
Data File : BP024468.D
Acq On : 30 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 11:50:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

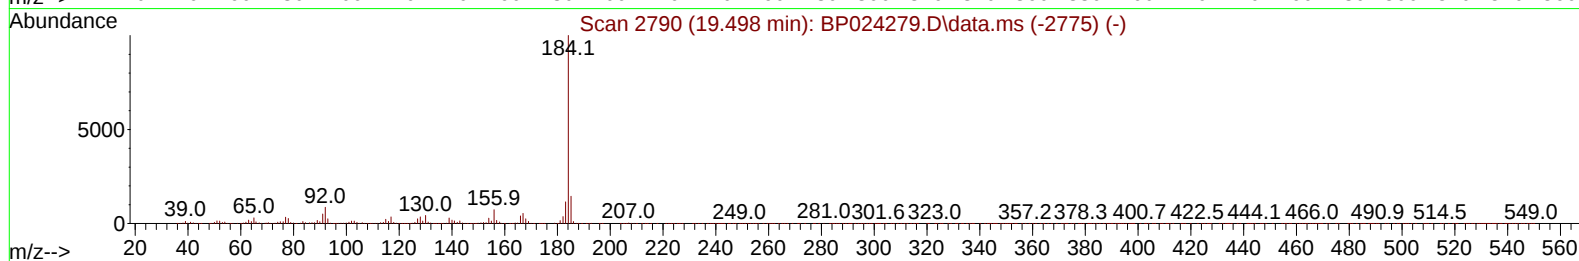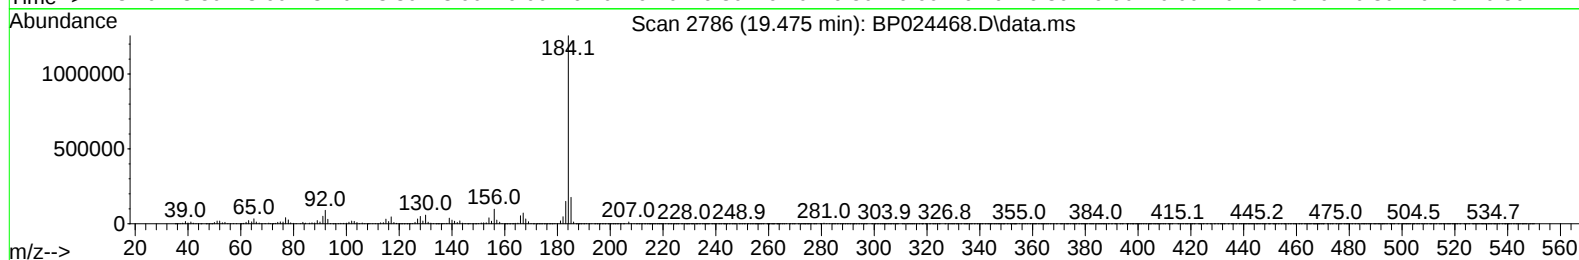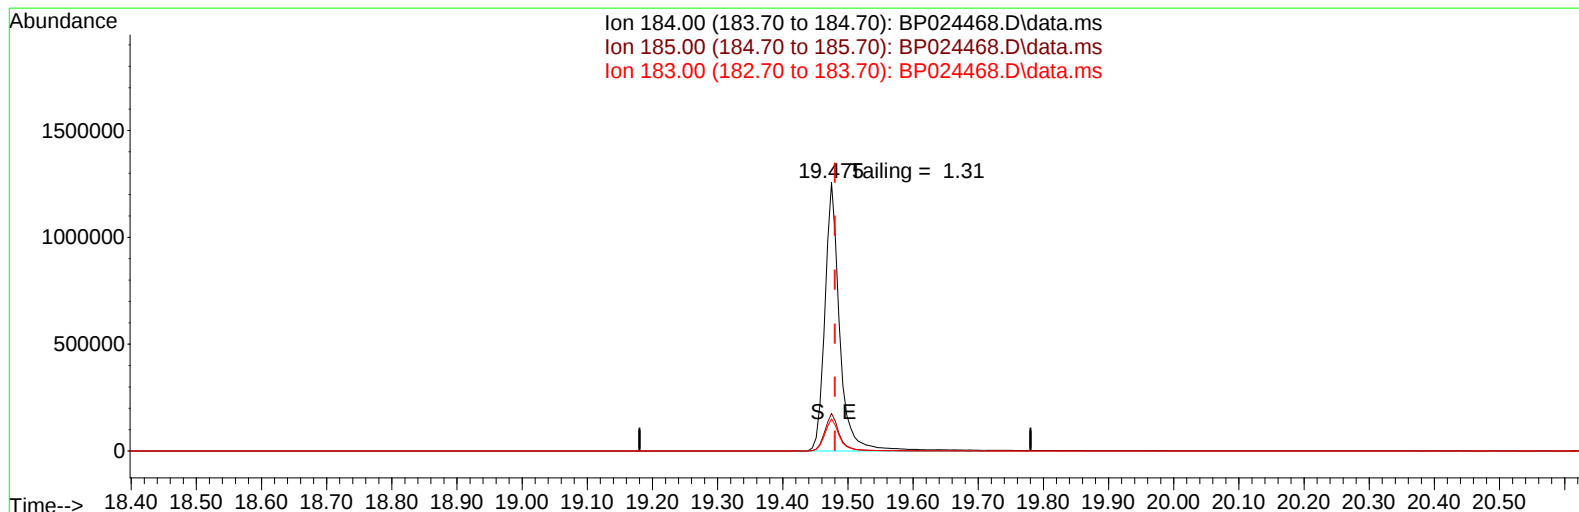

TIC: BP024468.D\data.ms

(77) Benzidine**19.475min (-0.006) 28743.64 ng****response 1983157**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.50	11.93
0.00	0.00	0.00