
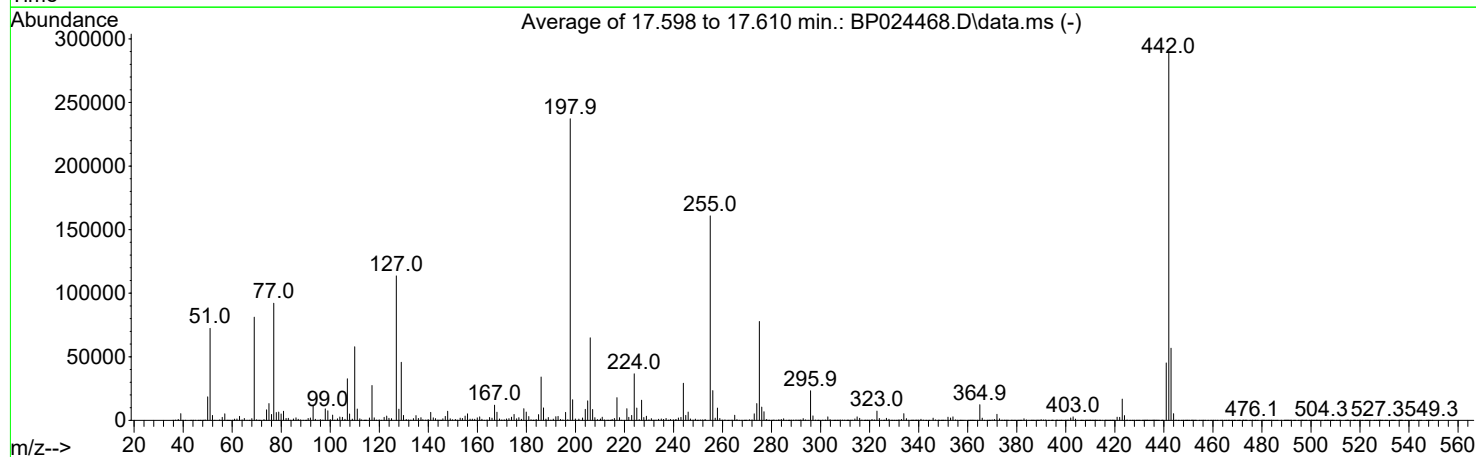


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043025\
Data File : BP024468.D
Acq On : 30 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 18 12:04:48 2025

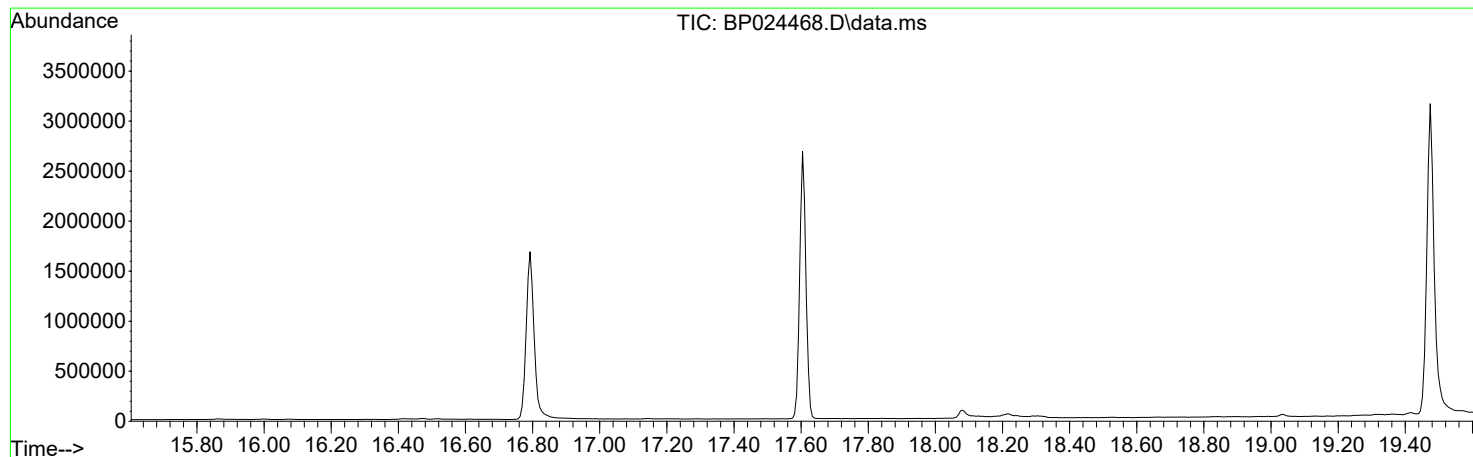

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	72376	PASS
68	69	0.00	2	1.8	1441	PASS
69	198	0.00	100	34.2	81206	PASS
70	69	0.00	2	0.6	514	PASS
127	198	10	80	47.9	113667	PASS
197	198	0.00	2	0.2	552	PASS
198	198	100	100	100.0	237217	PASS
199	198	5	9	6.8	16176	PASS
275	198	10	60	32.8	77785	PASS
365	198	1	100	5.2	12302	PASS
441	198	0.01	100	19.0	45120	PASS
442	442	100	100	100.0	289291	PASS
443	442	15	24	19.6	56794	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/30/2025	BNA_P	<u>BP024468.D</u>
Compound Name	Response	Retention Time
DDT	916900	20.769
DDD	29935	20.304
DDE	1565	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31500	948400	3.32

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043025\
Data File : BP024468.D
Acq On : 30 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 30 11:50:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

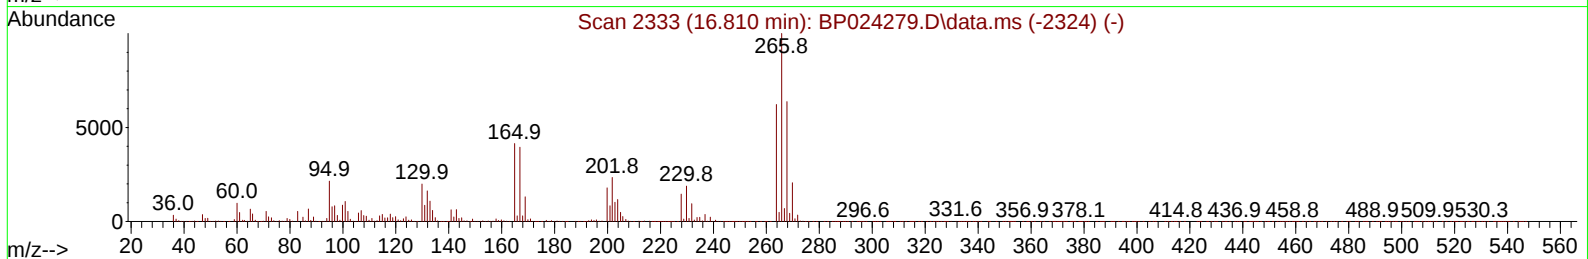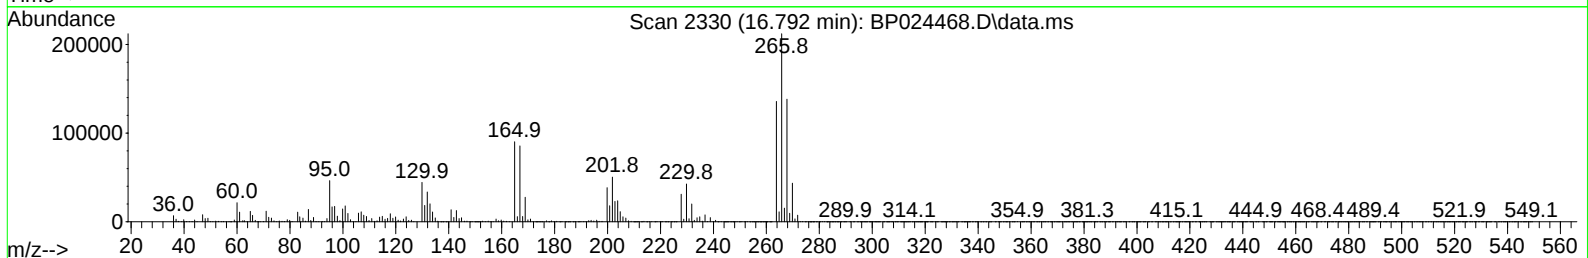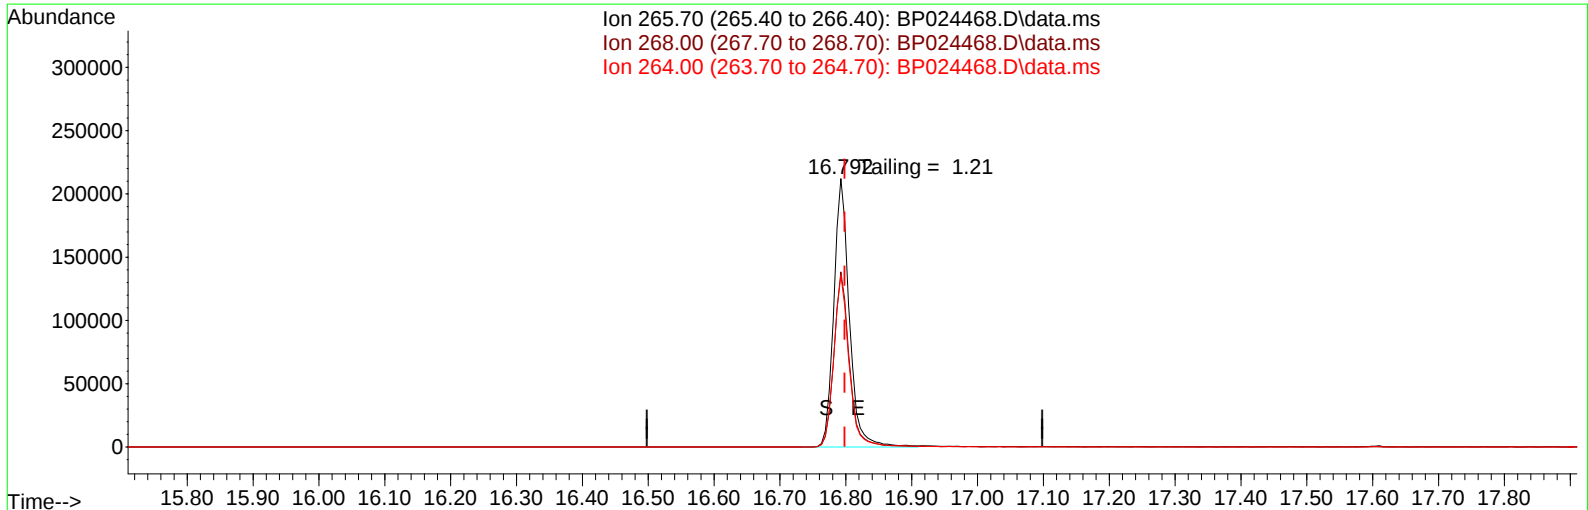

TIC: BP024468.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.006) 14308.85 ng




response 348711

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.21
264.00	62.20	63.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP043025\
Data File : BP024468.D
Acq On : 30 Apr 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 30 11:50:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

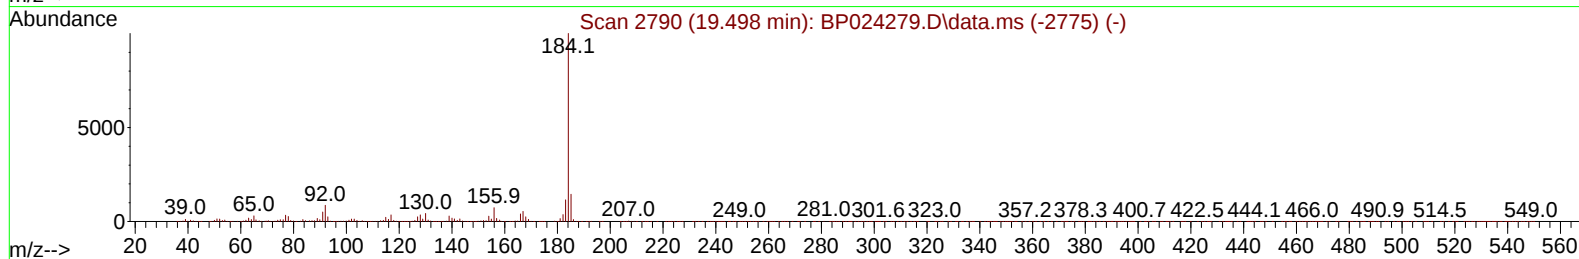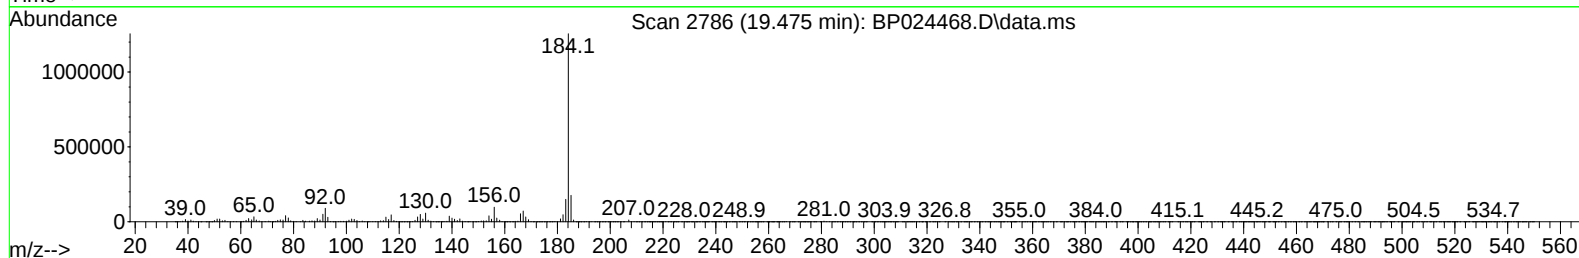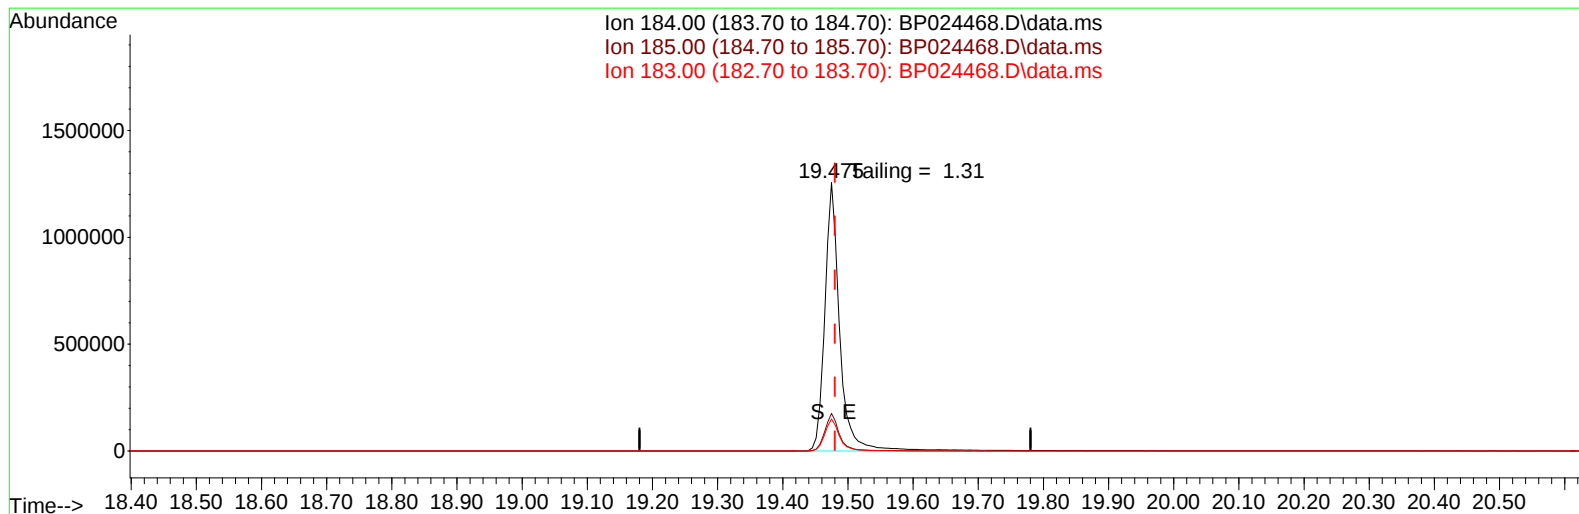

TIC: BP024468.D\data.ms

(77) Benzidine

19.475min (-0.006) 28743.64 ng

response 1983157

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.50	11.93
0.00	0.00	0.00