
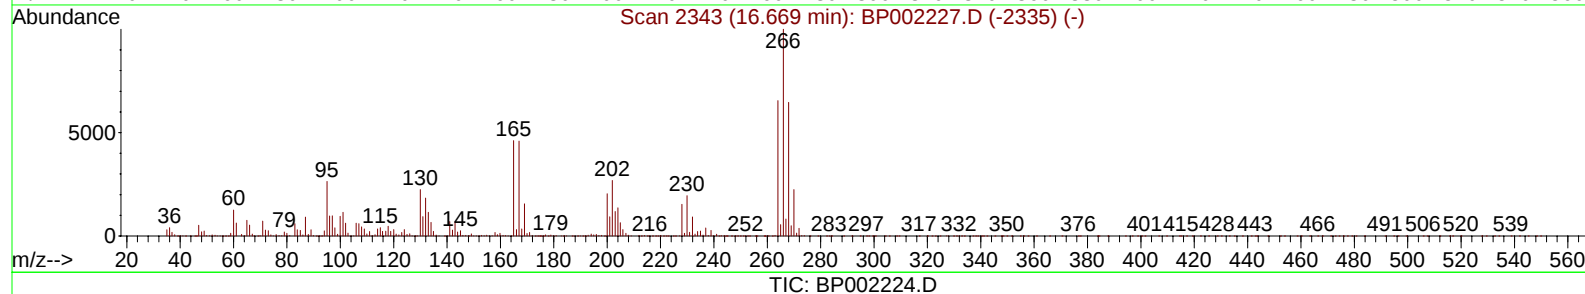
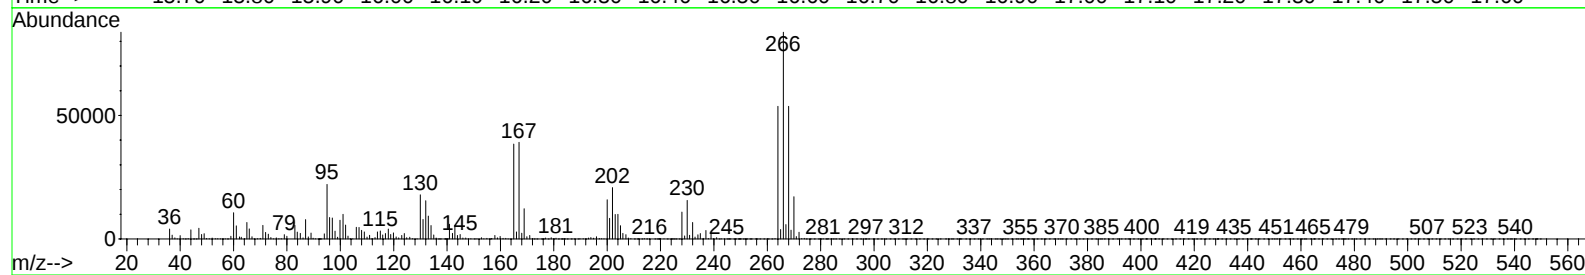


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050420\
Data File : BP002224.D
Acq On : 04 May 2020 14:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 05:34:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP050420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 04 19:53:54 2020
Response via : Initial Calibration

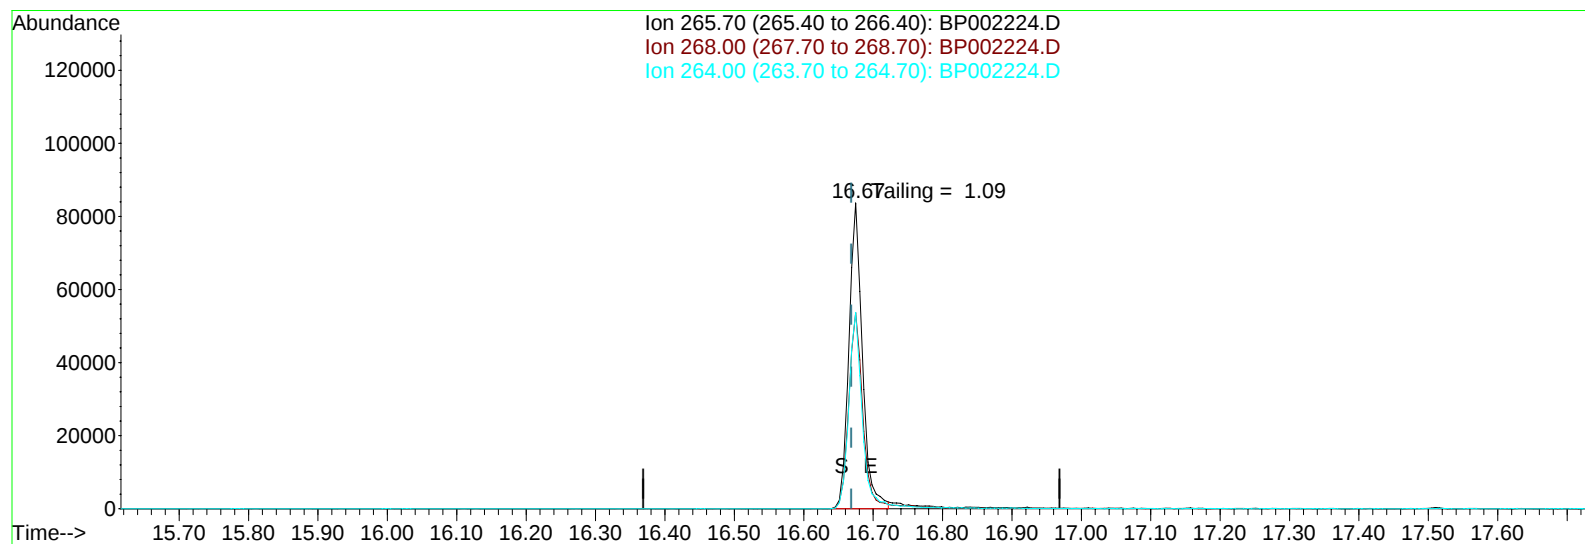

(70) Pentachlorophenol (C)




16.675min (+0.006) 1201716.41ng

response 114097

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	64.18
264.00	65.50	64.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050420\
 Data File : BP002224.D
 Acq On : 04 May 2020 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 05:34:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP050420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 04 19:53:54 2020
 Response via : Initial Calibration

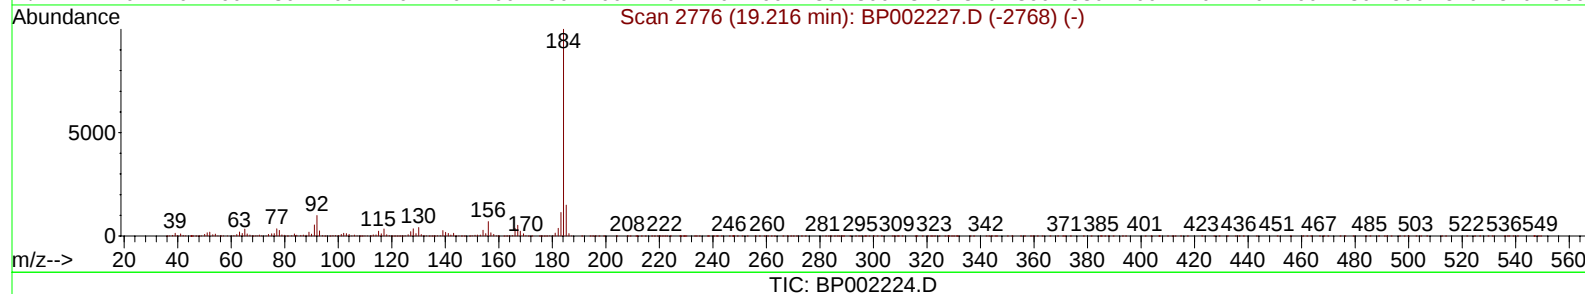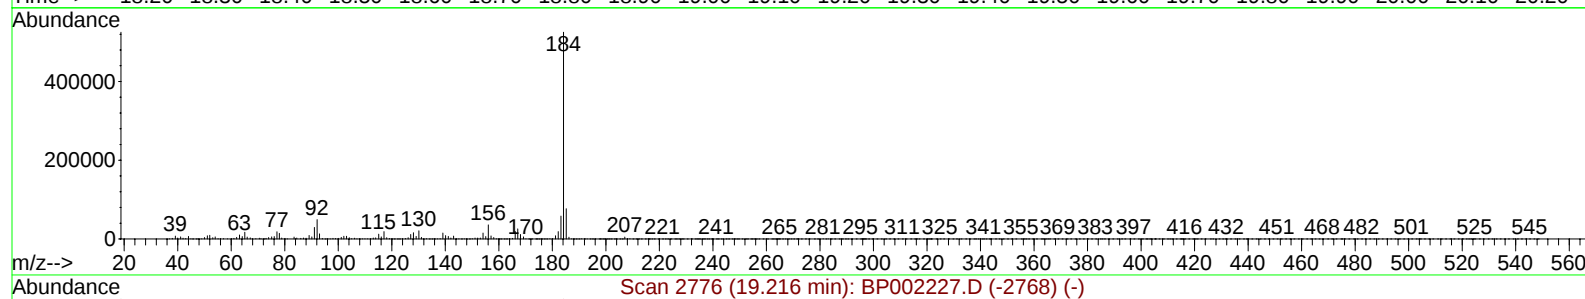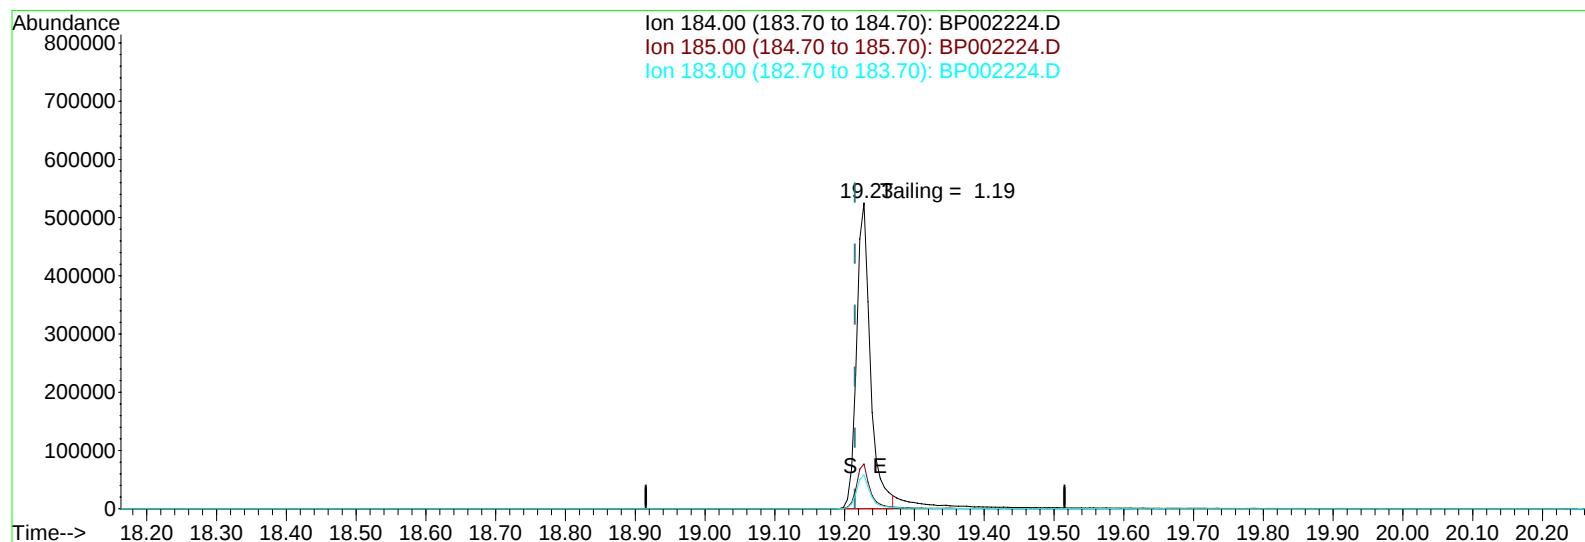

TIC: BP002224.D

(77) Benzidine

19.228min (+0.013) 8915.10ng

response 644792

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	14.65
183.00	11.40	11.10
0.00	0.00	0.00