


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP050420\
 Data File : BP002224.D
 Acq On : 04 May 2020 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP050420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 04 19:53:54 2020

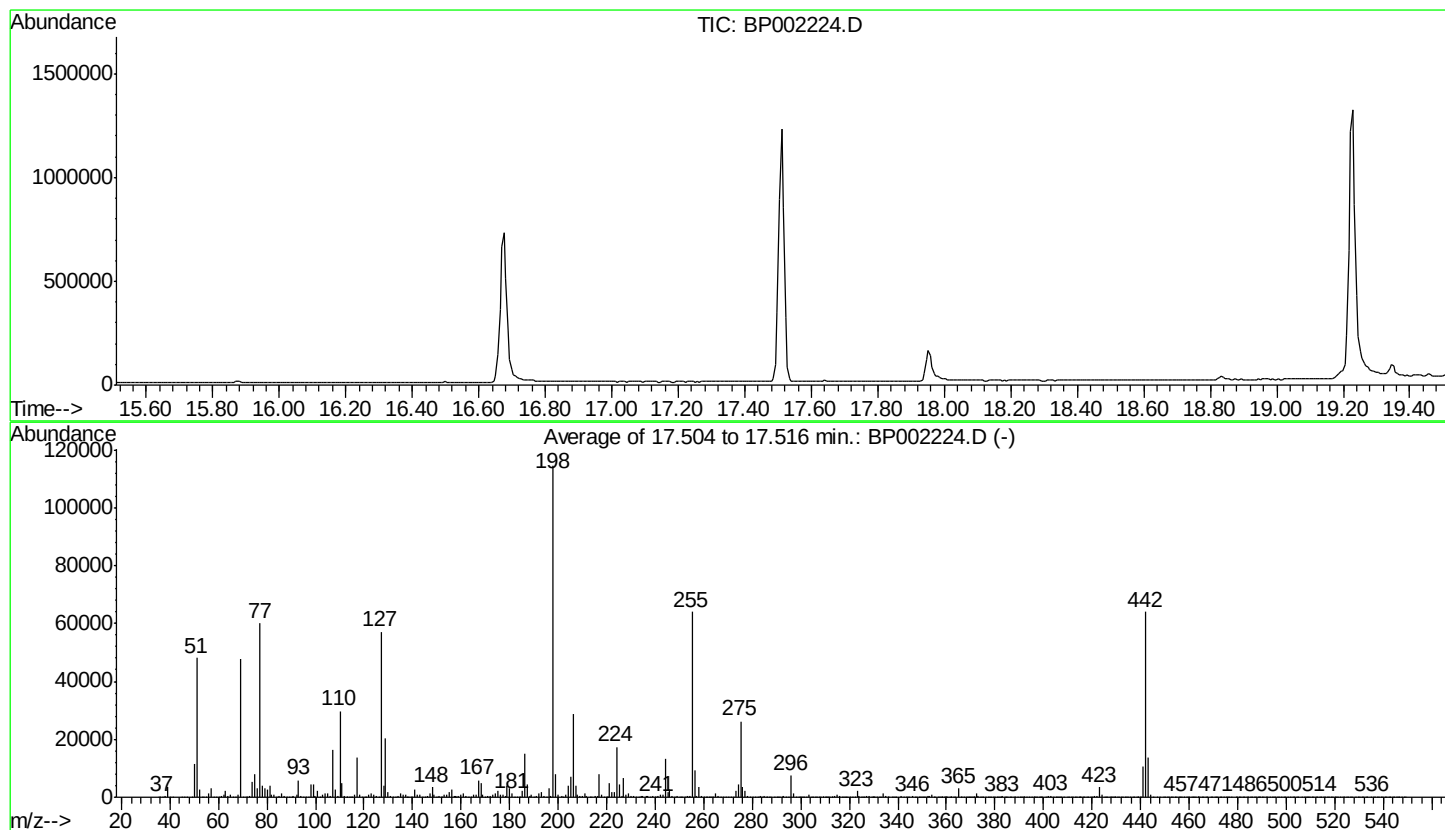

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	48101	PASS
68	69	0.00	2	1.6	750	PASS
69	198	0.00	100	41.9	47953	PASS
70	69	0.00	2	0.5	216	PASS
127	198	10	80	50.0	57242	PASS
197	198	0.00	2	0.3	324	PASS
198	198	100	100	100.0	114498	PASS
199	198	5	9	6.8	7824	PASS
275	198	10	60	22.9	26205	PASS
365	198	1	100	2.7	3070	PASS
441	198	0.01	100	9.4	10711	PASS
442	198	50	100	55.9	63973	PASS
443	442	15	24	21.2	13552	PASS