
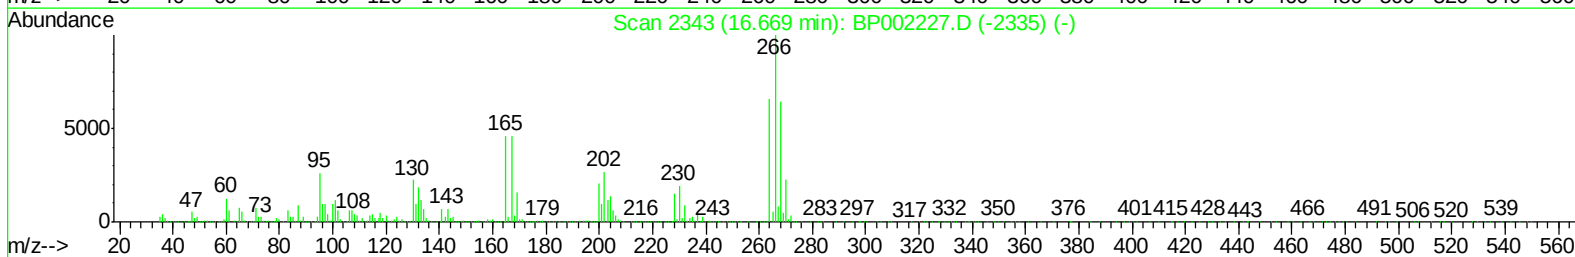
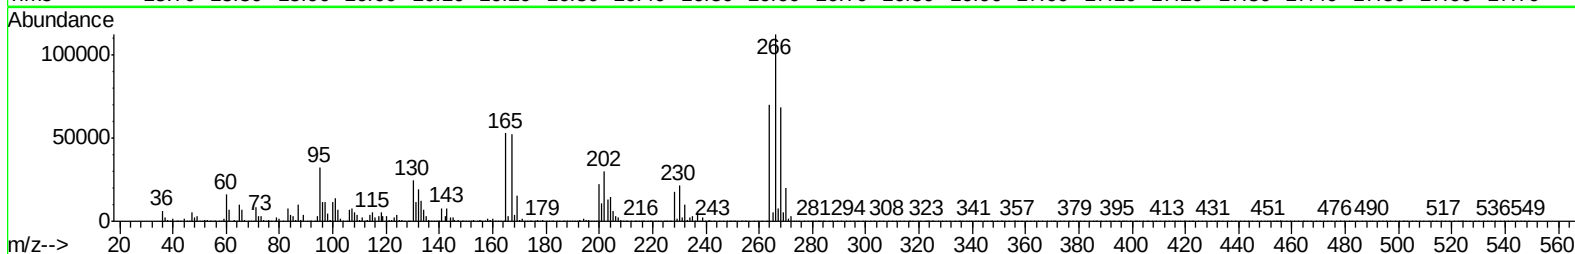


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
 Data File : BP002233.D
 Acq On : 05 May 2020 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 02:27:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP050420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 05 13:34:25 2020
 Response via : Initial Calibration

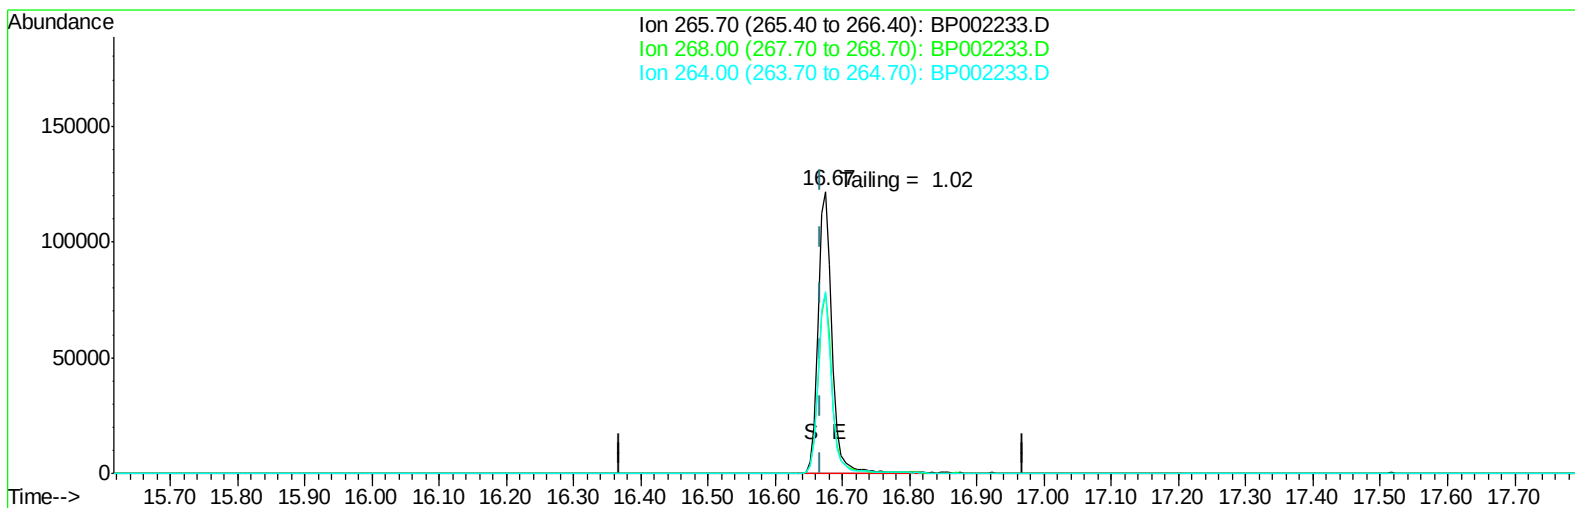

TIC: BP002233.D

(70) Pentachlorophenol (C)




16.675min (+0.006) 1387206.01ng

response 178747

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	64.11
264.00	65.50	64.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
 Data File : BP002233.D
 Acq On : 05 May 2020 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 02:27:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP050420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 05 13:34:25 2020
 Response via : Initial Calibration

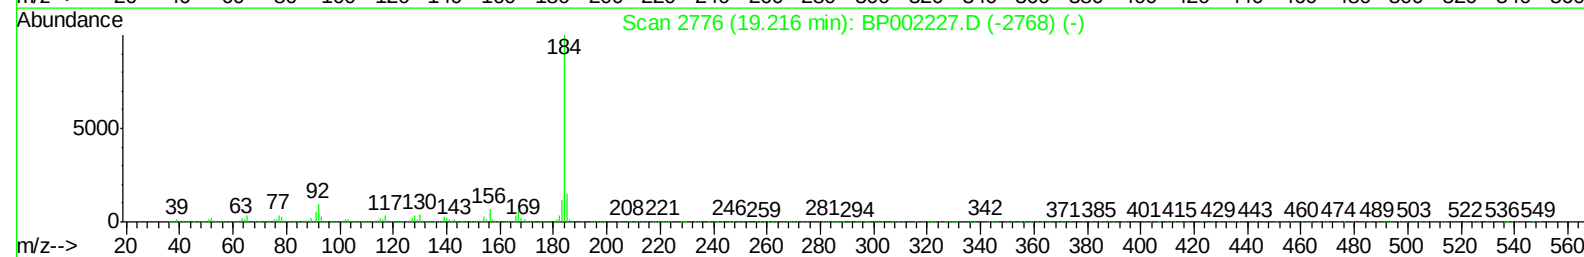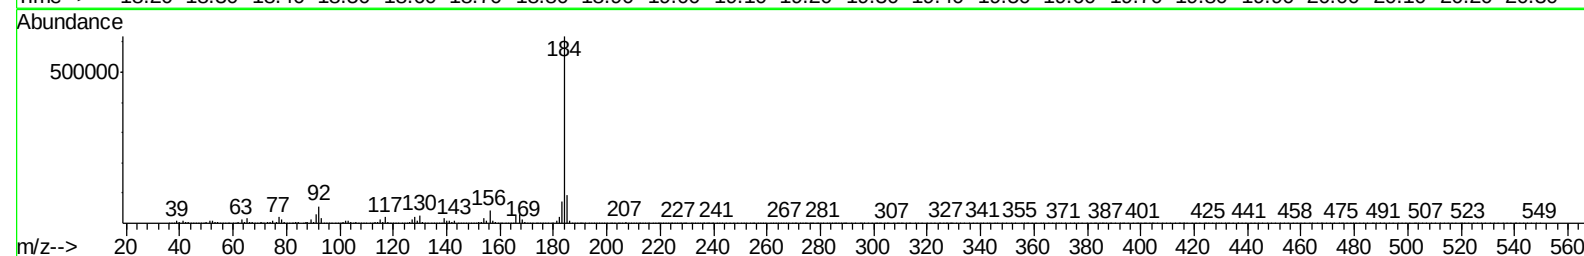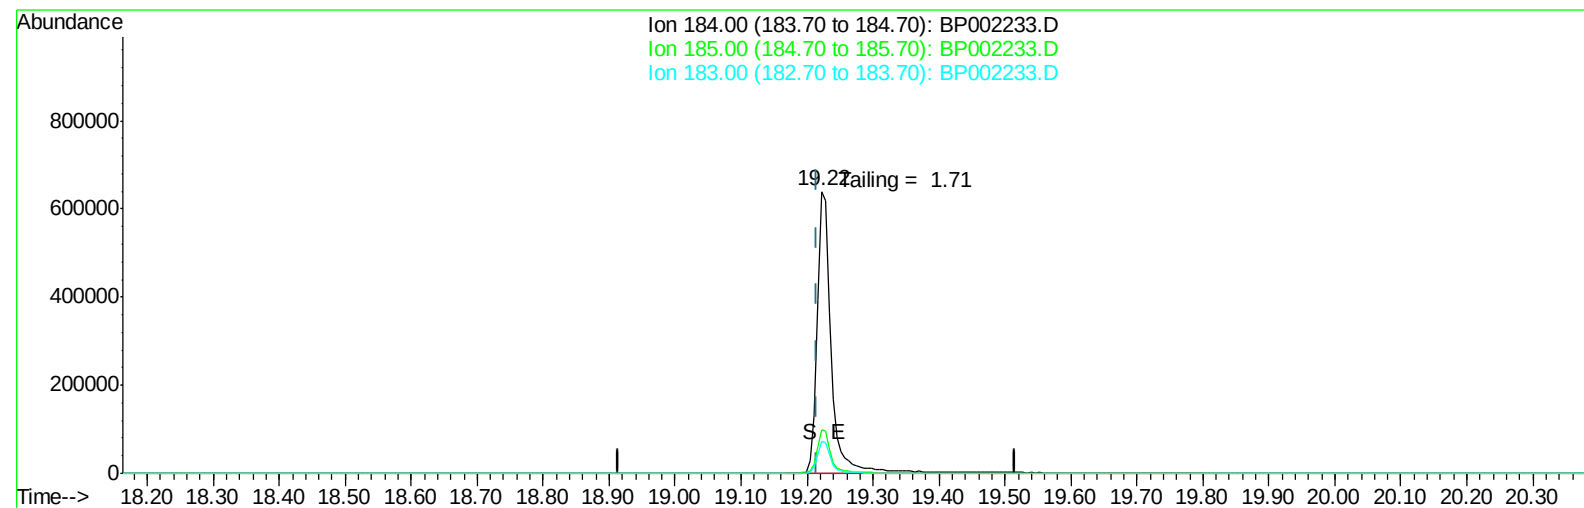

TIC: BP002233.D

(77) Benzidine

19.222min (+0.006) 1119.09ng

response 958214

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	15.35
183.00	11.40	11.27
0.00	0.00	0.00