

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
 Data File : BP002235.D
 Acq On : 05 May 2020 13:34
 Operator : CG/JU
 Sample : PB128656BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB128656BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP050420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	391	398	417	rBV	3556690	5617131	38.85%	8.155%
2	6.798	656	665	687	rBV	3749760	6196128	42.85%	8.996%
3	7.616	796	804	814	rBV	690038	1079411	7.47%	1.567%
4	7.934	850	858	866	rBV	3402627	5441655	37.64%	7.900%
5	8.757	989	998	1012	rBV	2758919	4522562	31.28%	6.566%
6	10.386	1267	1275	1289	rBV	978519	1605727	11.11%	2.331%
7	12.880	1691	1699	1714	rBV	6705283	10277812	71.08%	14.922%
8	14.257	1922	1933	1944	rBV	1542499	2276734	15.75%	3.305%
9	15.751	2180	2187	2208	rBV	4976317	7399692	51.18%	10.743%
10	17.010	2394	2401	2412	rBV	2075598	2858267	19.77%	4.150%
11	19.598	2835	2841	2859	rBV	10518355	14458568	100.00%	20.992%
12	21.109	3092	3098	3112	rBV	2797500	3470516	24.00%	5.039%
13	23.309	3465	3472	3485	rVB	1971565	3673206	25.41%	5.333%




Sum of corrected areas: 68877409

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
Data File : BP002235.D
Acq On : 05 May 2020 13:34
Operator : CG/JU
Sample : PB128656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB128656BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP050420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

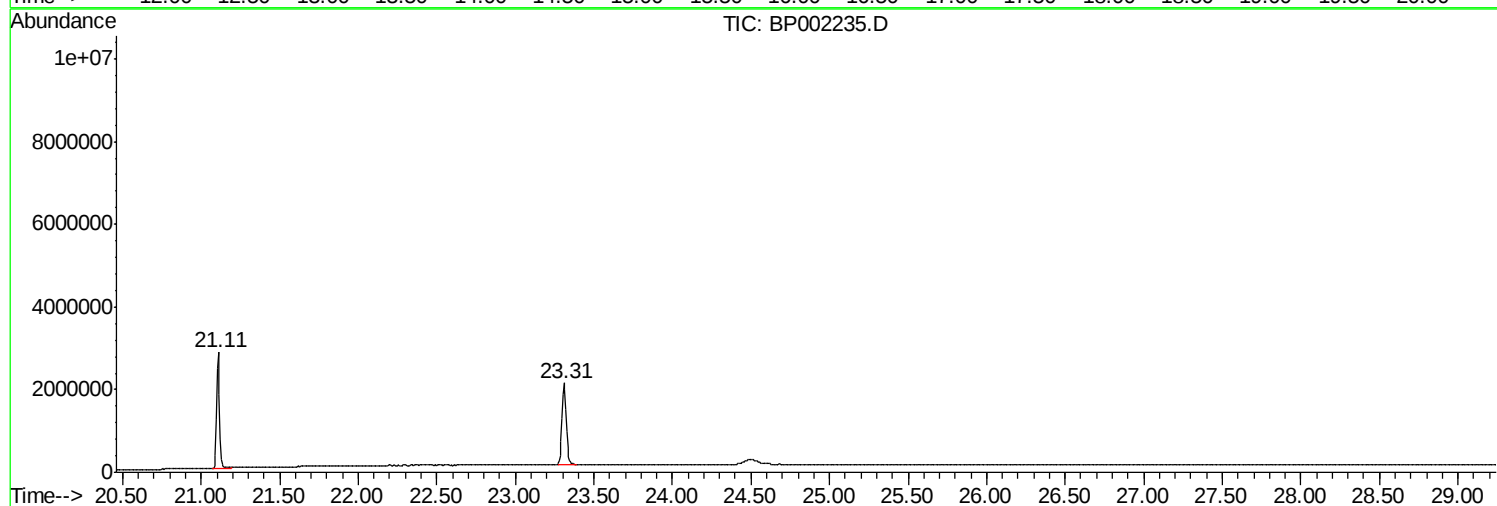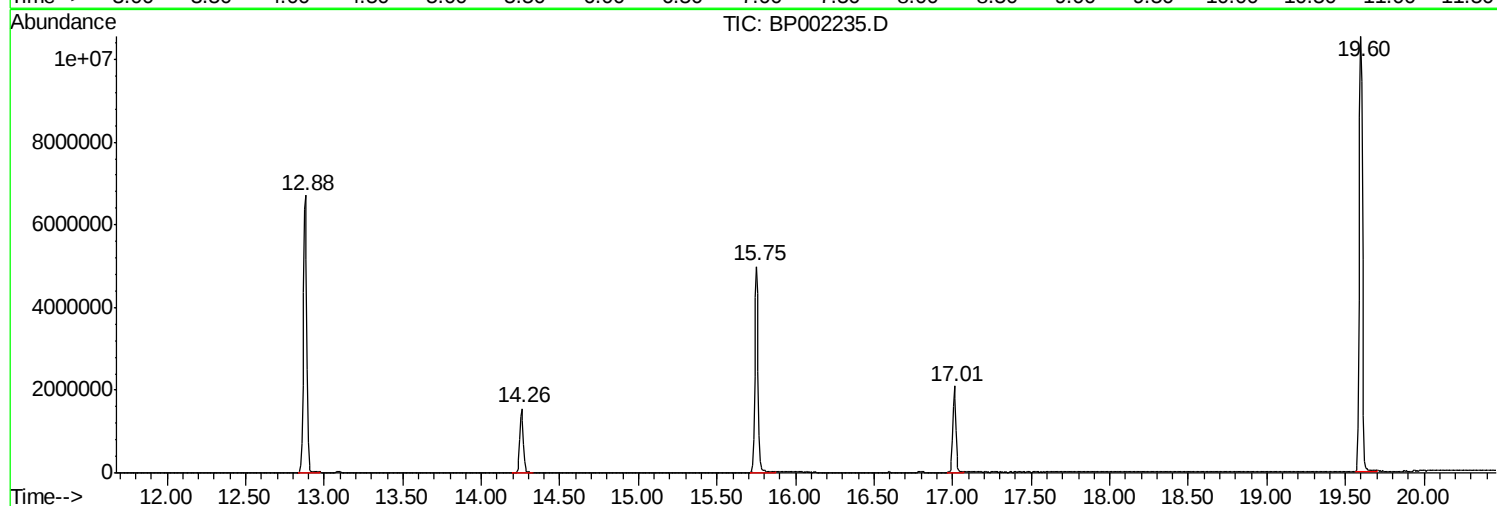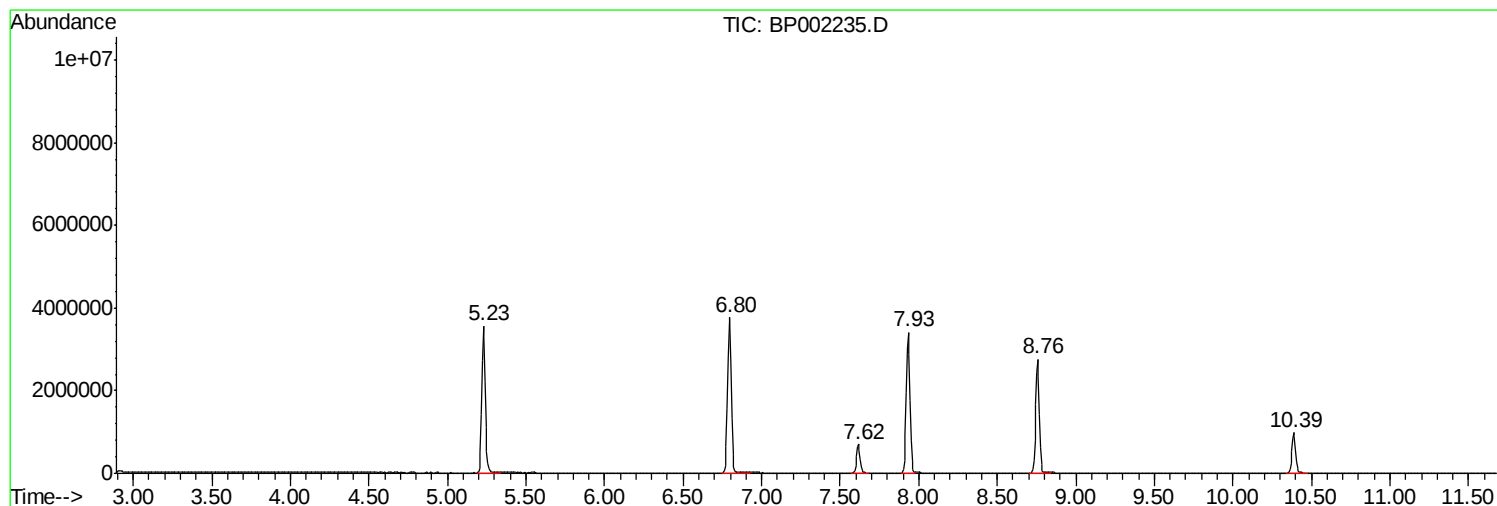

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP050520\
Data_File : BP002235.D
Acq_On : 05_May, 2020 13:344
Operator : CG/JUU
Sample : PB128656BLL
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
PB128656BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP050420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
