

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
 Data File : BP002246.D
 Acq On : 05 May 2020 20:27
 Operator : CG/JU
 Sample : L2483-02 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 6FT-TP-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP050420.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.916	3	5	10	rVB	60808	63319	1.14%	0.144%
2	5.228	392	398	412	rBV	767685	1153863	20.77%	2.618%
3	6.793	657	664	681	rBV	885538	1385039	24.93%	3.142%
4	7.616	797	804	812	rBV	976346	1570968	28.27%	3.564%
5	7.934	849	858	867	rBV	716092	1158348	20.85%	2.628%
6	8.751	990	997	1011	rBV	523612	864063	15.55%	1.960%
7	10.387	1266	1275	1282	rBV	1517342	2484180	44.71%	5.636%
8	12.875	1691	1698	1710	rBV	1626288	2323772	41.82%	5.272%
9	13.716	1834	1841	1847	rBV	202601	285361	5.14%	0.647%
10	13.975	1879	1885	1893	rVB	35825	58460	1.05%	0.133%
11	14.257	1926	1933	1940	rBV	2370658	3424396	61.63%	7.769%
12	14.316	1940	1943	1952	rVB	39132	61967	1.12%	0.141%
13	15.310	2106	2112	2119	rBV	44977	74648	1.34%	0.169%
14	15.745	2179	2186	2198	rBV	1048174	1519903	27.35%	3.448%
15	17.010	2394	2401	2405	rBV	2936100	4113147	74.02%	9.332%
16	17.051	2405	2408	2414	rVB	560952	729394	13.13%	1.655%
17	17.139	2419	2423	2429	rVB	119502	172534	3.11%	0.391%
18	17.886	2546	2550	2554	rBV	68579	88718	1.60%	0.201%
19	17.933	2554	2558	2566	rVV2	131938	204562	3.68%	0.464%
20	18.069	2576	2581	2585	rVV2	111879	186383	3.35%	0.423%
21	18.110	2585	2588	2592	rVB2	55007	73465	1.32%	0.167%
22	18.374	2629	2633	2636	rBV	48717	67164	1.21%	0.152%
23	18.780	2698	2702	2707	rBV2	47342	68096	1.23%	0.154%
24	18.910	2720	2724	2732	rVB3	34768	68322	1.23%	0.155%
25	19.027	2739	2744	2751	rBV	972931	1237378	22.27%	2.807%
26	19.380	2795	2804	2809	rBV	844142	1299278	23.38%	2.948%
27	19.457	2813	2817	2823	rVB2	33451	57489	1.03%	0.130%
28	19.592	2835	2840	2852	rVB	2923247	3516703	63.29%	7.979%
29	19.710	2854	2860	2864	rBV2	56086	128936	2.32%	0.293%
30	19.833	2877	2881	2884	rBV4	53025	90156	1.62%	0.205%
31	19.868	2884	2887	2892	rVB	120650	159952	2.88%	0.363%
32	19.968	2900	2904	2907	rVB	71861	84237	1.52%	0.191%
33	20.021	2909	2913	2918	rVB2	84239	120930	2.18%	0.274%
34	20.157	2933	2936	2940	rBV	48998	57139	1.03%	0.130%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
Data File : BP002246.D
Acq On : 05 May 2020 20:27
Operator : CG/JU
Sample : L2483-02 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
6FT-TP-1

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP050420.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	20.204	2940	2944	2950	rBV3	50302	76479	1.38%	0.174%
36	20.598	3008	3011	3018	rVB	66342	89942	1.62%	0.204%
37	20.798	3042	3045	3048	rVB	60124	64037	1.15%	0.145%
38	20.857	3048	3055	3057	rBV4	131723	246249	4.43%	0.559%
39	21.104	3091	3097	3101	rBV2	3784450	5556488	100.00%	12.607%
40	21.139	3101	3103	3112	rVB	477051	605419	10.90%	1.374%
41	21.257	3120	3123	3127	rBV	69408	75913	1.37%	0.172%
42	21.298	3127	3130	3137	rBV2	87971	116545	2.10%	0.264%
43	21.733	3201	3204	3208	rBV	91899	95066	1.71%	0.216%
44	22.198	3279	3283	3288	rVB	127908	163732	2.95%	0.371%
45	22.651	3355	3360	3365	rBV2	353427	812574	14.62%	1.844%
46	22.815	3385	3388	3394	rVB	80991	134123	2.41%	0.304%
47	23.115	3435	3439	3448	rVB	237058	432067	7.78%	0.980%
48	23.209	3450	3455	3462	rVV	315058	591577	10.65%	1.342%
49	23.309	3462	3472	3488	rVB	2638948	5416546	97.48%	12.289%
50	23.927	3573	3577	3583	rVB	114146	198471	3.57%	0.450%
51	25.527	3843	3849	3862	rVB4	124029	448836	8.08%	1.018%


Sum of corrected areas: 44076334

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP050520\
Data File : BP002246.D
Acq On : 05 May 2020 20:27
Operator : CG/JU
Sample : L2483-02 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
6FT-TP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP050420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

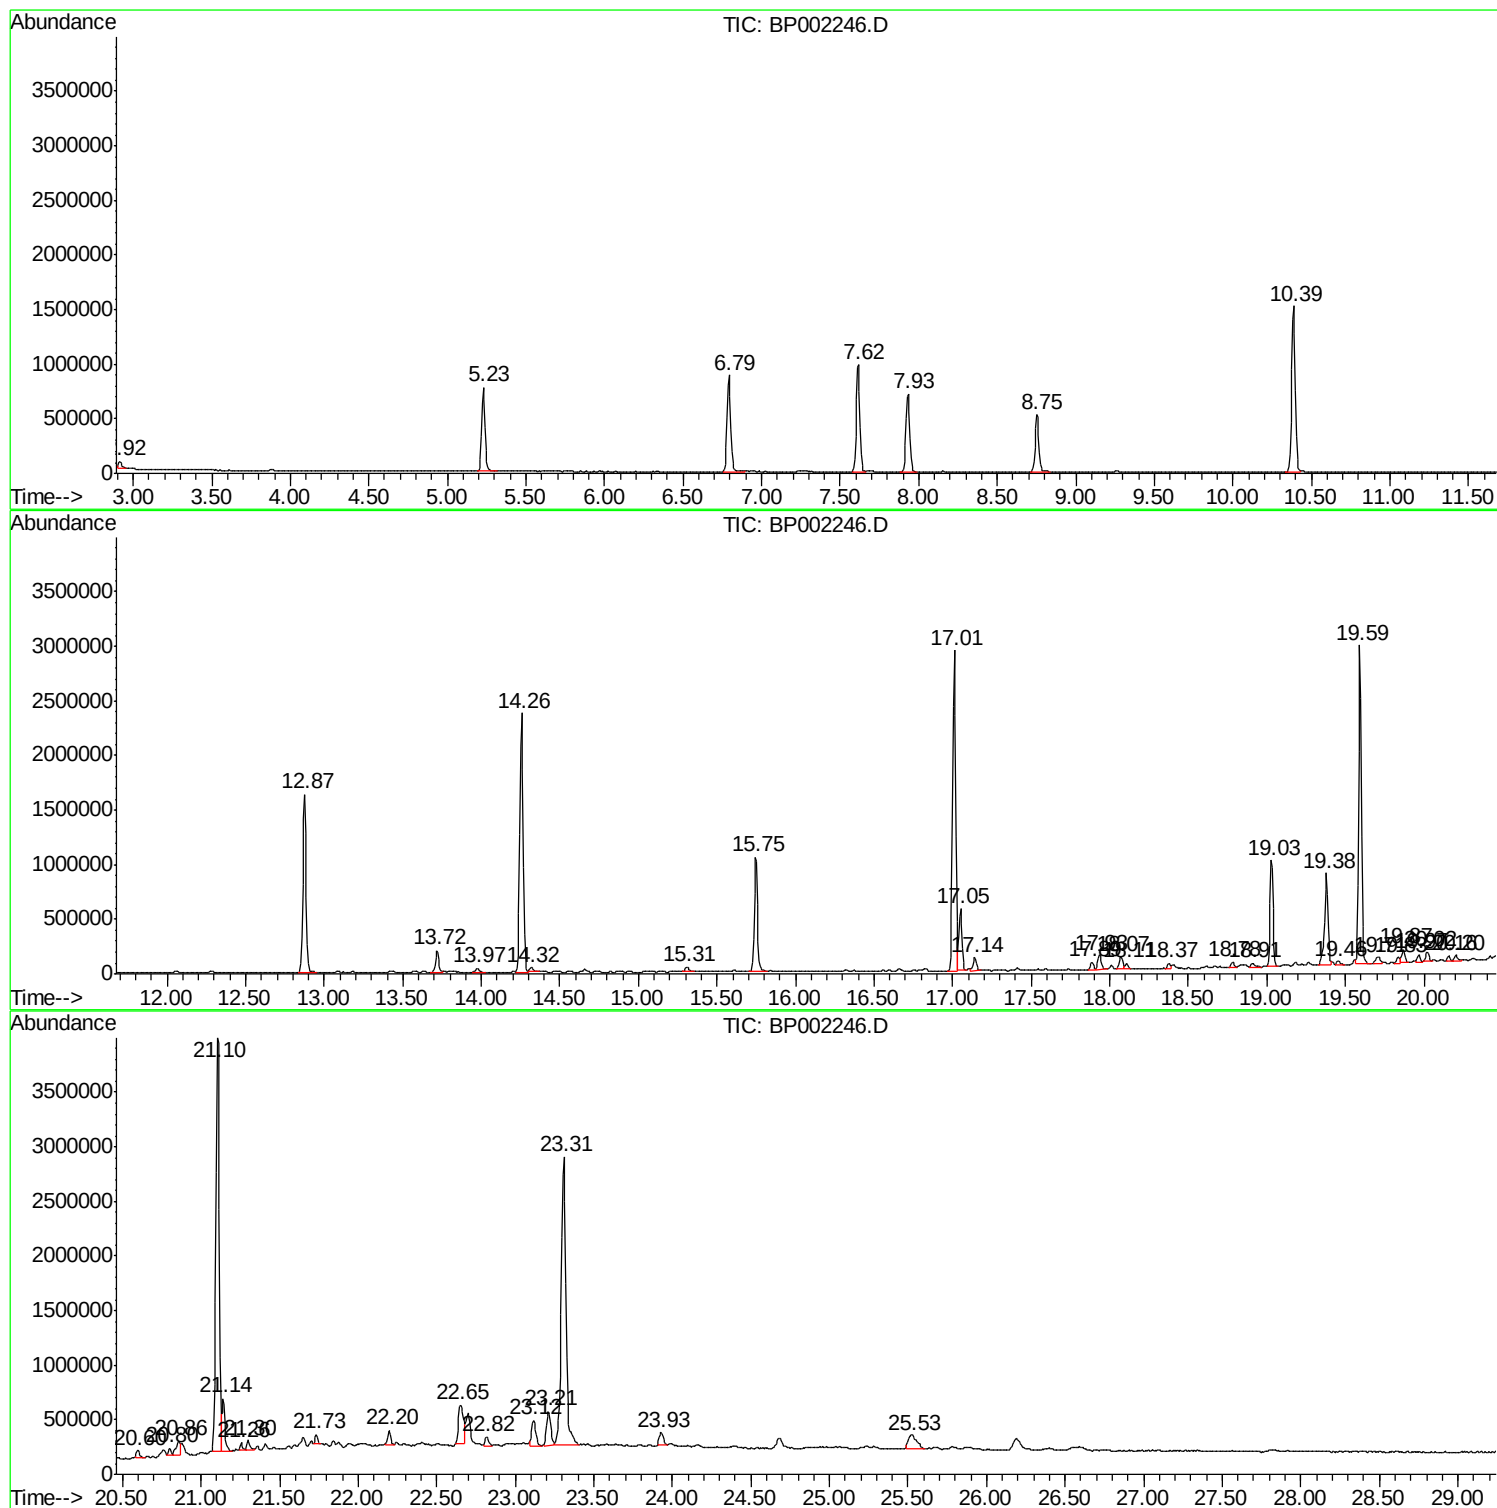

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP050520\
Data_File : BP002246.D
Acq_On : 05_May, 2020 20:277
Operator : CG/JUU
Sample : L2483-02_5XX
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
6FT-TP-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP050420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
