


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP050520\  
 Data File : BP002233.D  
 Acq On : 05 May 2020 12:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP050420.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue May 05 13:34:25 2020

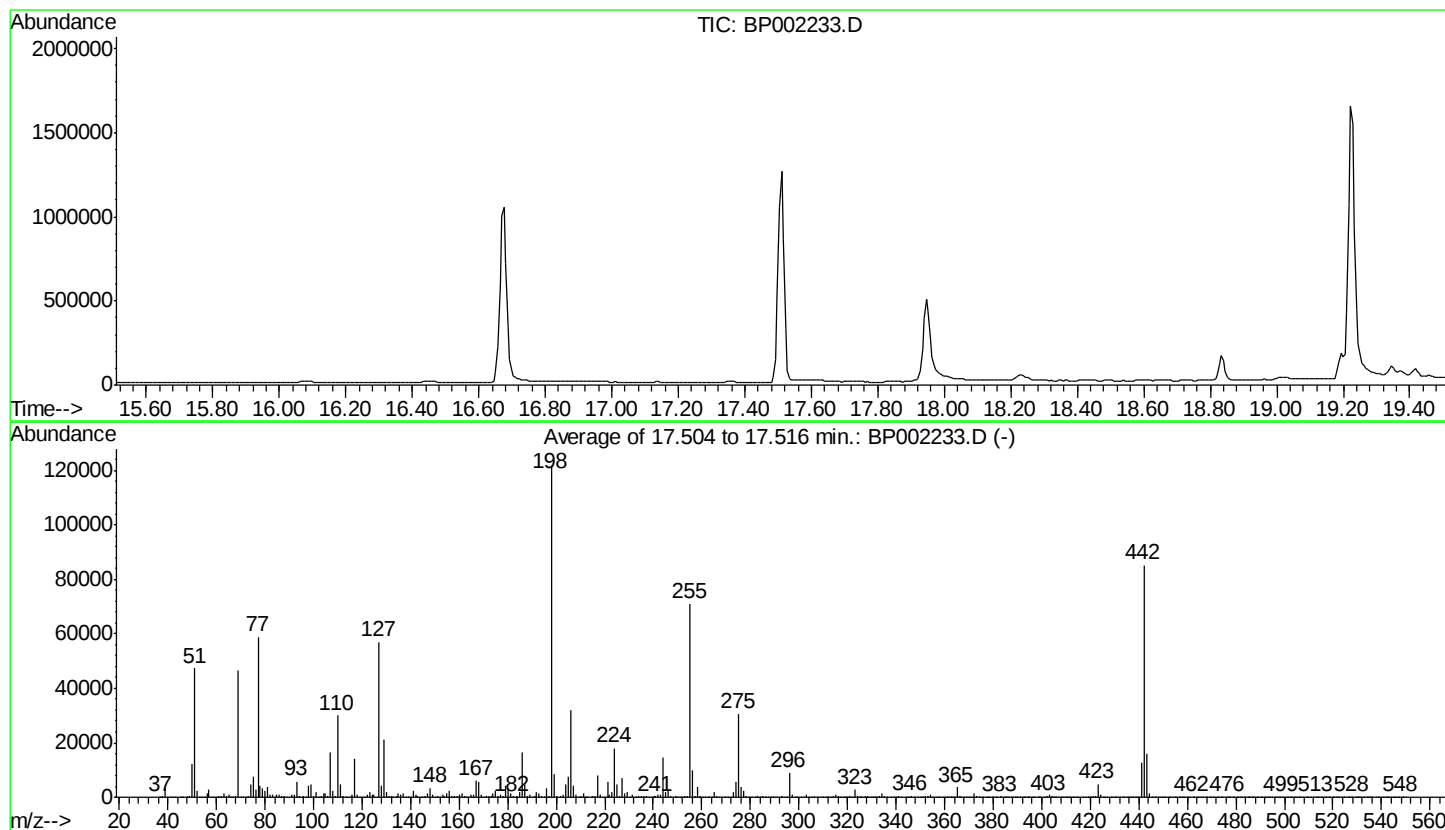

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2476

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 38.9      | 47411   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 666     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.1      | 46433   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 248     | PASS             |
| 127         | 198          | 10           | 80           | 46.9      | 57154   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 438     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 121829  | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 8559    | PASS             |
| 275         | 198          | 10           | 60           | 25.1      | 30576   | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 3652    | PASS             |
| 441         | 198          | 0.01         | 100          | 10.4      | 12637   | PASS             |
| 442         | 198          | 50           | 100          | 70.0      | 85322   | PASS             |
| 443         | 442          | 15           | 24           | 18.6      | 15873   | PASS             |