


1,4-Dioxane

Response Ratio

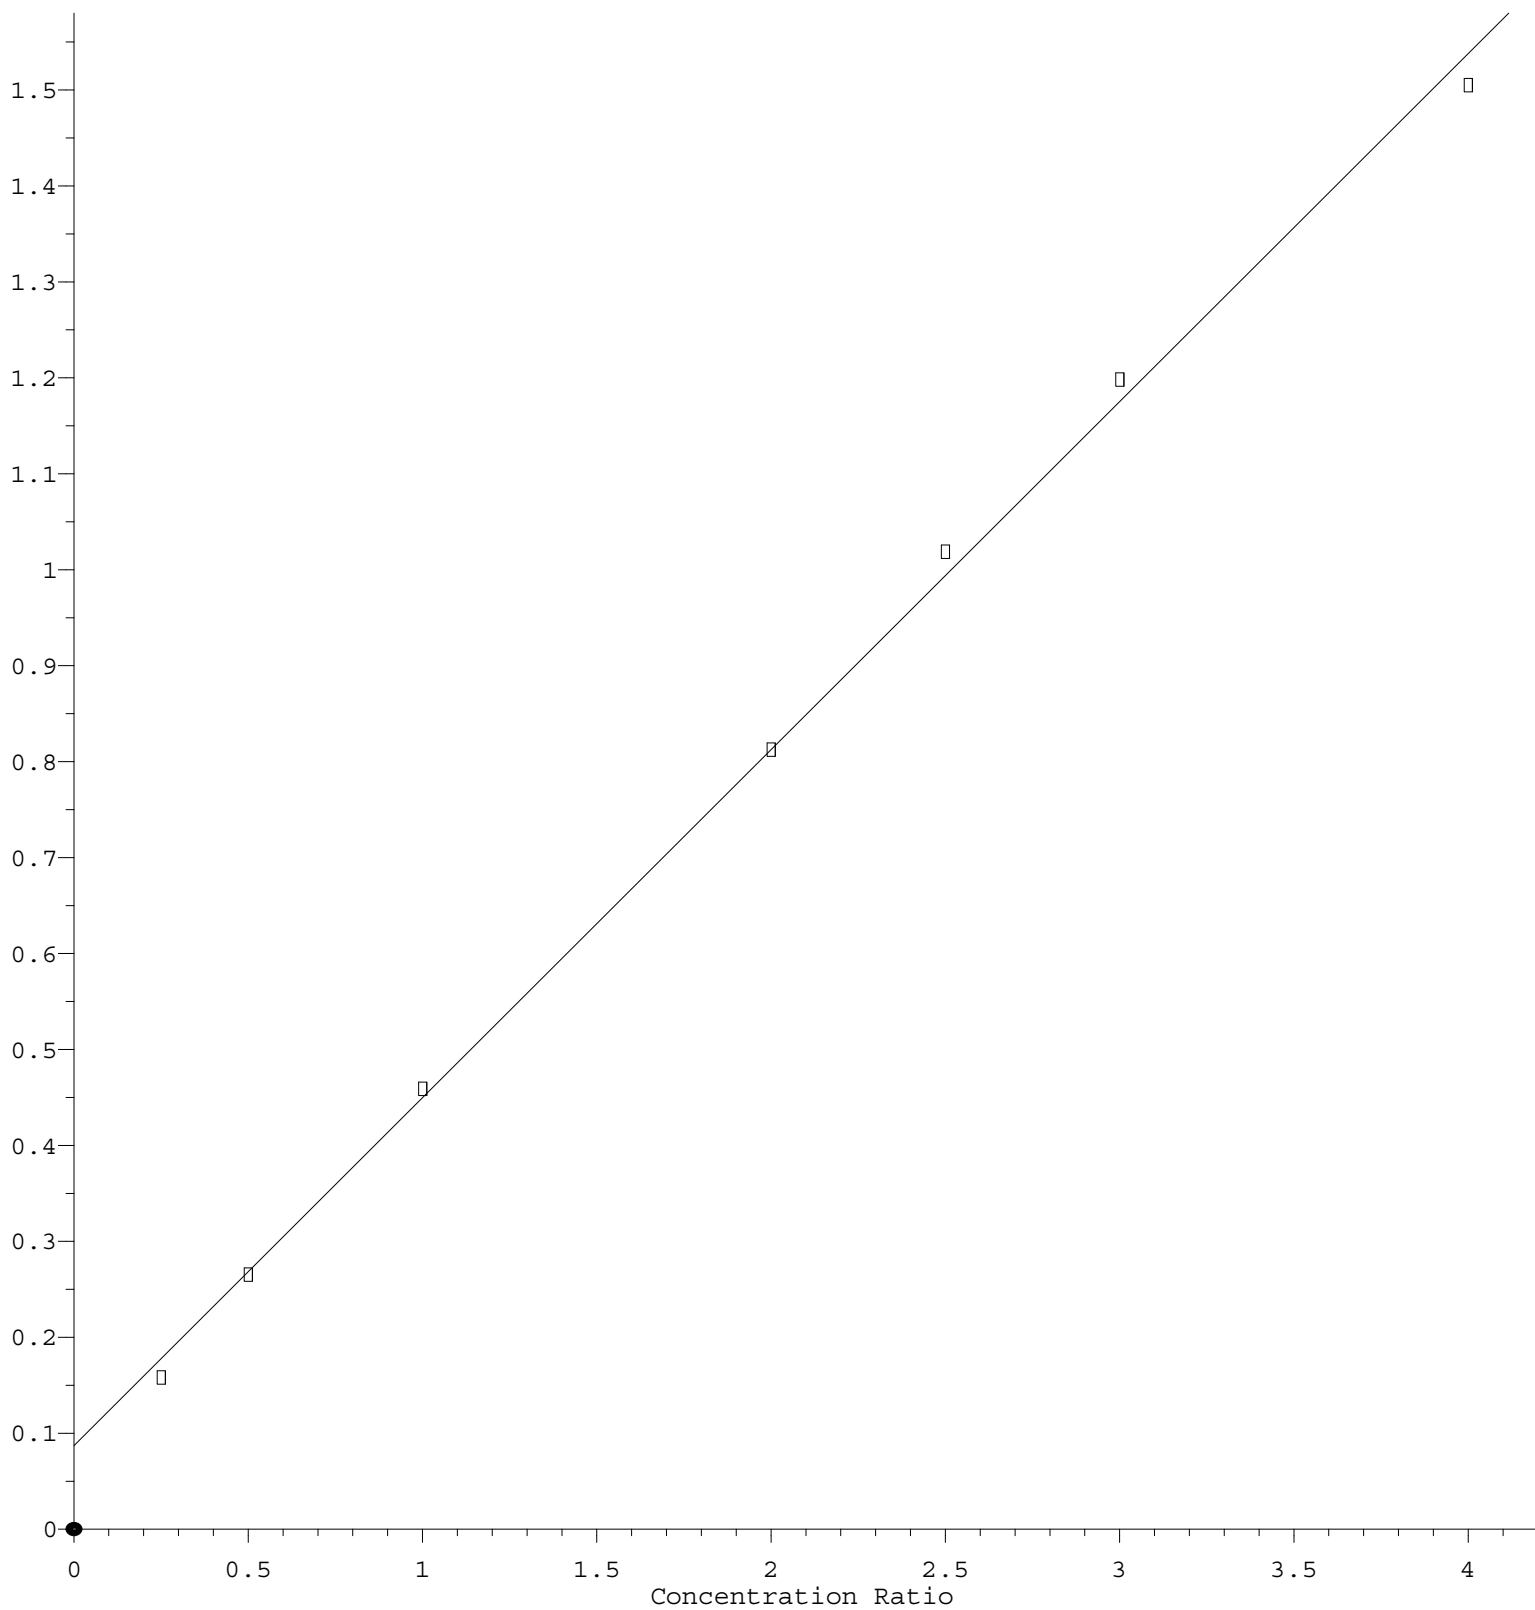

$$\text{Response} = 3.627\text{e-}001 * \text{Amt} + 8.726\text{e-}002$$


Coef of Det (r^2) = 0.998210 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP050521.M

Calibration Table Last Updated: Wed May 05 19:00:25 2021

Hexachlorocyclopentadiene

Response Ratio

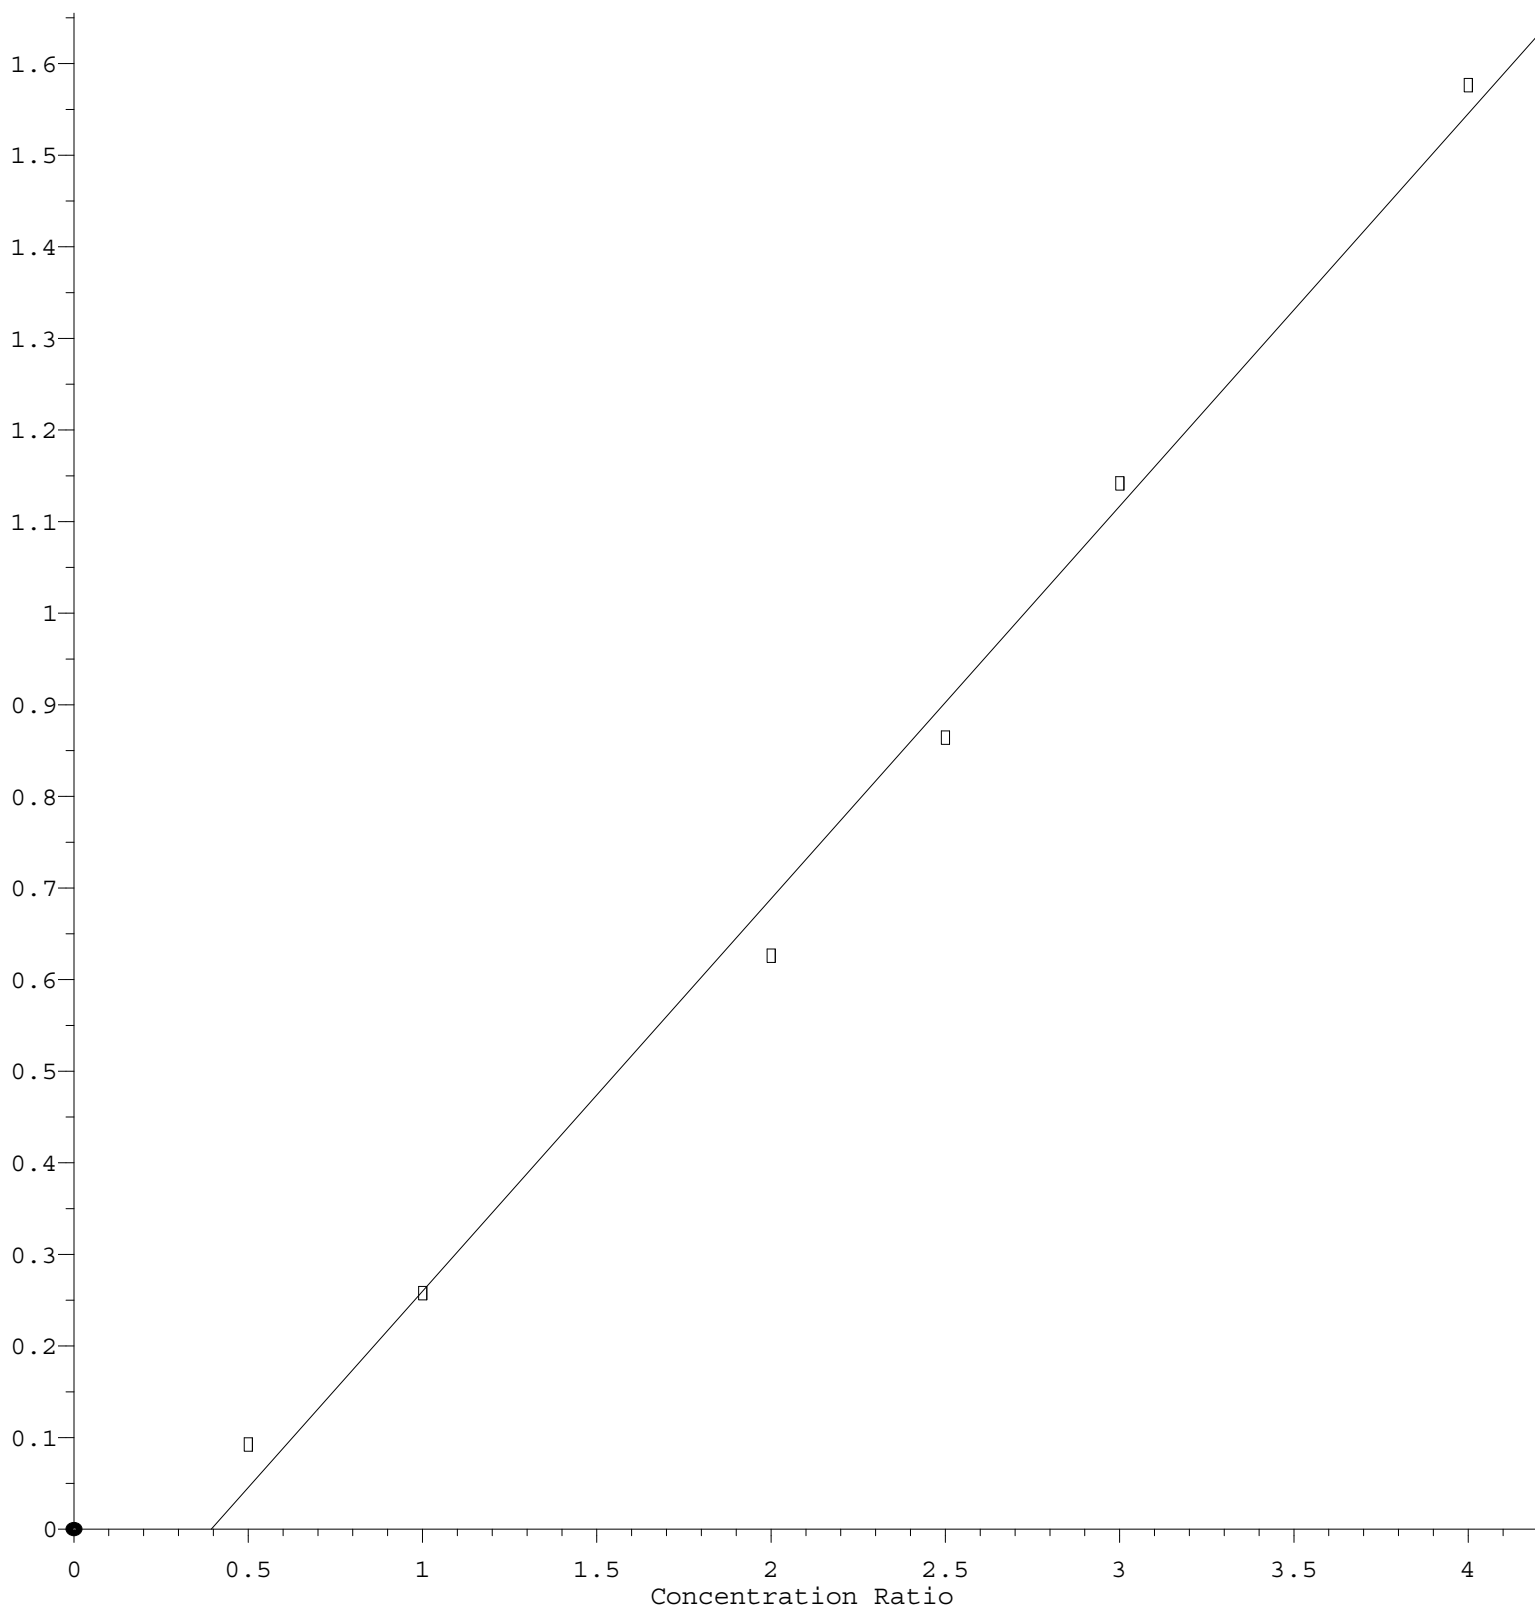

$$\text{Response} = 4.285\text{e-}001 * \text{Amt} - 1.686\text{e-}001$$


Coef of Det (r^2) = 0.994063 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP050521.M

Calibration Table Last Updated: Wed May 05 19:00:25 2021

Benzaldehyde

Response Ratio

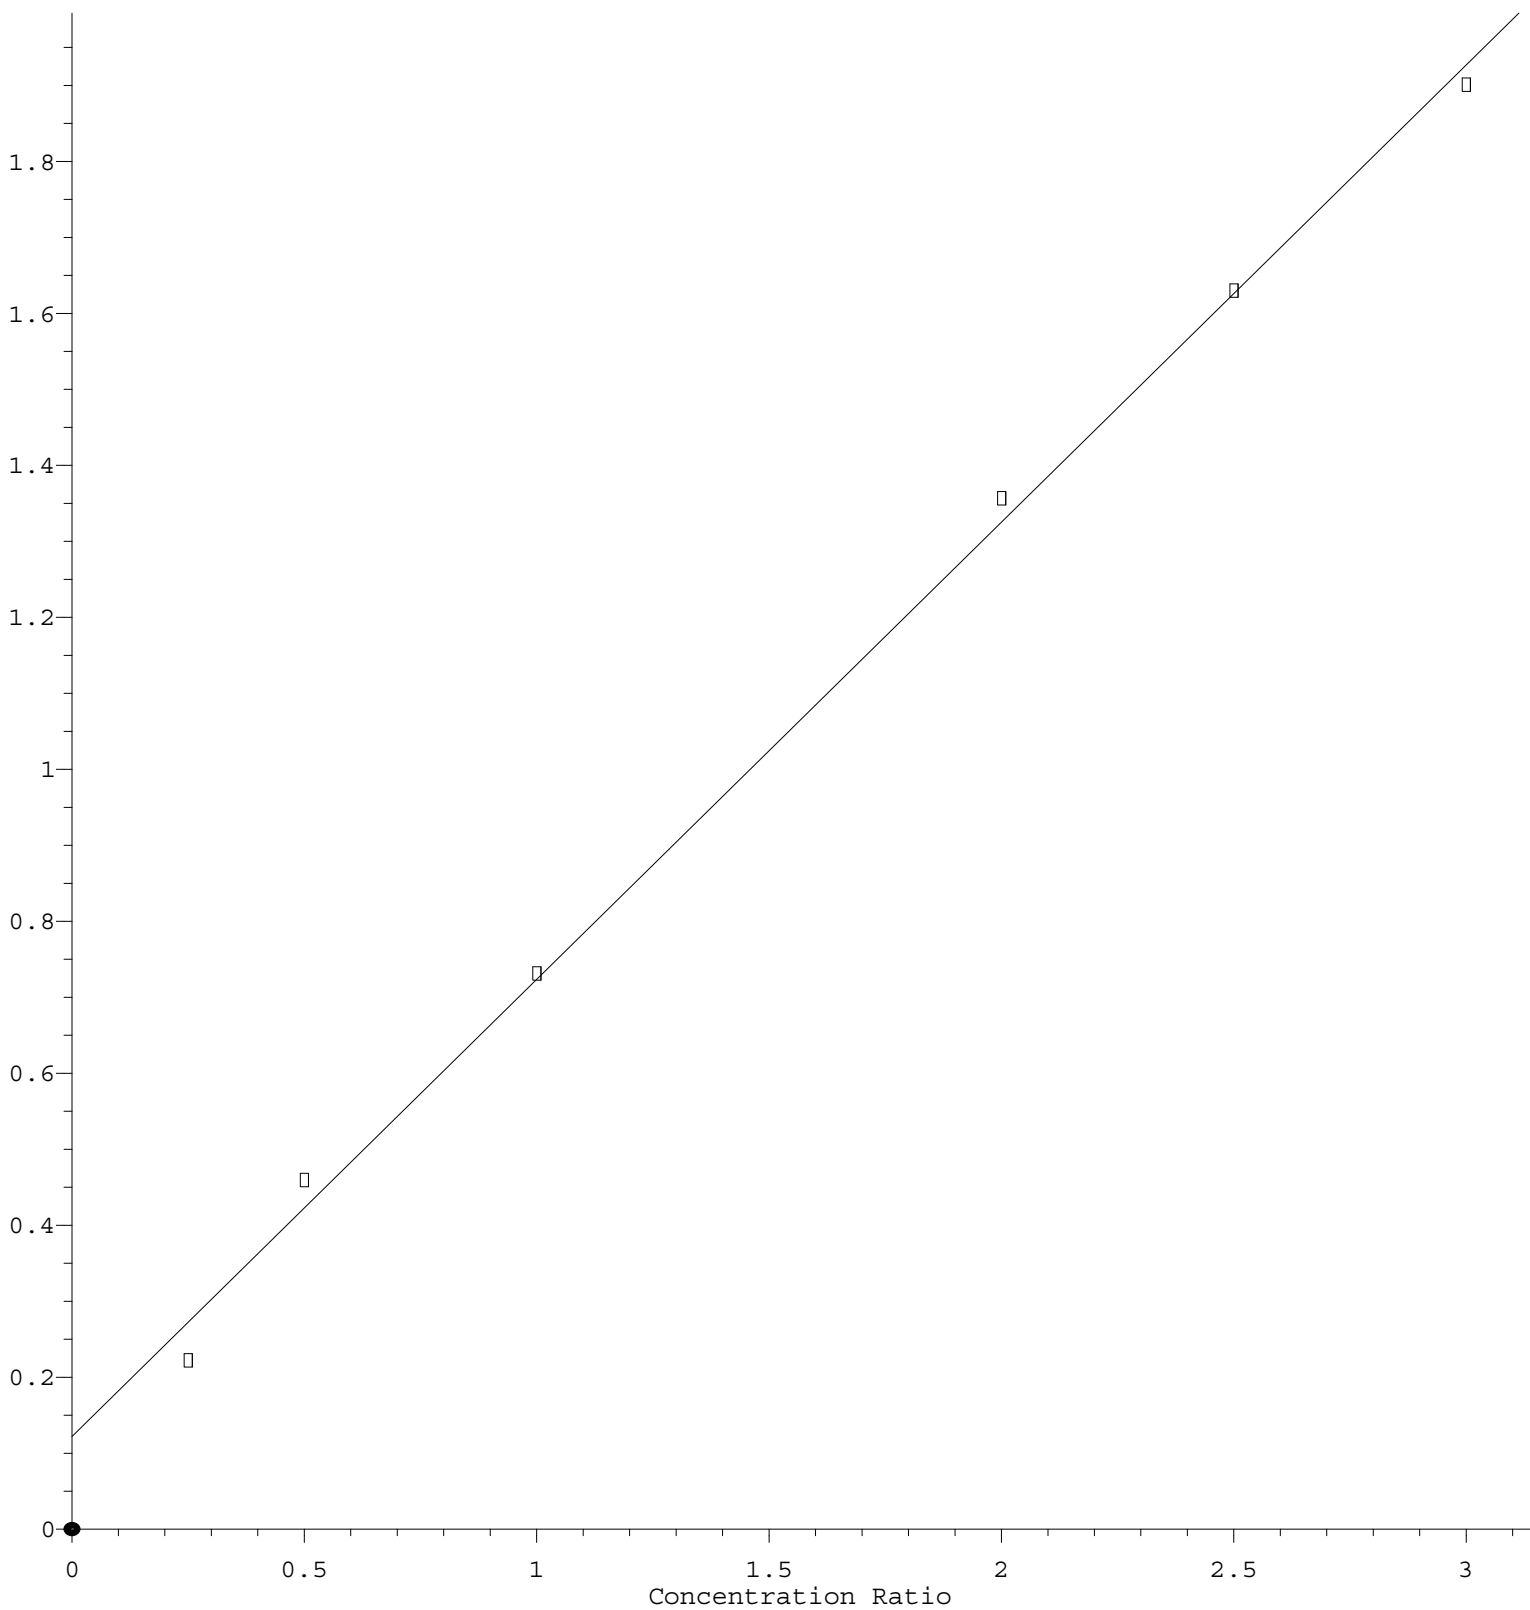

$$\text{Response} = 6.020\text{e-}001 * \text{Amt} + 1.219\text{e-}001$$

Coef of Det (r^2) = 0.997552 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP050521.M

Calibration Table Last Updated: Wed May 05 19:00:25 2021