
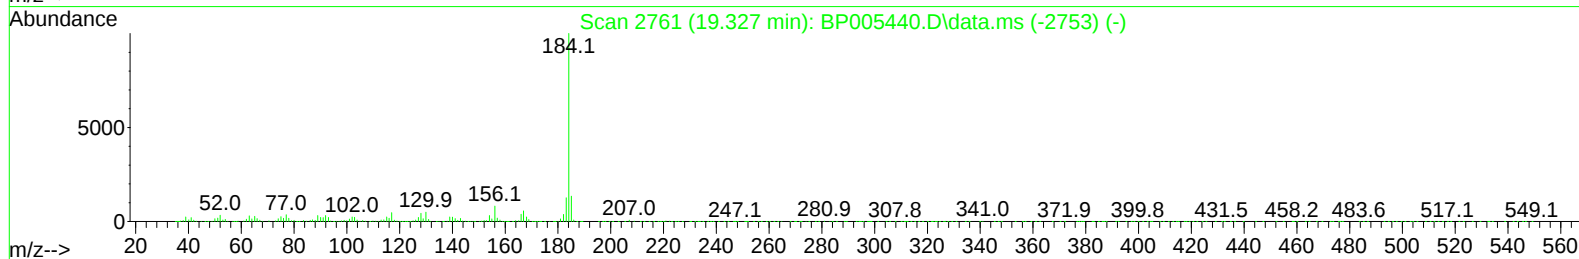
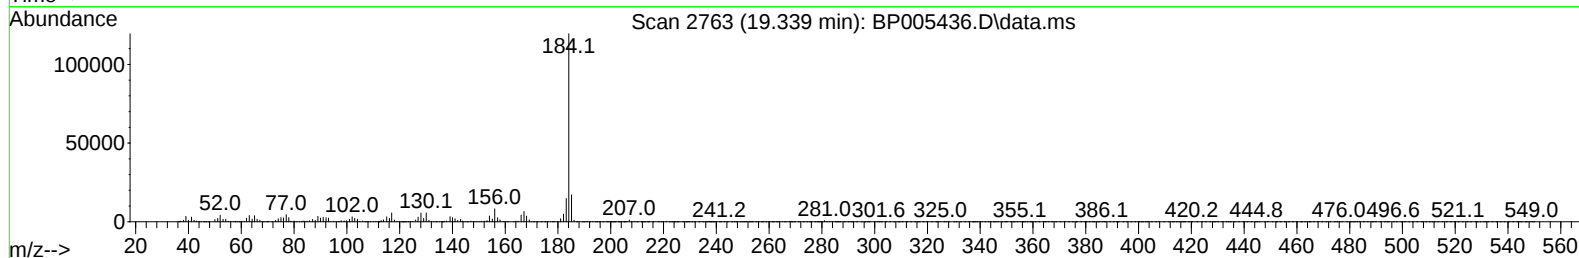


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050521\
 Data File : BP005436.D
 Acq On : 05 May 2021 14:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 17:38:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 17:06:09 2021
 Response via : Initial Calibration

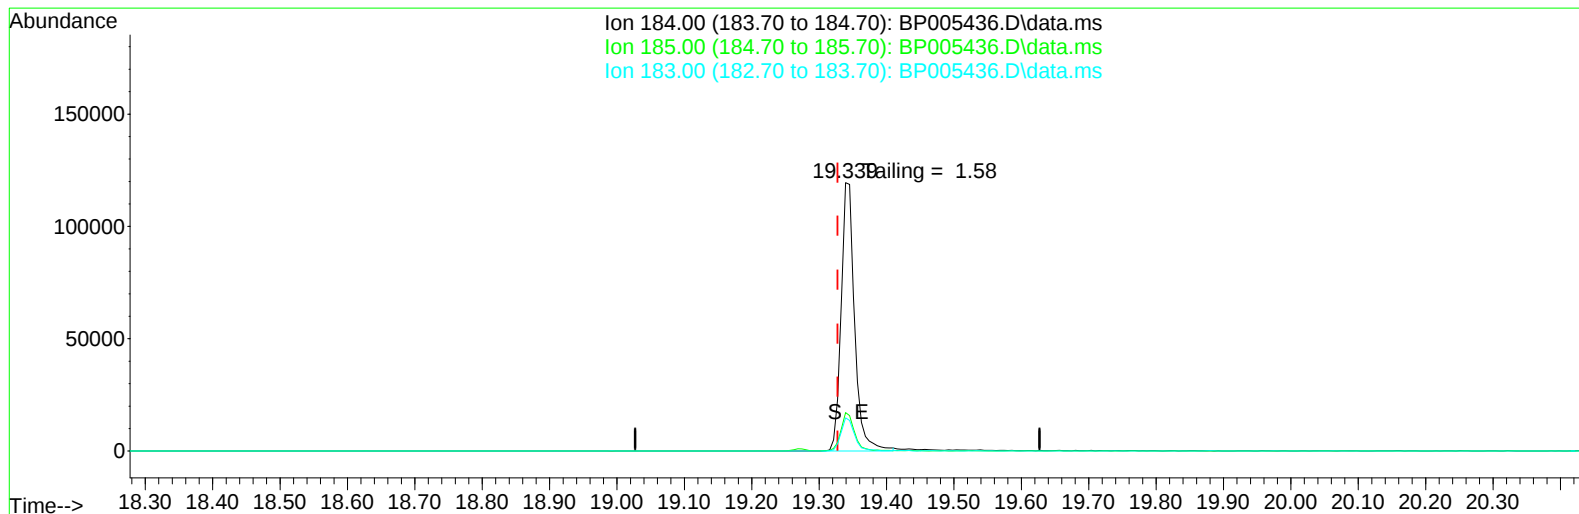




TIC: BP005436.D\data.ms

(77) Benzidine**19.339min (+ 0.012) 9783.56 ng****response 166980**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.30
183.00	12.30	12.36
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050521\  
Data File : BP05436.D  
Acq On    : 05 May 2021  14:04  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 05 17:38:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 17:06:09 2021
Response via : Initial Calibration

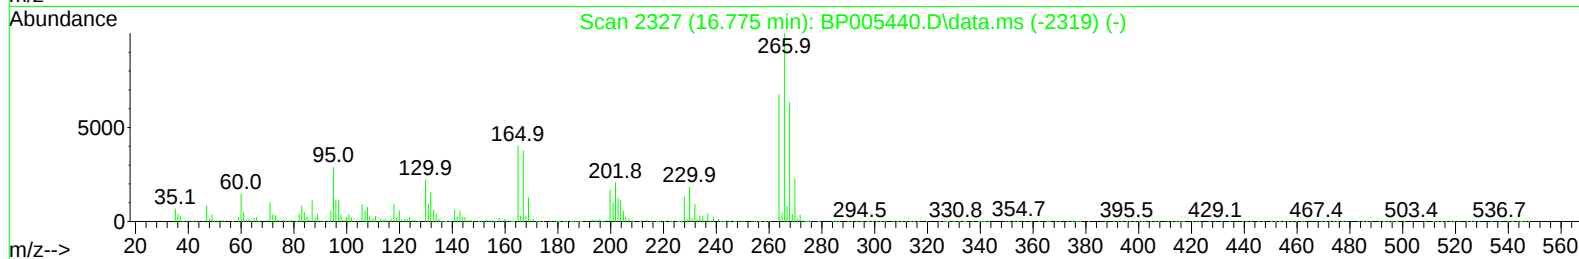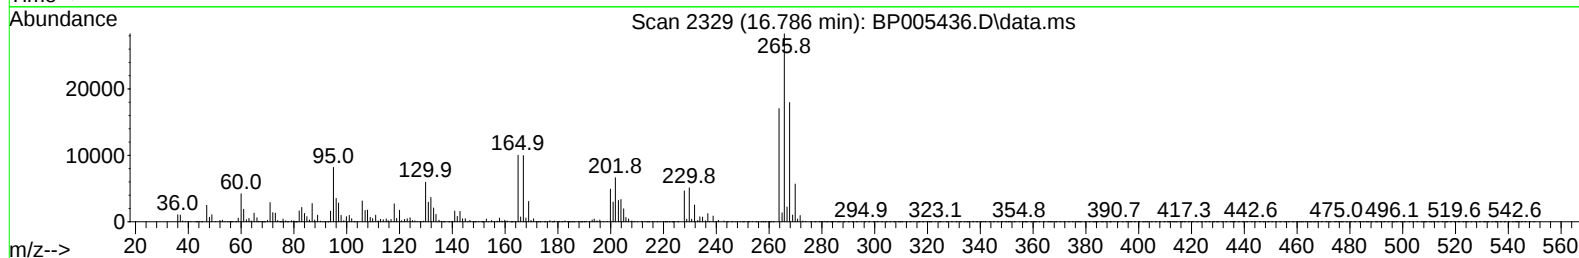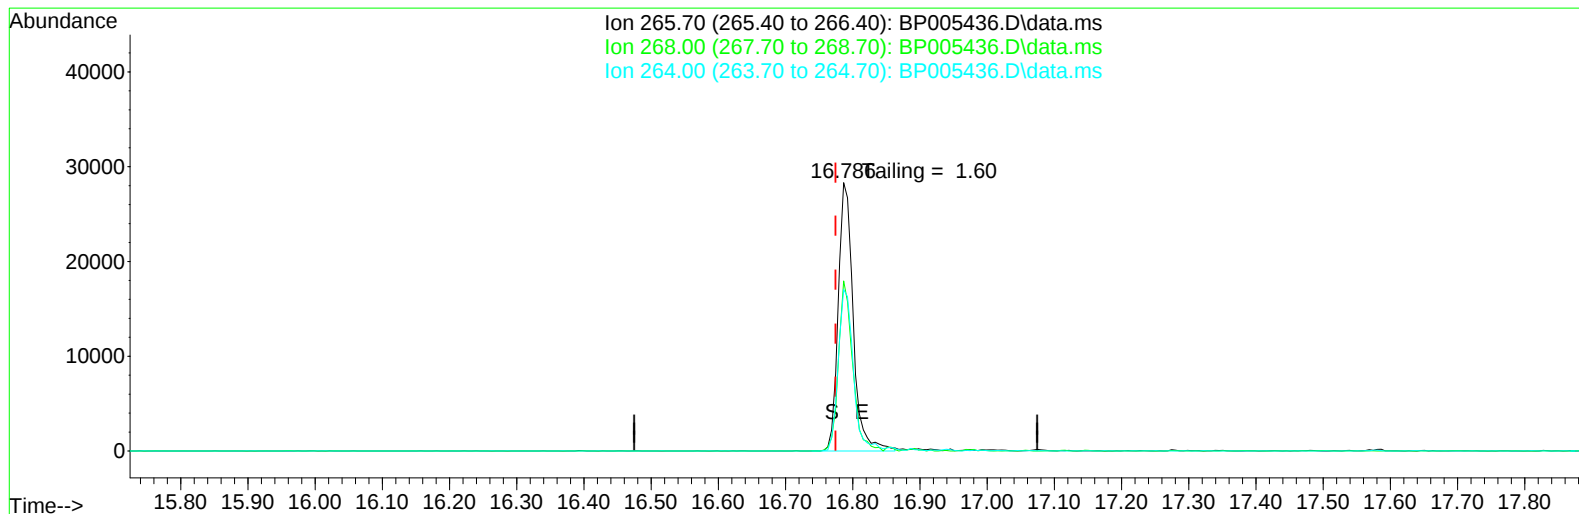

TIC: BP005436.D\data.ms

(70) **Pentachlorophenol (C)**

16.786min (+ 0.012) 362189.54 ng

response 44093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.39
264.00	67.10	60.17
0.00	0.00	0.00