
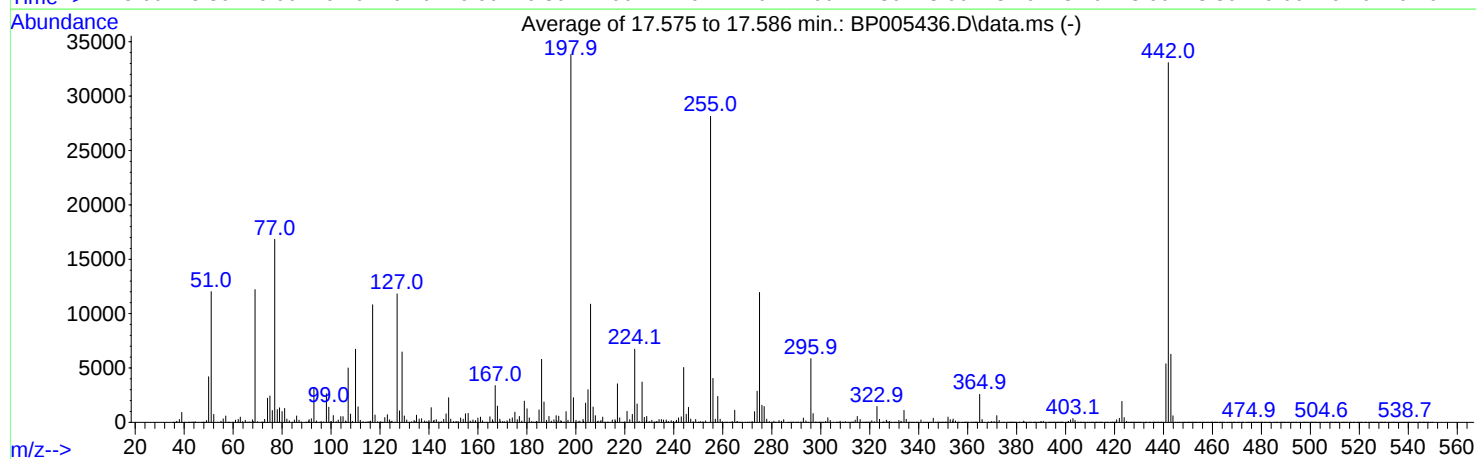


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050521\
 Data File : BP005436.D
 Acq On : 05 May 2021 14:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 05 19:00:25 2021

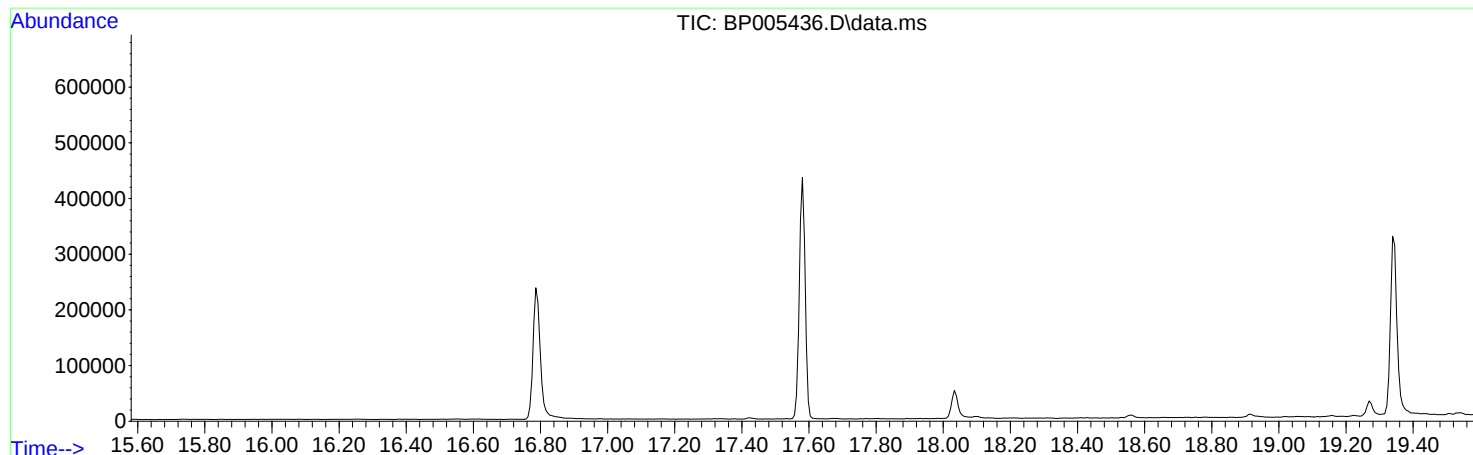




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	12016	PASS
68	69	0.00	2	2.0	242	PASS
69	198	0.00	100	36.1	12207	PASS
70	69	0.00	2	0.6	73	PASS
127	198	10	80	34.9	11812	PASS
197	198	0.00	2	0.6	198	PASS
198	198	100	100	100.0	33829	PASS
199	198	5	9	6.7	2271	PASS
275	198	10	60	35.3	11942	PASS
365	198	1	100	7.6	2577	PASS
441	198	0.01	100	15.9	5389	PASS
442	442	100	100	100.0	33080	PASS
443	442	15	24	18.9	6268	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050521\
Data File : BP005436.D
Acq On : 05 May 2021 14:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 05 17:38:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 17:06:09 2021
Response via : Initial Calibration

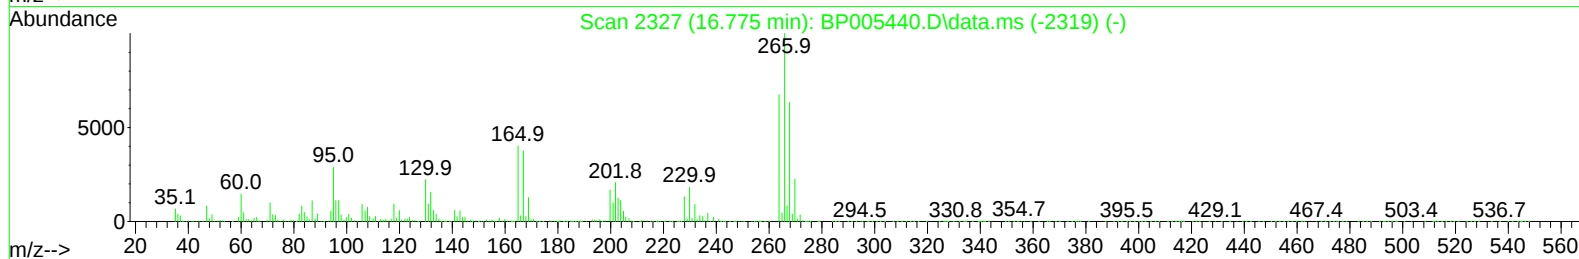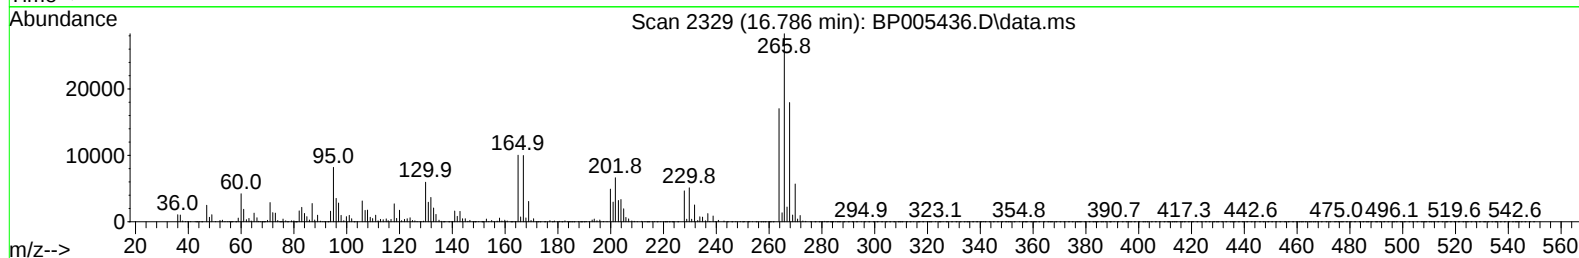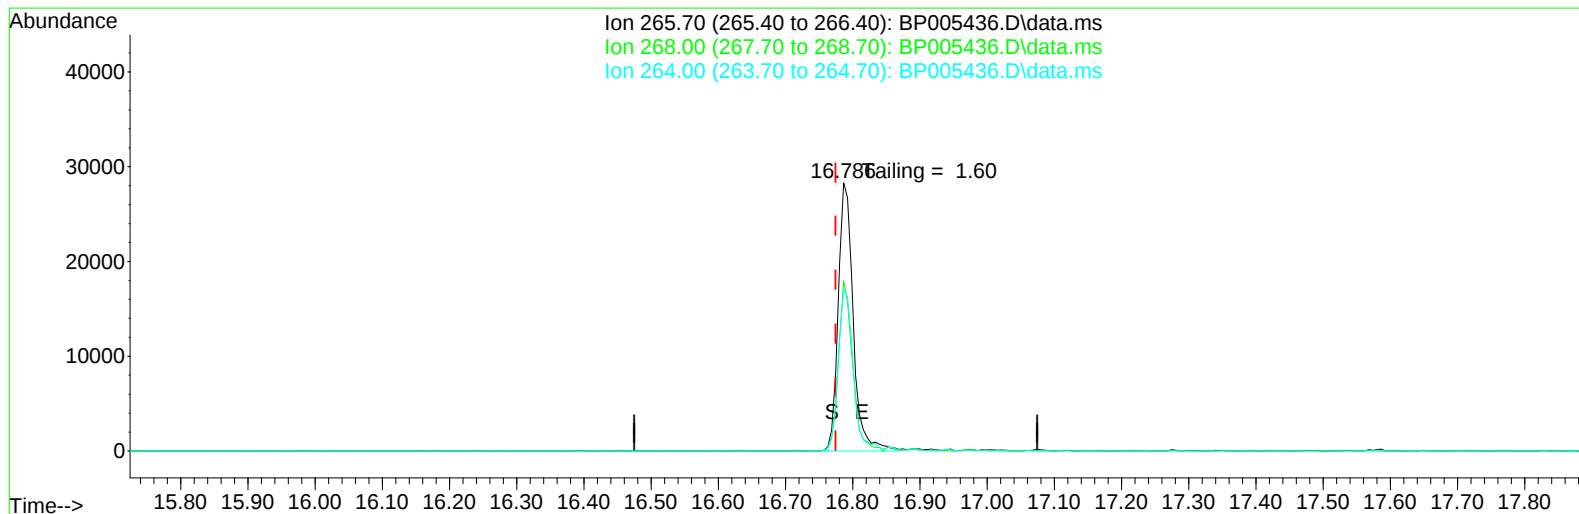

TIC: BP005436.D\data.ms

(70) Pentachlorophenol (C)

16.786min (+ 0.012) 362189.54 ng

response 44093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	63.39
264.00	67.10	60.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
05/05/2021	BNA_P	BP005436.D
Compound Name	Response	Retention Time
DDT	126098	20.53
DDD	1542	20.11
DDE	417	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1959	128057	1.53