




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010245.D
 Acq On : 05 May 2022 14:03
 Operator : CG/JU
 Sample : N2668-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL66

Manual IntegrationsAPPROVED

Quant Time: May 06 01:07:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

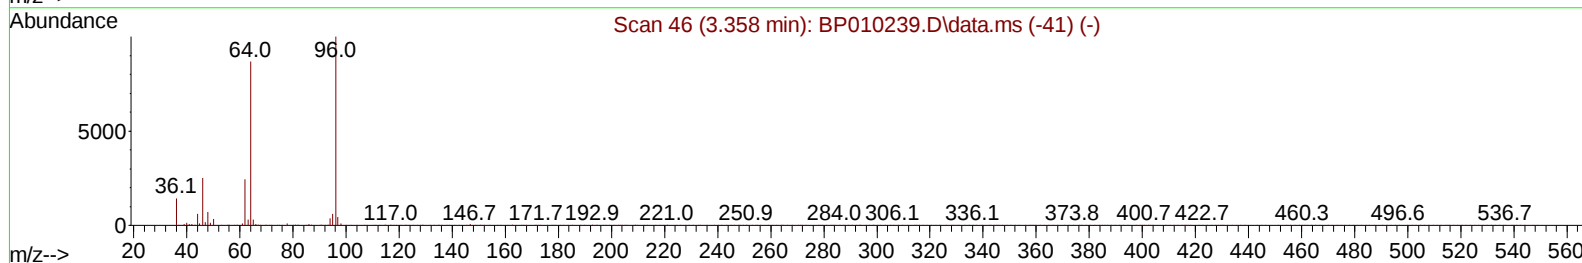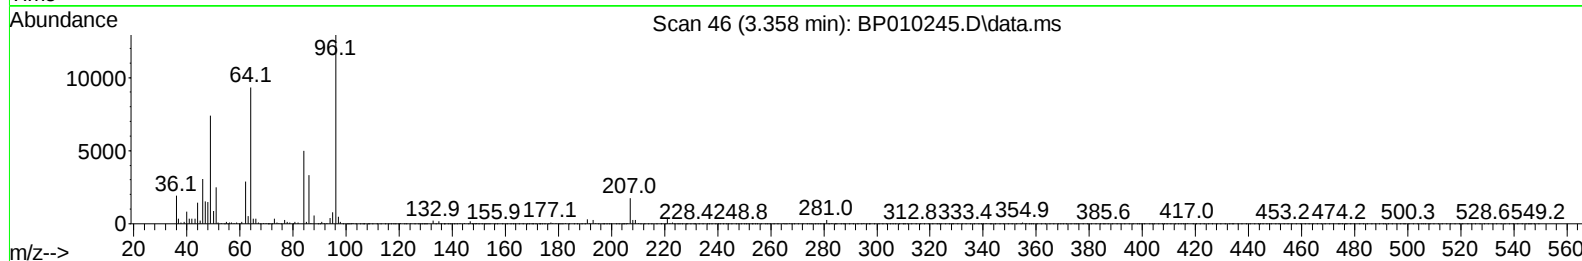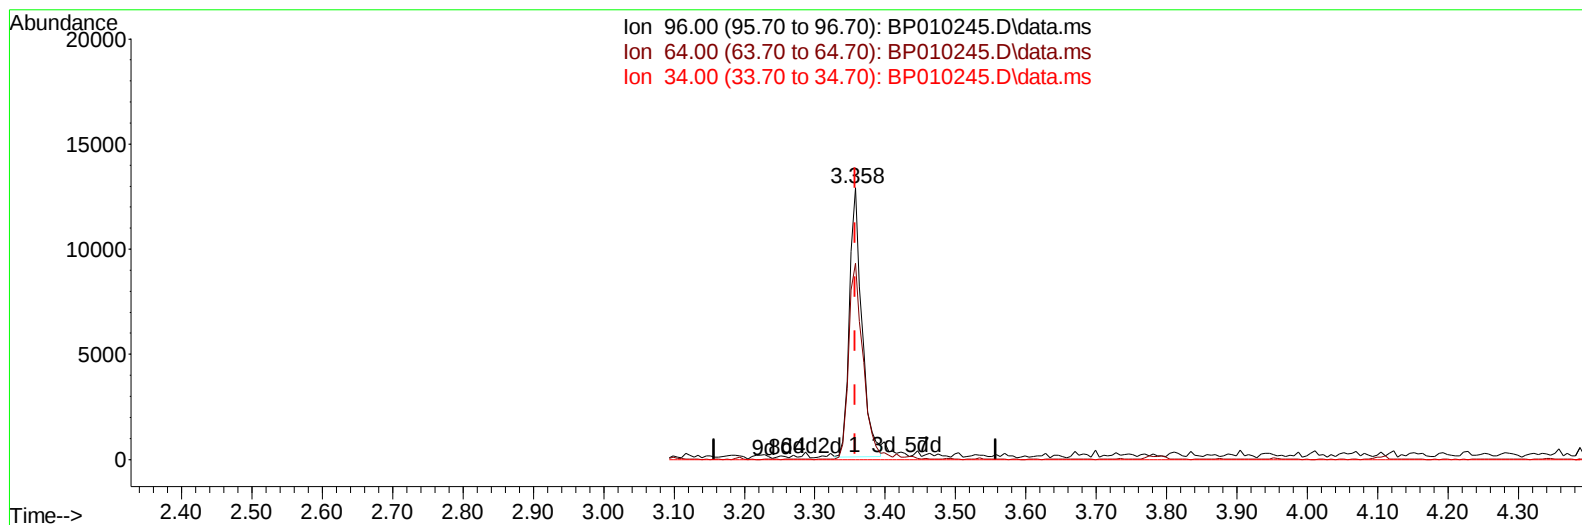

TIC: BP010245.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 4.42 ng/uL

response 15816

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	72.24#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010245.D
 Acq On : 05 May 2022 14:03
 Operator : CG/JU
 Sample : N2668-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL66

Manual IntegrationsAPPROVED

Quant Time: May 06 01:07:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

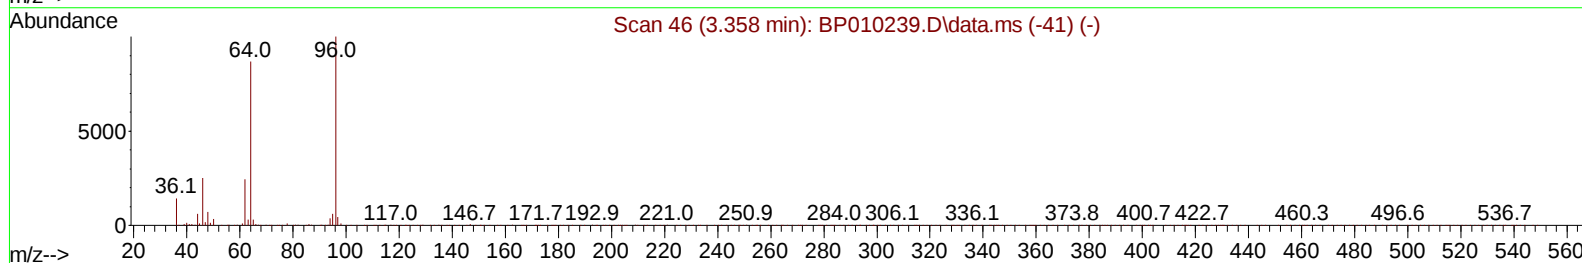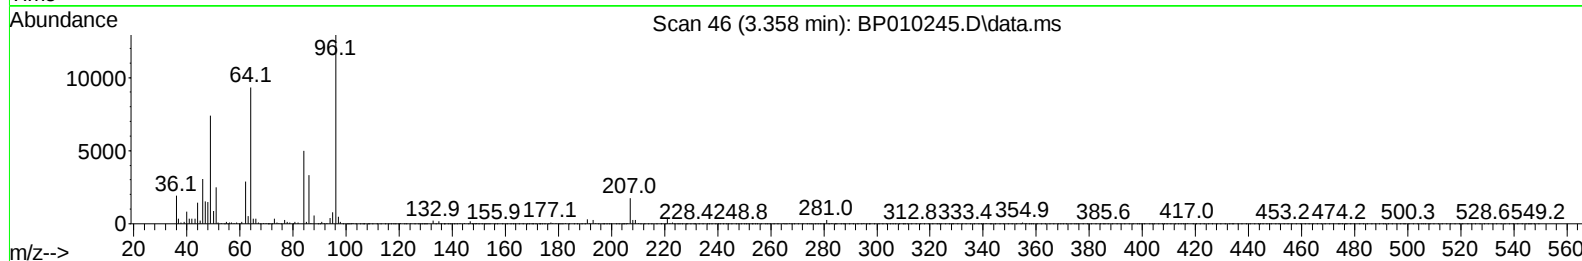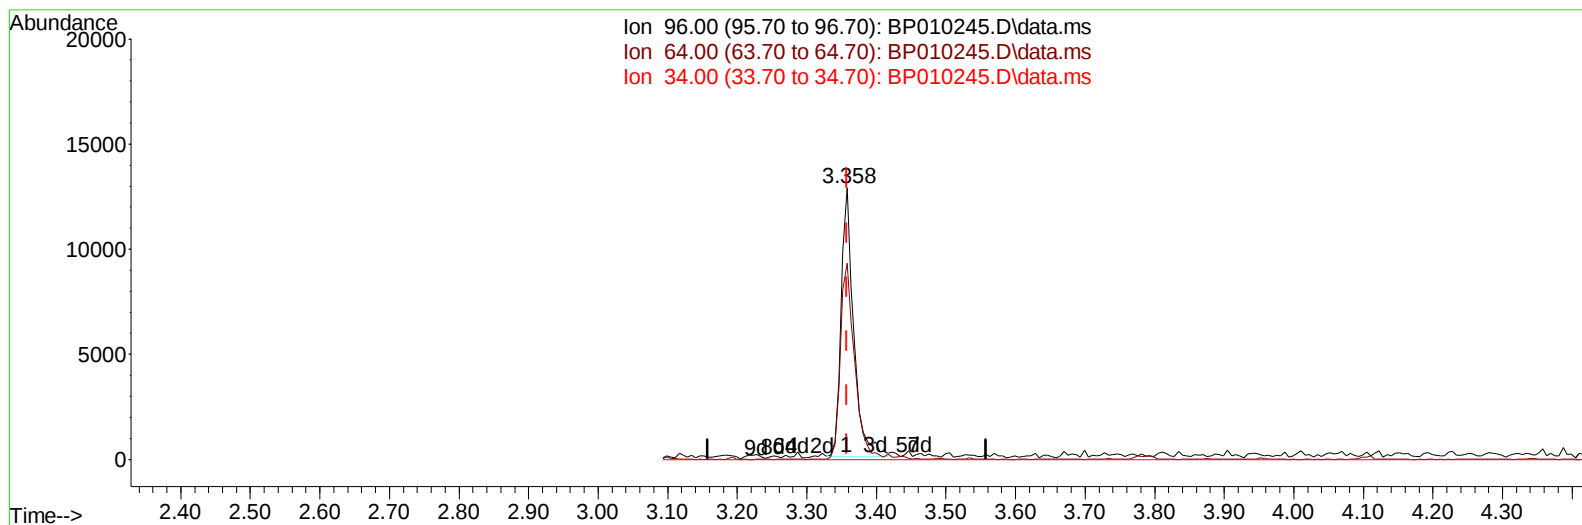

TIC: BP010245.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (-0.000) 4.54 ng/uL m

response 16236

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	72.24#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010245.D
 Acq On : 05 May 2022 14:03
 Operator : CG/JU
 Sample : N2668-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL66

Manual IntegrationsAPPROVED

Quant Time: May 06 01:07:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

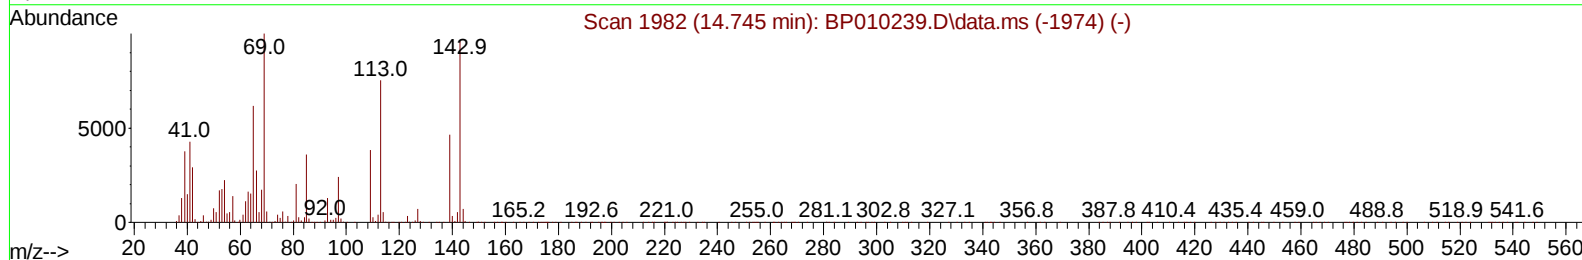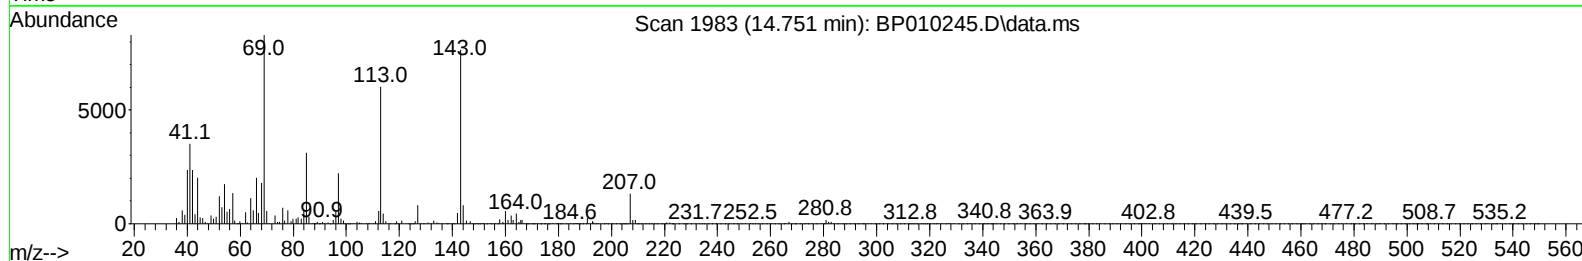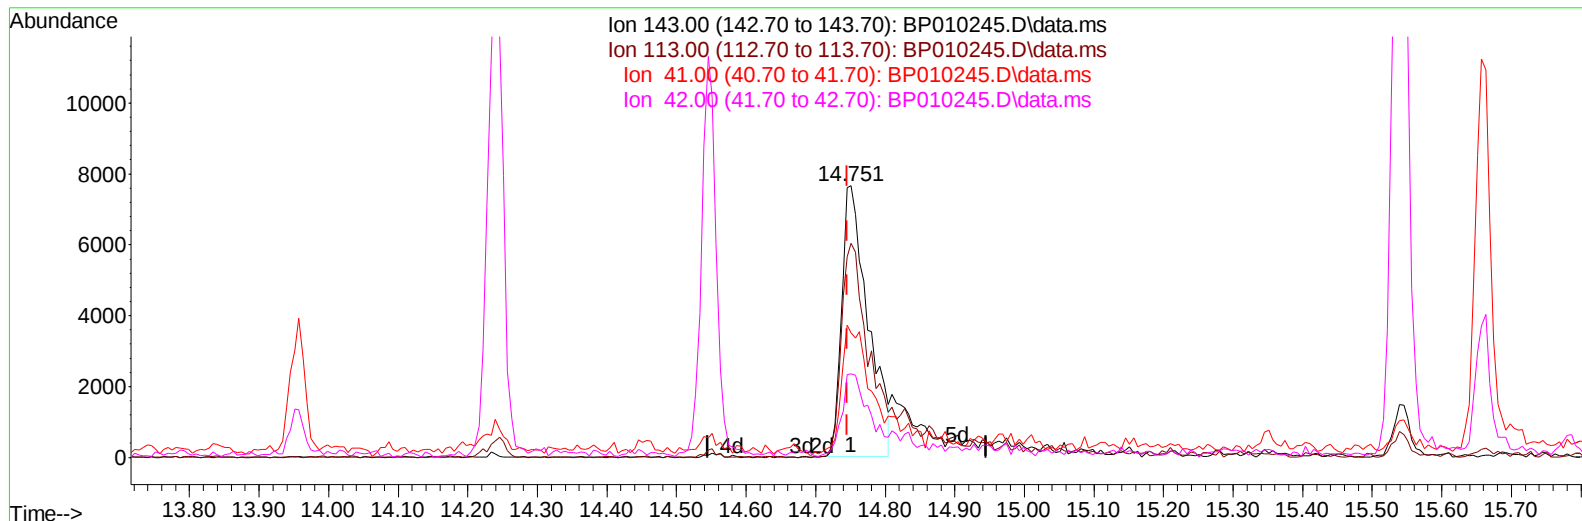

TIC: BP010245.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.006) 2.99 ng/u1

response 20075

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	78.78#
41.00	23.20	45.92#
42.00	18.00	30.77#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010245.D
Acq On : 05 May 2022 14:03
Operator : CG/JU
Sample : N2668-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL66

Manual IntegrationsAPPROVED

Quant Time: May 06 01:07:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

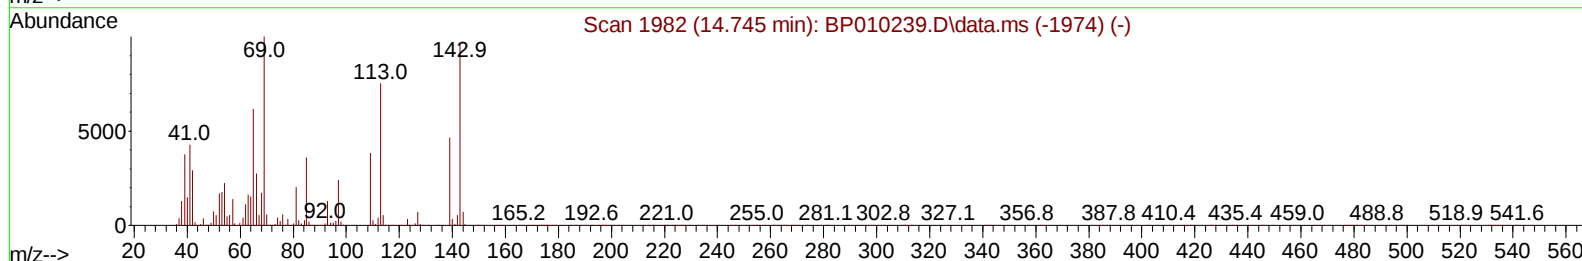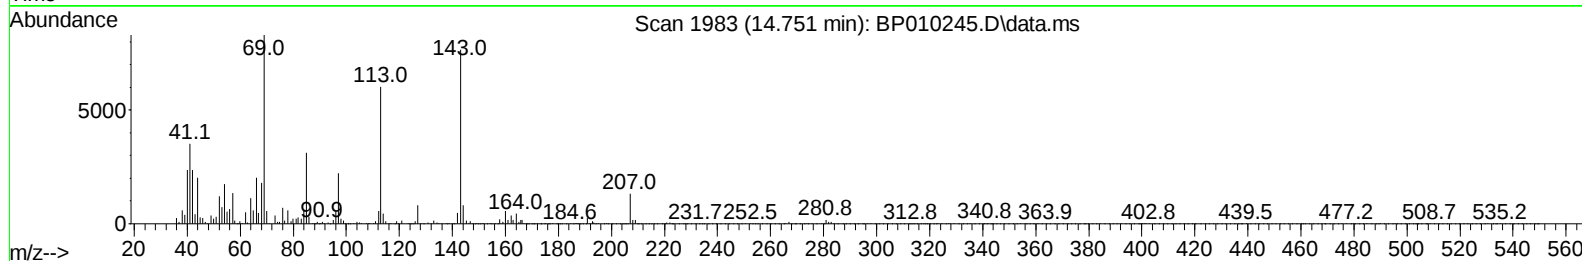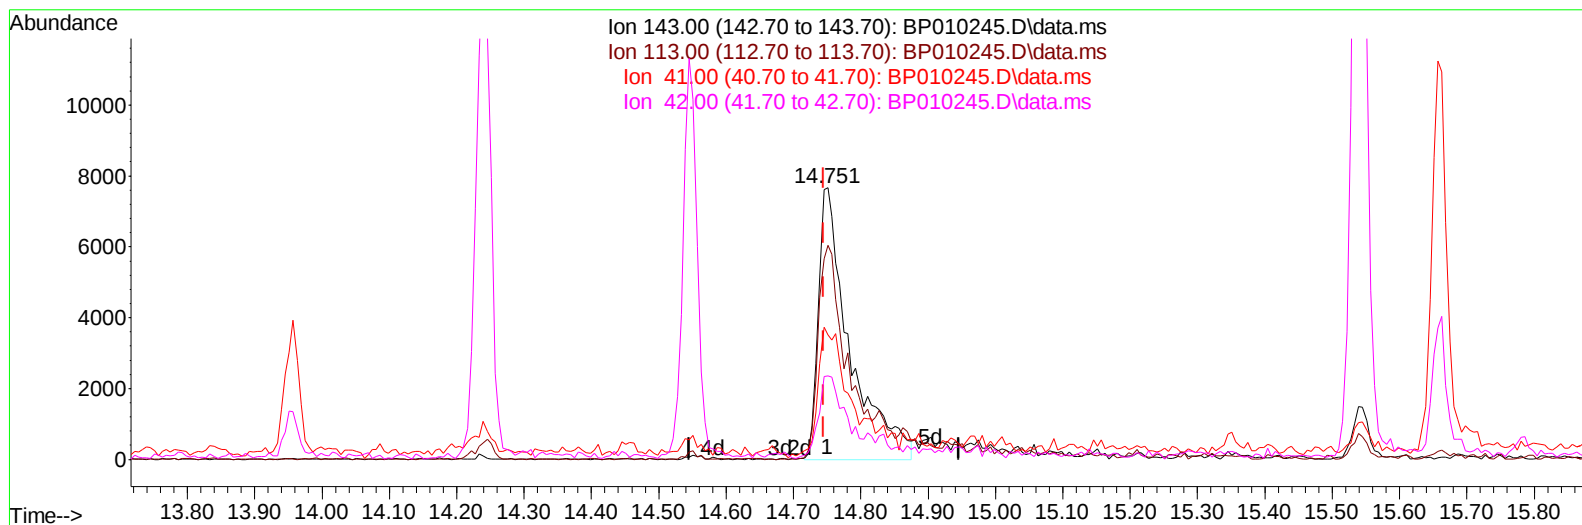

TIC: BP010245.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.006) 3.68 ng/ul m

response 24701

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	78.78#
41.00	23.20	45.92#
42.00	18.00	30.77#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010245.D
 Acq On : 05 May 2022 14:03
 Operator : CG/JU
 Sample : N2668-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL66

Manual IntegrationsAPPROVED

Quant Time: May 06 01:07:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	155981	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136	689302	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	468466	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	955543	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.380	240	684146	20.000	ng/ul	# 0.00
88) Perylene-d12	23.821	264	592996	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	16236m	4.539	ng/uL	0.00
4) Pyridine-d5	3.781	84	93503	9.292	ng/ul	0.01
7) Phenol-d5	7.081	99	81637	5.754	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	322257	37.853	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	273776	26.055	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	176494	15.014	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	196950	35.924	ng/ul	0.00
24) 2-Nitrophenol-d4	9.798	143	207163	34.600	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	324967	27.880	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	452957	27.102	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1366569	37.500	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	1520084	34.466	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	24701m	3.682	ng/ul	0.00
60) Fluorene-d10	15.539	176	1206466	38.487	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	183319	30.341	ng/ul	0.00
73) Anthracene-d10	17.398	188	1899057	41.080	ng/ul	0.00
81) Pyrene-d10	19.627	212	2013735	51.757	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.662	264	1384851	44.546	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010245.D
Acq On : 05 May 2022 14:03
Operator : CG/JU
Sample : N2668-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL66

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 01:07:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

