




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010247.D
 Acq On : 05 May 2022 15:10
 Operator : CG/JU
 Sample : N2678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A2

Manual IntegrationsAPPROVED

Quant Time: May 06 02:10:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

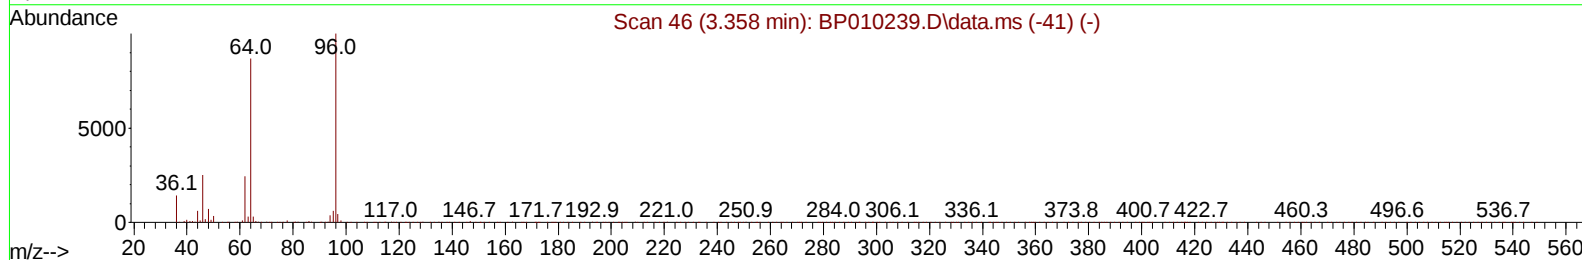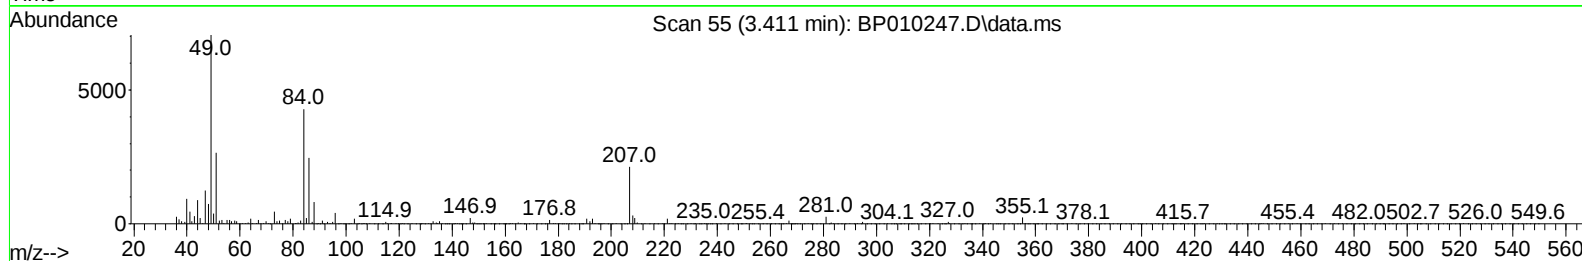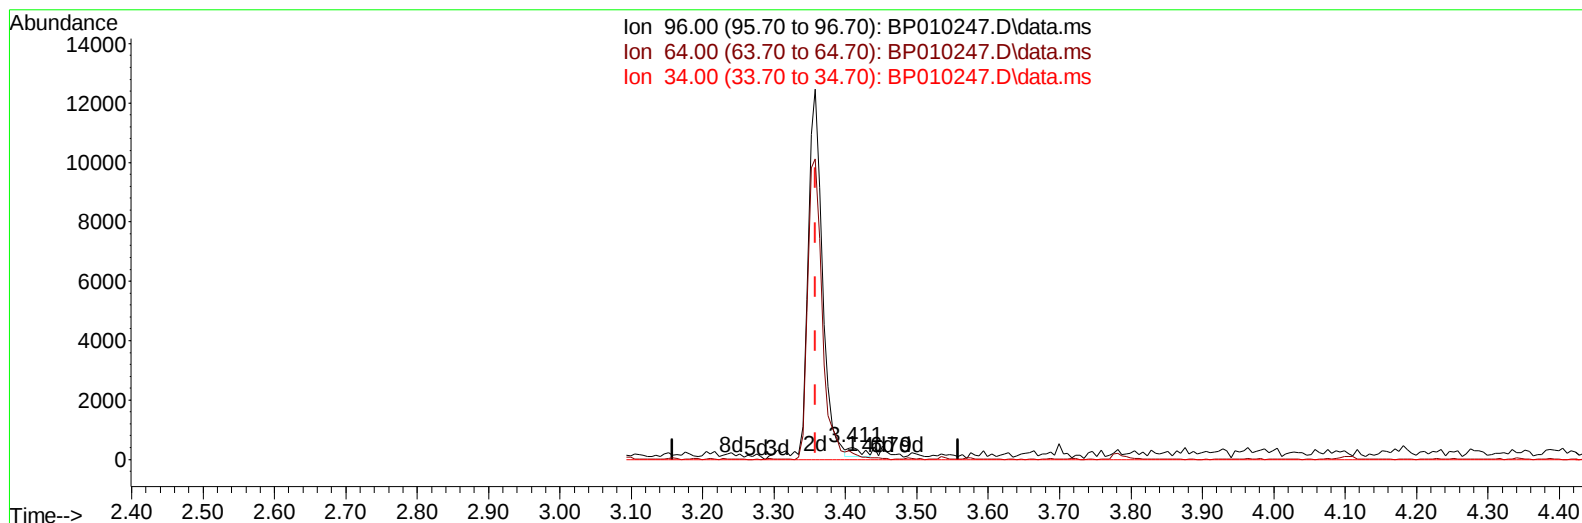

TIC: BP010247.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.411min (+ 0.053) 0.11 ng/uL

response 406

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	49.51
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010247.D
 Acq On : 05 May 2022 15:10
 Operator : CG/JU
 Sample : N2678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A2

Manual IntegrationsAPPROVED

Quant Time: May 06 02:10:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

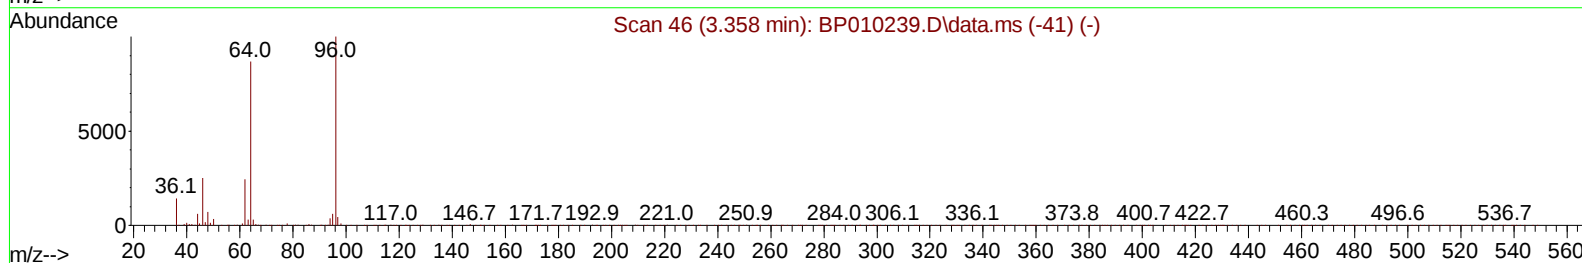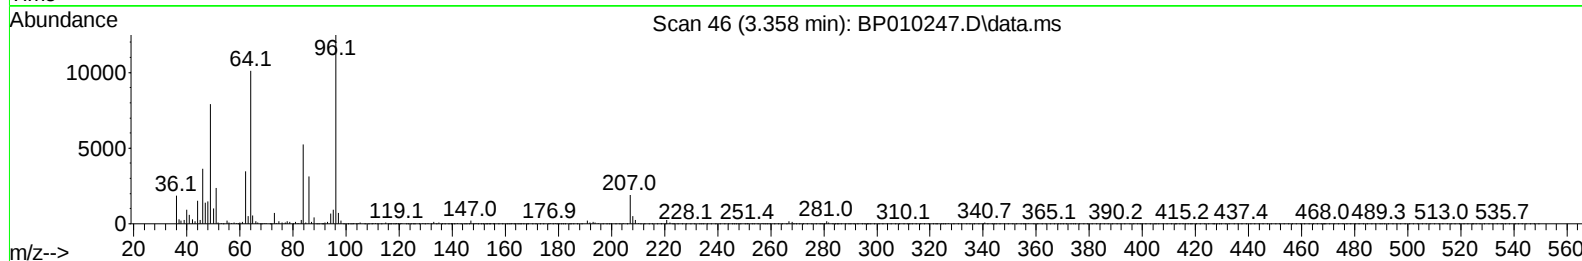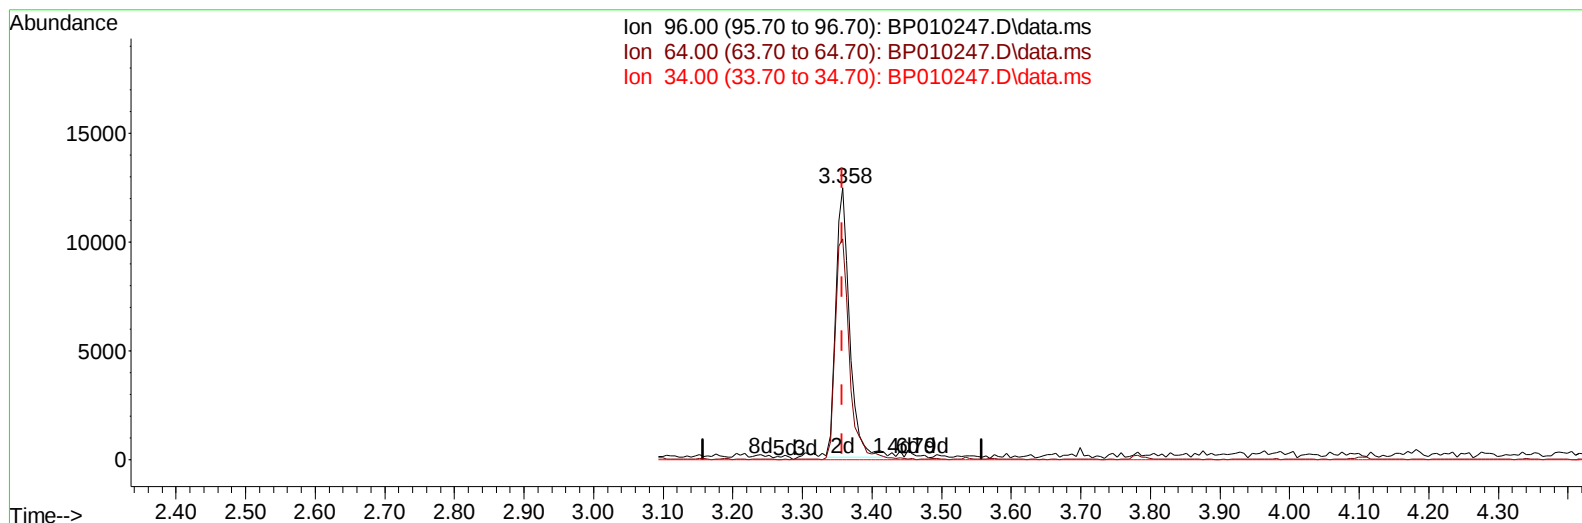

TIC: BP010247.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (+ 0.000) 4.75 ng/uL m

response 17037

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	81.18#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Manual IntegrationsAPPROVED

Quant Time: May 06 02:10:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

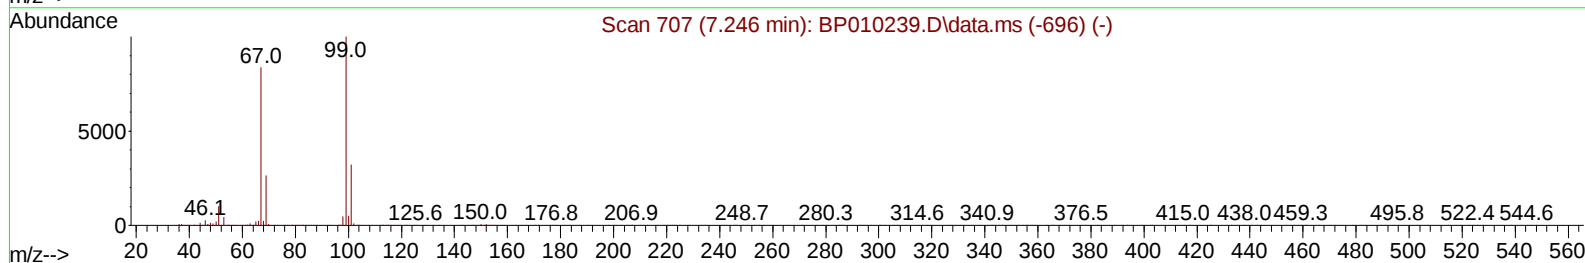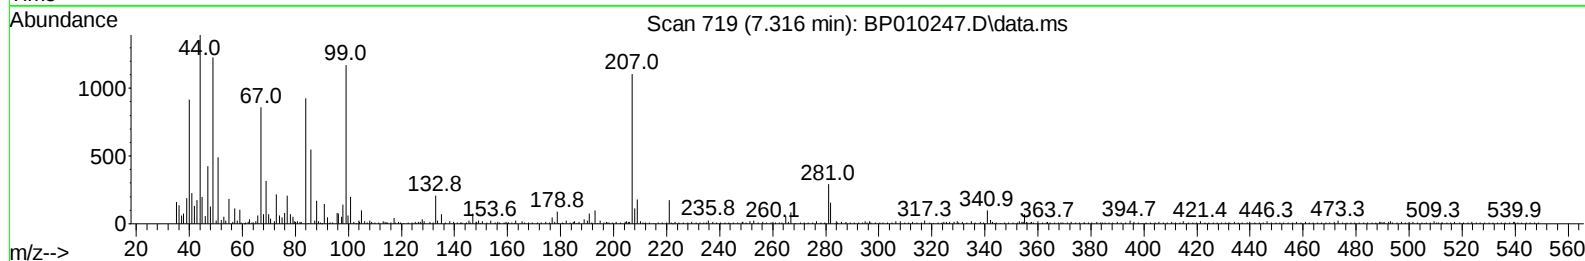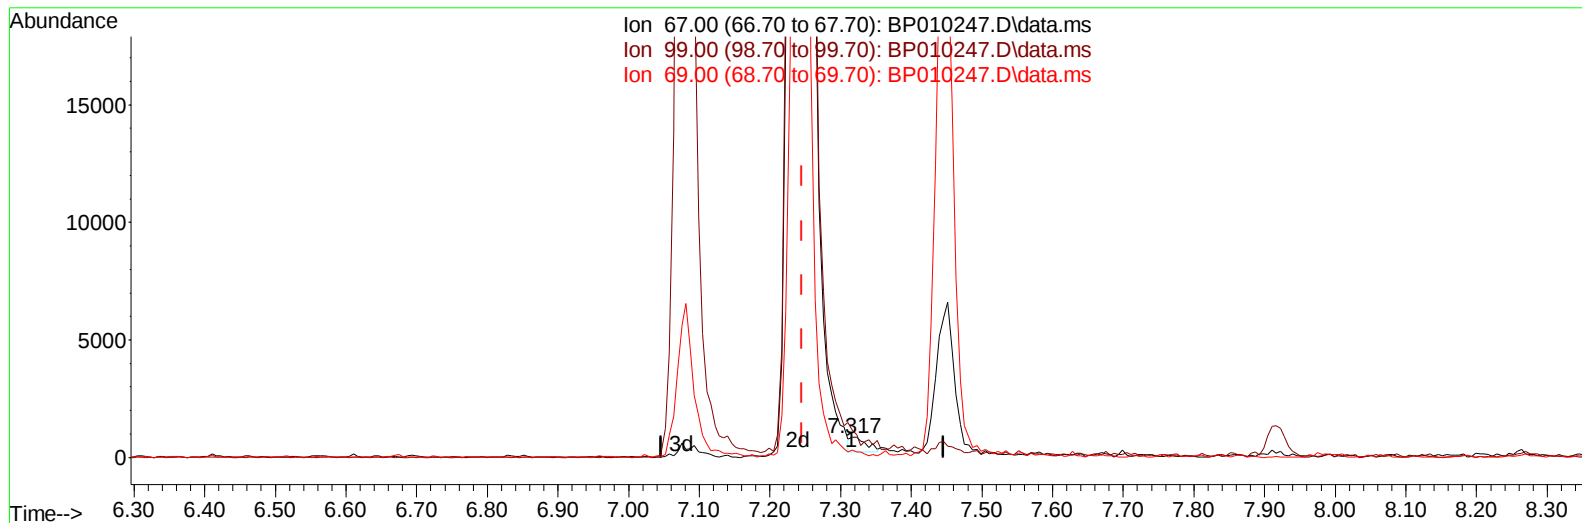

TIC: BP010247.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.316min (+ 0.071) 0.12 ng/u1

response 1003

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	136.55
69.00	40.10	37.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010247.D
 Acq On : 05 May 2022 15:10
 Operator : CG/JU
 Sample : N2678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A2

Manual IntegrationsAPPROVED

Quant Time: May 06 02:10:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

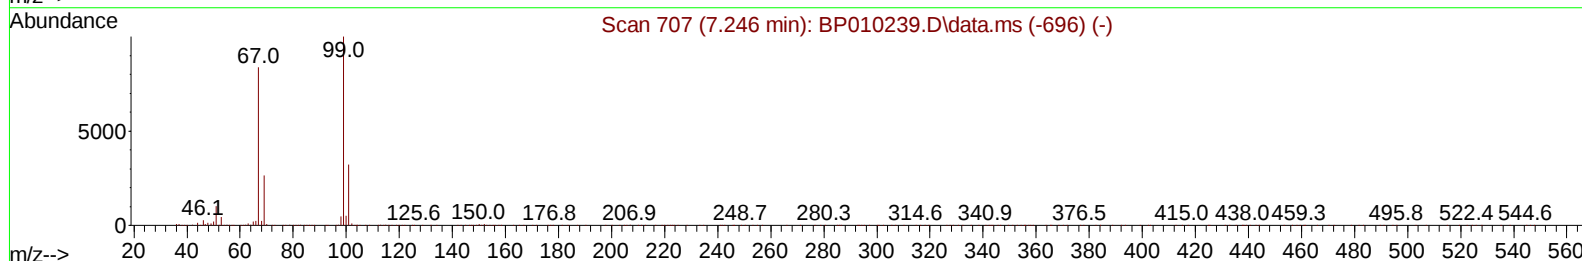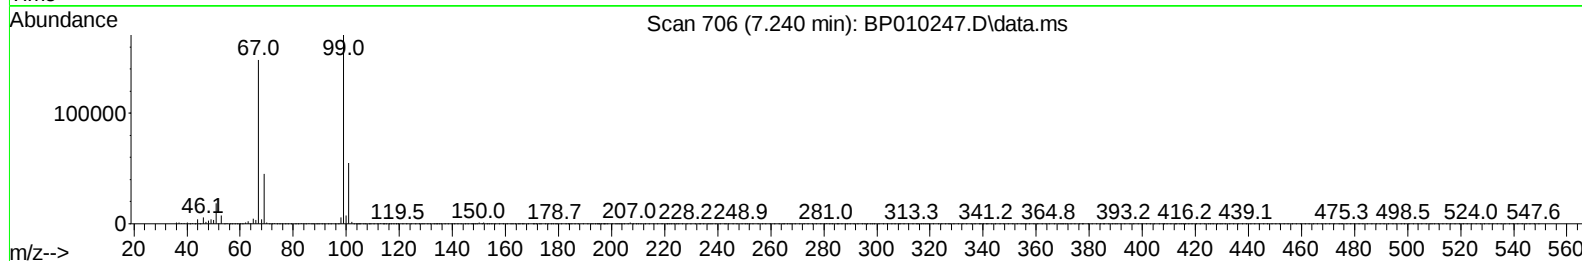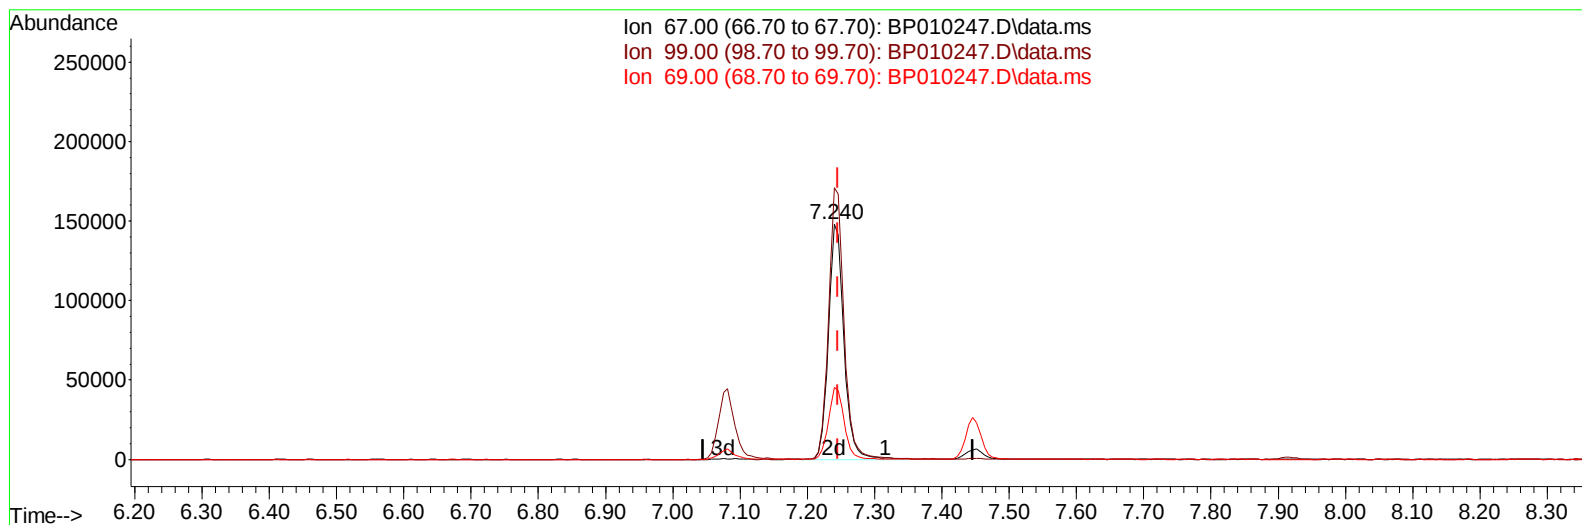

TIC: BP010247.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.240min (-0.006) 28.05 ng/ul m

response 239502

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	115.39#
69.00	40.10	30.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Manual IntegrationsAPPROVED

Quant Time: May 06 02:10:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

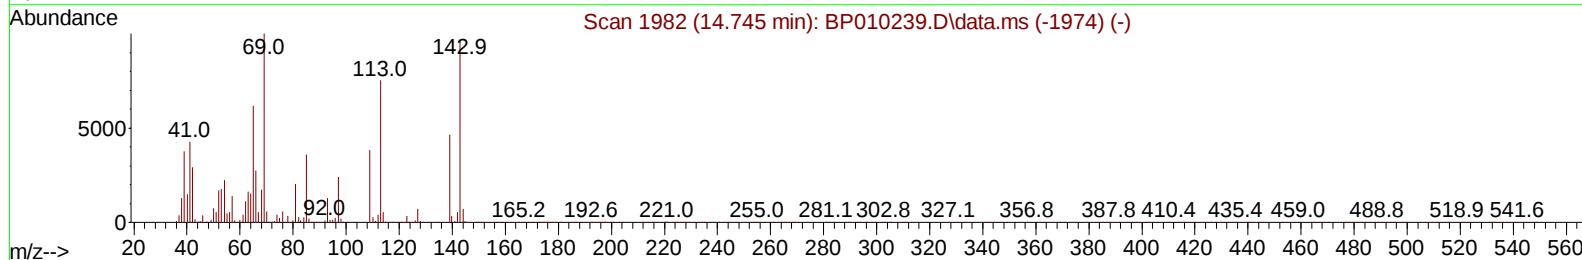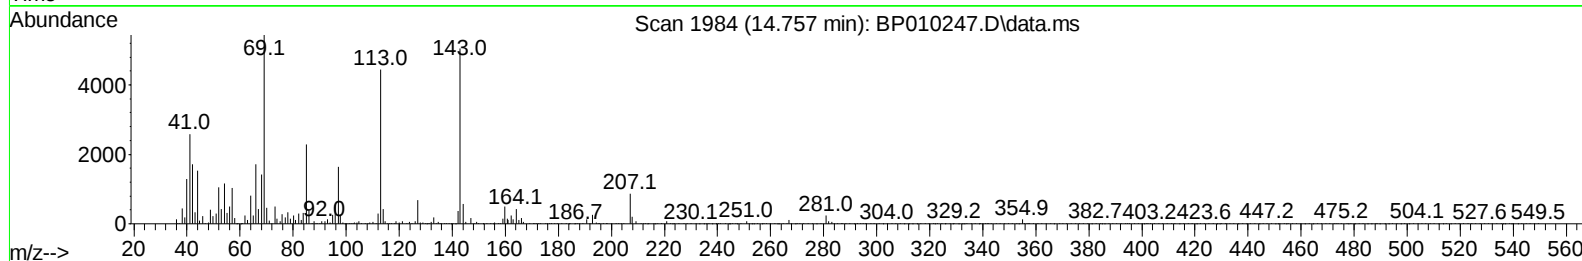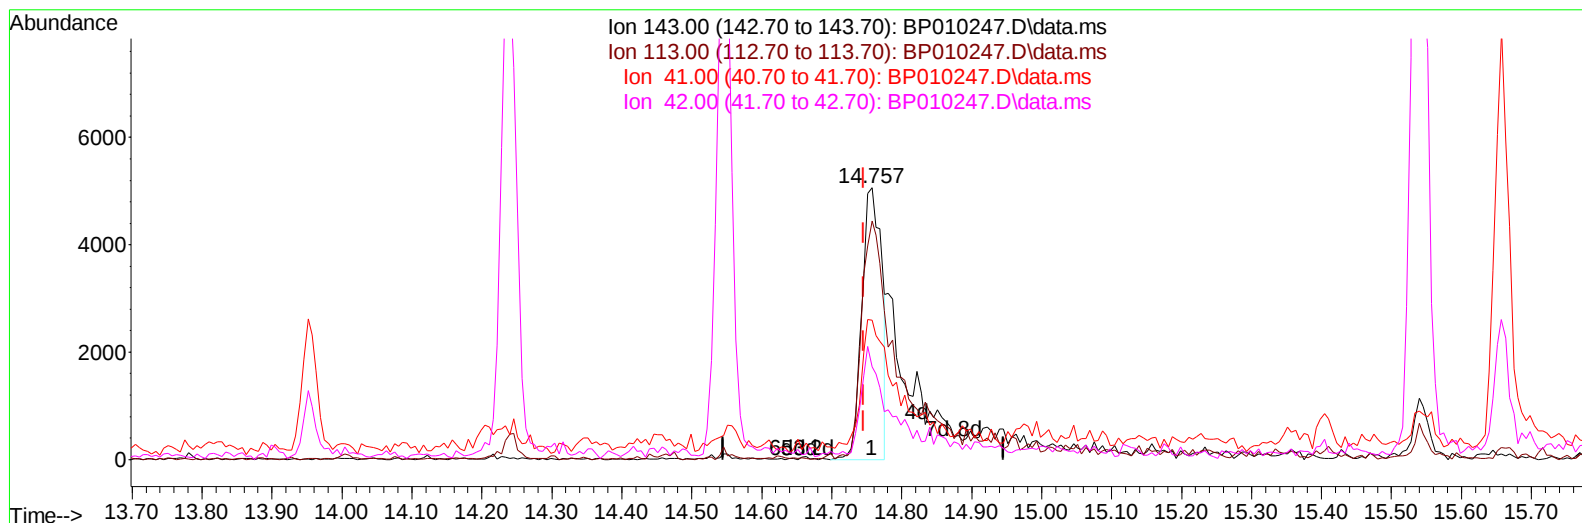

TIC: BP010247.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.012) 1.56 ng/u1

response 9997

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	87.71#
41.00	23.20	51.20#
42.00	18.00	34.02#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Manual IntegrationsAPPROVED

Quant Time: May 06 02:10:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

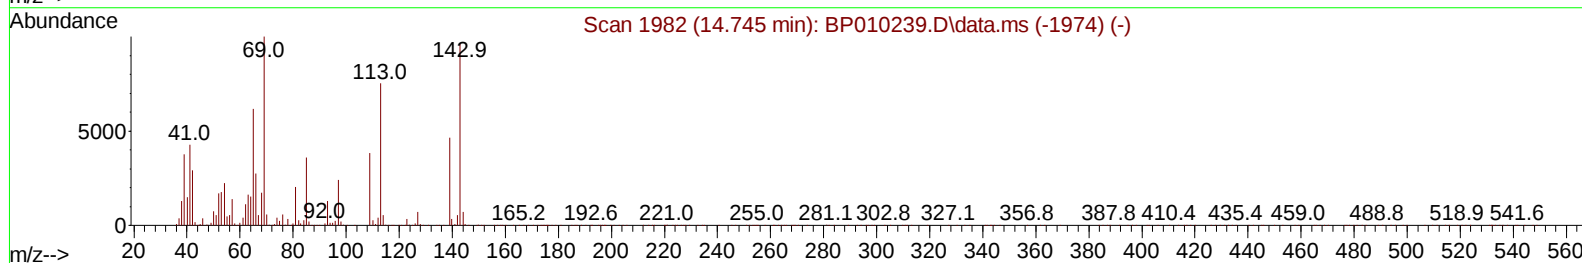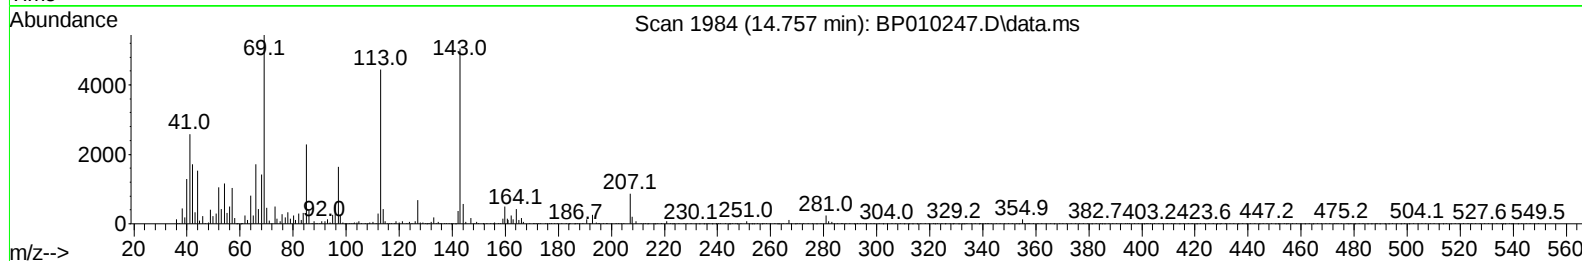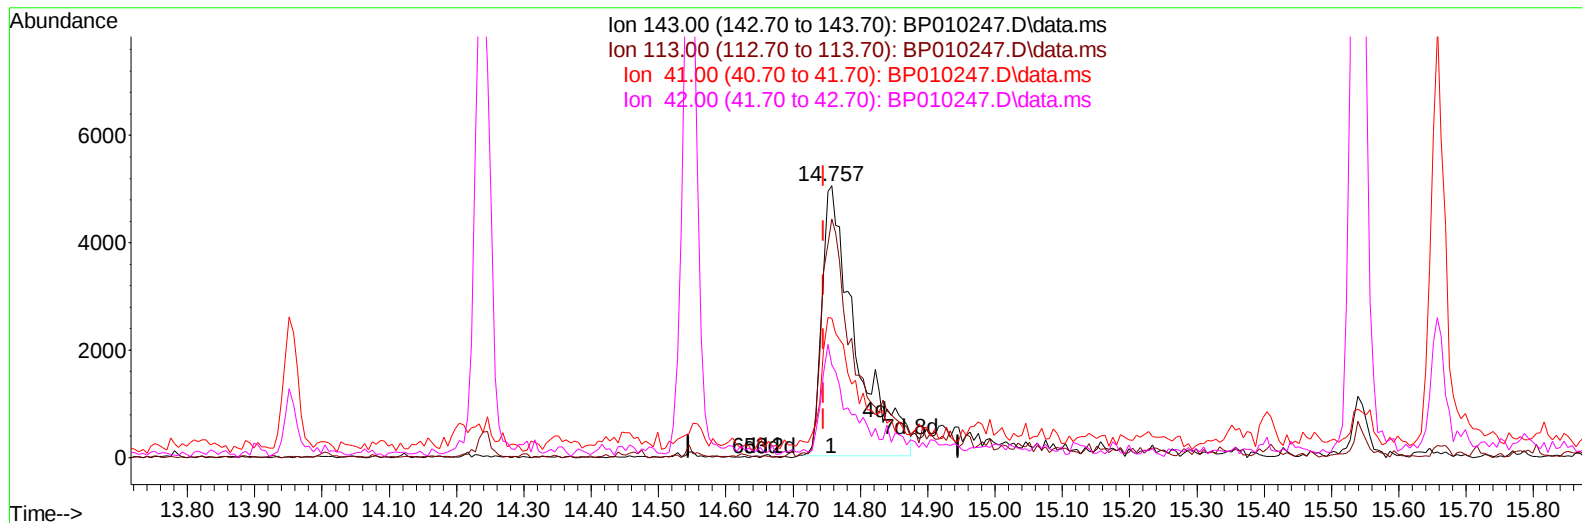

TIC: BP010247.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.012) 2.72 ng/ul m

response 17444

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	87.71#
41.00	23.20	51.20#
42.00	18.00	34.02#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010247.D
 Acq On : 05 May 2022 15:10
 Operator : CG/JU
 Sample : N2678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 02:10:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	156462	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136	676276	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.546	164	448565	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	843759	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.380	240	614010	20.000	ng/ul	0.00
88) Perylene-d12	23.822	264	588799	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	17037m	4.748	ng/uL	0.00
4) Pyridine-d5	3.781	84	68603	6.797	ng/ul	0.01
7) Phenol-d5	7.081	99	74715	5.250	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	239502m	28.046	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	217302	20.617	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	148626	12.605	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	145581	27.066	ng/ul	0.00
24) 2-Nitrophenol-d4	9.799	143	147056	25.034	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	244976	21.422	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	216723	13.217	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	977457	28.013	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	1050876	24.884	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	17444m	2.716	ng/ul	0.01
60) Fluorene-d10	15.540	176	821011	27.353	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	110701	20.749	ng/ul	0.00
73) Anthracene-d10	17.398	188	1248274	30.580	ng/ul	0.00
81) Pyrene-d10	19.628	212	1306712	37.421	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.663	264	1014480	32.865	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 02:10:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

