




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010254.D
 Acq On : 05 May 2022 19:06
 Operator : CG/JU
 Sample : N2678-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B8

Manual IntegrationsAPPROVED

Quant Time: May 06 02:07:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

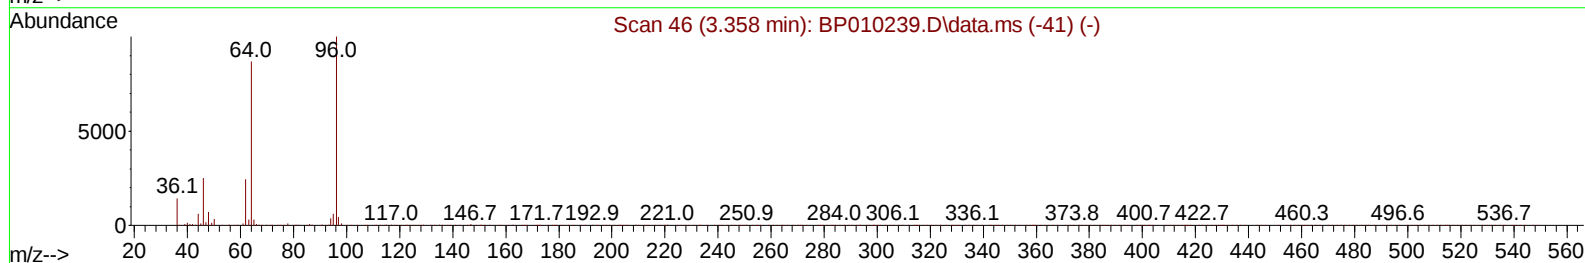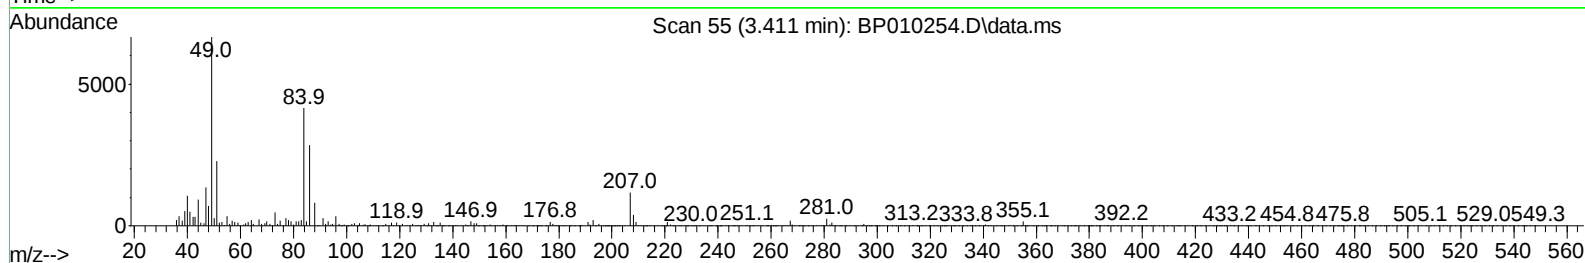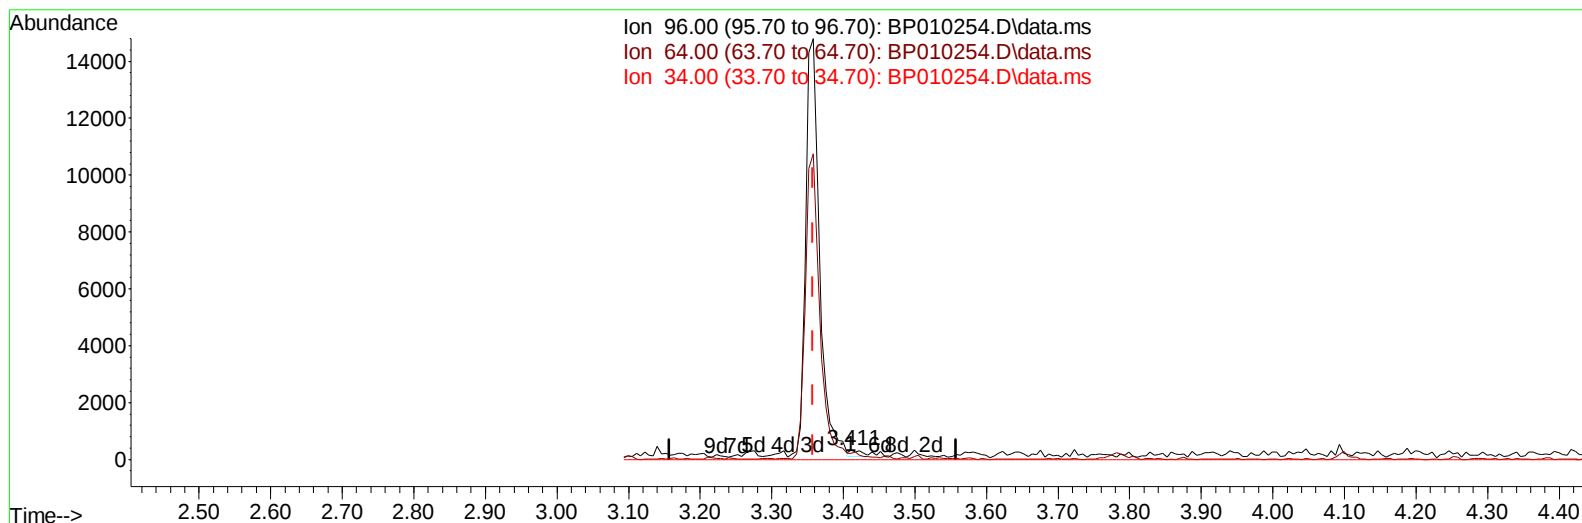

TIC: BP010254.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.411min (+ 0.053) 0.06 ng/uL

response 243

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	61.72
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010254.D
 Acq On : 05 May 2022 19:06
 Operator : CG/JU
 Sample : N2678-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B8

Manual IntegrationsAPPROVED

Quant Time: May 06 02:07:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

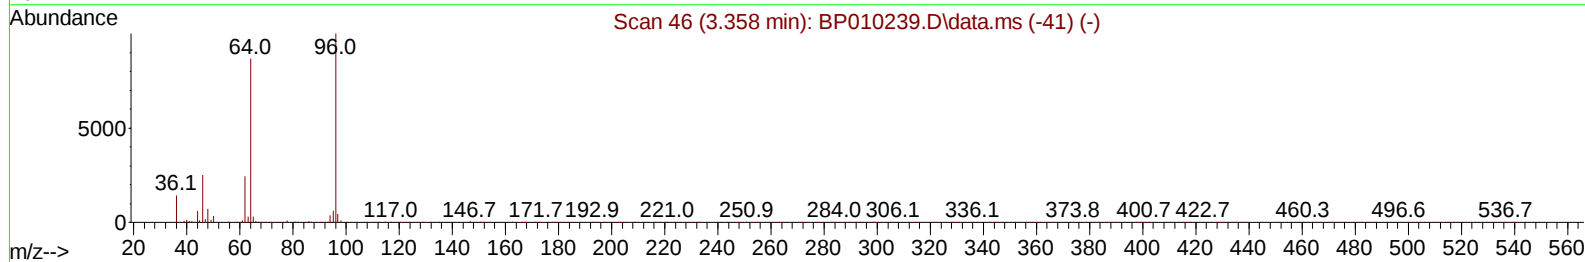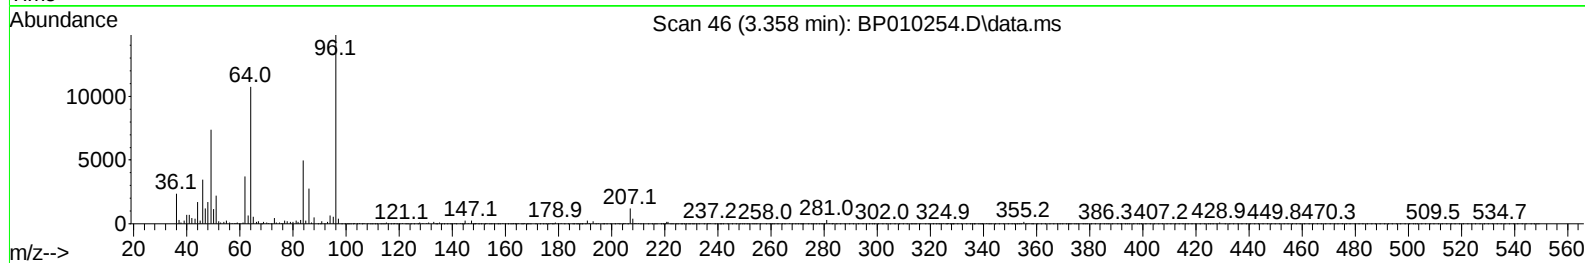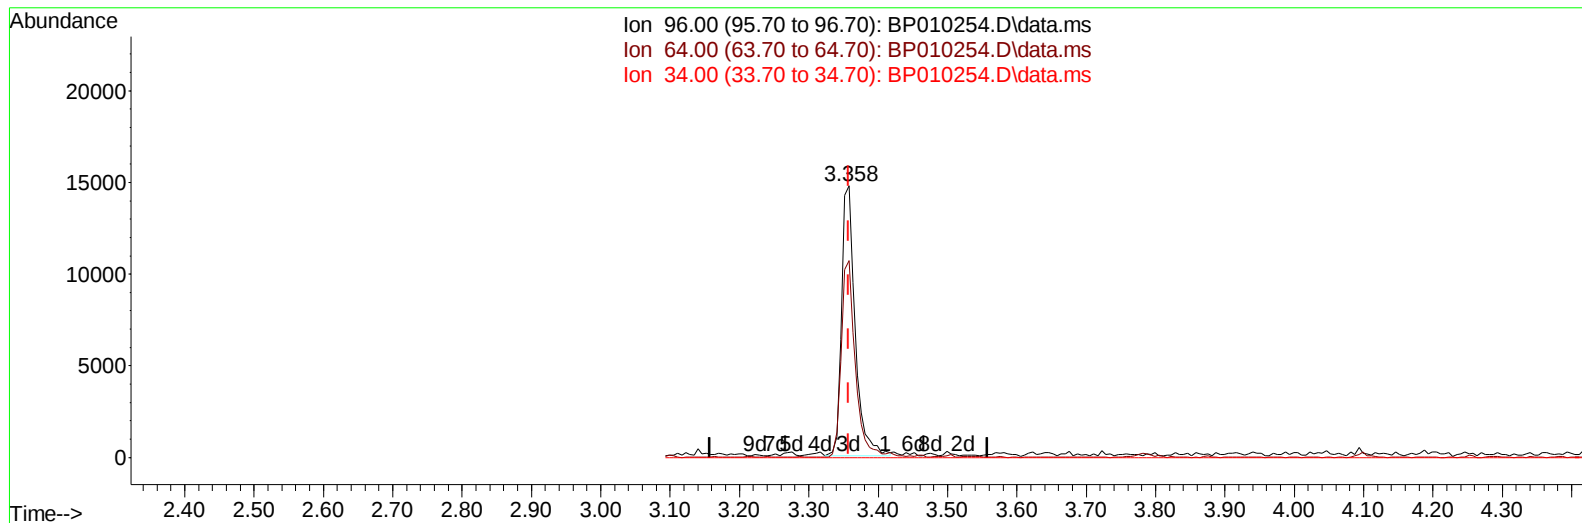

TIC: BP010254.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.358min (+ 0.000) 4.75 ng/uL m

response 20077

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	72.53#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010254.D
Acq On : 05 May 2022 19:06
Operator : CG/JU
Sample : N2678-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B8

Manual IntegrationsAPPROVED

Quant Time: May 06 02:07:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

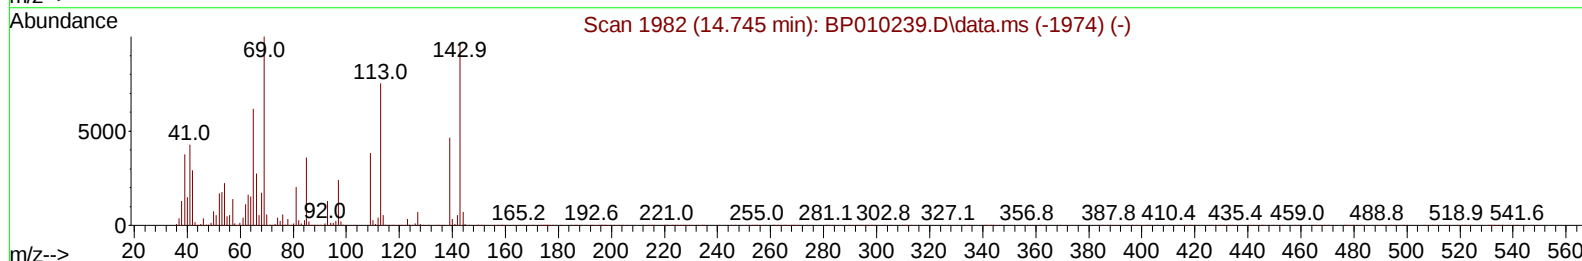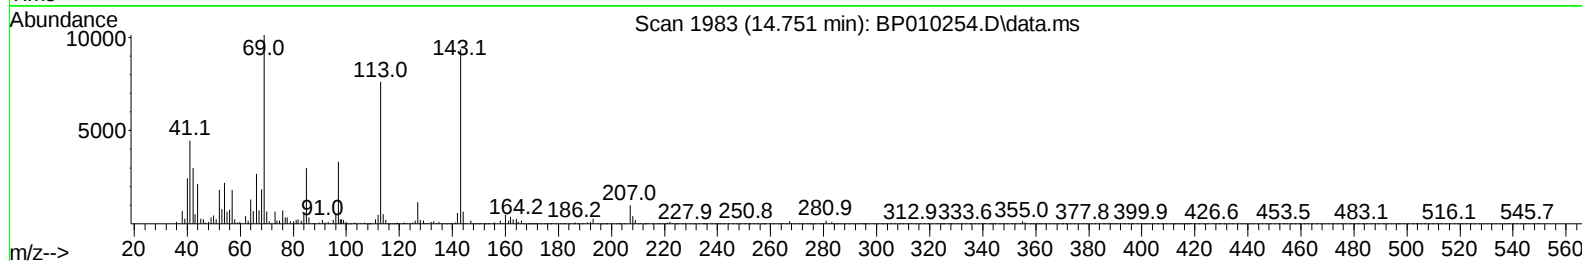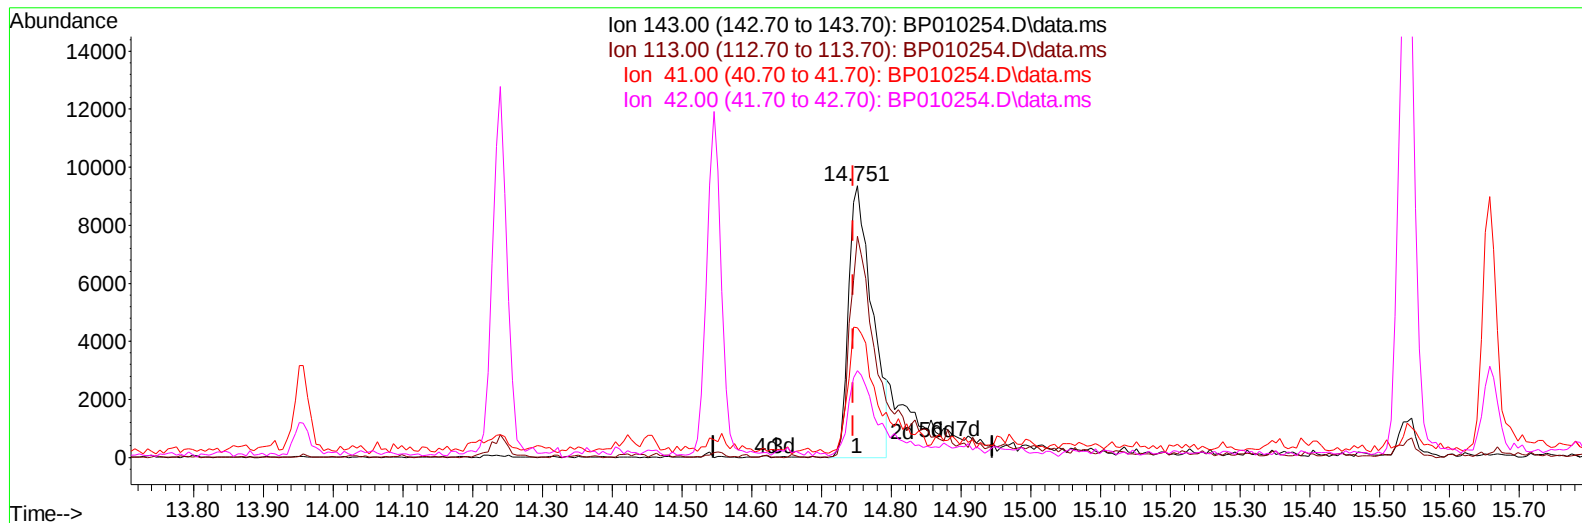

TIC: BP010254.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.006) 2.93 ng/u1

response 22141

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.56#
41.00	23.20	47.73#
42.00	18.00	32.08#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010254.D
Acq On : 05 May 2022 19:06
Operator : CG/JU
Sample : N2678-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B8

Manual IntegrationsAPPROVED

Quant Time: May 06 02:07:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

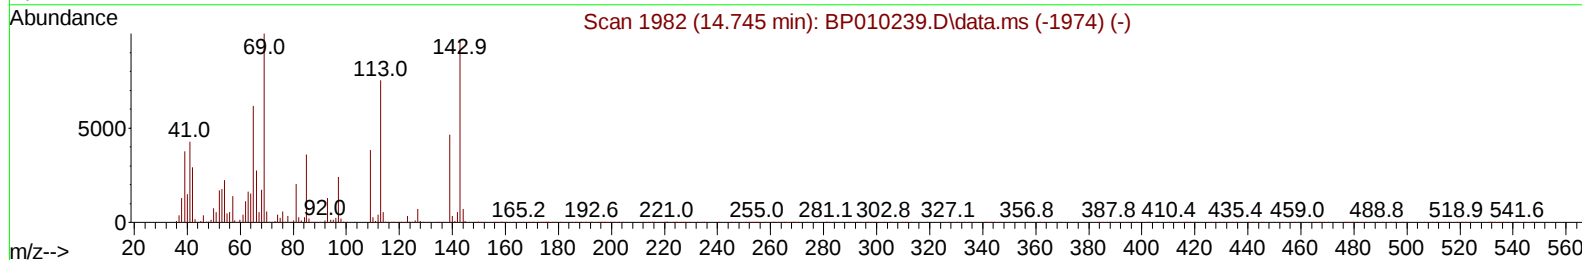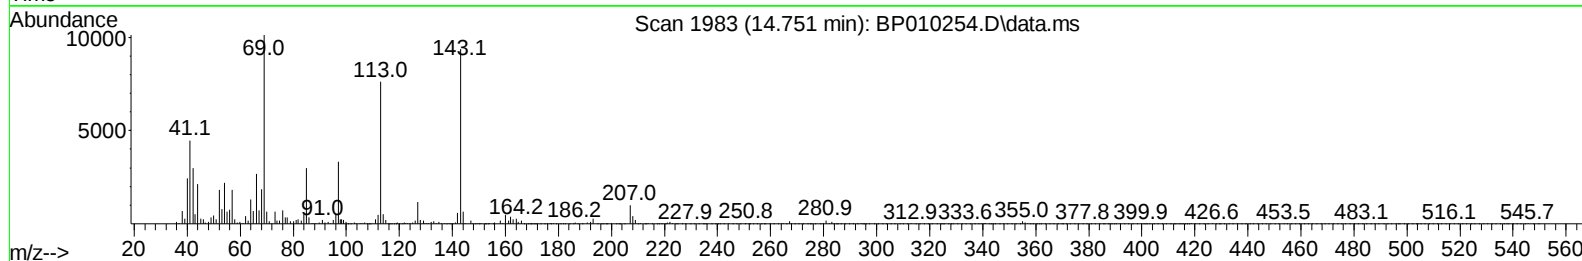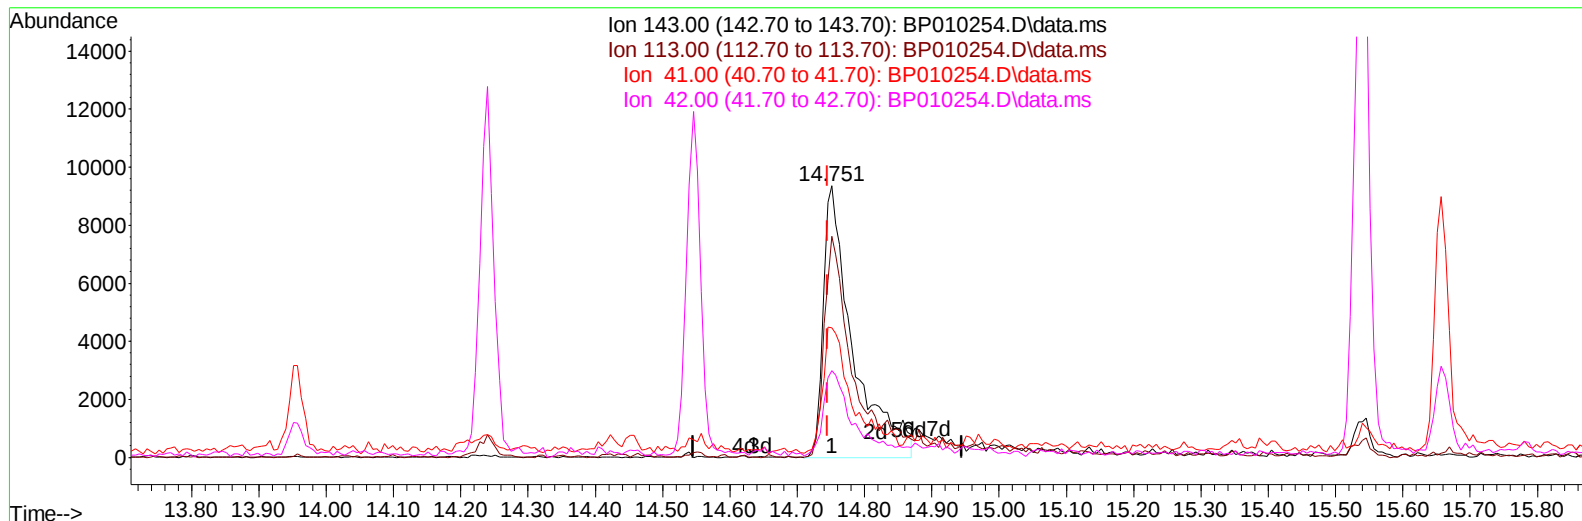

TIC: BP010254.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.751min (+ 0.006) 3.80 ng/ul m

response 28737

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.56#
41.00	23.20	47.73#
42.00	18.00	32.08#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010254.D
Acq On : 05 May 2022 19:06
Operator : CG/JU
Sample : N2678-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B8

Manual IntegrationsAPPROVED

Quant Time: May 06 02:07:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

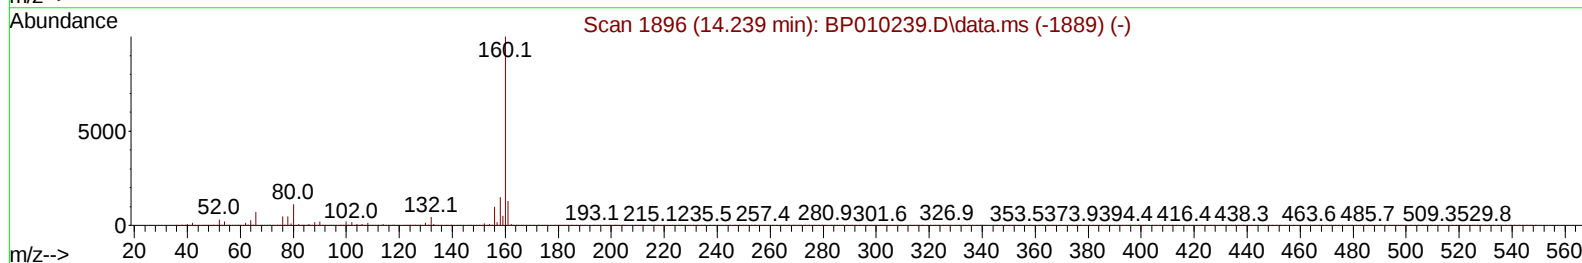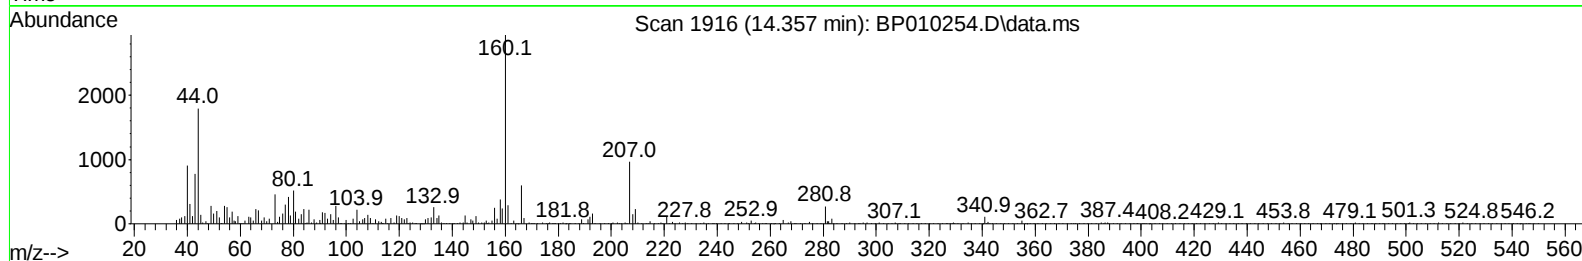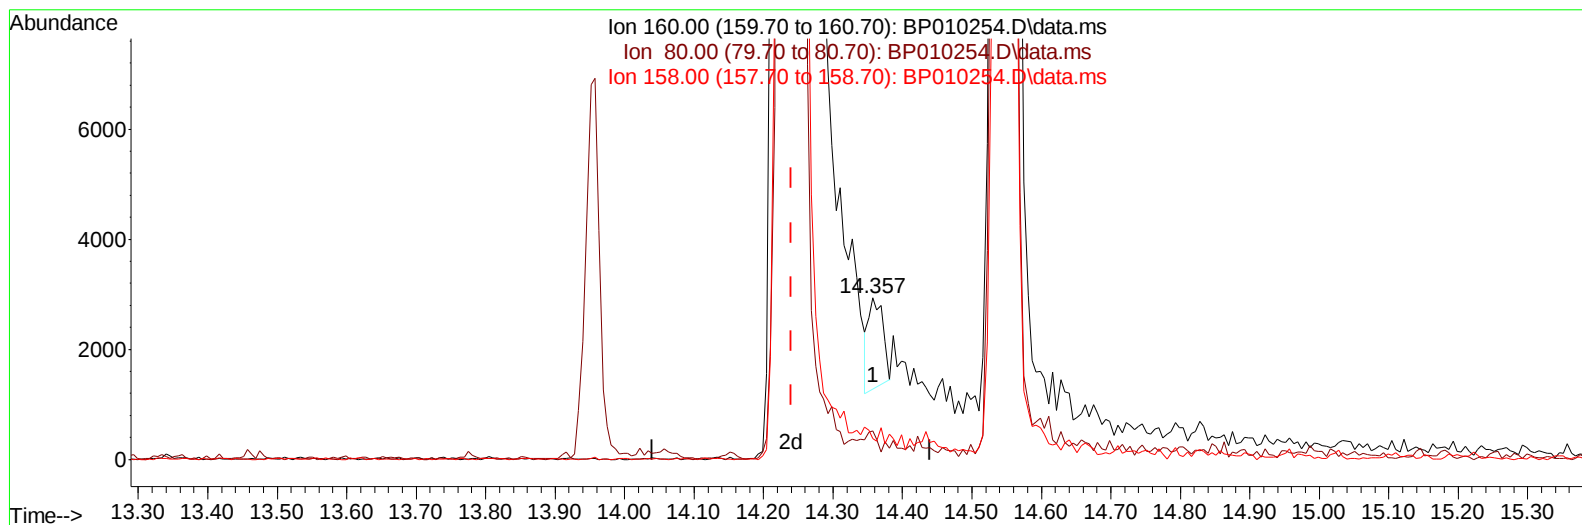

TIC: BP010254.D\data.ms

(49) Acenaphthylene-d8 (S)

14.357min (+ 0.118) 0.05 ng/u1

response 2366

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	17.00	17.50
158.00	13.10	12.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010254.D
Acq On : 05 May 2022 19:06
Operator : CG/JU
Sample : N2678-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B8

Manual IntegrationsAPPROVED

Quant Time: May 06 02:07:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

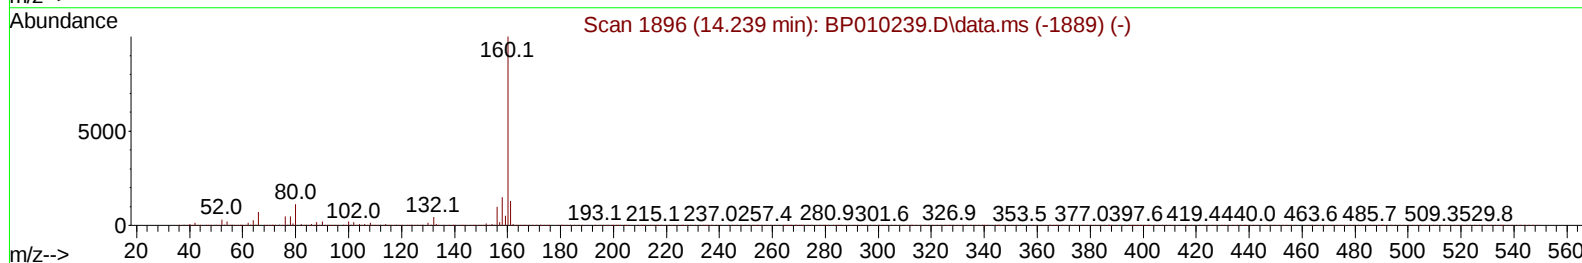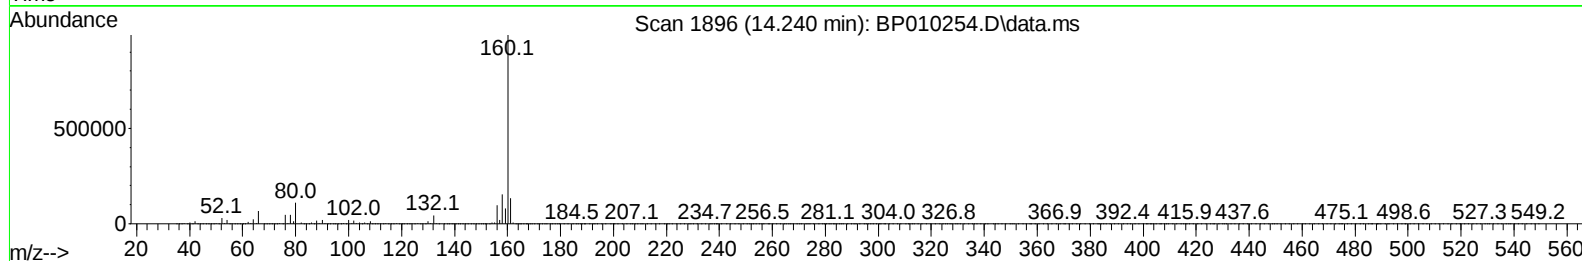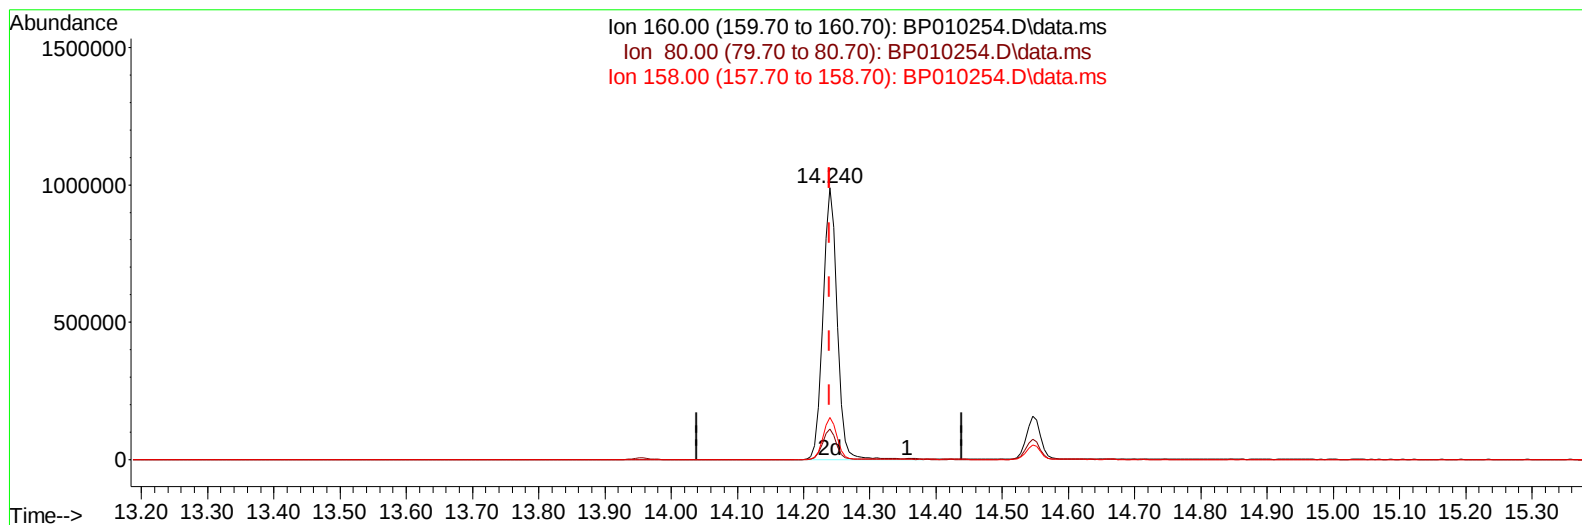

TIC: BP010254.D\data.ms

(49) Acenaphthylene-d8 (S)

14.240min (+ 0.000) 30.03 ng/ul m

response 1492396

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	17.00	11.26#
158.00	13.10	15.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010254.D
 Acq On : 05 May 2022 19:06
 Operator : CG/JU
 Sample : N2678-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 02:07:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	184301	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136	814426	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.546	164	527829	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1026004	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.380	240	649502	20.000	ng/ul	0.00
88) Perylene-d12	23.822	264	612196	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	20077m	4.750	ng/uL	0.00
4) Pyridine-d5	3.781	84	88945	7.481	ng/ul	0.01
7) Phenol-d5	7.081	99	103137	6.152	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	318436	31.657	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	294382	23.711	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	201175	14.484	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	201638	31.129	ng/ul	0.00
24) 2-Nitrophenol-d4	9.799	143	207576	29.342	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	338372	24.570	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	323207	16.368	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1341894	32.682	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	1492396m	30.032	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	28737m	3.802	ng/ul	0.00
60) Fluorene-d10	15.540	176	1143238	32.369	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	139074	21.437	ng/ul	0.00
73) Anthracene-d10	17.398	188	1763655	35.531	ng/ul	0.00
81) Pyrene-d10	19.628	212	1710012	46.295	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.669	264	1190602	37.096	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010254.D
Acq On : 05 May 2022 19:06
Operator : CG/JU
Sample : N2678-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 02:07:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

