




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010255.D
Acq On : 05 May 2022 19:40
Operator : CG/JU
Sample : N2678-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B9

Manual IntegrationsAPPROVED

Quant Time: May 06 02:08:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

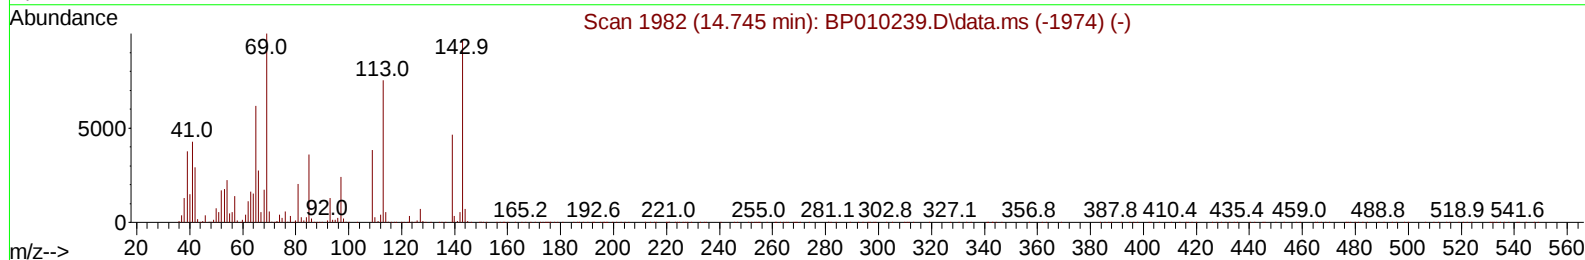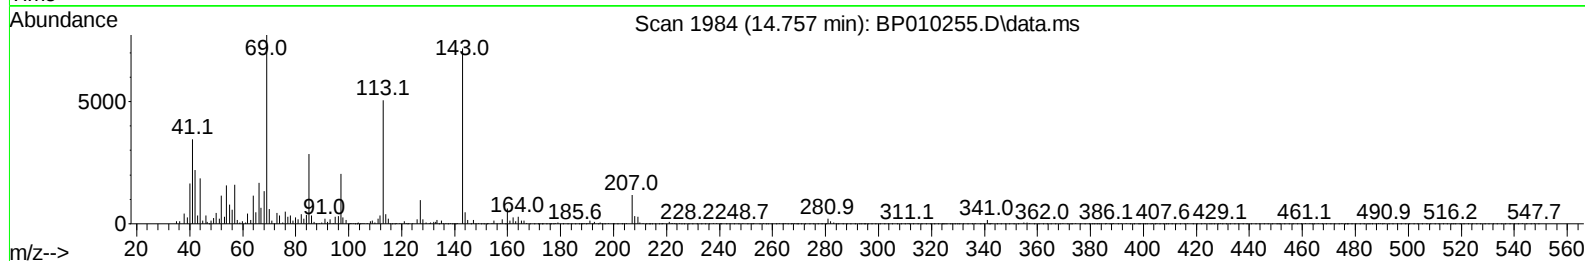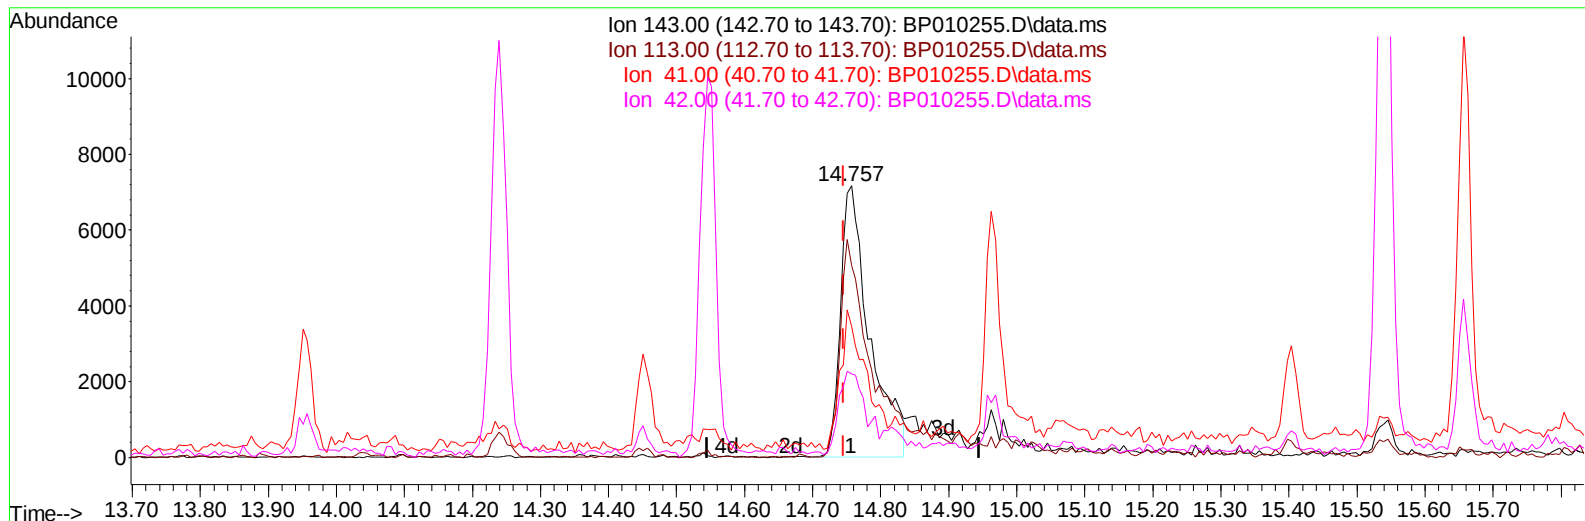

TIC: BP010255.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.012) 3.08 ng/u1

response 21302

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	70.68#
41.00	23.20	48.34#
42.00	18.00	30.72#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010255.D
Acq On : 05 May 2022 19:40
Operator : CG/JU
Sample : N2678-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B9

Manual IntegrationsAPPROVED

Quant Time: May 06 02:08:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

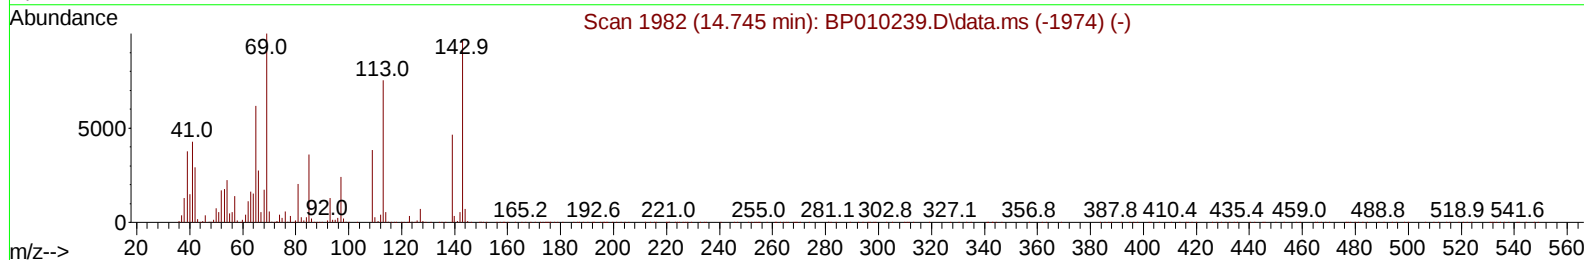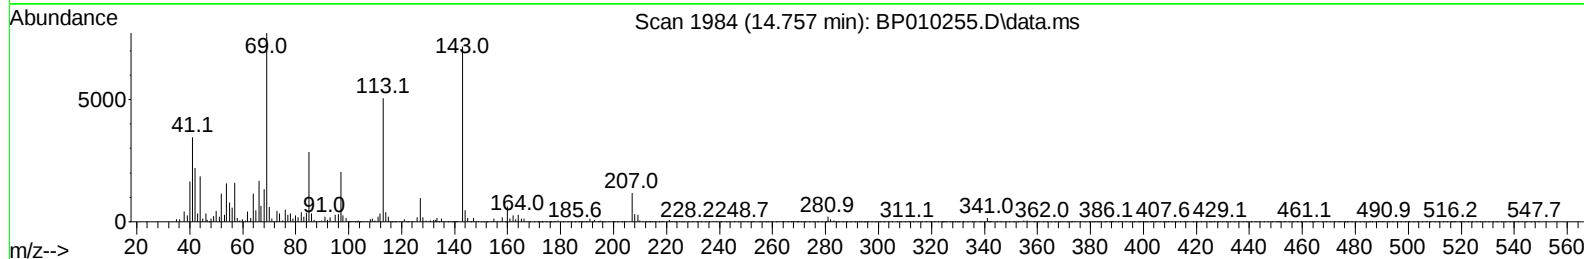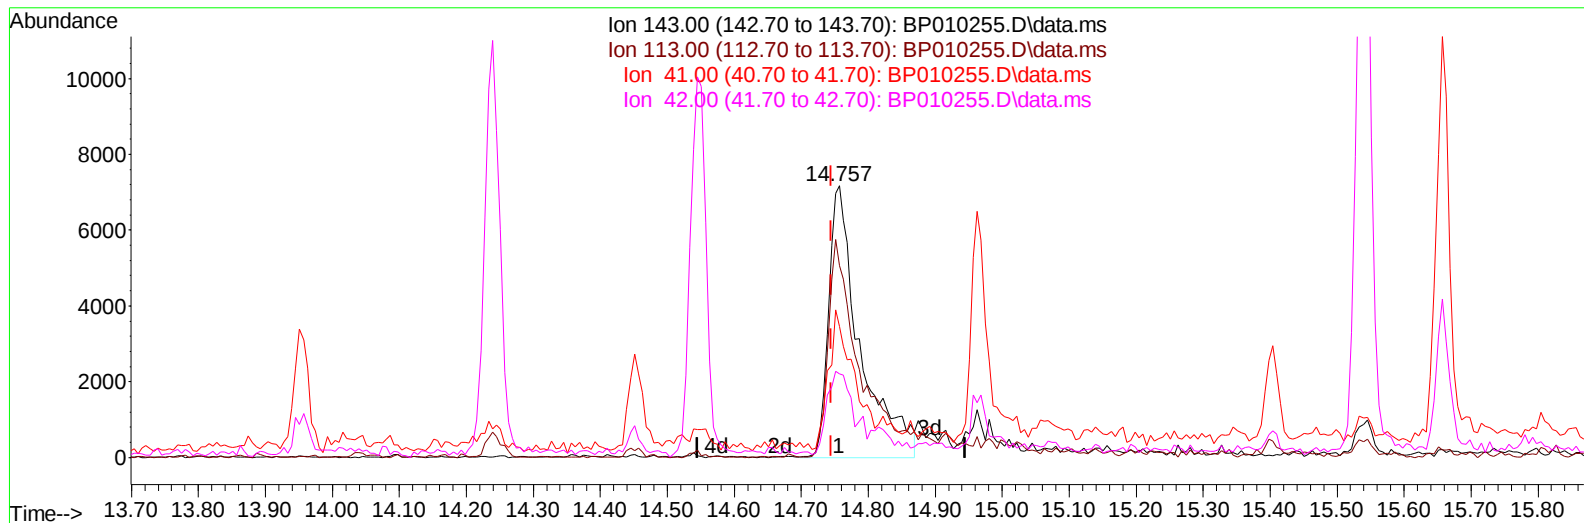

TIC: BP010255.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (+ 0.012) 3.37 ng/ul m

response 23290

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	70.68#
41.00	23.20	48.34#
42.00	18.00	30.72#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010255.D
 Acq On : 05 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0B9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
 Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 02:08:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 06 01:05:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	170566	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136	748779	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.545	164	482266	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	908782	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.380	240	593610	20.000	ng/ul	# 0.00
88) Perylene-d12	23.821	264	588374	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.358	96	15930	4.073	ng/uL	0.00
4) Pyridine-d5	3.781	84	52732	4.792	ng/ul	0.01
7) Phenol-d5	7.081	99	86119	5.551	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	298031	32.014	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	259439	22.580	ng/ul	0.00
15) 4-Methylphenol-d8	8.622	113	173540	13.501	ng/ul	0.00
21) Nitrobenzene-d5	9.075	128	188015	31.571	ng/ul	0.00
24) 2-Nitrophenol-d4	9.798	143	190138	29.234	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	308013	24.326	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	275942	15.199	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1223123	32.604	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	1346958	29.667	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	23290m	3.372	ng/ul	0.01
60) Fluorene-d10	15.539	176	1022763	31.693	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	160539	27.938	ng/ul	0.00
73) Anthracene-d10	17.398	188	1595098	36.280	ng/ul	0.00
81) Pyrene-d10	19.627	212	1556843	46.117	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.662	264	1170019	37.931	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010255.D
Acq On : 05 May 2022 19:40
Operator : CG/JU
Sample : N2678-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0B9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/10/2022
Supervised By :mohammad ahmed 05/10/2022

Quant Time: May 06 02:08:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 06 01:05:07 2022
Response via : Initial Calibration

