

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010240.D
 Acq On : 05 May 2022 11:15
 Operator : CG/JU
 Sample : PB144597BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	54	rVB	48141	65909	1.94%	0.162%
2	3.775	114	117	133	rBV	460041	759547	22.32%	1.870%
3	4.105	169	173	177	rVB2	12852	15807	0.46%	0.039%
4	6.075	505	508	513	rVB6	2050	3866	0.11%	0.010%
5	7.081	672	679	694	rBV	695608	1142727	33.58%	2.813%
6	7.246	700	707	721	rBV	590960	947898	27.85%	2.333%
7	7.446	735	741	756	rBV	731805	1191045	34.99%	2.932%
8	7.916	814	821	833	rVB	658493	1053647	30.96%	2.594%
9	8.622	933	941	957	rBV	906770	1511089	44.40%	3.720%
10	9.075	1008	1018	1031	rBV	762135	1281009	37.64%	3.154%
11	9.799	1134	1141	1155	rBV	589358	1038516	30.51%	2.557%
12	10.340	1225	1233	1253	rBV	802127	1517072	44.57%	3.735%
13	10.722	1290	1298	1312	rBV	951576	1625050	47.75%	4.000%
14	10.857	1313	1321	1344	rBV	545130	1117919	32.85%	2.752%
15	12.016	1511	1518	1521	rBV9	1990	3471	0.10%	0.009%
16	12.316	1564	1569	1578	rBV3	12690	26966	0.79%	0.066%
17	13.957	1841	1848	1861	rBV	1687344	2426909	71.31%	5.974%
18	14.240	1887	1896	1909	rBV	1810620	2728463	80.17%	6.717%
19	14.551	1942	1949	1959	rBV	1421209	2200149	64.64%	5.416%
20	14.745	1975	1982	1999	rBV	337286	794761	23.35%	1.957%
21	15.181	2053	2056	2057	rBV3	2939	3641	0.11%	0.009%
22	15.363	2082	2087	2092	rBV9	2554	5634	0.17%	0.014%
23	15.539	2110	2117	2132	rBV	2170296	3403472	100.00%	8.379%
24	15.663	2132	2138	2150	rVV	493410	785118	23.07%	1.933%
25	15.781	2155	2158	2167	rVB	27952	47187	1.39%	0.116%
26	16.328	2246	2251	2261	rVB8	10393	19017	0.56%	0.047%
27	16.981	2357	2362	2367	rBV9	4914	9512	0.28%	0.023%
28	17.092	2375	2381	2383	rBV7	3891	6244	0.18%	0.015%
29	17.298	2408	2416	2427	rBV	1507448	2327581	68.39%	5.730%
30	17.398	2427	2433	2453	rVB	2202026	3382510	99.38%	8.327%
31	19.210	2737	2741	2747	rBV3	24811	35983	1.06%	0.089%
32	19.280	2750	2753	2761	rVB2	19132	27209	0.80%	0.067%
33	19.633	2807	2813	2826	rBV	2438614	3303250	97.06%	8.132%
34	21.386	3106	3111	3124	rBV	1226498	1770201	52.01%	4.358%
35	23.668	3492	3499	3506	rBV2	1171658	2460751	72.30%	6.058%
36	23.827	3519	3526	3539	rVB2	729128	1582317	46.49%	3.895%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010240.D
Acq On : 05 May 2022 11:15
Operator : CG/JU
Sample : PB144597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 40621447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010240.D
Acq On : 05 May 2022 11:15
Operator : CG/JU
Sample : PB144597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

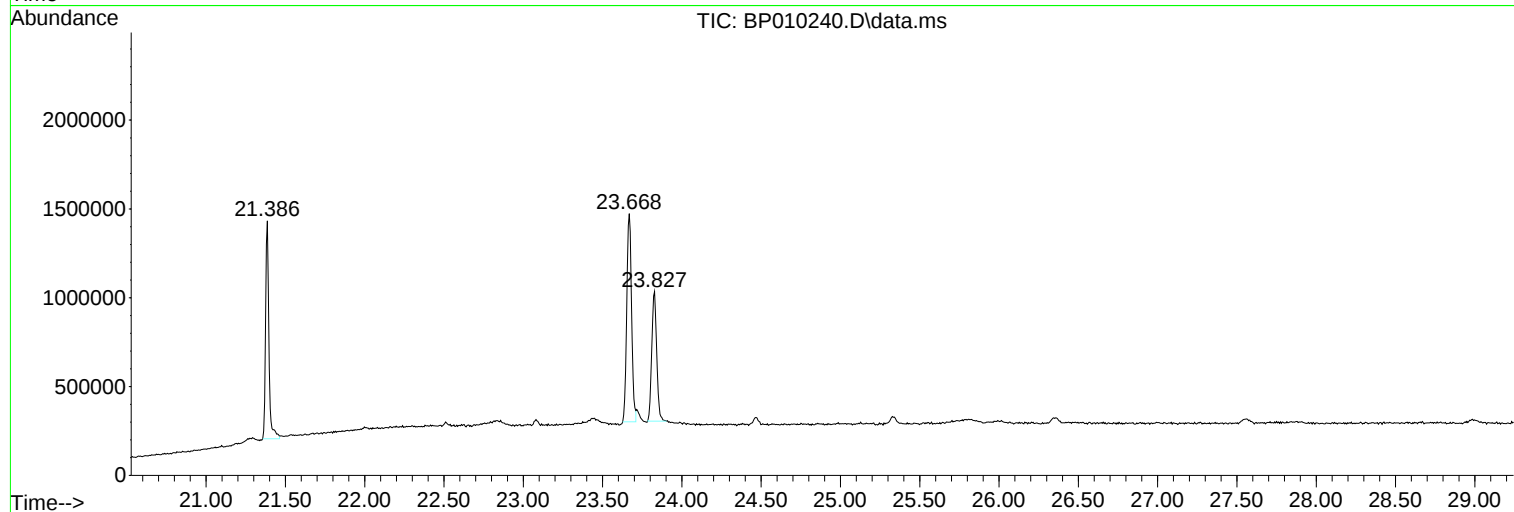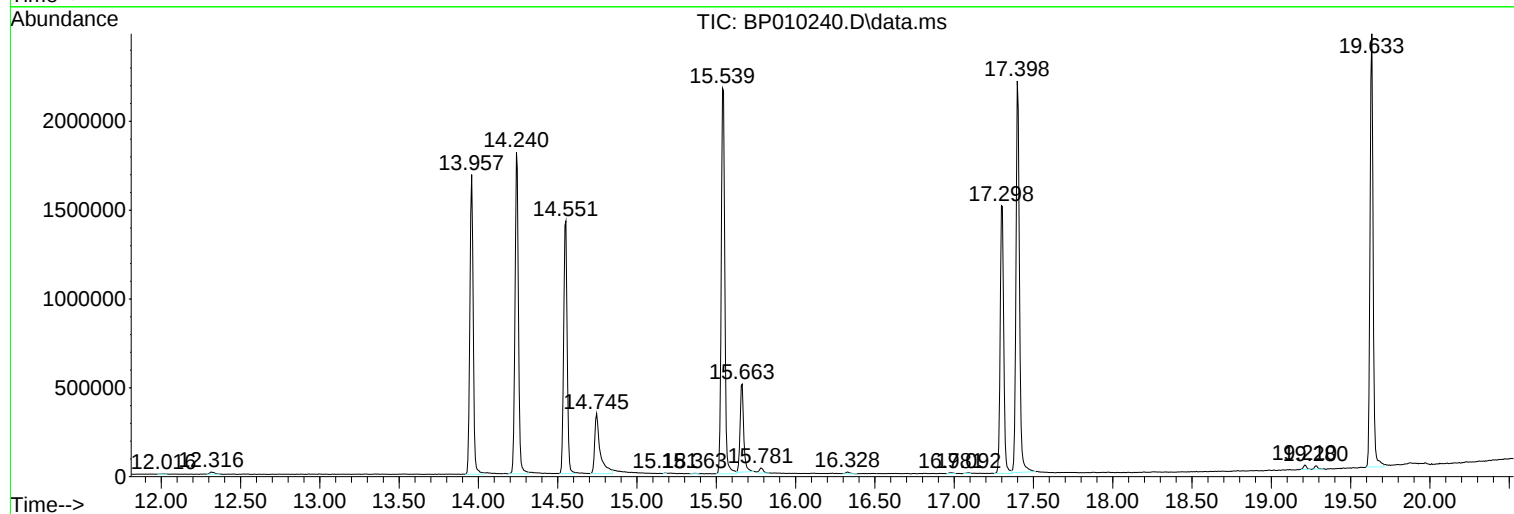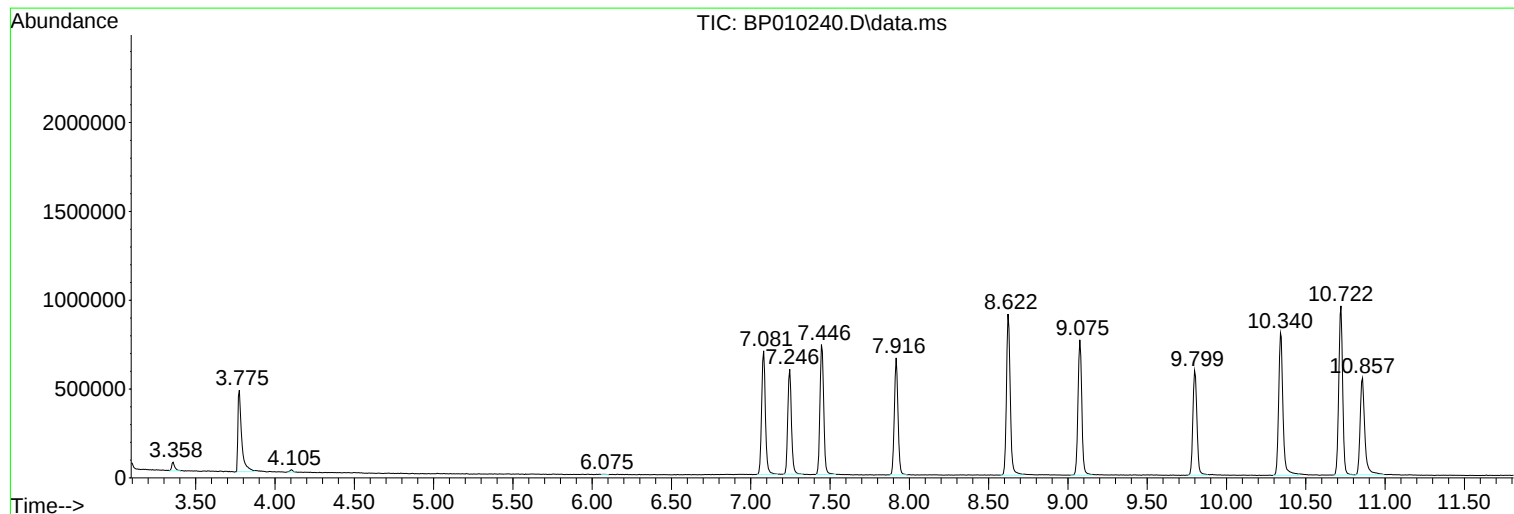

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010240.D
Acq On : 05 May 2022 11:15
Operator : CG/JU
Sample : PB144597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010240.D
Acq On : 05 May 2022 11:15
Operator : CG/JU
Sample : PB144597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc