

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010244.D
 Acq On : 05 May 2022 13:29
 Operator : CG/JU
 Sample : N2668-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	50	rVB	32344	38526	0.96%	0.095%
2	3.781	115	118	139	rVB	105293	190018	4.76%	0.469%
3	4.011	152	157	160	rBV4	6328	9900	0.25%	0.024%
4	4.105	169	173	179	rVB2	12213	20287	0.51%	0.050%
5	5.028	325	330	339	rVB5	4469	10821	0.27%	0.027%
6	6.334	549	552	555	rBV5	3107	5206	0.13%	0.013%
7	6.822	631	635	640	rBV8	1682	4159	0.10%	0.010%
8	7.081	672	679	689	rBV	146371	250938	6.29%	0.619%
9	7.240	700	706	720	rBV	684036	1125398	28.19%	2.778%
10	7.446	734	741	753	rBV	649377	1043465	26.14%	2.576%
11	7.546	756	758	763	rVB6	3707	4628	0.12%	0.011%
12	7.916	813	821	831	rBV	580919	949644	23.79%	2.344%
13	8.622	934	941	953	rBV	464413	781343	19.57%	1.929%
14	9.075	1010	1018	1032	rBV	877277	1507742	37.76%	3.722%
15	9.522	1087	1094	1101	rVB7	8366	14805	0.37%	0.037%
16	9.799	1133	1141	1155	rBV	685223	1171369	29.34%	2.892%
17	10.340	1226	1233	1251	rBV	856814	1540931	38.60%	3.804%
18	10.716	1289	1297	1311	rBV	824495	1415561	35.46%	3.495%
19	10.852	1313	1320	1343	rVV	619558	1237387	30.99%	3.055%
20	11.557	1436	1440	1445	rBV7	1992	4374	0.11%	0.011%
21	12.316	1562	1569	1578	rVB2	14186	30314	0.76%	0.075%
22	12.522	1599	1604	1607	rBV7	2452	4521	0.11%	0.011%
23	13.163	1709	1713	1718	rVV7	3038	4054	0.10%	0.010%
24	13.381	1745	1750	1754	rVB4	5351	6698	0.17%	0.017%
25	13.451	1759	1762	1767	rBV7	2157	4334	0.11%	0.011%
26	13.957	1840	1848	1862	rBV	1924634	2713019	67.95%	6.698%
27	14.051	1862	1864	1867	rVB3	3558	4789	0.12%	0.012%
28	14.240	1888	1896	1918	rBV	1960690	3047882	76.34%	7.524%
29	14.546	1942	1948	1961	rBV	1210467	1790555	44.85%	4.420%
30	14.757	1978	1984	2005	rBV3	31648	117924	2.95%	0.291%
31	15.363	2083	2087	2092	rVB2	11924	17186	0.43%	0.042%
32	15.540	2110	2117	2131	rBV	2656615	3867839	96.88%	9.548%
33	15.657	2131	2137	2154	rVV	667515	1085828	27.20%	2.681%
34	15.781	2154	2158	2173	rVV	36314	78173	1.96%	0.193%
35	15.910	2176	2180	2184	rVB5	5934	10644	0.27%	0.026%
36	16.328	2247	2251	2258	rVB6	9154	15511	0.39%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010244.D
 Acq On : 05 May 2022 13:29
 Operator : CG/JU
 Sample : N2668-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	16.640	2300	2304	2308	rVB7	2761	4388	0.11%	0.011%
38	16.934	2350	2354	2358	rBV7	3943	6979	0.17%	0.017%
39	16.975	2358	2361	2366	rVV6	4704	7816	0.20%	0.019%
40	17.087	2378	2380	2388	rVB8	4505	7525	0.19%	0.019%
41	17.298	2409	2416	2426	rBV	1257624	1828490	45.80%	4.514%
42	17.398	2426	2433	2452	rVB2	2537622	3835726	96.07%	9.469%
43	17.869	2510	2513	2517	rBV6	3268	5595	0.14%	0.014%
44	18.192	2563	2568	2570	rBV6	5446	9281	0.23%	0.023%
45	18.369	2596	2598	2601	rBV3	3516	4321	0.11%	0.011%
46	19.210	2736	2741	2745	rBV3	32578	43746	1.10%	0.108%
47	19.281	2748	2753	2759	rVV	28540	43073	1.08%	0.106%
48	19.634	2806	2813	2828	rBV	2772159	3992433	100.00%	9.856%
49	21.380	3105	3110	3123	rBV	1088632	1598370	40.03%	3.946%
50	23.663	3491	3498	3516	rBV2	1606238	3490528	87.43%	8.617%
51	23.822	3519	3525	3540	rVB2	698661	1503547	37.66%	3.712%


Sum of corrected areas: 40507591

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010244.D
Acq On : 05 May 2022 13:29
Operator : CG/JU
Sample : N2668-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

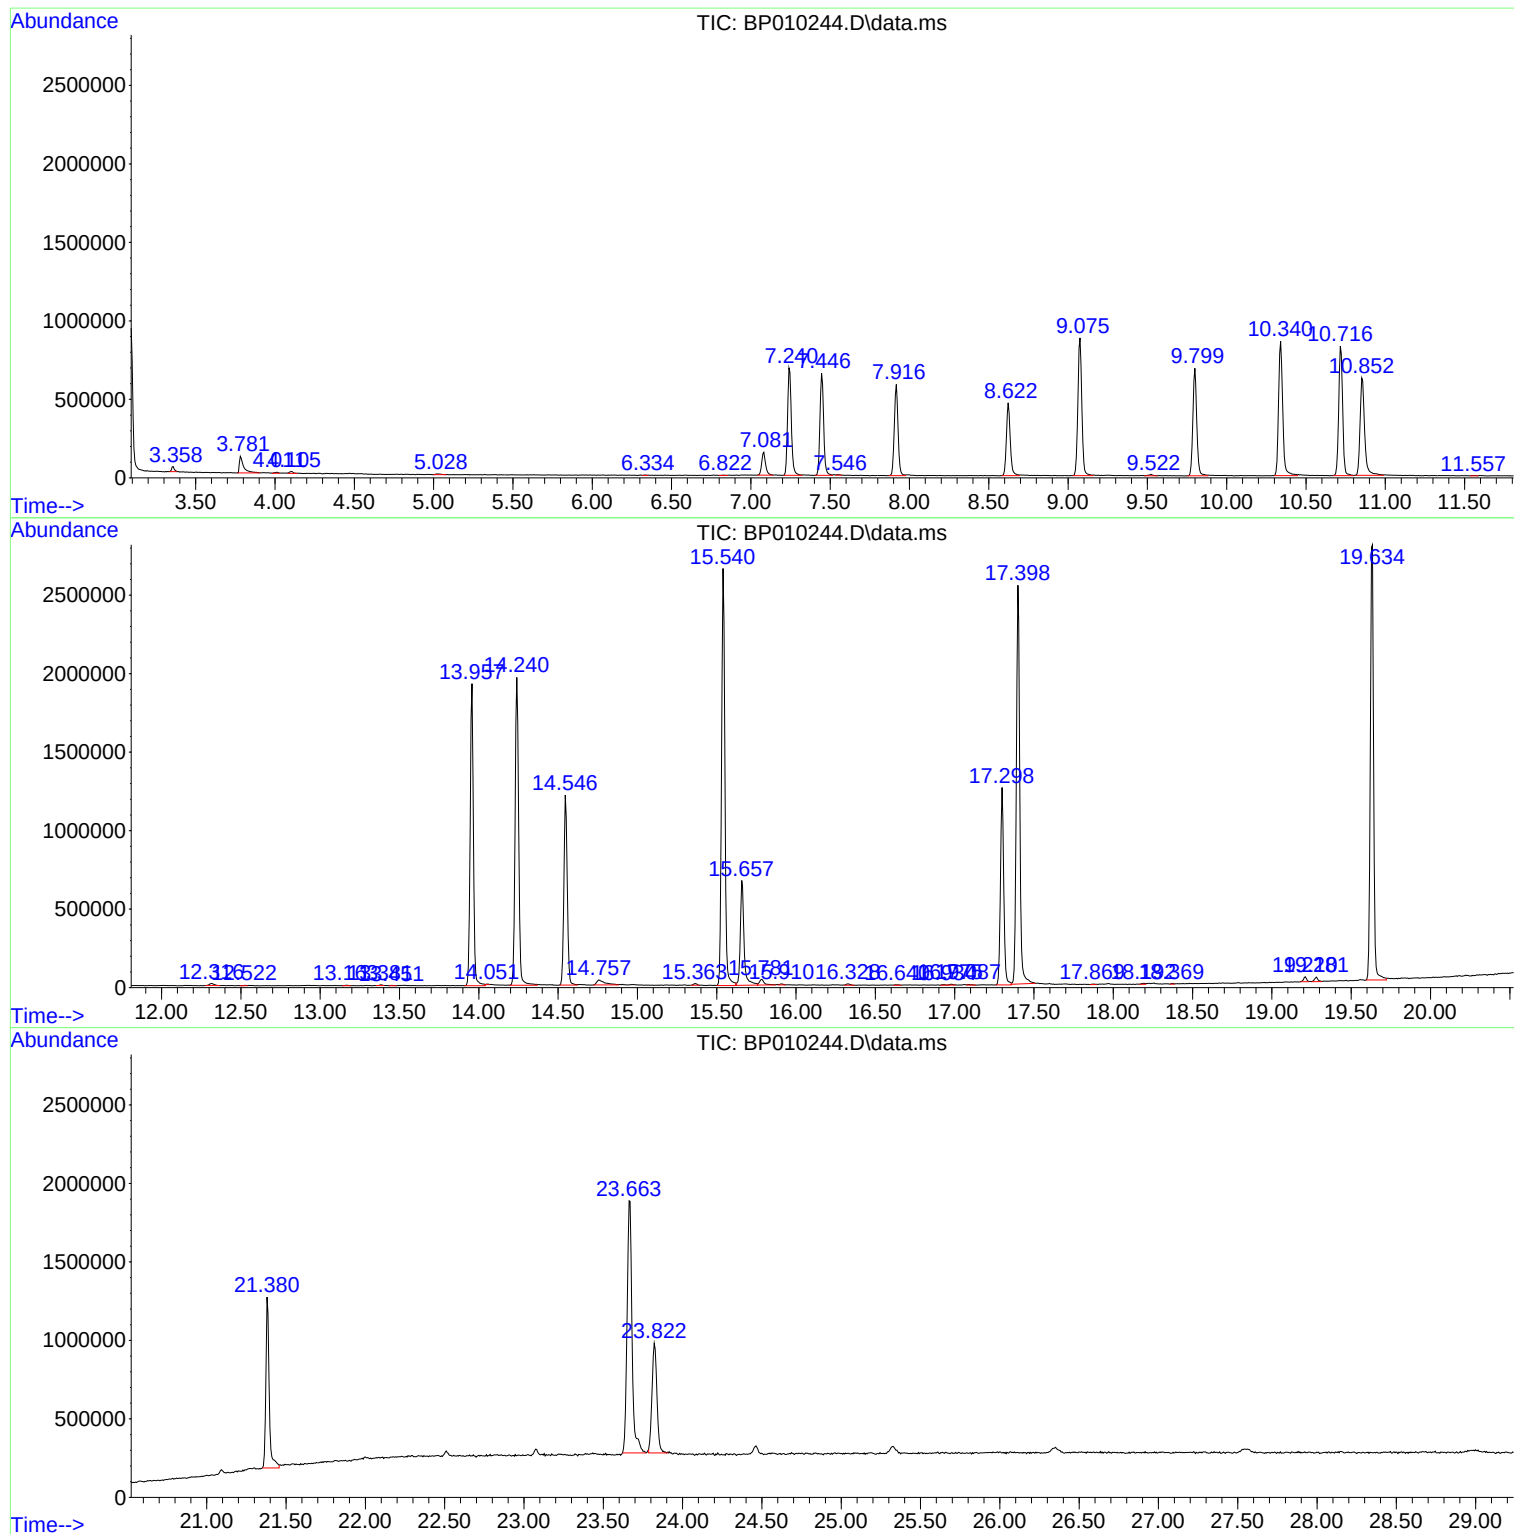

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010244.D
Acq On : 05 May 2022 13:29
Operator : CG/JU
Sample : N2668-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010244.D
Acq On : 05 May 2022 13:29
Operator : CG/JU
Sample : N2668-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc