

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010245.D
 Acq On : 05 May 2022 14:03
 Operator : CG/JU
 Sample : N2668-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	52	rVB	33336	42663	0.83%	0.091%
2	3.781	114	118	134	rBV	161368	307283	5.95%	0.655%
3	3.940	143	145	151	rVB7	4293	5819	0.11%	0.012%
4	4.011	155	157	161	rVB5	7059	8426	0.16%	0.018%
5	4.099	169	172	178	rVB2	12131	19169	0.37%	0.041%
6	5.022	325	329	336	rBV3	6182	10930	0.21%	0.023%
7	7.081	673	679	690	rBV	151890	254213	4.92%	0.542%
8	7.246	697	707	719	rBV	673588	1132118	21.91%	2.412%
9	7.446	734	741	754	rBV	649466	1053042	20.38%	2.243%
10	7.552	756	759	765	rVB8	4921	8924	0.17%	0.019%
11	7.916	814	821	829	rBV	594560	973553	18.84%	2.074%
12	7.993	830	834	841	rVB	12220	21309	0.41%	0.045%
13	8.622	933	941	954	rBV	481199	827838	16.02%	1.764%
14	9.075	1009	1018	1032	rBV	918896	1545638	29.91%	3.293%
15	9.522	1089	1094	1101	rVB2	14241	22582	0.44%	0.048%
16	9.798	1133	1141	1156	rBV	716986	1232146	23.84%	2.625%
17	10.075	1183	1188	1191	rBV7	2714	5635	0.11%	0.012%
18	10.340	1225	1233	1245	rBV	911968	1609056	31.14%	3.428%
19	10.716	1290	1297	1311	rBV	875607	1508297	29.19%	3.213%
20	10.851	1313	1320	1334	rBV	845470	1577099	30.52%	3.360%
21	11.545	1430	1438	1441	rBV10	3620	8634	0.17%	0.018%
22	12.157	1538	1542	1551	rVB9	4739	9828	0.19%	0.021%
23	12.310	1559	1568	1574	rBV3	17031	32603	0.63%	0.069%
24	12.916	1667	1671	1675	rVV7	3455	5370	0.10%	0.011%
25	13.104	1696	1703	1710	rBV7	2291	6047	0.12%	0.013%
26	13.163	1710	1713	1719	rVB4	6221	7650	0.15%	0.016%
27	13.381	1746	1750	1756	rVB3	11014	16278	0.32%	0.035%
28	13.451	1758	1762	1766	rBV7	4555	6677	0.13%	0.014%
29	13.734	1805	1810	1815	rBV7	2879	6242	0.12%	0.013%
30	13.957	1841	1848	1861	rBV	2167298	3053510	59.09%	6.505%
31	14.239	1887	1896	1912	rBV	2257197	3386465	65.53%	7.214%
32	14.345	1912	1914	1919	rVB6	4981	6835	0.13%	0.015%
33	14.451	1930	1932	1938	rVB7	7007	10213	0.20%	0.022%
34	14.545	1940	1948	1960	rBV	1368982	2041132	39.50%	4.348%
35	14.751	1976	1983	1999	rBV2	56259	172042	3.33%	0.367%
36	14.963	2017	2019	2026	rVB8	6504	9032	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010245.D
 Acq On : 05 May 2022 14:03
 Operator : CG/JU
 Sample : N2668-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	15.292	2071	2075	2080	rBV2	9984	14912	0.29%	0.032%
38	15.369	2080	2088	2093	rVV2	35686	56628	1.10%	0.121%
39	15.539	2110	2117	2131	rBV	2959979	4492085	86.93%	9.570%
40	15.657	2131	2137	2151	rVV	908899	1403477	27.16%	2.990%
41	15.780	2154	2158	2171	rVV	38492	84912	1.64%	0.181%
42	15.910	2174	2180	2183	rVB7	6024	10805	0.21%	0.023%
43	16.245	2230	2237	2239	rBV8	3449	7368	0.14%	0.016%
44	16.328	2246	2251	2257	rVB4	11388	18840	0.36%	0.040%
45	16.980	2356	2362	2365	rBV8	7495	13314	0.26%	0.028%
46	17.298	2407	2416	2427	rBV	1582773	2360284	45.68%	5.028%
47	17.398	2427	2433	2455	rVB	3342028	4941065	95.62%	10.526%
48	17.586	2462	2465	2469	rBV2	5802	8066	0.16%	0.017%
49	17.969	2526	2530	2533	rVB6	12040	15041	0.29%	0.032%
50	18.186	2562	2567	2570	rBV6	16413	26488	0.51%	0.056%
51	18.227	2570	2574	2576	rVV	16408	25353	0.49%	0.054%
52	18.257	2576	2579	2583	rVB	14744	17888	0.35%	0.038%
53	19.210	2736	2741	2748	rBV2	45361	68422	1.32%	0.146%
54	19.274	2748	2752	2758	rVV	33141	46356	0.90%	0.099%
55	19.563	2798	2801	2806	rBV7	7894	9181	0.18%	0.020%
56	19.627	2806	2812	2833	rBV	3667895	5167558	100.00%	11.009%
57	21.092	3057	3061	3069	rBV3	71984	126145	2.44%	0.269%
58	21.380	3105	3110	3126	rBV	1204335	1877611	36.33%	4.000%
59	23.662	3491	3498	3514	rBV2	1665768	3651837	70.67%	7.780%
60	23.821	3519	3525	3535	rVB2	721447	1553076	30.05%	3.309%


Sum of corrected areas: 46941010

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010245.D
Acq On : 05 May 2022 14:03
Operator : CG/JU
Sample : N2668-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

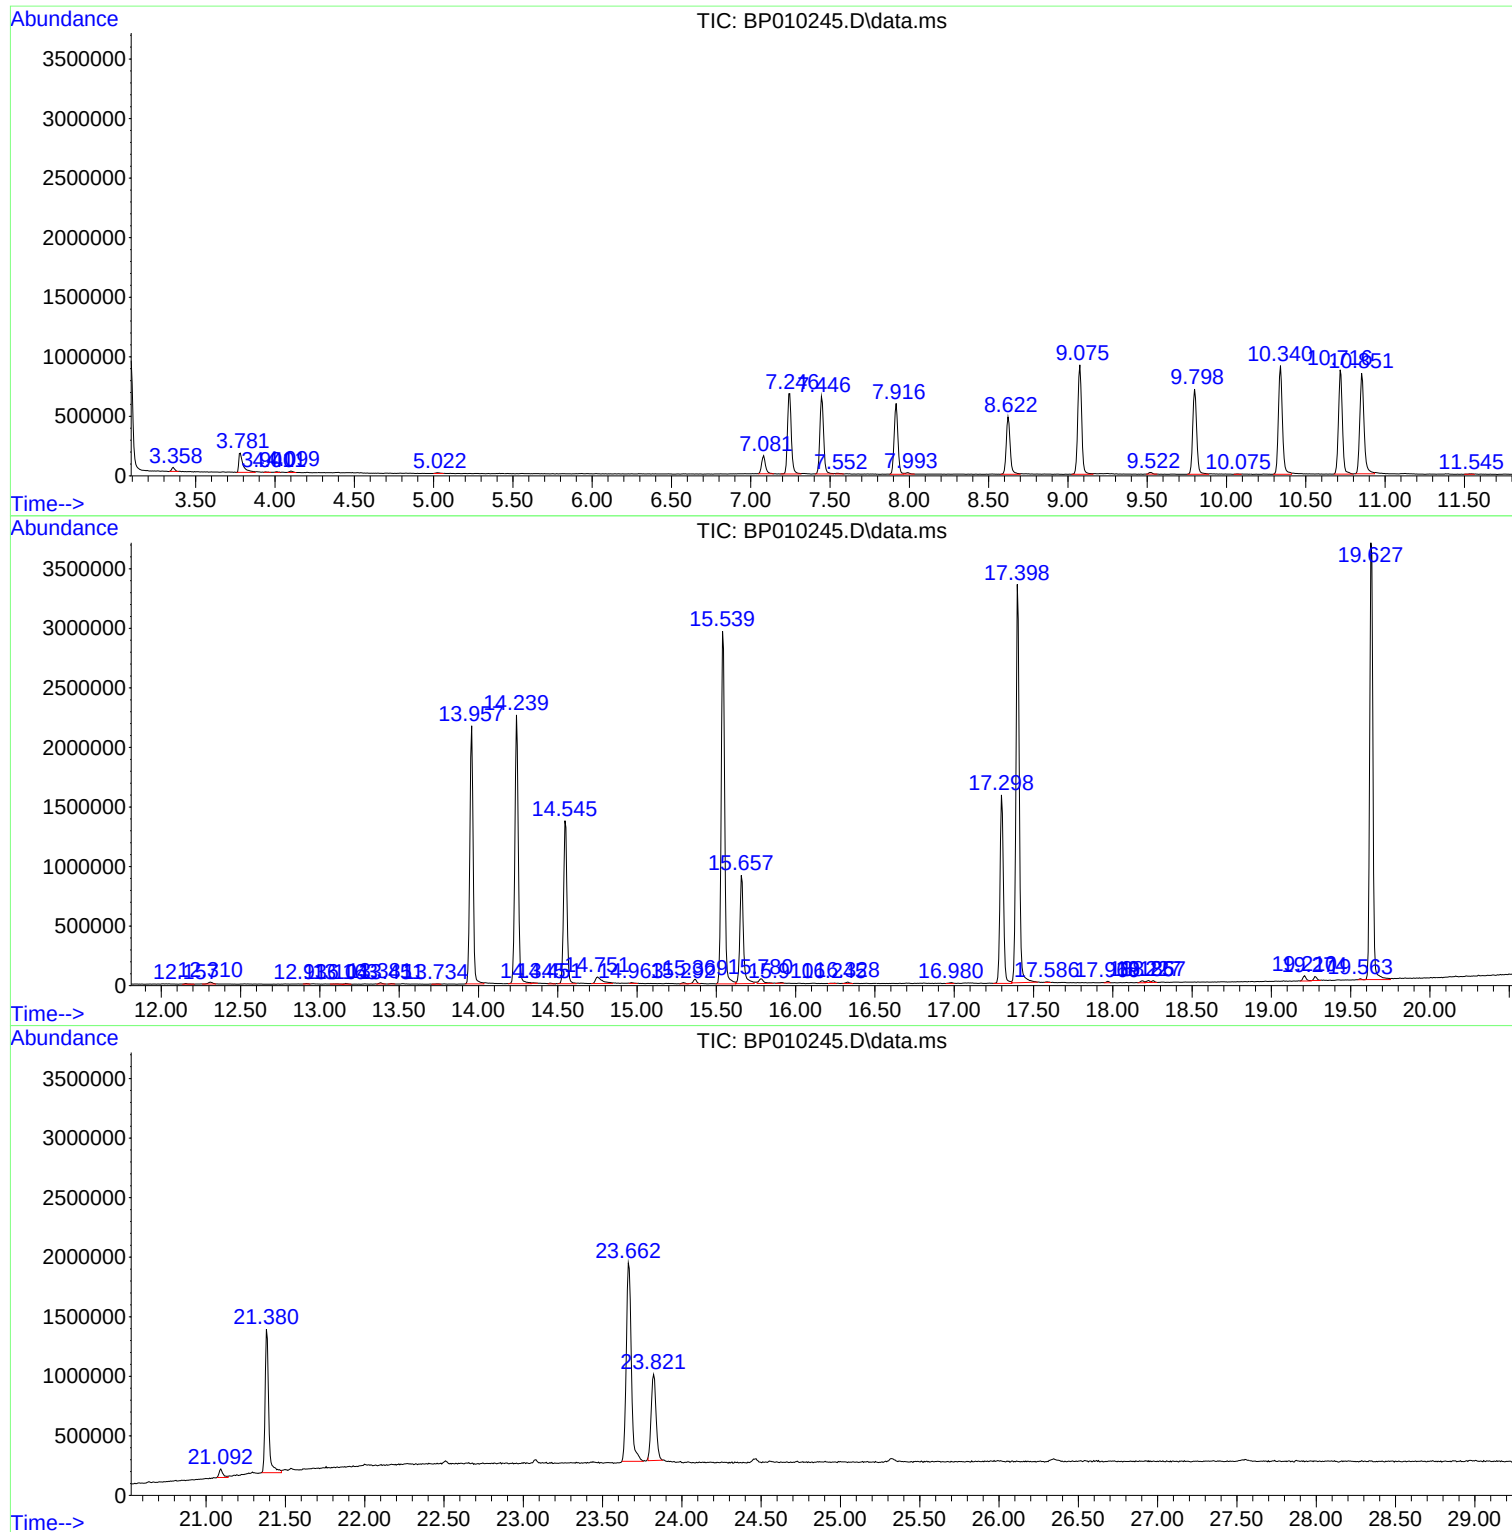

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010245.D
Acq On : 05 May 2022 14:03
Operator : CG/JU
Sample : N2668-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010245.D
Acq On : 05 May 2022 14:03
Operator : CG/JU
Sample : N2668-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc