

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010247.D
 Acq On : 05 May 2022 15:10
 Operator : CG/JU
 Sample : N2678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	50	rBV	37598	48607	1.44%	0.137%
2	3.652	94	96	100	rBV4	4014	5413	0.16%	0.015%
3	3.781	115	118	139	rVB	124420	225206	6.65%	0.634%
4	4.099	169	172	176	rVB	10636	14043	0.41%	0.040%
5	4.540	241	247	254	rVB2	27879	45127	1.33%	0.127%
6	5.017	326	328	339	rVB5	6230	13682	0.40%	0.039%
7	5.281	370	373	376	rVB4	2995	4022	0.12%	0.011%
8	6.022	495	499	502	rVB6	3627	5662	0.17%	0.016%
9	7.081	671	679	692	rVB	133427	250094	7.39%	0.704%
10	7.240	700	706	722	rVB	506295	840445	24.83%	2.365%
11	7.446	735	741	754	rBV	517893	842376	24.88%	2.371%
12	7.916	813	821	831	rBV	590073	978949	28.92%	2.755%
13	7.987	831	833	838	rVB4	6154	8563	0.25%	0.024%
14	8.264	875	880	885	rBV5	4878	9108	0.27%	0.026%
15	8.622	933	941	958	rBV	408284	698325	20.63%	1.965%
16	8.734	958	960	969	rVB10	4788	10624	0.31%	0.030%
17	8.840	974	978	983	rVB5	5316	9653	0.29%	0.027%
18	9.075	1010	1018	1036	rBV	655792	1147523	33.90%	3.229%
19	9.246	1044	1047	1054	rVV9	3531	7172	0.21%	0.020%
20	9.316	1054	1059	1065	rVB	12356	20256	0.60%	0.057%
21	9.522	1089	1094	1099	rVB5	6892	11485	0.34%	0.032%
22	9.799	1133	1141	1159	rBV	521725	901706	26.64%	2.538%
23	10.340	1225	1233	1243	rBV	688296	1212836	35.83%	3.413%
24	10.510	1256	1262	1273	rBV2	42557	109464	3.23%	0.308%
25	10.716	1288	1297	1308	rBV	843149	1449013	42.80%	4.078%
26	10.852	1313	1320	1338	rBV	401580	770066	22.75%	2.167%
27	11.375	1406	1409	1415	rVB2	8276	14860	0.44%	0.042%
28	11.722	1465	1468	1472	rBV6	1859	3633	0.11%	0.010%
29	12.016	1511	1518	1519	rBV7	3068	4770	0.14%	0.013%
30	12.304	1561	1567	1574	rBV3	11965	26626	0.79%	0.075%
31	12.869	1656	1663	1665	rBV8	1888	3747	0.11%	0.011%
32	12.916	1667	1671	1678	rVB10	3395	6217	0.18%	0.017%
33	13.140	1705	1709	1712	rBV5	5706	8808	0.26%	0.025%
34	13.163	1712	1713	1720	rVB7	5585	6909	0.20%	0.019%
35	13.287	1729	1734	1737	rVB7	2930	4707	0.14%	0.013%
36	13.387	1747	1751	1756	rVB7	3156	5681	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010247.D
 Acq On : 05 May 2022 15:10
 Operator : CG/JU
 Sample : N2678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	13.446	1756	1761	1767	rBV7	4878	9305	0.27%	0.026%
38	13.522	1769	1774	1780	rBV10	3812	8343	0.25%	0.023%
39	13.604	1782	1788	1798	rVV	59675	92017	2.72%	0.259%
40	13.957	1839	1848	1862	rBV	1488625	2210043	65.28%	6.219%
41	14.240	1886	1896	1912	rBV	1553699	2364931	69.86%	6.655%
42	14.422	1924	1927	1929	rBV3	6397	7462	0.22%	0.021%
43	14.451	1931	1932	1937	rVB5	6545	6569	0.19%	0.018%
44	14.546	1941	1948	1959	rBV	1267855	1938321	57.26%	5.455%
45	14.710	1971	1976	1978	rBV6	4753	6557	0.19%	0.018%
46	14.757	1978	1984	1997	rBV3	35636	115498	3.41%	0.325%
47	14.898	2006	2008	2013	rBV6	2440	3827	0.11%	0.011%
48	15.140	2047	2049	2054	rVB6	3182	3530	0.10%	0.010%
49	15.187	2054	2057	2061	rVB6	2862	3583	0.11%	0.010%
50	15.357	2080	2086	2091	rBV8	7375	13238	0.39%	0.037%
51	15.404	2091	2094	2100	rVB4	7441	9736	0.29%	0.027%
52	15.540	2110	2117	2131	rBV	2070142	3095957	91.45%	8.713%
53	15.657	2131	2137	2154	rVV	568294	895305	26.45%	2.520%
54	15.781	2154	2158	2169	rVB3	26492	55793	1.65%	0.157%
55	15.963	2186	2189	2192	rVV5	3517	5086	0.15%	0.014%
56	15.993	2192	2194	2198	rVB5	5504	6427	0.19%	0.018%
57	16.234	2231	2235	2237	rBV4	3299	4042	0.12%	0.011%
58	16.263	2237	2240	2247	rVV9	6683	14120	0.42%	0.040%
59	16.328	2247	2251	2257	rVB8	9589	15593	0.46%	0.044%
60	16.387	2257	2261	2265	rVB7	3812	5479	0.16%	0.015%
61	16.440	2265	2270	2276	rVB10	7477	14204	0.42%	0.040%
62	16.504	2278	2281	2285	rVV5	2717	3531	0.10%	0.010%
63	16.545	2286	2288	2293	rVB5	2690	3451	0.10%	0.010%
64	16.710	2312	2316	2319	rBV6	3775	6087	0.18%	0.017%
65	16.775	2323	2327	2329	rBV5	3431	5107	0.15%	0.014%
66	16.975	2357	2361	2364	rBV6	5835	7335	0.22%	0.021%
67	17.063	2374	2376	2380	rBV5	4371	6203	0.18%	0.017%
68	17.110	2380	2384	2389	rVB6	8534	13366	0.39%	0.038%
69	17.298	2410	2416	2426	rBV	1383581	2055962	60.73%	5.786%
70	17.398	2427	2433	2450	rVB2	2153194	3243116	95.80%	9.127%
71	17.616	2468	2470	2475	rVB6	4338	5300	0.16%	0.015%
72	17.975	2527	2531	2536	rVB3	16645	21930	0.65%	0.062%
73	18.181	2563	2566	2572	rBV4	29433	46479	1.37%	0.131%
74	19.210	2737	2741	2747	rBV5	28793	42615	1.26%	0.120%
75	19.275	2749	2752	2757	rVV2	20041	30087	0.89%	0.085%
76	19.410	2772	2775	2778	rBV5	12394	18002	0.53%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Title : SVOA CALIBRATION

77	19.628	2806	2812	2825	rBV	2464262	3385376	100.00%	9.527%
78	21.092	3057	3061	3069	rBV4	80175	134599	3.98%	0.379%
79	21.380	3105	3110	3125	rBV	1135761	1684903	49.77%	4.742%
80	23.663	3491	3498	3506	rBV2	1233795	2645582	78.15%	7.445%
81	23.822	3519	3525	3537	rVB2	745946	1545036	45.64%	4.348%




Sum of corrected areas: 35534411

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

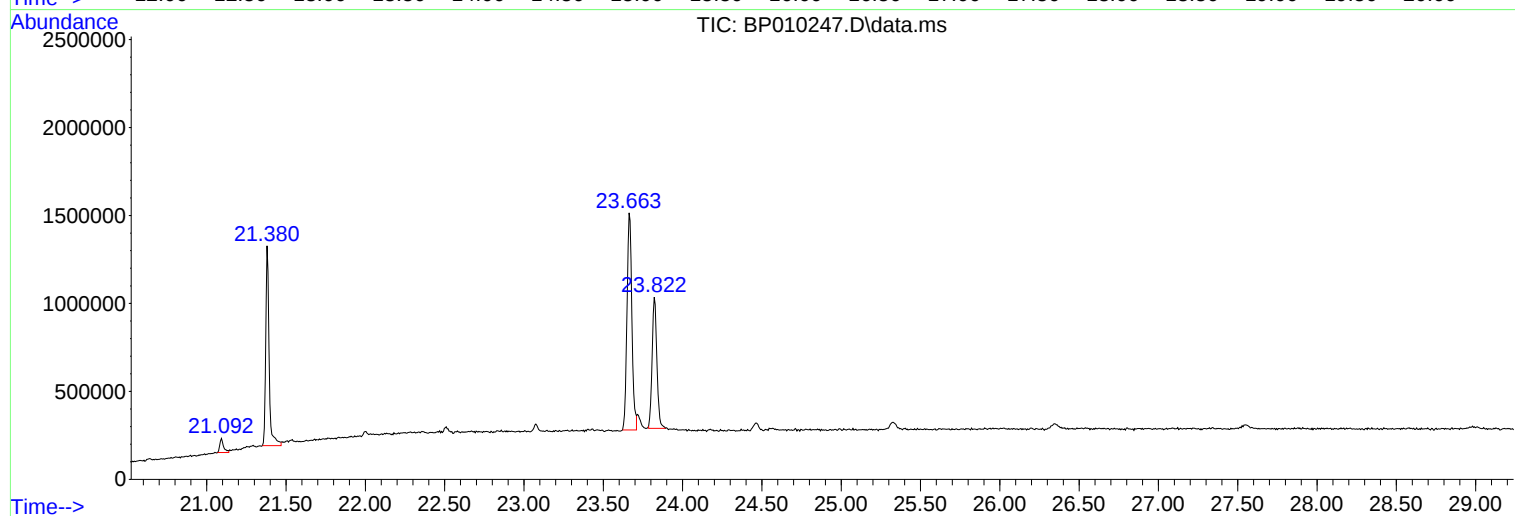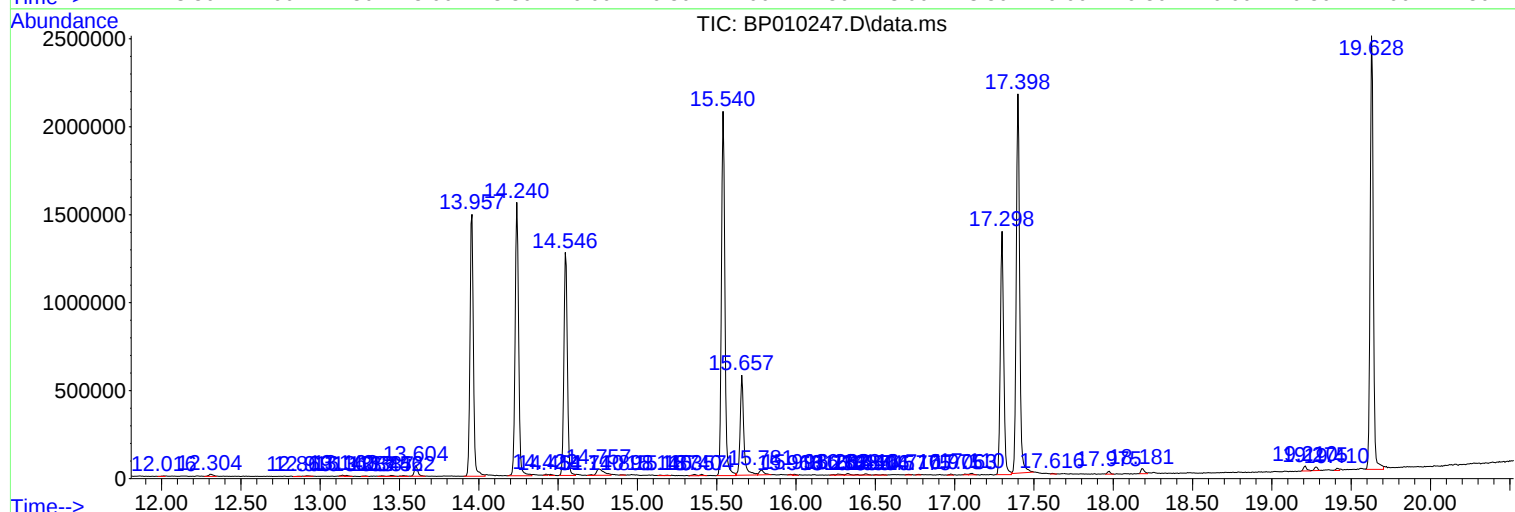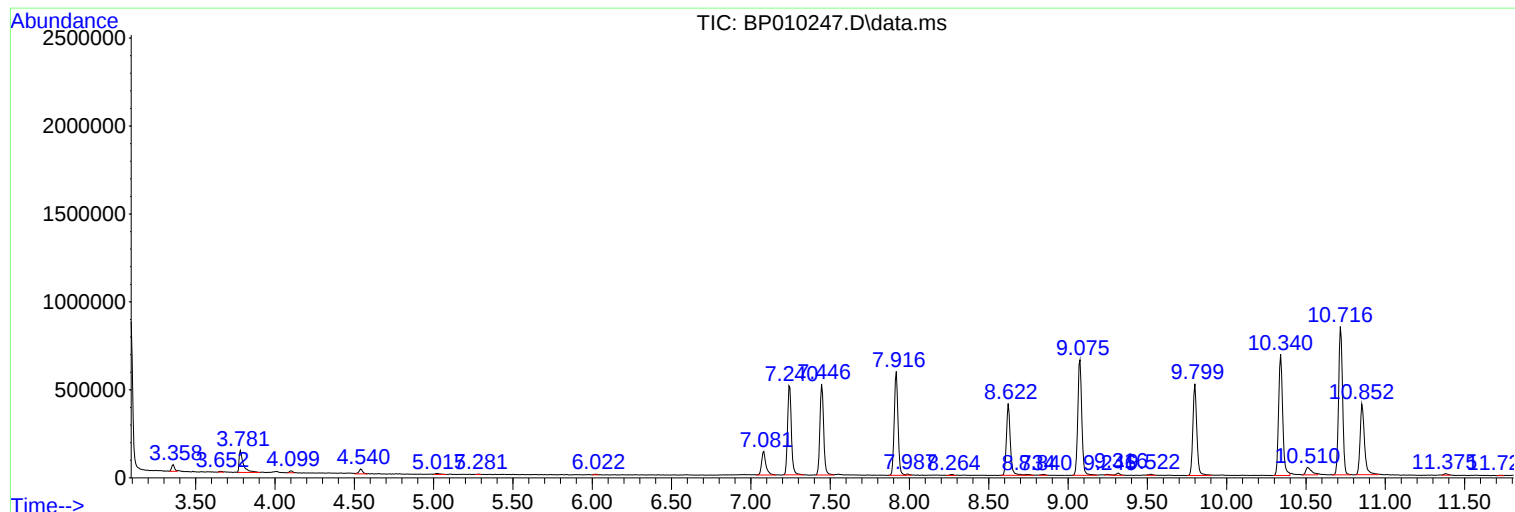

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010247.D
Acq On : 05 May 2022 15:10
Operator : CG/JU
Sample : N2678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0A2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc