

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010248.D
 Acq On : 05 May 2022 15:44
 Operator : CG/JU
 Sample : N2697-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	54	rVB	31234	43947	1.21%	0.112%
2	3.781	114	118	131	rBV	168901	303228	8.32%	0.776%
3	3.875	131	134	140	rVB4	19744	29584	0.81%	0.076%
4	4.011	154	157	164	rVB5	10452	16044	0.44%	0.041%
5	4.105	168	173	181	rVB3	18106	29826	0.82%	0.076%
6	4.322	206	210	215	rBV2	15185	21886	0.60%	0.056%
7	4.734	276	280	284	rVB5	6494	8236	0.23%	0.021%
8	5.016	324	328	335	rBV2	33378	49882	1.37%	0.128%
9	5.122	342	346	351	rBV6	4015	7675	0.21%	0.020%
10	6.781	622	628	634	rBV10	3631	8125	0.22%	0.021%
11	7.081	672	679	700	rVB	516183	875602	24.02%	2.240%
12	7.240	700	706	717	rBV	426676	718412	19.71%	1.838%
13	7.446	734	741	753	rBV	564078	903852	24.80%	2.312%
14	7.546	755	758	763	rVB5	5592	8772	0.24%	0.022%
15	7.916	809	821	830	rBV	660261	1078493	29.59%	2.759%
16	7.993	831	834	840	rVV5	5702	8766	0.24%	0.022%
17	8.057	841	845	850	rVB8	2179	4372	0.12%	0.011%
18	8.622	934	941	949	rBV	643485	1085000	29.77%	2.776%
19	8.746	958	962	968	rVB5	6371	9955	0.27%	0.025%
20	9.075	1010	1018	1028	rVV	561954	960368	26.35%	2.457%
21	9.163	1030	1033	1037	rVB5	4625	6551	0.18%	0.017%
22	9.246	1043	1047	1052	rBV8	2850	4878	0.13%	0.012%
23	9.516	1088	1093	1100	rBV4	7511	12861	0.35%	0.033%
24	9.799	1133	1141	1156	rBV	446105	788041	21.62%	2.016%
25	10.087	1183	1190	1193	rBV9	3182	5707	0.16%	0.015%
26	10.340	1226	1233	1249	rBV	649649	1151773	31.60%	2.947%
27	10.716	1289	1297	1312	rBV	939338	1626460	44.62%	4.161%
28	10.851	1312	1320	1336	rBV	507939	1004718	27.56%	2.570%
29	11.569	1437	1442	1448	rVB9	2600	5400	0.15%	0.014%
30	11.651	1455	1456	1464	rVB7	2910	5294	0.15%	0.014%
31	11.763	1470	1475	1483	rVB4	6950	14159	0.39%	0.036%
32	12.010	1516	1517	1521	rVV4	4130	4340	0.12%	0.011%
33	12.151	1532	1541	1548	rBV4	15059	29128	0.80%	0.075%
34	12.310	1560	1568	1573	rBV5	11322	24756	0.68%	0.063%
35	12.381	1576	1580	1587	rVB8	5163	11473	0.31%	0.029%
36	12.516	1600	1603	1610	rBV9	2365	4745	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010248.D
 Acq On : 05 May 2022 15:44
 Operator : CG/JU
 Sample : N2697-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	12.598	1610	1617	1620	rBV8	4676	8144	0.22%	0.021%
38	12.910	1668	1670	1674	rVV5	3905	5163	0.14%	0.013%
39	12.957	1675	1678	1682	rVB6	3042	4923	0.14%	0.013%
40	13.045	1689	1693	1696	rBV5	3825	5141	0.14%	0.013%
41	13.098	1698	1702	1707	rVV7	8625	14067	0.39%	0.036%
42	13.157	1711	1712	1717	rVB5	3855	4591	0.13%	0.012%
43	13.287	1727	1734	1740	rBV5	3495	8946	0.25%	0.023%
44	13.381	1746	1750	1759	rBV2	21804	37100	1.02%	0.095%
45	13.875	1830	1834	1839	rVB6	6473	10043	0.28%	0.026%
46	13.957	1839	1848	1858	rBV	1218784	1791730	49.15%	4.584%
47	14.040	1859	1862	1867	rVV4	14904	21453	0.59%	0.055%
48	14.157	1880	1882	1886	rVB5	4351	4851	0.13%	0.012%
49	14.240	1889	1896	1907	rVV	1340645	2024105	55.53%	5.178%
50	14.451	1928	1932	1938	rBV	28687	37737	1.04%	0.097%
51	14.545	1940	1948	1956	rBV	1450853	2157514	59.19%	5.520%
52	14.745	1976	1982	2002	rBV2	230004	571863	15.69%	1.463%
53	14.957	2014	2018	2024	rVB7	16369	31725	0.87%	0.081%
54	15.075	2034	2038	2045	rVB10	10726	18758	0.51%	0.048%
55	15.181	2050	2056	2059	rVV7	6536	15410	0.42%	0.039%
56	15.210	2059	2061	2066	rVB5	6320	7579	0.21%	0.019%
57	15.351	2080	2085	2090	rBV	29857	46679	1.28%	0.119%
58	15.404	2090	2094	2098	rVB	32490	41592	1.14%	0.106%
59	15.539	2111	2117	2131	rBV	1787698	2634641	72.28%	6.740%
60	15.657	2131	2137	2147	rVV	426035	624202	17.12%	1.597%
61	15.781	2154	2158	2162	rBV3	17965	29440	0.81%	0.075%
62	15.957	2186	2188	2193	rBV6	5570	7950	0.22%	0.020%
63	16.034	2197	2201	2209	rVB10	8714	18715	0.51%	0.048%
64	16.110	2211	2214	2215	rBV3	4790	5171	0.14%	0.013%
65	16.269	2237	2241	2243	rBV	40586	53053	1.46%	0.136%
66	16.292	2243	2245	2248	rVB3	24619	26602	0.73%	0.068%
67	16.834	2335	2337	2342	rBV6	6399	7726	0.21%	0.020%
68	16.875	2342	2344	2349	rVB6	6022	5619	0.15%	0.014%
69	16.957	2353	2358	2364	rBV6	12981	22050	0.60%	0.056%
70	17.063	2372	2376	2381	rVV2	34911	47301	1.30%	0.121%
71	17.116	2381	2385	2390	rVB2	22208	30553	0.84%	0.078%
72	17.198	2396	2399	2407	rVB10	7181	14585	0.40%	0.037%
73	17.298	2410	2416	2421	rVV	1614159	2435799	66.82%	6.232%
74	17.339	2421	2423	2427	rVV	200151	264773	7.26%	0.677%
75	17.398	2427	2433	2446	rVV2	1836842	2770896	76.01%	7.089%
76	17.498	2447	2450	2455	rVB2	22068	31177	0.86%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010248.D
 Acq On : 05 May 2022 15:44
 Operator : CG/JU
 Sample : N2697-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

77	17.710	2482	2486	2495	rVB	17994	38384	1.05%	0.098%
78	17.804	2498	2502	2508	rVB2	33513	47039	1.29%	0.120%
79	17.875	2512	2514	2517	rBV4	5020	6313	0.17%	0.016%
80	17.969	2527	2530	2533	rVB4	10192	12746	0.35%	0.033%
81	18.180	2560	2566	2569	rBV2	93930	141958	3.89%	0.363%
82	18.351	2591	2595	2599	rBV2	37152	66868	1.83%	0.171%
83	18.475	2612	2616	2619	rBV	30942	36104	0.99%	0.092%
84	18.651	2642	2646	2649	rBV	18699	24163	0.66%	0.062%
85	18.686	2649	2652	2660	rVB5	19424	29525	0.81%	0.076%
86	18.886	2684	2686	2689	rVB4	11940	10831	0.30%	0.028%
87	19.051	2711	2714	2716	rBV3	18086	22664	0.62%	0.058%
88	19.080	2716	2719	2725	rVB	30546	36574	1.00%	0.094%
89	19.204	2734	2740	2748	rBV6	36084	74338	2.04%	0.190%
90	19.304	2749	2757	2763	rBV	535428	756463	20.75%	1.935%
91	19.363	2764	2767	2771	rVB5	26169	34844	0.96%	0.089%
92	19.416	2771	2776	2779	rBV6	23782	42170	1.16%	0.108%
93	19.627	2807	2812	2826	rBV2	2191464	3645200	100.00%	9.326%
94	20.139	2895	2899	2906	rVB3	66981	143447	3.94%	0.367%
95	20.233	2913	2915	2919	rVB	32197	34949	0.96%	0.089%
96	21.092	3056	3061	3069	rBV4	392521	625455	17.16%	1.600%
97	21.380	3104	3110	3115	rBV	1509610	2289590	62.81%	5.858%
98	23.074	3394	3398	3404	rBV2	356877	660133	18.11%	1.689%
99	23.663	3492	3498	3504	rBV	943693	1887058	51.77%	4.828%
100	23.821	3519	3525	3532	rBV	830917	1648393	45.22%	4.217%




Sum of corrected areas: 39086885

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010248.D
Acq On : 05 May 2022 15:44
Operator : CG/JU
Sample : N2697-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBP8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

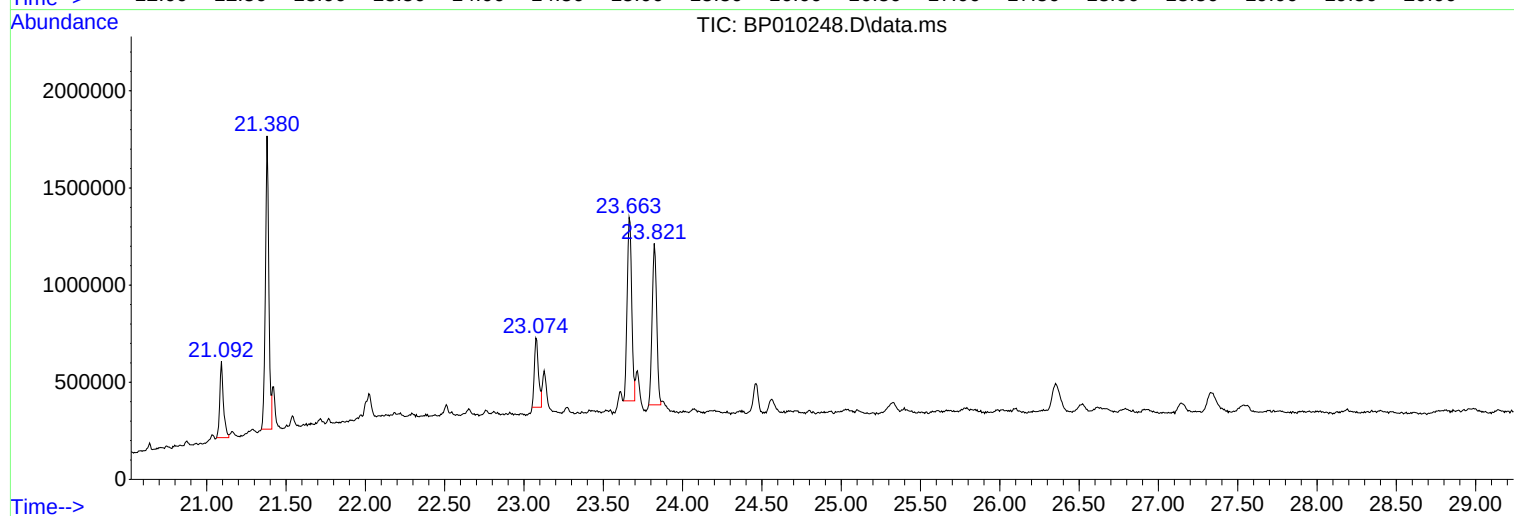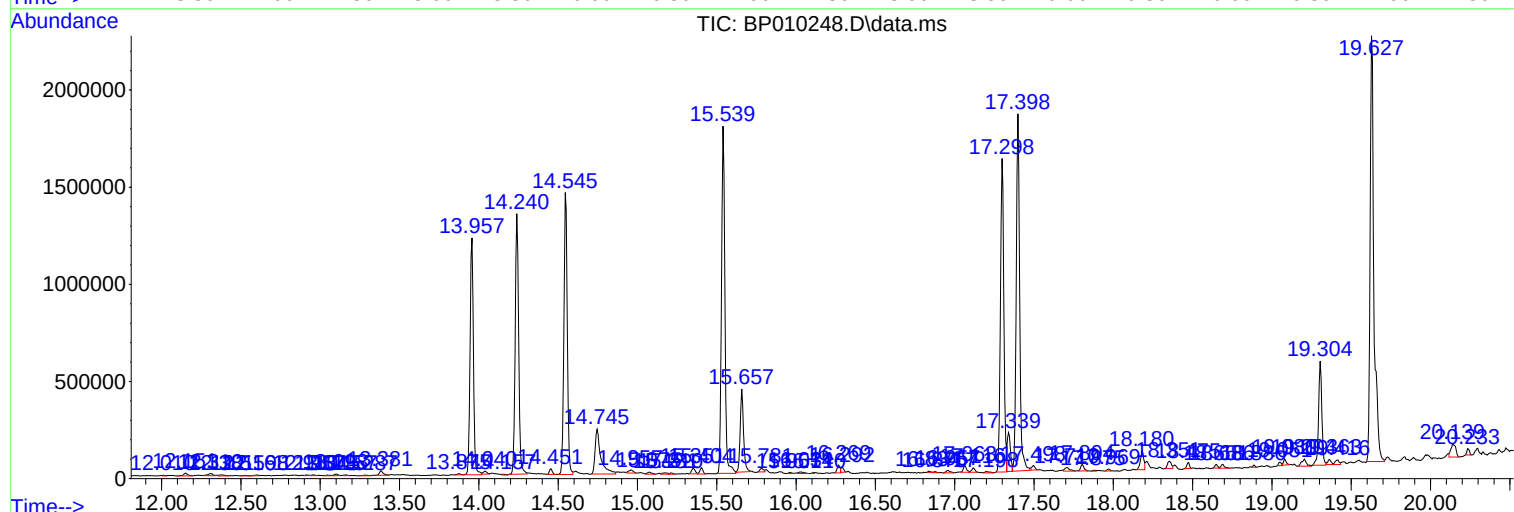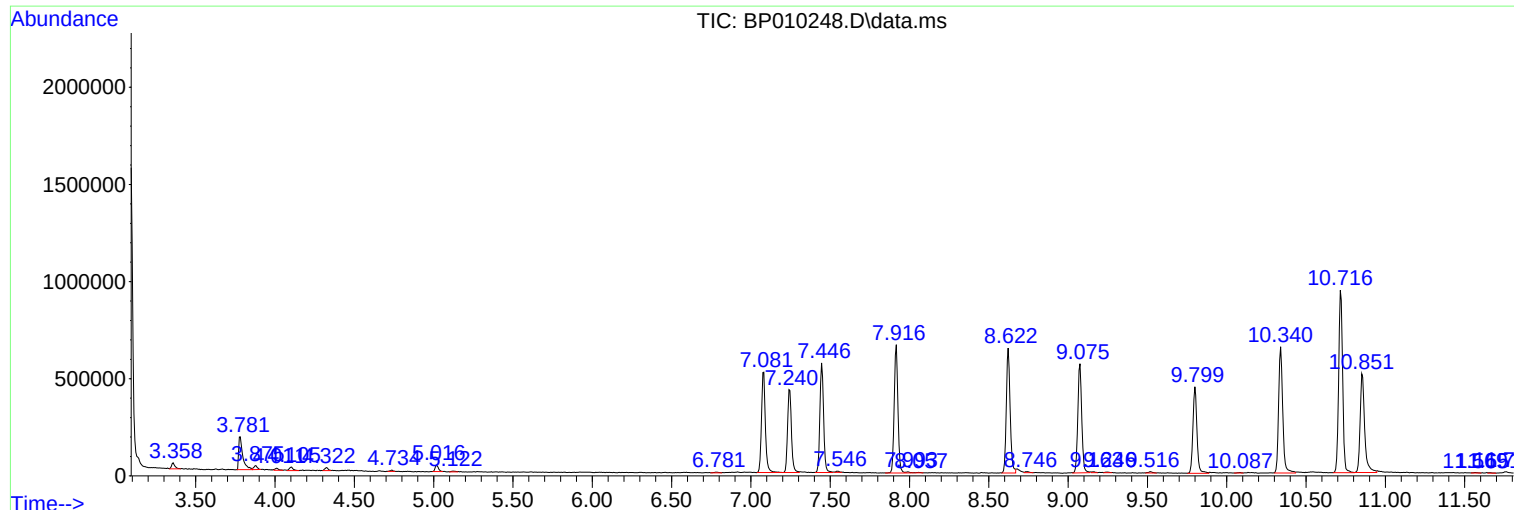

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010248.D
Acq On : 05 May 2022 15:44
Operator : CG/JU
Sample : N2697-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBP8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	5.46 ng/ul	625455	Chrysene-d12	21.380

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Docosene			308	C22H44	001599-67-3	96
2	Pentadecafluorooctanoic acid, oc...			666	C26H37F15O2	1000406-04-8	94
3	Heptadecyl heptafluorobutyrate			452	C21H35F7O2	959085-66-6	93
4	Eicosyl trifluoroacetate			394	C22H41F3O2	1000351-75-2	91
5	Nonadecyl trifluoroacetate			380	C21H39F3O2	1000351-76-3	91

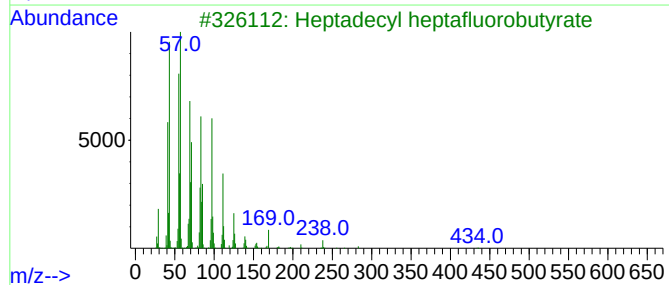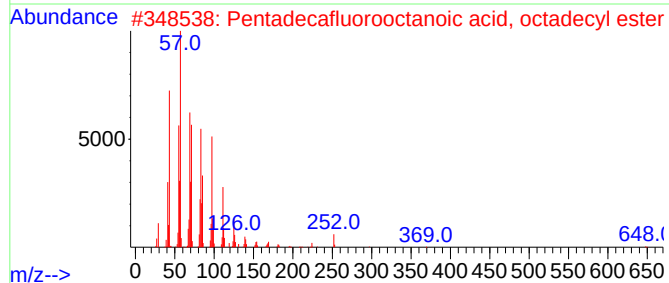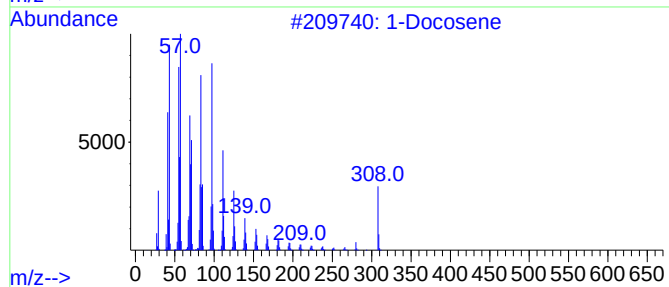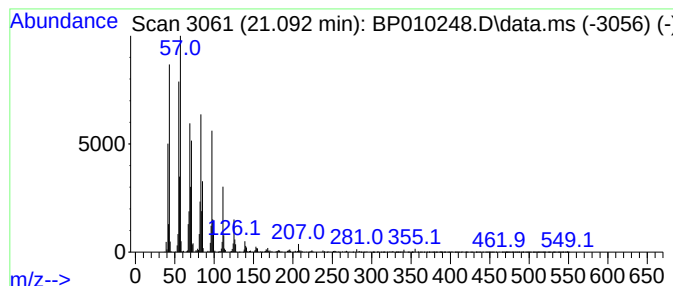

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010248.D
Acq On : 05 May 2022 15:44
Operator : CG/JU
Sample : N2697-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBP8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.092	5.5	ng/u1	625455	5	21.380	2289590	20.0