

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010250.D
 Acq On : 05 May 2022 16:51
 Operator : CG/JU
 Sample : N2697-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	38	rVB5	11801	19206	0.51%	0.045%
2	3.358	42	46	56	rVB	39370	59864	1.58%	0.141%
3	3.781	114	118	131	rBV	136797	241688	6.36%	0.567%
4	3.876	132	134	138	rVB4	9644	10332	0.27%	0.024%
5	4.011	153	157	161	rVB4	10095	15036	0.40%	0.035%
6	4.099	168	172	181	rVB	24762	35013	0.92%	0.082%
7	4.323	206	210	216	rBV5	11563	18499	0.49%	0.043%
8	4.734	277	280	286	rVB8	4518	7340	0.19%	0.017%
9	5.017	323	328	338	rVB	42220	67436	1.77%	0.158%
10	5.417	394	396	401	rVB6	2995	4523	0.12%	0.011%
11	6.605	595	598	604	rVB8	2948	5625	0.15%	0.013%
12	7.081	671	679	696	rBV	617943	1072541	28.23%	2.518%
13	7.240	700	706	717	rBV	532627	868507	22.86%	2.039%
14	7.446	734	741	752	rBV	683178	1097234	28.88%	2.576%
15	7.546	755	758	763	rVB6	8111	12170	0.32%	0.029%
16	7.916	810	821	829	rBV	674647	1098729	28.91%	2.580%
17	8.058	840	845	850	rVB7	4099	7998	0.21%	0.019%
18	8.622	934	941	956	rBV	831794	1406649	37.02%	3.303%
19	8.740	956	961	970	rVB	42889	75122	1.98%	0.176%
20	9.075	1010	1018	1031	rBV	680200	1167890	30.73%	2.742%
21	9.246	1045	1047	1055	rVB9	5240	7870	0.21%	0.018%
22	9.516	1089	1093	1101	rVB3	8739	14737	0.39%	0.035%
23	9.799	1131	1141	1156	rBV	554274	966112	25.42%	2.268%
24	10.093	1184	1191	1193	rVB6	3823	6442	0.17%	0.015%
25	10.340	1225	1233	1253	rBV	806866	1448243	38.11%	3.400%
26	10.716	1289	1297	1312	rBV	964988	1695916	44.63%	3.982%
27	10.852	1312	1320	1334	rBV	627978	1275578	33.57%	2.995%
28	11.763	1470	1475	1478	rVB6	2635	4658	0.12%	0.011%
29	12.146	1537	1540	1545	rVB6	4235	6687	0.18%	0.016%
30	12.310	1560	1568	1575	rBV	14638	28403	0.75%	0.067%
31	12.599	1613	1617	1621	rBV7	3026	5144	0.14%	0.012%
32	12.722	1633	1638	1643	rBV9	3478	7185	0.19%	0.017%
33	13.063	1690	1696	1698	rBV7	2601	4467	0.12%	0.010%
34	13.163	1708	1713	1718	rBV7	4457	7328	0.19%	0.017%
35	13.381	1744	1750	1759	rBV6	11420	22354	0.59%	0.052%
36	13.728	1803	1809	1813	rBV9	2310	4015	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010250.D
 Acq On : 05 May 2022 16:51
 Operator : CG/JU
 Sample : N2697-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBQ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	13.875	1831	1834	1837	rVV5	5648	6699	0.18%	0.016%
38	13.957	1841	1848	1857	rVV	1577704	2301827	60.58%	5.404%
39	14.040	1860	1862	1867	rVB6	4962	6672	0.18%	0.016%
40	14.240	1886	1896	1914	rBV	1742324	2681421	70.57%	6.296%
41	14.451	1929	1932	1938	rVB7	8135	10872	0.29%	0.026%
42	14.546	1941	1948	1957	rBV	1513596	2268235	59.69%	5.326%
43	14.746	1976	1982	1997	rBV	314936	705168	18.56%	1.656%
44	14.969	2014	2020	2026	rVB4	18572	35095	0.92%	0.082%
45	15.275	2068	2072	2074	rBV5	2999	3918	0.10%	0.009%
46	15.357	2081	2086	2091	rVB4	12189	21217	0.56%	0.050%
47	15.398	2091	2093	2102	rVB5	6924	11127	0.29%	0.026%
48	15.540	2111	2117	2132	rBV	2298648	3359574	88.41%	7.888%
49	15.657	2132	2137	2152	rVV	570689	854968	22.50%	2.007%
50	15.781	2154	2158	2167	rVB	27713	49837	1.31%	0.117%
51	15.893	2175	2177	2183	rVB7	4863	7911	0.21%	0.019%
52	16.040	2197	2202	2204	rBV6	5049	6260	0.16%	0.015%
53	16.110	2212	2214	2219	rVB6	4672	5527	0.15%	0.013%
54	16.269	2238	2241	2243	rBV4	7205	9158	0.24%	0.022%
55	16.328	2247	2251	2256	rVB8	10127	18264	0.48%	0.043%
56	16.434	2267	2269	2272	rVB4	4407	4811	0.13%	0.011%
57	16.628	2296	2302	2309	rVB9	7365	16405	0.43%	0.039%
58	16.704	2312	2315	2319	rVB6	4402	5294	0.14%	0.012%
59	16.840	2336	2338	2341	rVV4	3578	4880	0.13%	0.011%
60	16.957	2353	2358	2366	rVB2	50543	82819	2.18%	0.194%
61	17.063	2373	2376	2381	rBV6	7505	15426	0.41%	0.036%
62	17.116	2382	2385	2389	rVB2	10430	15724	0.41%	0.037%
63	17.298	2410	2416	2421	rBV	1711734	2481763	65.31%	5.827%
64	17.340	2421	2423	2427	rVV	174586	230571	6.07%	0.541%
65	17.398	2427	2433	2446	rVV2	2291171	3441132	90.56%	8.079%
66	17.498	2446	2450	2455	rVB7	24353	43945	1.16%	0.103%
67	17.587	2463	2465	2471	rVB5	7817	11267	0.30%	0.026%
68	17.704	2480	2485	2489	rBV2	12754	25015	0.66%	0.059%
69	17.804	2499	2502	2510	rVB8	9731	17669	0.46%	0.041%
70	17.881	2513	2515	2518	rBV4	5053	6843	0.18%	0.016%
71	17.969	2527	2530	2536	rVB6	19201	23357	0.61%	0.055%
72	18.181	2561	2566	2570	rBV4	73266	116337	3.06%	0.273%
73	18.357	2592	2596	2599	rBV2	27940	39266	1.03%	0.092%
74	18.469	2613	2615	2620	rBV5	11403	13067	0.34%	0.031%
75	18.651	2643	2646	2648	rBV2	12654	14237	0.37%	0.033%
76	18.692	2650	2653	2658	rVV7	12287	19190	0.51%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010250.D
 Acq On : 05 May 2022 16:51
 Operator : CG/JU
 Sample : N2697-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M

Title : SVOA CALIBRATION

77	19.081	2717	2719	2722	rVB3	16339	15408	0.41%	0.036%
78	19.204	2738	2740	2747	rVB3	40250	53457	1.41%	0.126%
79	19.304	2749	2757	2762	rBV	383347	532795	14.02%	1.251%
80	19.628	2807	2812	2826	rBV	2482029	3799911	100.00%	8.922%
81	21.092	3057	3061	3070	rBV2	297286	420754	11.07%	0.988%
82	21.380	3105	3110	3115	rBV	1280981	1748083	46.00%	4.104%
83	23.080	3394	3399	3403	rBV2	264067	454750	11.97%	1.068%
84	23.669	3492	3499	3504	rBV2	1085989	2195827	57.79%	5.156%
85	23.822	3519	3525	3538	rVB2	725576	1580897	41.60%	3.712%


Sum of corrected areas: 42591191

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010250.D
Acq On : 05 May 2022 16:51
Operator : CG/JU
Sample : N2697-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

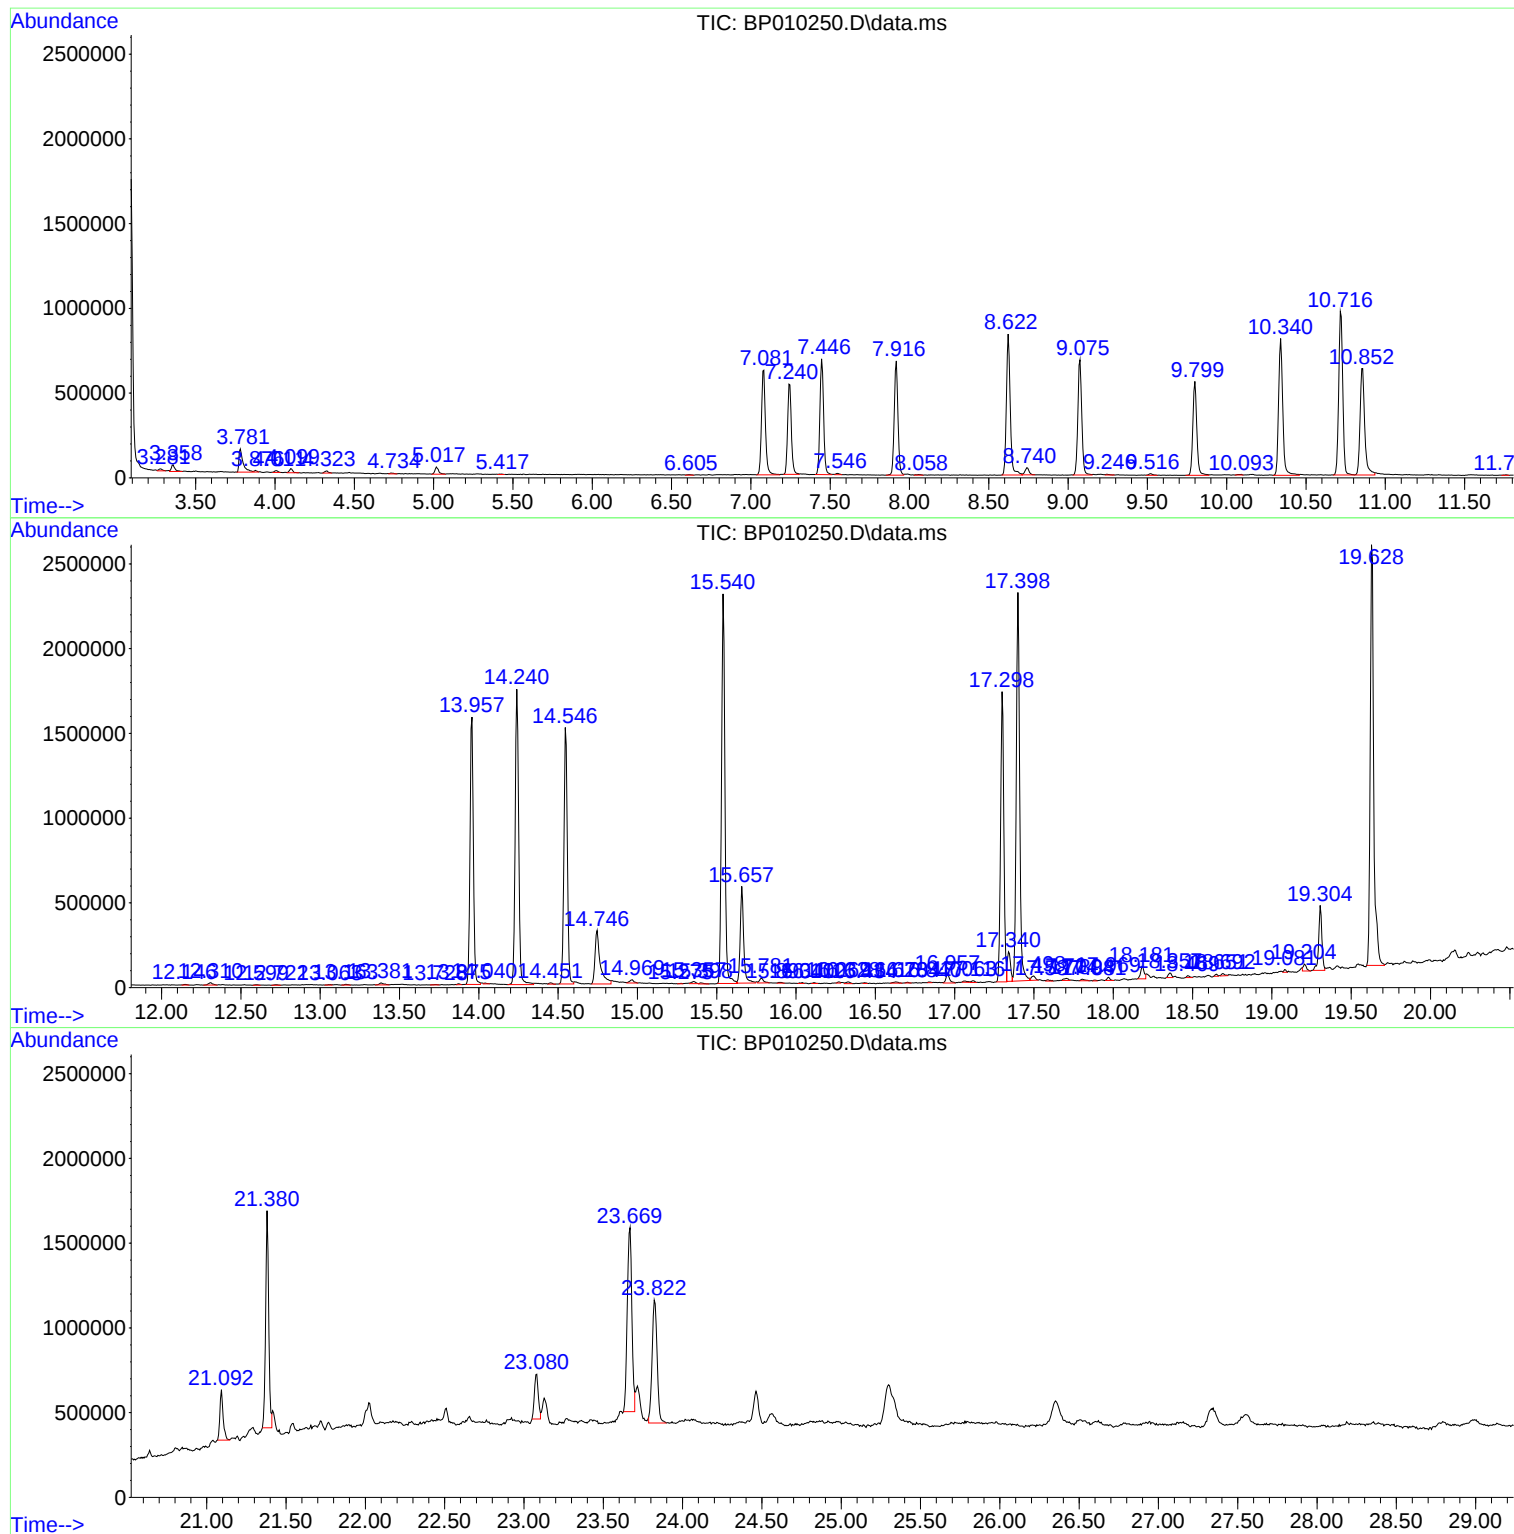

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010250.D
Acq On : 05 May 2022 16:51
Operator : CG/JU
Sample : N2697-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	4.81 ng/ul	420754	Chrysene-d12	21.381

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene			364	C26H52	018835-33-1	99
2	1-Tetracosene			336	C24H48	010192-32-2	97
3	Cyclotetracosane			336	C24H48	000297-03-0	96
4	5-Octadecene, (E)-			252	C18H36	007206-21-5	93
5	Eicosyl trifluoroacetate			394	C22H41F3O2	1000351-75-2	91

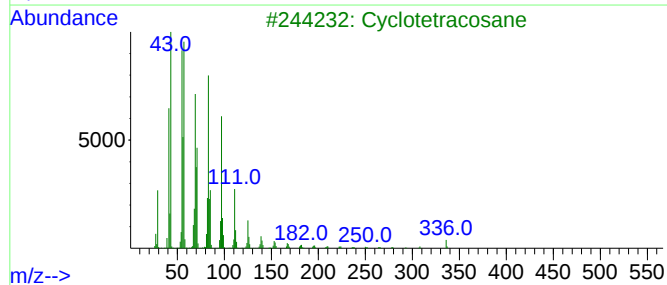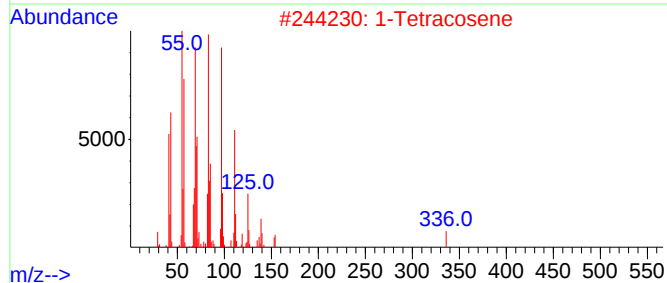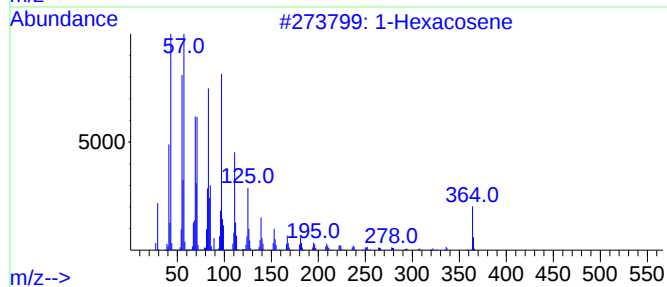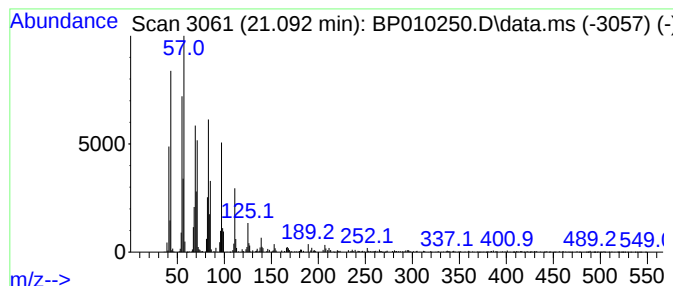

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010250.D
Acq On : 05 May 2022 16:51
Operator : CG/JU
Sample : N2697-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.092	4.8	ng/u1	420754	5	21.381	1748080	20.0