

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010252.D
 Acq On : 05 May 2022 17:59
 Operator : CG/JU
 Sample : N2697-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	42	46	51	rVB	21579	27643	1.29%	0.103%
2	3.793	117	120	128	rBV	32904	58696	2.74%	0.218%
3	3.875	132	134	139	rVB4	8867	9214	0.43%	0.034%
4	4.099	169	172	177	rVB	16905	22845	1.07%	0.085%
5	4.322	207	210	216	rVB3	11048	14538	0.68%	0.054%
6	4.652	263	266	267	rBV3	3207	2828	0.13%	0.011%
7	5.017	324	328	335	rVB	28185	41431	1.93%	0.154%
8	5.122	344	346	348	rVB3	2473	2204	0.10%	0.008%
9	5.269	369	371	374	rBV4	1871	2401	0.11%	0.009%
10	5.781	456	458	461	rVB4	2257	2283	0.11%	0.008%
11	7.075	671	678	691	rBV	328492	583753	27.24%	2.170%
12	7.240	699	706	720	rBV	297604	489923	22.86%	1.821%
13	7.446	730	741	753	rBV	373504	616041	28.74%	2.290%
14	7.546	755	758	766	rVB7	7094	14379	0.67%	0.053%
15	7.605	766	768	774	rBV7	1658	3616	0.17%	0.013%
16	7.652	774	776	779	rVV4	2139	2368	0.11%	0.009%
17	7.916	810	821	831	rBV	664034	1090820	50.90%	4.055%
18	8.063	840	846	853	rVB6	6987	14570	0.68%	0.054%
19	8.146	857	860	862	rBV4	2614	2976	0.14%	0.011%
20	8.222	869	873	875	rBV5	1708	2485	0.12%	0.009%
21	8.363	894	897	901	rVV6	2547	3222	0.15%	0.012%
22	8.422	904	907	912	rVB7	2451	3301	0.15%	0.012%
23	8.622	935	941	956	rVV	434206	761023	35.51%	2.829%
24	8.740	956	961	969	rVB	27494	51130	2.39%	0.190%
25	9.075	1011	1018	1035	rVB	360648	646468	30.16%	2.403%
26	9.252	1045	1048	1055	rVB7	3329	6725	0.31%	0.025%
27	9.322	1059	1060	1063	rVB3	2870	2463	0.11%	0.009%
28	9.522	1090	1094	1101	rVB8	6545	13263	0.62%	0.049%
29	9.799	1132	1141	1152	rBV	280279	502215	23.43%	1.867%
30	9.875	1152	1154	1156	rVB3	2750	2407	0.11%	0.009%
31	10.081	1185	1189	1196	rBV7	3631	6556	0.31%	0.024%
32	10.163	1199	1203	1208	rVB8	3954	7655	0.36%	0.028%
33	10.340	1226	1233	1247	rBV	409540	752414	35.11%	2.797%
34	10.716	1290	1297	1312	rBV	974661	1650080	76.99%	6.134%
35	10.857	1314	1321	1336	rBV	318338	654177	30.52%	2.432%
36	11.404	1412	1414	1417	rVB4	2179	2589	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010252.D
 Acq On : 05 May 2022 17:59
 Operator : CG/JU
 Sample : N2697-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	11.563	1434	1441	1443	rVV8	2273	3841	0.18%	0.014%
38	11.751	1470	1473	1474	rVV3	2515	2548	0.12%	0.009%
39	11.769	1474	1476	1483	rVB8	2520	4629	0.22%	0.017%
40	12.069	1523	1527	1531	rBV5	2003	2256	0.11%	0.008%
41	12.310	1561	1568	1575	rBV5	8566	15517	0.72%	0.058%
42	12.375	1575	1579	1582	rBV6	3019	4082	0.19%	0.015%
43	12.598	1613	1617	1621	rVB7	3181	3388	0.16%	0.013%
44	12.663	1624	1628	1630	rBV5	1637	2320	0.11%	0.009%
45	13.051	1691	1694	1696	rBV4	2207	2292	0.11%	0.009%
46	13.104	1699	1703	1706	rVV6	2972	4701	0.22%	0.017%
47	13.169	1709	1714	1719	rVB8	3051	5775	0.27%	0.021%
48	13.287	1728	1734	1739	rBV10	2357	3914	0.18%	0.015%
49	13.381	1747	1750	1756	rBV5	6738	10142	0.47%	0.038%
50	13.451	1756	1762	1767	rVB9	3531	7899	0.37%	0.029%
51	13.669	1796	1799	1801	rBV4	1680	2316	0.11%	0.009%
52	13.834	1824	1827	1830	rBV5	2900	3260	0.15%	0.012%
53	13.875	1832	1834	1837	rVB4	2366	2874	0.13%	0.011%
54	13.957	1840	1848	1861	rBV	829623	1198904	55.94%	4.457%
55	14.040	1861	1862	1865	rVV3	5189	4085	0.19%	0.015%
56	14.075	1866	1868	1876	rVB9	4906	7919	0.37%	0.029%
57	14.240	1886	1896	1907	rBV	913662	1388656	64.79%	5.162%
58	14.457	1928	1933	1937	rVB6	7306	8435	0.39%	0.031%
59	14.545	1939	1948	1958	rBV	1370553	2143175	100.00%	7.967%
60	14.751	1977	1983	2001	rBV2	92727	278732	13.01%	1.036%
61	14.963	2017	2019	2026	rVB8	9295	16063	0.75%	0.060%
62	15.298	2072	2076	2077	rBV4	2810	2568	0.12%	0.010%
63	15.351	2080	2085	2090	rVV2	19770	31145	1.45%	0.116%
64	15.404	2090	2094	2097	rVB4	6291	7066	0.33%	0.026%
65	15.540	2110	2117	2131	rBV	1098471	1725508	80.51%	6.414%
66	15.657	2132	2137	2150	rVV	214362	356102	16.62%	1.324%
67	15.781	2154	2158	2163	rVB3	12262	18940	0.88%	0.070%
68	16.057	2203	2205	2209	rVB5	4430	4318	0.20%	0.016%
69	16.116	2212	2215	2217	rBV4	3457	3549	0.17%	0.013%
70	16.269	2237	2241	2242	rBV4	8410	9049	0.42%	0.034%
71	16.381	2256	2260	2264	rBV	10158	15256	0.71%	0.057%
72	16.439	2264	2270	2276	rVB5	10153	21859	1.02%	0.081%
73	16.498	2276	2280	2285	rBV5	8643	12971	0.61%	0.048%
74	16.545	2285	2288	2292	rBV4	6217	8184	0.38%	0.030%
75	16.628	2299	2302	2304	rBV4	4408	5414	0.25%	0.020%
76	16.704	2310	2315	2319	rBV7	10246	17021	0.79%	0.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010252.D
 Acq On : 05 May 2022 17:59
 Operator : CG/JU
 Sample : N2697-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBQ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

77	16.769	2322	2326	2329	rBV3	9537	13315	0.62%	0.049%
78	16.804	2330	2332	2335	rVB4	2929	2573	0.12%	0.010%
79	16.851	2335	2340	2343	rBV6	6004	10001	0.47%	0.037%
80	17.028	2367	2370	2371	rBV3	3350	2907	0.14%	0.011%
81	17.063	2373	2376	2379	rVV5	10822	16252	0.76%	0.060%
82	17.116	2383	2385	2389	rVB5	7789	9423	0.44%	0.035%
83	17.222	2401	2403	2407	rVB5	3592	4654	0.22%	0.017%
84	17.298	2410	2416	2421	rVV	1421028	2095355	97.77%	7.789%
85	17.339	2421	2423	2428	rVV	87265	126174	5.89%	0.469%
86	17.398	2428	2433	2446	rVB	1048271	1572944	73.39%	5.847%
87	17.645	2474	2475	2479	rBV4	3861	4490	0.21%	0.017%
88	17.798	2499	2501	2504	rBV3	8391	11335	0.53%	0.042%
89	17.969	2526	2530	2536	rVB9	8508	13222	0.62%	0.049%
90	18.181	2561	2566	2570	rBV4	32476	58968	2.75%	0.219%
91	18.357	2592	2596	2599	rBV5	14195	22670	1.06%	0.084%
92	19.081	2717	2719	2722	rBV3	14572	13028	0.61%	0.048%
93	19.304	2749	2757	2764	rBV	179139	276772	12.91%	1.029%
94	19.628	2807	2812	2826	rBV2	1202989	1862862	86.92%	6.925%
95	21.092	3057	3061	3067	rBV2	185992	246897	11.52%	0.918%
96	21.380	3105	3110	3115	rBV	1213656	1646842	76.84%	6.122%
97	22.004	3213	3216	3225	rVB4	105233	224522	10.48%	0.835%
98	23.074	3394	3398	3403	rBV2	262963	442765	20.66%	1.646%
99	23.663	3492	3498	3504	rBV2	609958	1234529	57.60%	4.589%
100	23.821	3519	3525	3536	rVB2	753406	1550906	72.36%	5.765%




Sum of corrected areas: 26900781

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010252.D
Acq On : 05 May 2022 17:59
Operator : CG/JU
Sample : N2697-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

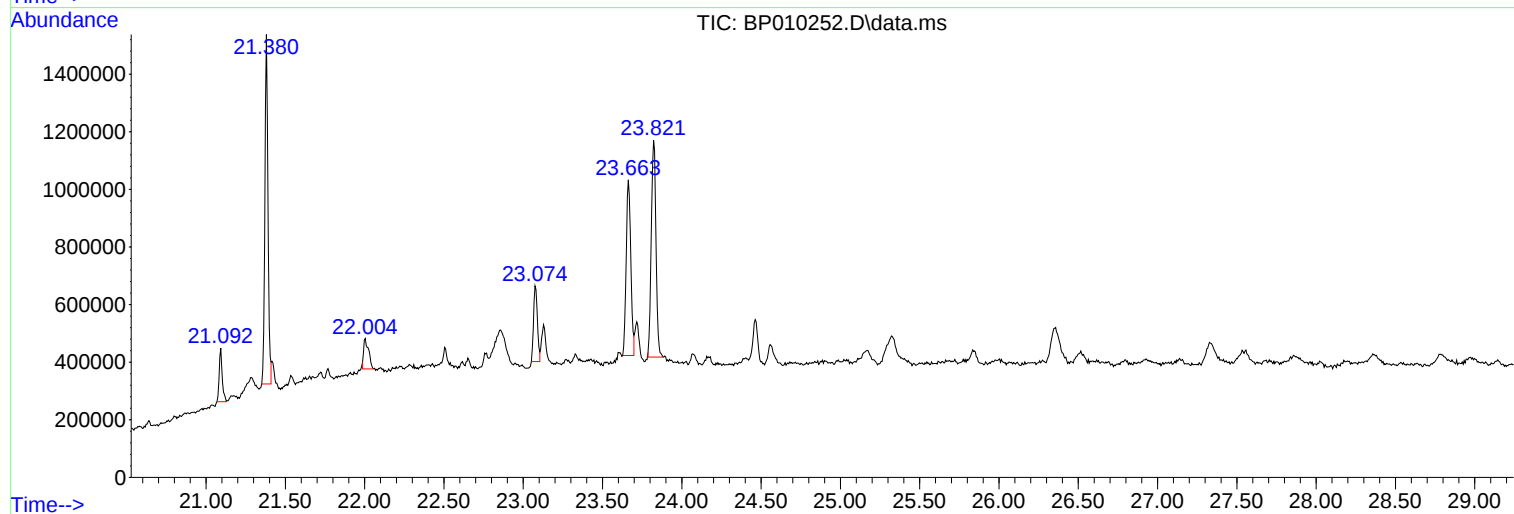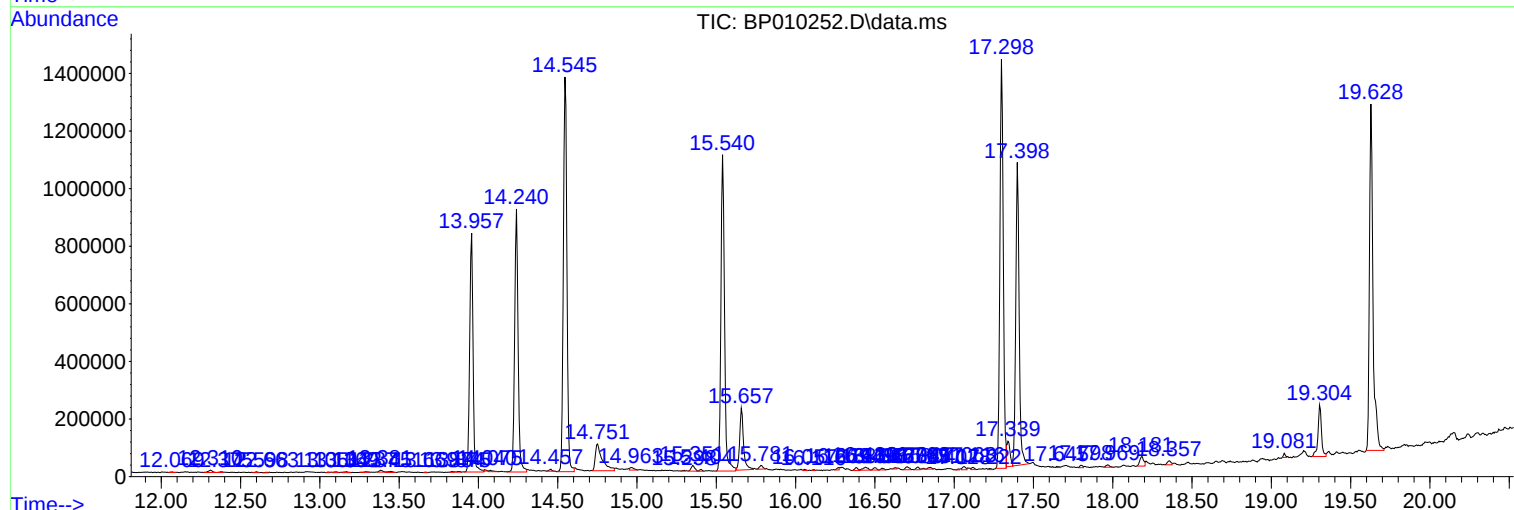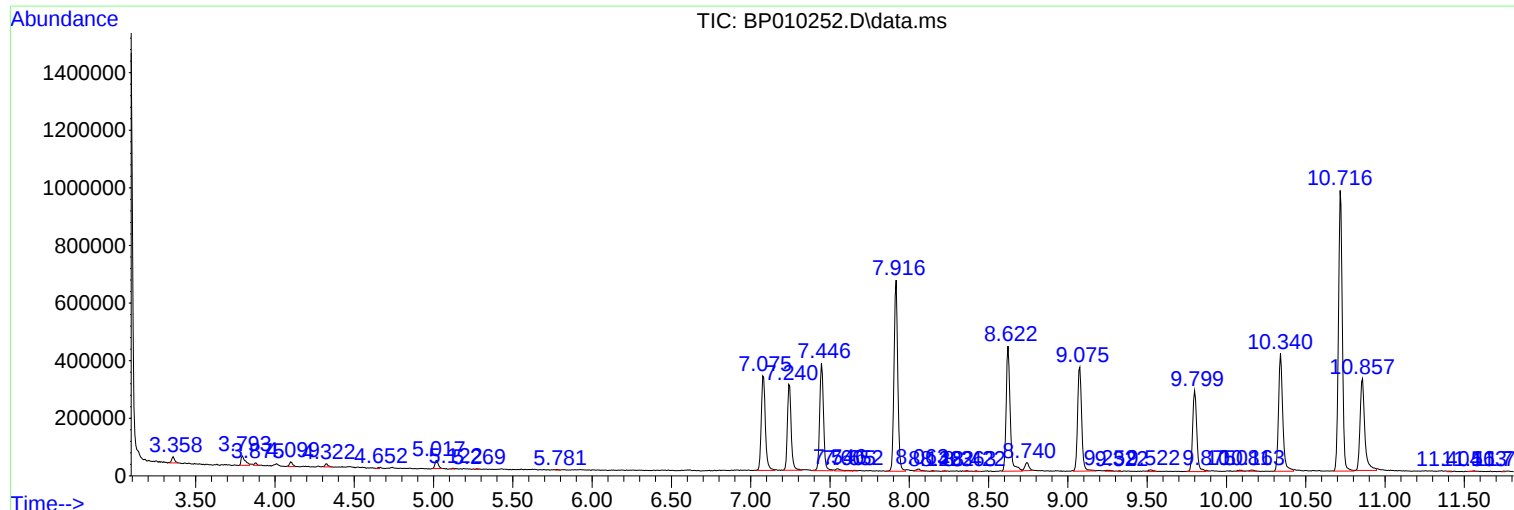

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010252.D
Acq On : 05 May 2022 17:59
Operator : CG/JU
Sample : N2697-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tricosyl heptafluorobutyrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.092	3.00 ng/ul	246897	Chrysene-d12	21.380

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tricosyl heptafluorobutyrate	536	C27H47F7O2	1000351-83-4	91
2			Oxalic acid, hexadecyl propyl ester	356	C21H40O4	1000309-26-9	91
3			Tetracosyl heptafluorobutyrate	550	C28H49F7O2	1000351-83-7	91
4			Oxalic acid, isobutyl octadecyl ...	398	C24H46O4	1000309-38-3	91
5			Tricosyl trifluoroacetate	436	C25H47F3O2	1000351-75-1	91

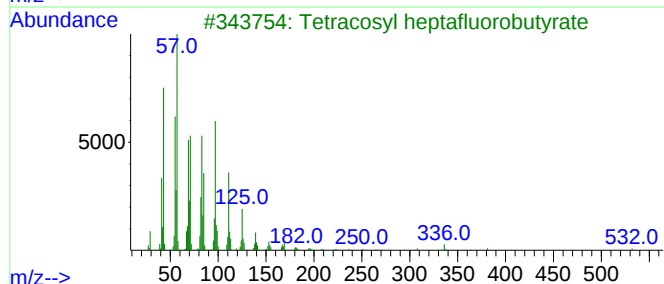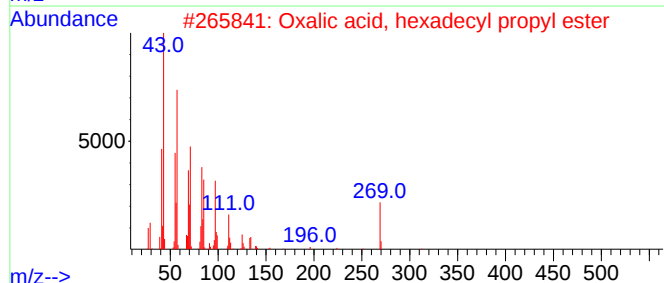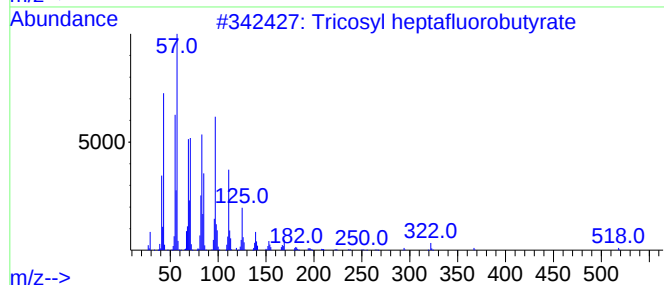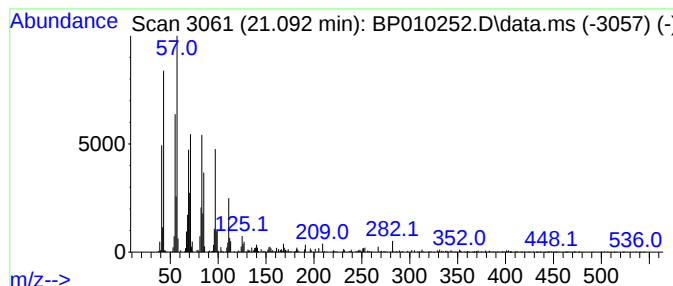

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010252.D
Acq On : 05 May 2022 17:59
Operator : CG/JU
Sample : N2697-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.004	2.73 ng/ul	224522	Chrysene-d12	21.380

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonadecane	268	C19H40	000629-92-5	95
2			Eicosane	282	C20H42	000112-95-8	95
3			Heneicosane	296	C21H44	000629-94-7	94
4			Heneicosane	296	C21H44	000629-94-7	93
5			Nonadecane	268	C19H40	000629-92-5	90

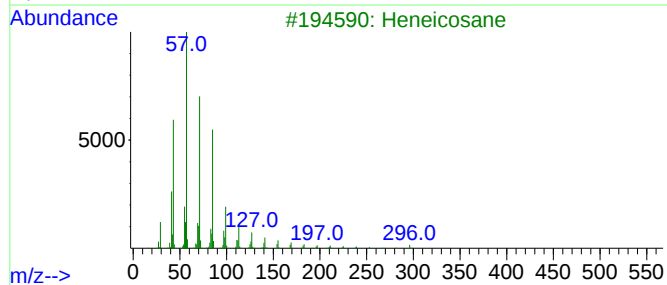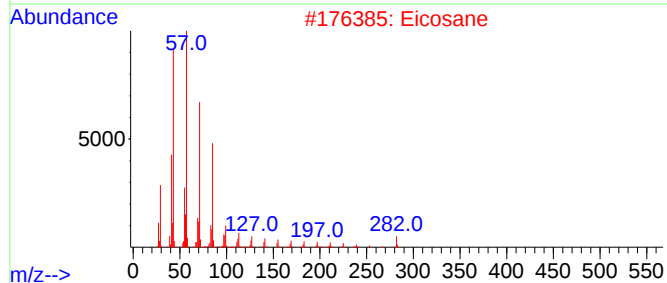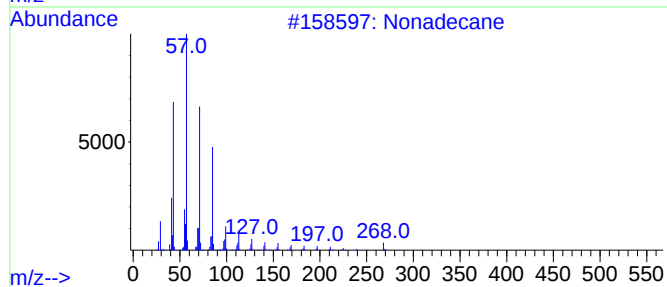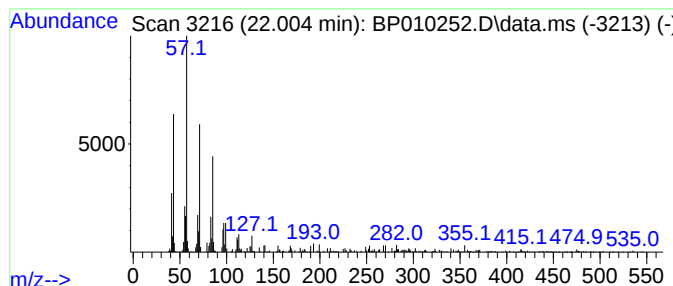

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010252.D
Acq On : 05 May 2022 17:59
Operator : CG/JU
Sample : N2697-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tricosyl heptaf...	21.092	3.0	ng/u1	246897	5	21.380	1646840	20.0
(DEL) Alkane: S...	22.004	2.7	ng/u1	224522	5	21.380	1646840	20.0