

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010256.D
 Acq On : 05 May 2022 20:14
 Operator : CG/JU
 Sample : N2678-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	43	46	51	rBV	42360	48337	1.19%	0.120%
2	3.781	115	118	129	rBV	126906	204069	5.01%	0.507%
3	4.099	168	172	176	rVB3	12782	18400	0.45%	0.046%
4	5.016	326	328	335	rVB2	8348	12436	0.31%	0.031%
5	7.081	673	679	693	rVB	176318	305626	7.50%	0.759%
6	7.240	700	706	723	rBV	669495	1112372	27.29%	2.762%
7	7.445	732	741	754	rBV	671420	1101210	27.01%	2.735%
8	7.551	754	759	764	rVB9	6165	11524	0.28%	0.029%
9	7.916	814	821	831	rBV	612509	984984	24.16%	2.446%
10	7.992	831	834	838	rVB5	4463	5778	0.14%	0.014%
11	8.622	935	941	959	rBV	503549	874303	21.45%	2.171%
12	8.734	959	960	967	rVB7	3460	5721	0.14%	0.014%
13	9.075	1008	1018	1029	rBV	842211	1436590	35.24%	3.568%
14	9.522	1088	1094	1098	rBV5	6060	10269	0.25%	0.026%
15	9.798	1132	1141	1158	rBV	663037	1150193	28.21%	2.856%
16	10.339	1225	1233	1249	rBV	840593	1498365	36.75%	3.721%
17	10.528	1259	1265	1273	rBV8	11497	29367	0.72%	0.073%
18	10.716	1290	1297	1309	rBV	817296	1396607	34.26%	3.468%
19	10.851	1313	1320	1334	rBV	432128	859512	21.08%	2.134%
20	11.381	1404	1410	1412	rBV6	3906	6834	0.17%	0.017%
21	12.145	1537	1540	1546	rVB8	5424	9016	0.22%	0.022%
22	12.310	1561	1568	1580	rBV	15087	31690	0.78%	0.079%
23	12.922	1667	1672	1676	rBV7	4230	7390	0.18%	0.018%
24	13.169	1709	1714	1717	rBV7	3926	5231	0.13%	0.013%
25	13.380	1745	1750	1760	rBV2	21762	34408	0.84%	0.085%
26	13.780	1812	1818	1821	rBV7	3153	5512	0.14%	0.014%
27	13.957	1841	1848	1860	rBV	1629854	2384462	58.49%	5.921%
28	14.086	1865	1870	1875	rVB6	17950	29979	0.74%	0.074%
29	14.239	1886	1896	1910	rBV	1863809	2742304	67.27%	6.810%
30	14.451	1926	1932	1937	rVB	40556	55225	1.35%	0.137%
31	14.545	1940	1948	1961	rBV	1124511	1701234	41.73%	4.225%
32	14.751	1977	1983	2002	rBV	53303	163289	4.01%	0.406%
33	14.963	2016	2019	2024	rVB6	6145	9910	0.24%	0.025%
34	15.074	2031	2038	2044	rVB2	27096	42107	1.03%	0.105%
35	15.204	2053	2060	2064	rBV4	28352	44445	1.09%	0.110%
36	15.363	2081	2087	2090	rBV8	5432	13331	0.33%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
 Data File : BP010256.D
 Acq On : 05 May 2022 20:14
 Operator : CG/JU
 Sample : N2678-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
 Title : SVOA CALIBRATION

37	15.404	2090	2094	2098	rVB2	44839	59098	1.45%	0.147%
38	15.539	2110	2117	2131	rBV	2243367	3345769	82.07%	8.309%
39	15.657	2131	2137	2152	rVV	687878	1096712	26.90%	2.724%
40	15.780	2154	2158	2168	rVV4	35770	89820	2.20%	0.223%
41	15.851	2168	2170	2174	rVV5	7101	10022	0.25%	0.025%
42	15.904	2174	2179	2185	rVV9	6772	17016	0.42%	0.042%
43	15.963	2185	2189	2196	rVV7	7066	17577	0.43%	0.044%
44	16.021	2197	2199	2209	rVV7	7293	13230	0.32%	0.033%
45	16.104	2211	2213	2219	rVB7	4309	6930	0.17%	0.017%
46	16.263	2236	2240	2248	rVV	44686	75953	1.86%	0.189%
47	16.327	2248	2251	2256	rVB6	11186	16966	0.42%	0.042%
48	16.974	2359	2361	2366	rBV6	3527	4611	0.11%	0.011%
49	17.063	2371	2376	2381	rBV3	33456	45723	1.12%	0.114%
50	17.298	2409	2416	2426	rBV	1158744	1731194	42.46%	4.299%
51	17.398	2426	2433	2455	rVB	2366234	3584010	87.91%	8.900%
52	17.733	2485	2490	2493	rBV7	4604	7818	0.19%	0.019%
53	17.804	2499	2502	2507	rVB2	19416	20902	0.51%	0.052%
54	18.063	2543	2546	2547	rBV3	4781	5362	0.13%	0.013%
55	18.180	2562	2566	2574	rBV3	15264	30413	0.75%	0.076%
56	18.474	2612	2616	2621	rBV5	11598	16085	0.39%	0.040%
57	19.210	2737	2741	2747	rBV3	32273	49754	1.22%	0.124%
58	19.274	2749	2752	2758	rVB2	25750	37396	0.92%	0.093%
59	19.627	2806	2812	2827	rBV	2951703	4076824	100.00%	10.124%
60	21.086	3057	3060	3065	rBV4	61015	88153	2.16%	0.219%
61	21.380	3105	3110	3126	rBV	1243960	1789609	43.90%	4.444%
62	23.662	3491	3498	3513	rBV2	1821971	3937028	96.57%	9.777%
63	23.821	3518	3525	3536	rVB2	826998	1742044	42.73%	4.326%




Sum of corrected areas: 40268049

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010256.D
Acq On : 05 May 2022 20:14
Operator : CG/JU
Sample : N2678-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

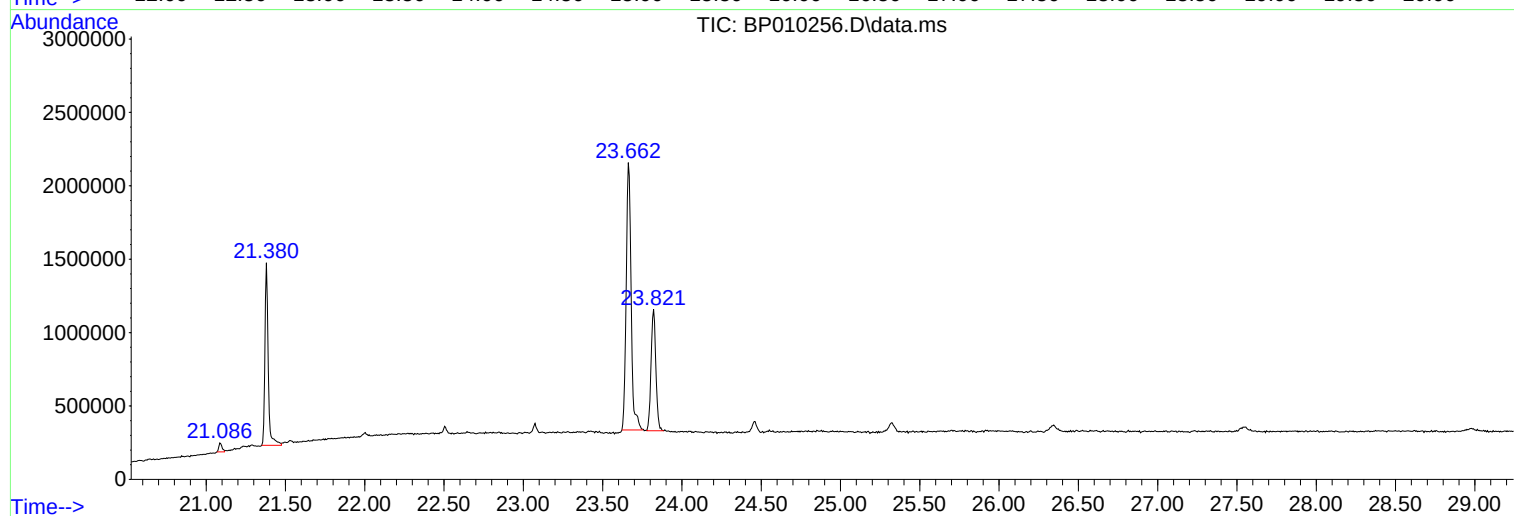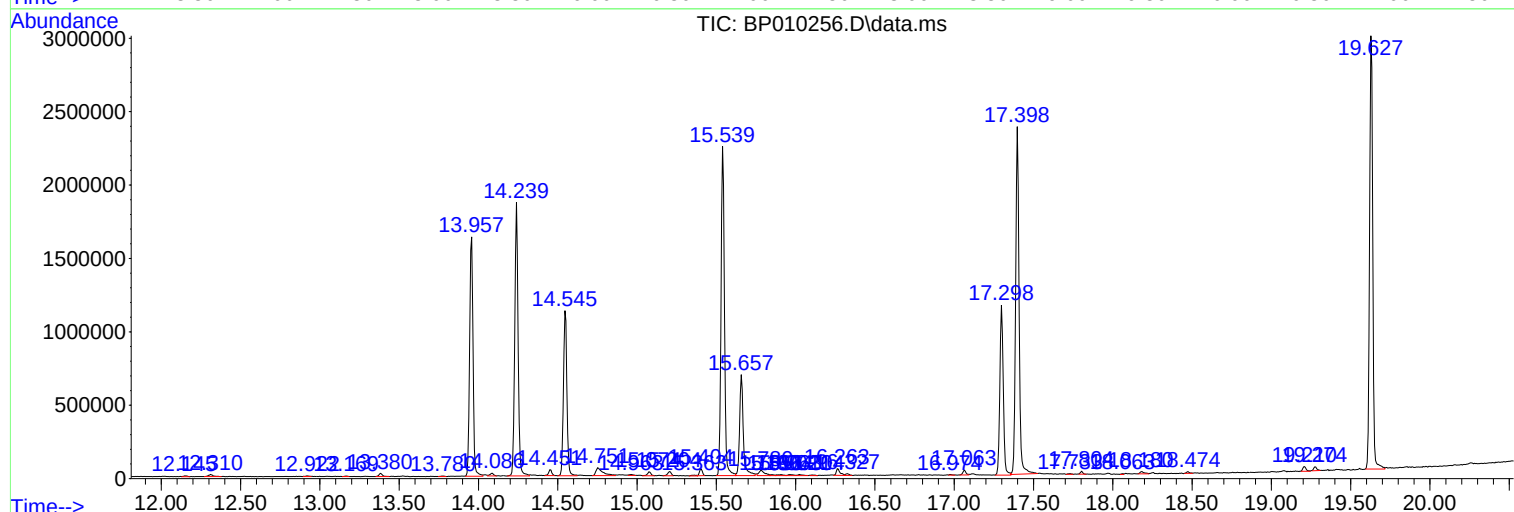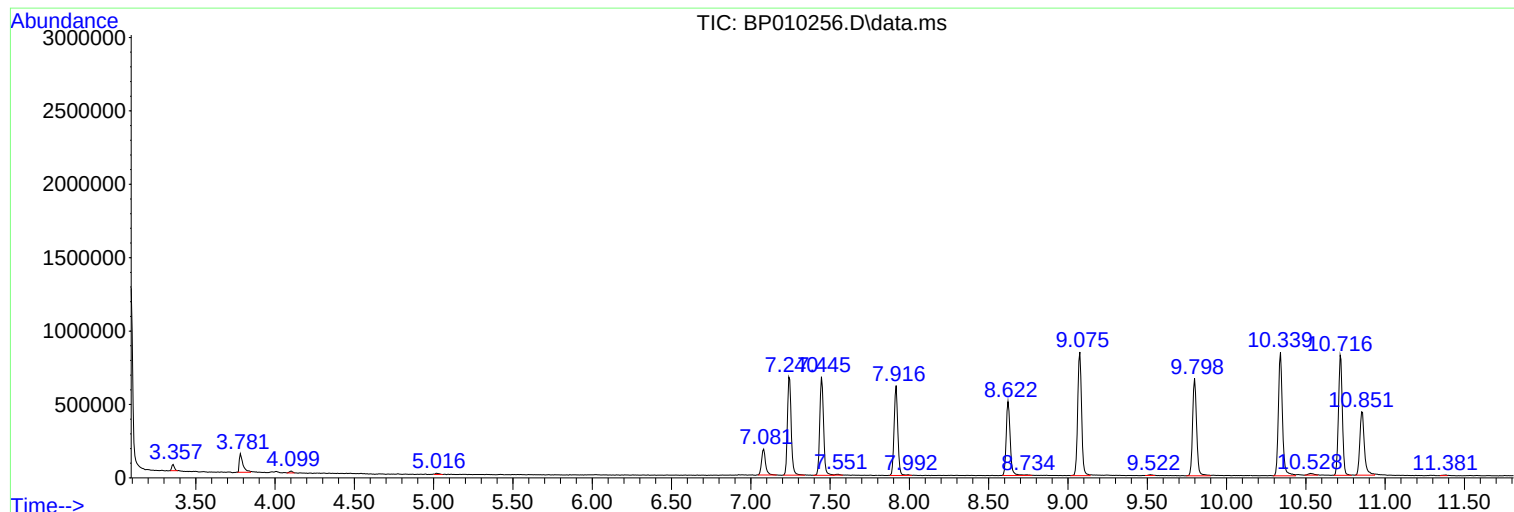

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010256.D
Acq On : 05 May 2022 20:14
Operator : CG/JU
Sample : N2678-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050522\
Data File : BP010256.D
Acq On : 05 May 2022 20:14
Operator : CG/JU
Sample : N2678-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP042122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc