




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020265.D
Acq On : 09 May 2024 11:29
Operator : MA/JU
Sample : P2369-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43X7

Manual IntegrationsAPPROVED

Quant Time: May 09 12:04:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/09/2024
Supervised By :mohammad ahmed 05/11/2024

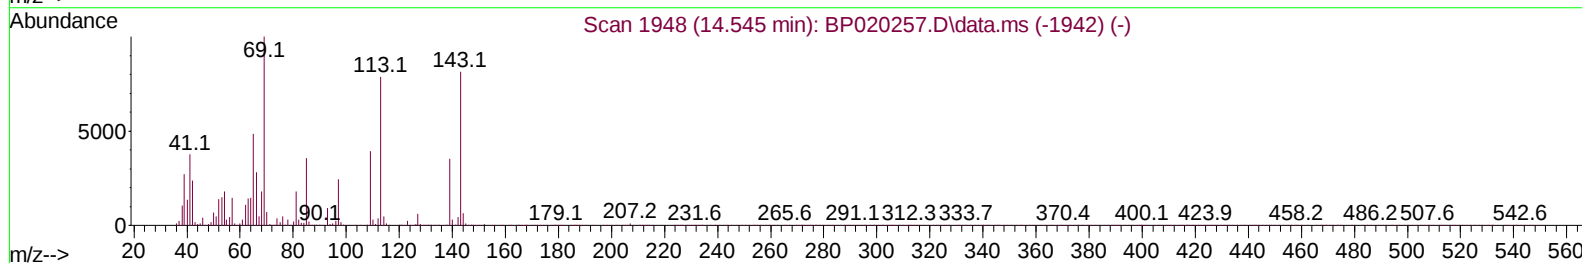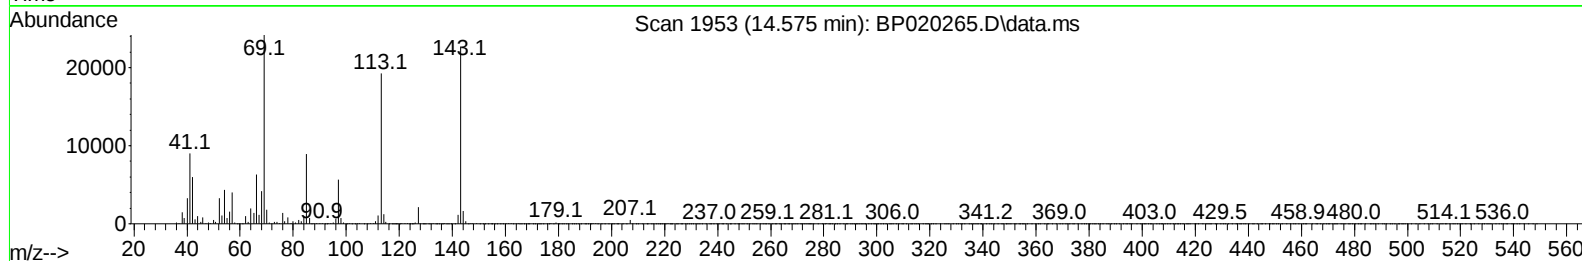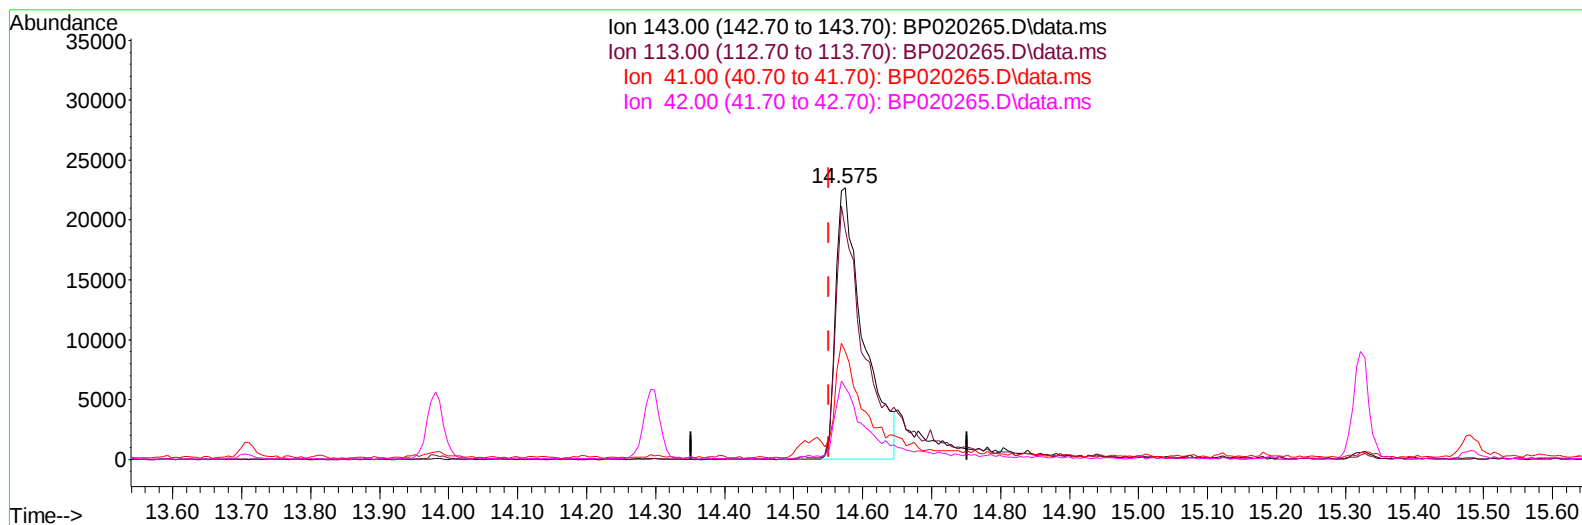

TIC: BP020265.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.575min (+ 0.023) 18.96 ng/u1

response 62934

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	84.83
41.00	50.30	39.76#
42.00	32.50	26.51




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020265.D
Acq On : 09 May 2024 11:29
Operator : MA/JU
Sample : P2369-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43X7

Manual IntegrationsAPPROVED

Quant Time: May 09 12:04:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/09/2024
Supervised By :mohammad ahmed 05/11/2024

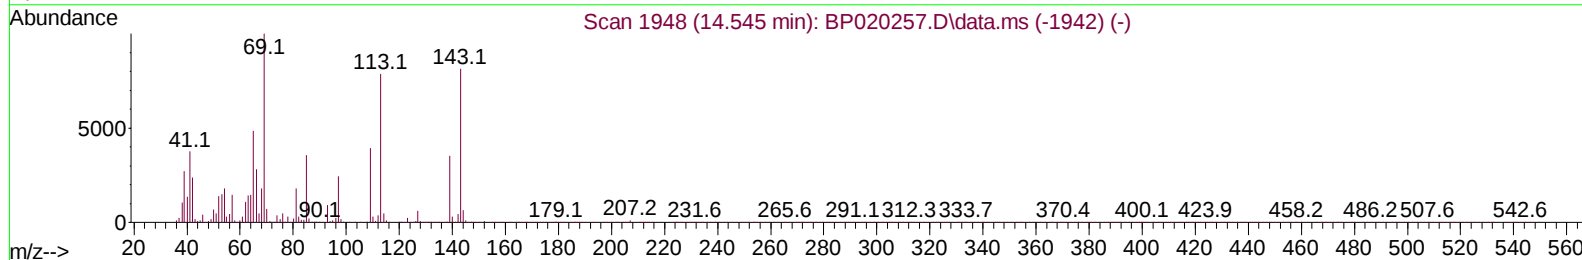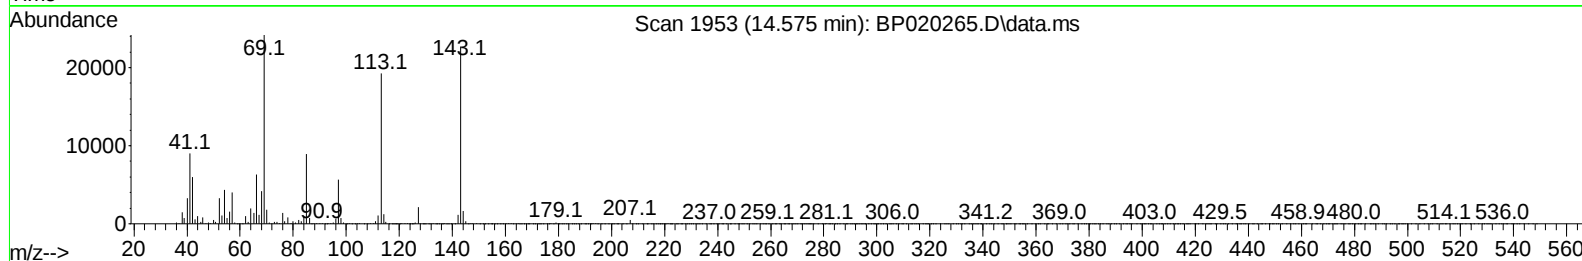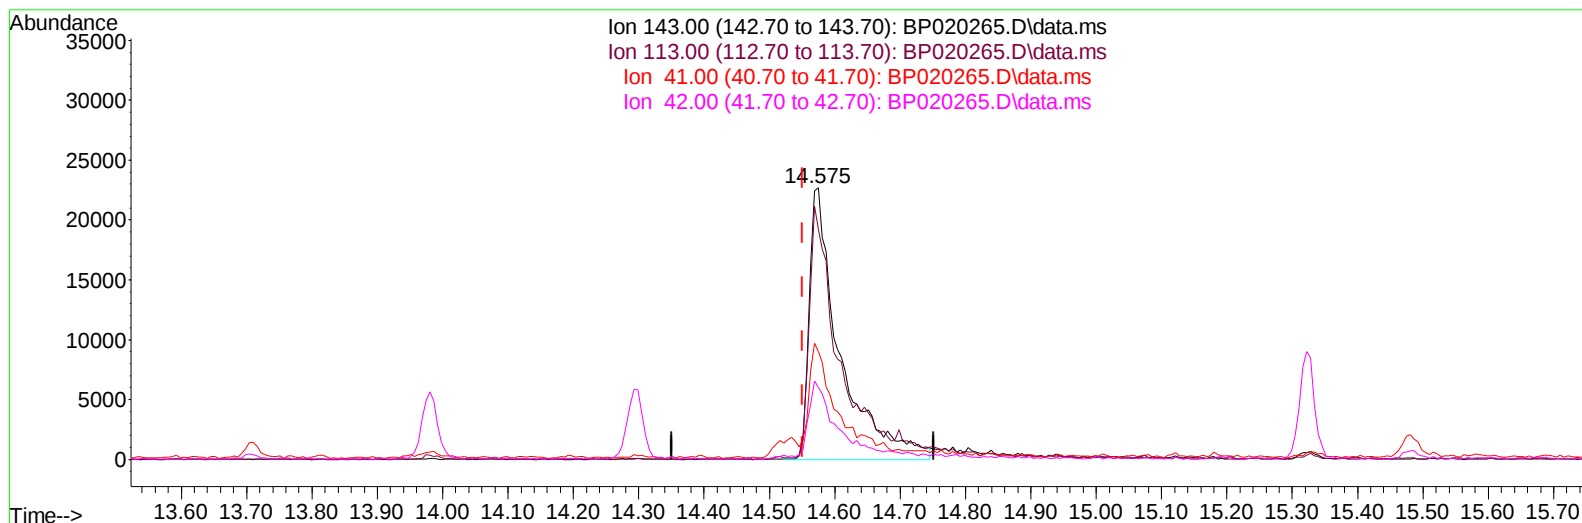

TIC: BP020265.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.575min (+ 0.023) 22.36 ng/ul m

response 74211

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	84.83
41.00	50.30	39.76#
42.00	32.50	26.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
 Data File : BP020265.D
 Acq On : 09 May 2024 11:29
 Operator : MA/JU
 Sample : P2369-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43X7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/09/2024
 Supervised By :mohammad ahmed 05/11/2024

Quant Time: May 09 12:05:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	94617	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	413513	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164	295691	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.139	188	650651	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	521103	20.000	ng/ul	0.00
88) Perylene-d12	25.009	264	554276	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	9630	4.298	ng/uL	0.00
4) Pyridine-d5	3.617	84	127551	19.594	ng/ul	0.00
7) Phenol-d5	6.810	99	197171	24.265	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	119145	24.138	ng/ul	0.00
11) 2-Chlorophenol-d4	7.157	132	156301	26.908	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	168345	25.626	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	80504	25.998	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	91649	25.846	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	169055	26.126	ng/ul	0.00
31) 4-Chloroaniline-d4	10.551	131	221279	24.433	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	610591	28.277	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	751286	31.496	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	74211m	22.361	ng/ul	0.02
60) Fluorene-d10	15.322	176	528485	29.343	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	46613	11.290	ng/ul	0.00
73) Anthracene-d10	17.245	188	812777	28.876	ng/ul	0.00
81) Pyrene-d10	19.639	212	964625	31.667	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.768	264	778808	29.060	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020265.D
Acq On : 09 May 2024 11:29
Operator : MA/JU
Sample : P2369-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43X7

Manual IntegrationsAPPROVED

Quant Time: May 09 12:05:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/09/2024
Supervised By :mohammad ahmed 05/11/2024

