

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
 Data File : BP020236.D
 Acq On : 08 May 2024 10:33
 Operator : MA/JU
 Sample : P2369-23
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y5

Quant Time: May 08 13:14:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	100104	20.000	ng/u1	0.02
20) Naphthalene-d8	10.393	136	429878	20.000	ng/u1	0.02
38) Acenaphthene-d10	14.298	164	309498	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.145	188	689666	20.000	ng/u1	0.00
79) Chrysene-d12	21.633	240	623353	20.000	ng/u1	0.00
88) Perylene-d12	24.998	264	570064	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	7526	3.175	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.805	99	214489	24.950	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.975	67	130862	25.058	ng/u1	0.02
11) 2-Chlorophenol-d4	7.152	132	157610	25.646	ng/u1	0.01
15) 4-Methylphenol-d8	8.340	113	180316	25.944	ng/u1	0.03
21) Nitrobenzene-d5	8.781	128	85945	26.699	ng/u1	0.02
24) 2-Nitrophenol-d4	9.487	143	98395	26.692	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.022	165	224954	33.441	ng/u1	0.01
31) 4-Chloroaniline-d4	10.557	131	213498	22.677	ng/u1	0.02
46) Dimethylphthalate-d6	13.710	166	726549	32.146	ng/u1	0.00
49) Acenaphthylene-d8	13.987	160	738225	29.568	ng/u1	0.00
54) 4-Nitrophenol-d4	14.551	143	120559	34.707	ng/u1	0.00
60) Fluorene-d10	15.328	176	621568	32.972	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.487	200	124133	28.364	ng/u1	0.01
73) Anthracene-d10	17.251	188	1053484	35.310	ng/u1	0.01
81) Pyrene-d10	19.645	212	1275556	35.006	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.780	264	980670	35.579	ng/u1	0.02
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.787	266	985583	188.456	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020236.D
Acq On : 08 May 2024 10:33
Operator : MA/JU
Sample : P2369-23
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43Y5

Quant Time: May 08 13:14:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

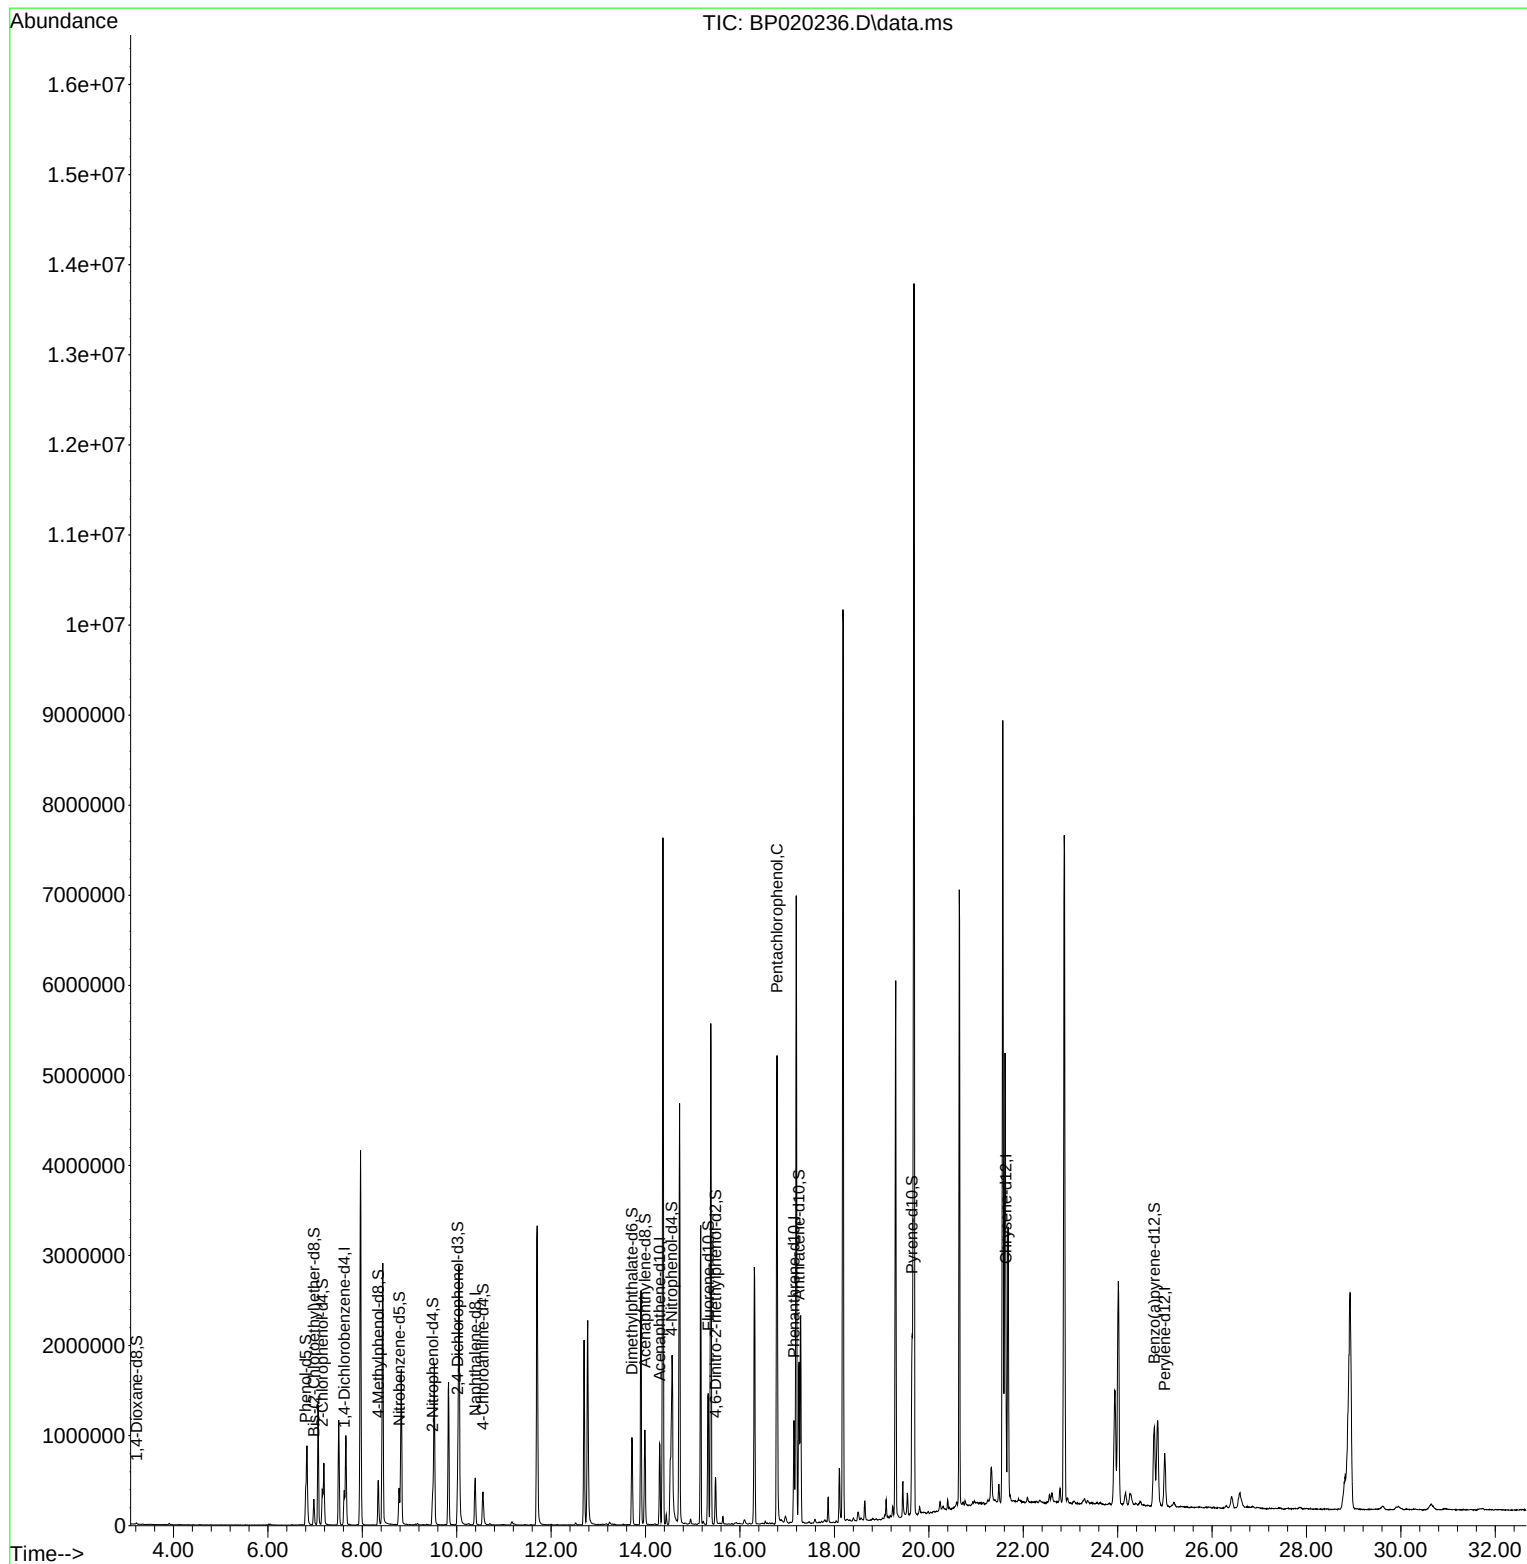

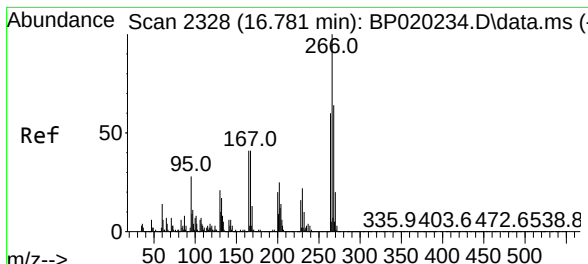

#71
 Pentachlorophenol
 Concen: 188.456 ng/ul
 RT: 16.787 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP020236.D
 Acq: 08 May 2024 10:33

Instrument :
 BNA_P
 ClientSampleId :
 A43Y5

Tgt Ion:	266	Resp:	985583
Ion Ratio	Lower	Upper	
266	100		
264	62.5	49.8	74.6
268	63.0	50.4	75.6

