

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
 Data File : BP020264.D
 Acq On : 09 May 2024 10:45
 Operator : MA/JU
 Sample : P2369-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43N2

Quant Time: May 09 11:13:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	110949	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	487192	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.293	164	347124	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.134	188	772812	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	617922	20.000	ng/ul	0.00
88) Perylene-d12	25.004	264	629141	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	10038	3.821	ng/uL	0.00
4) Pyridine-d5	3.617	84	168980	22.137	ng/ul	0.00
7) Phenol-d5	6.805	99	238473	25.028	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	153106	26.452	ng/ul	0.00
11) 2-Chlorophenol-d4	7.158	132	192650	28.283	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113	188460	24.465	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	108152	29.645	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	126637	30.312	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	236485	31.019	ng/ul	0.00
31) 4-Chloroaniline-d4	10.552	131	293752	27.530	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	857754	33.838	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	936835	33.456	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	116788	29.977	ng/ul	0.00
60) Fluorene-d10	15.316	176	743151	35.148	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	98803	20.147	ng/ul	0.00
73) Anthracene-d10	17.234	188	1132582	33.877	ng/ul	-0.01
81) Pyrene-d10	19.633	212	1363545	37.750	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.763	264	1063049	34.946	ng/ul	-0.01
Target Compounds						
71) Pentachlorophenol	16.769	266	405450	69.186	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020264.D
Acq On : 09 May 2024 10:45
Operator : MA/JU
Sample : P2369-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43N2

Quant Time: May 09 11:13:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

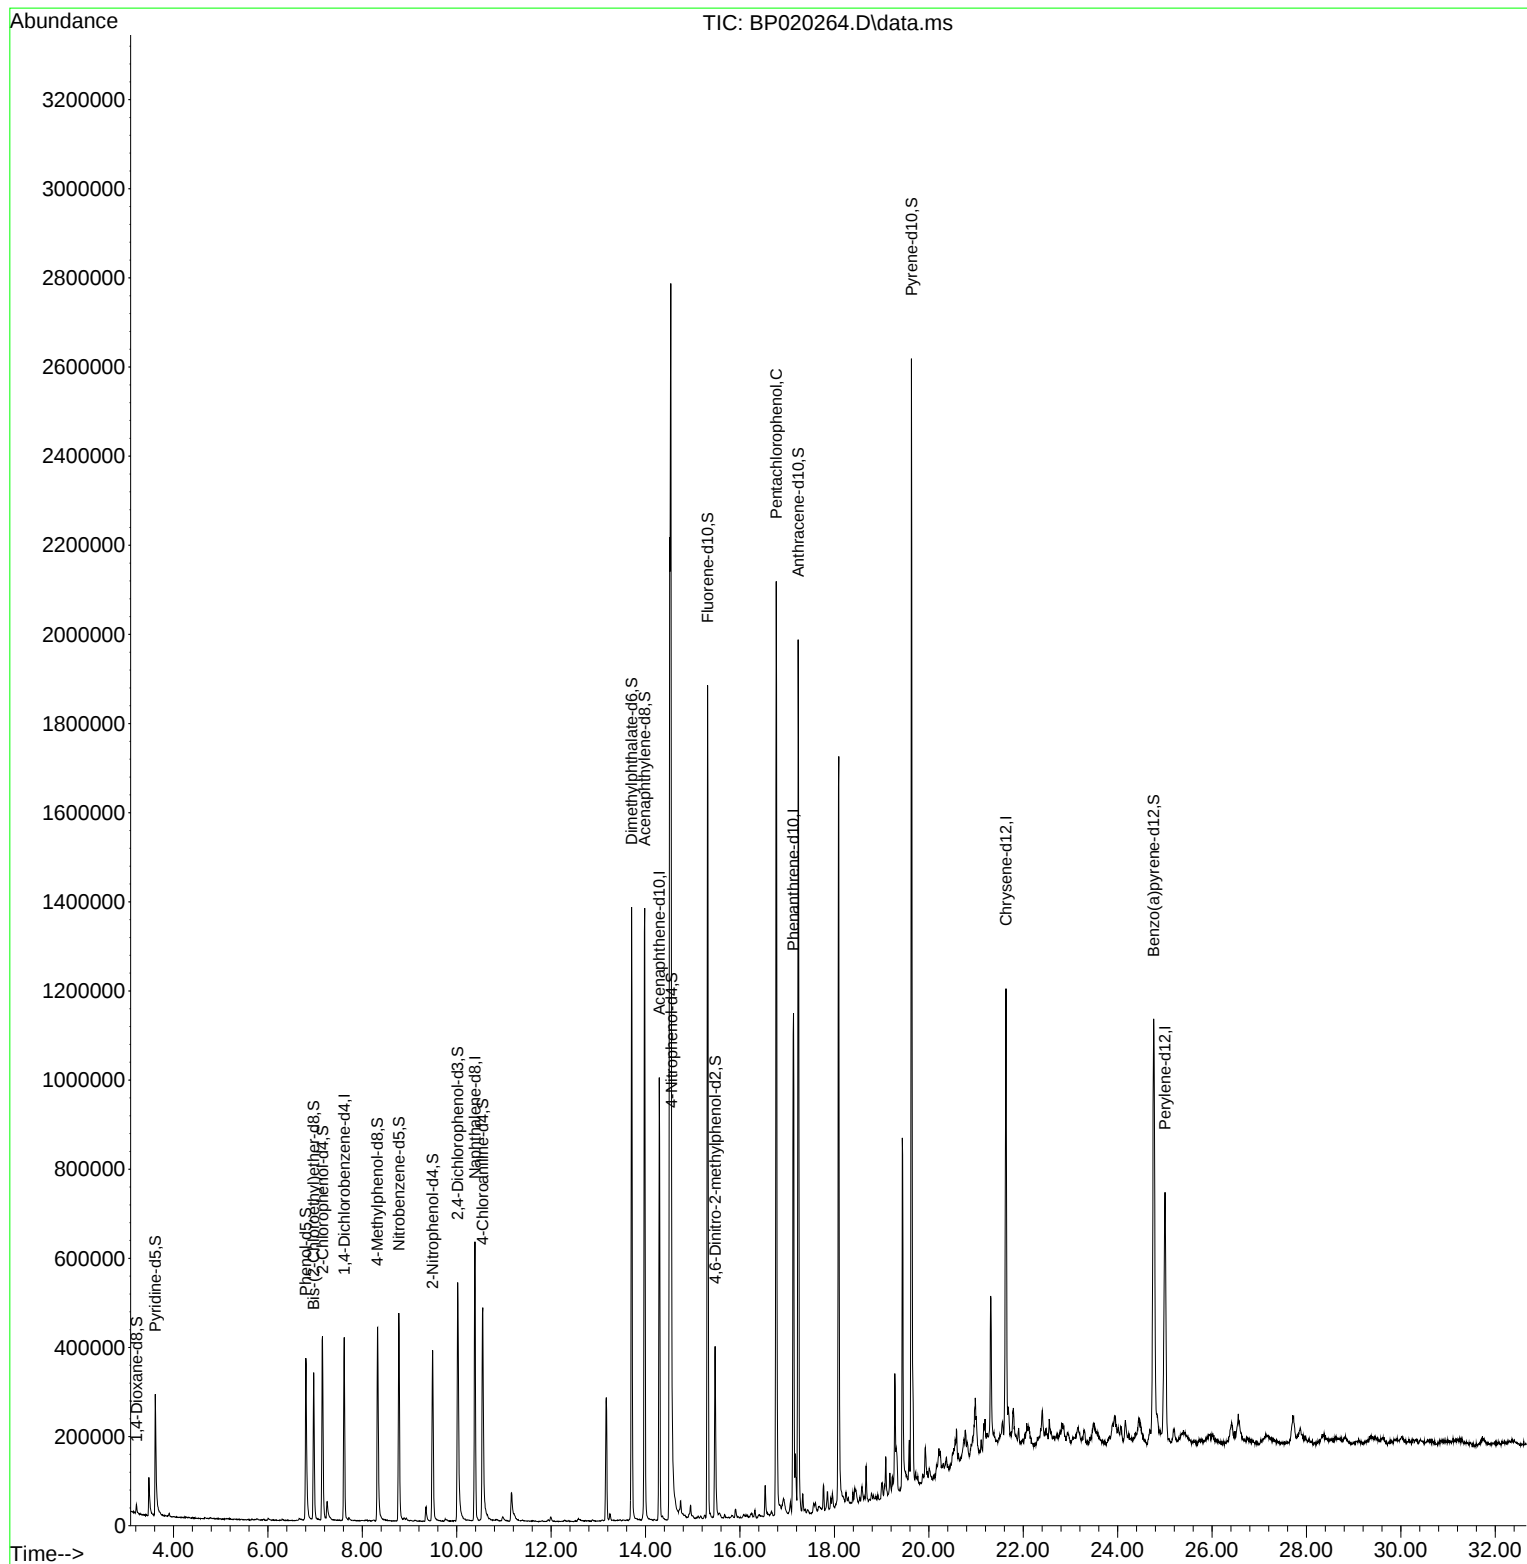

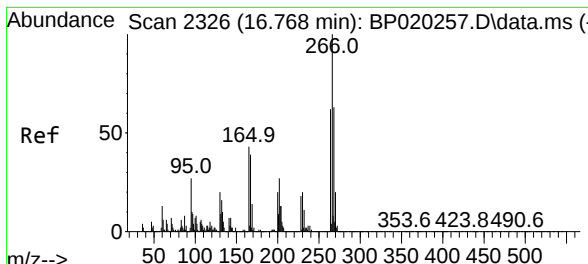

#71
 Pentachlorophenol
 Concen: 69.186 ng/ul
 RT: 16.769 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP020264.D
 Acq: 09 May 2024 10:45

Instrument :
 BNA_P
 ClientSampleId :
 A43N2

Tgt Ion:	266	Resp:	405450
Ion	Ratio	Lower	Upper
266	100		
264	62.8	49.8	74.6
268	63.5	50.4	75.6

