

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
 Data File : BP020258.D
 Acq On : 09 May 2024 06:21
 Operator : MA/JU
 Sample : PB160727BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	30	rVB	17093	28985	1.06%	0.105%
2	3.617	87	90	111	rBV	227521	484945	17.68%	1.758%
3	3.911	135	140	144	rBV5	7655	12539	0.46%	0.045%
4	6.805	624	632	650	rBV	306603	640702	23.36%	2.322%
5	6.975	655	661	677	rVB	260300	456540	16.65%	1.655%
6	7.158	685	692	707	rBV	325838	627812	22.89%	2.276%
7	7.616	763	770	782	rBV	340320	633787	23.11%	2.297%
8	8.328	885	891	915	rBV	423193	807344	29.44%	2.927%
9	8.781	960	968	984	rBV	338477	653663	23.83%	2.369%
10	9.493	1081	1089	1109	rBV	311481	575570	20.99%	2.086%
11	10.028	1173	1180	1199	rBV	360719	833563	30.39%	3.022%
12	10.387	1234	1241	1252	rBV	506313	925804	33.75%	3.356%
13	10.552	1261	1269	1304	rBV	389842	924089	33.69%	3.350%
14	12.022	1512	1519	1523	rBV3	4799	11413	0.42%	0.041%
15	13.704	1798	1805	1825	rBV	816888	1397723	50.96%	5.067%
16	13.975	1842	1851	1868	rBV	989615	1565338	57.07%	5.674%
17	14.287	1897	1904	1916	rBV	861479	1346220	49.08%	4.880%
18	14.557	1944	1950	1973	rBV	181033	619507	22.59%	2.246%
19	15.304	2070	2077	2096	rBV	1240858	1996382	72.79%	7.237%
20	15.475	2099	2106	2118	rBV	239814	456645	16.65%	1.655%
21	15.563	2118	2121	2129	rVB7	8959	18410	0.67%	0.067%
22	16.128	2212	2217	2223	rBV9	2866	5618	0.20%	0.020%
23	16.804	2327	2332	2340	rVB9	3858	8852	0.32%	0.032%
24	16.910	2345	2350	2355	rBV8	3417	7644	0.28%	0.028%
25	17.128	2380	2387	2398	rBV	1102904	1686645	61.49%	6.114%
26	17.234	2398	2405	2423	rVB	1516214	2320022	84.59%	8.410%
27	18.110	2550	2554	2558	rBV6	4082	6965	0.25%	0.025%
28	19.186	2732	2737	2742	rBV3	22445	37770	1.38%	0.137%
29	19.263	2746	2750	2755	rBV	15561	23402	0.85%	0.085%
30	19.633	2807	2813	2826	rBV	1826930	2742746	100.00%	9.942%
31	21.627	3145	3152	3163	rBV	956824	1776691	64.78%	6.440%
32	24.763	3676	3685	3701	rVB2	881411	2368191	86.34%	8.584%
33	24.986	3713	3723	3737	rVB	502317	1585577	57.81%	5.748%




Sum of corrected areas: 27587104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020258.D
Acq On : 09 May 2024 06:21
Operator : MA/JU
Sample : PB160727BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

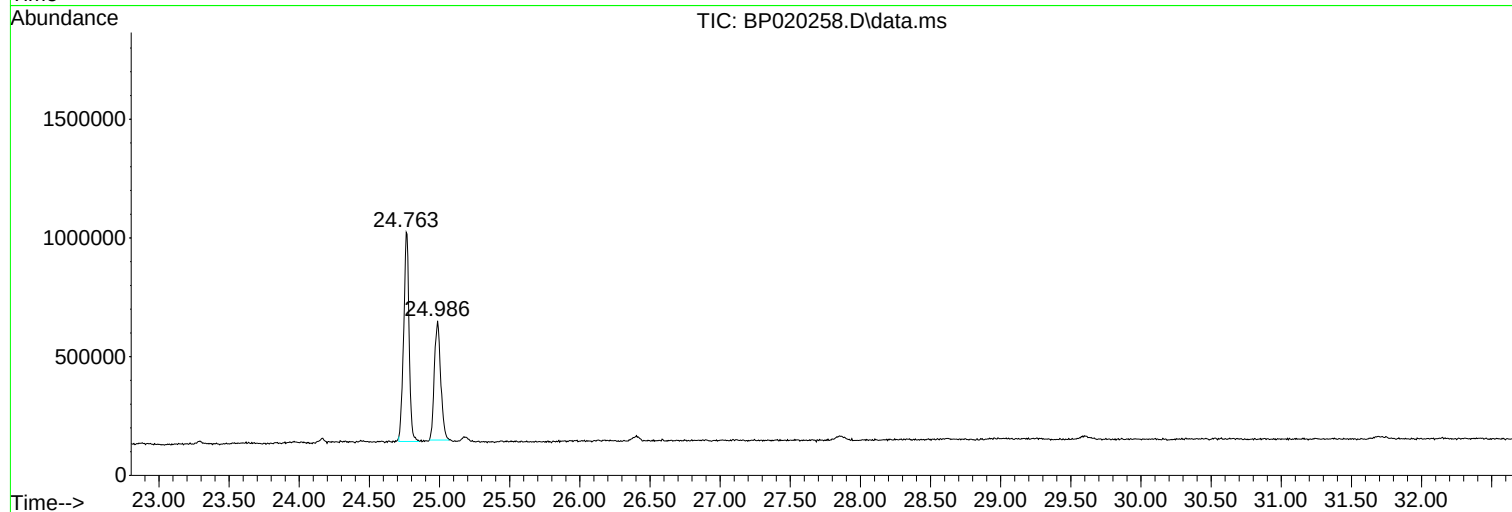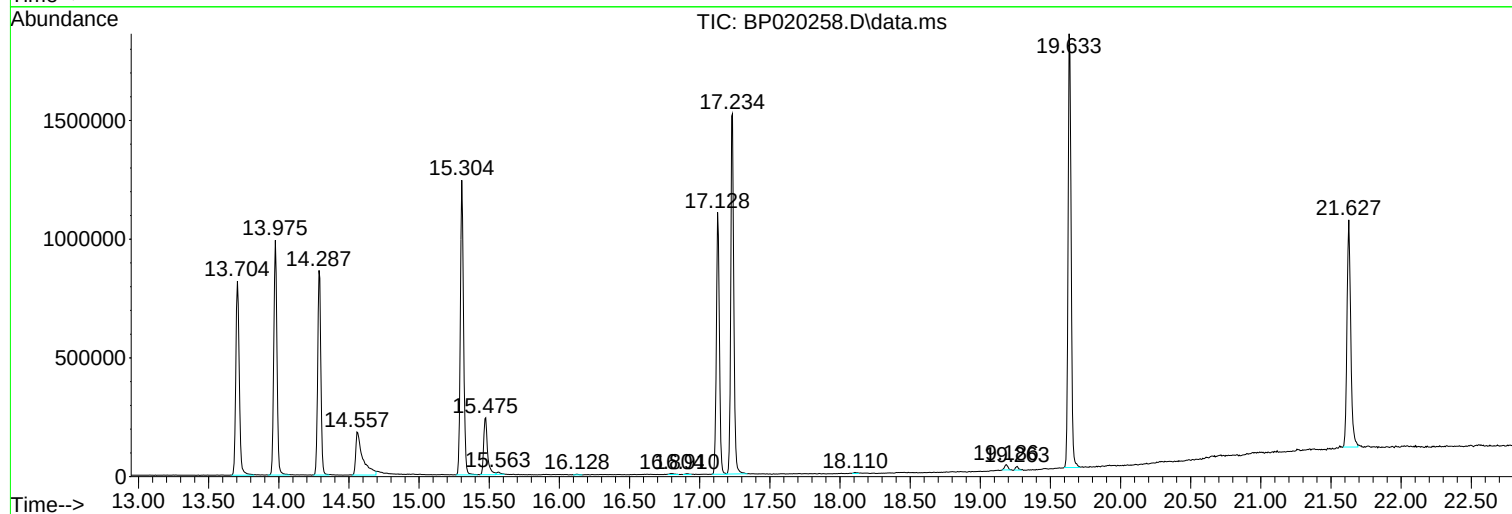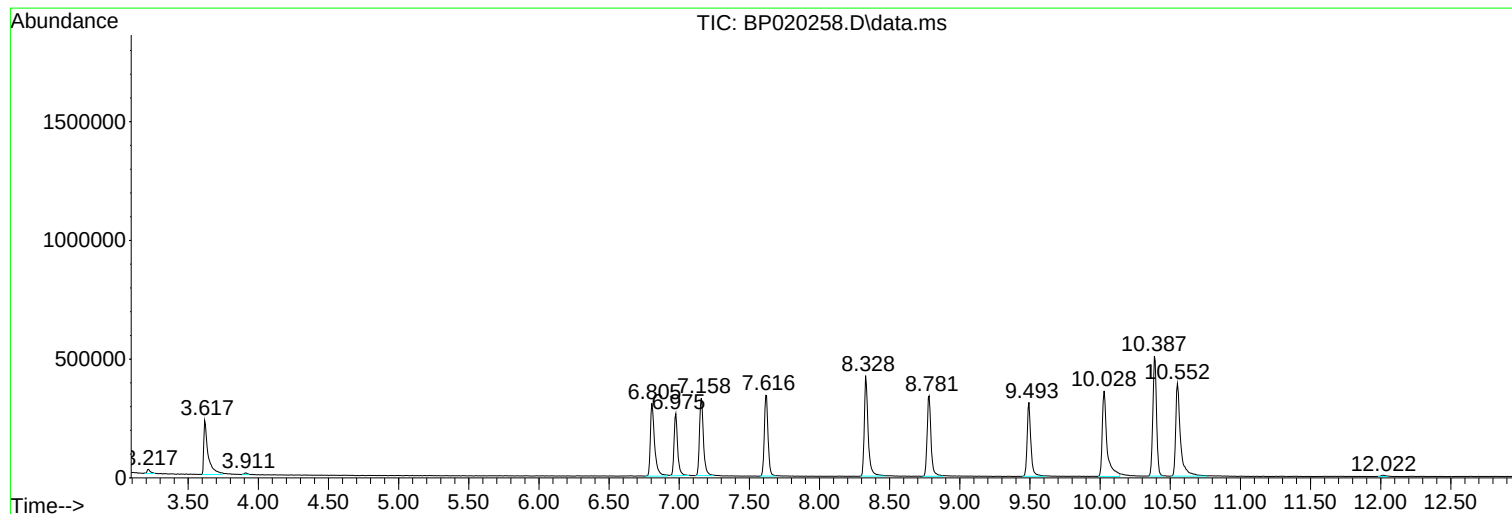

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020258.D
Acq On : 09 May 2024 06:21
Operator : MA/JU
Sample : PB160727BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020258.D
Acq On : 09 May 2024 06:21
Operator : MA/JU
Sample : PB160727BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc