

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
 Data File : BP020267.D
 Acq On : 09 May 2024 12:57
 Operator : MA/JU
 Sample : P2369-15DL 30X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43N9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.911	137	140	144	rBV5	4742	6024	0.13%	0.048%
2	6.881	636	645	646	rBV8	3237	5938	0.13%	0.047%
3	6.999	660	665	668	rBV7	3337	6790	0.15%	0.054%
4	7.187	691	697	705	rBV10	5338	14444	0.31%	0.115%
5	7.293	709	715	720	rVV9	2526	5151	0.11%	0.041%
6	7.622	763	771	788	rBV	275131	539935	11.71%	4.284%
7	8.816	969	974	976	rBV6	3522	5428	0.12%	0.043%
8	8.881	981	985	989	rBV7	4325	7851	0.17%	0.062%
9	9.375	1064	1069	1075	rBV7	3990	7589	0.16%	0.060%
10	9.516	1087	1093	1095	rBV7	3591	6459	0.14%	0.051%
11	10.134	1190	1198	1199	rBV7	3571	6567	0.14%	0.052%
12	10.393	1234	1242	1263	rBV	396872	801300	17.38%	6.357%
13	13.234	1720	1725	1730	rBV9	2826	4778	0.10%	0.038%
14	13.445	1756	1761	1766	rVB4	10155	14760	0.32%	0.117%
15	13.510	1768	1772	1776	rBV5	4317	5995	0.13%	0.048%
16	13.598	1783	1787	1789	rBV5	3996	5535	0.12%	0.044%
17	13.722	1801	1808	1814	rBV2	20494	43442	0.94%	0.345%
18	13.904	1835	1839	1841	rBV4	12178	18103	0.39%	0.144%
19	13.934	1841	1844	1847	rVV4	15385	21630	0.47%	0.172%
20	13.981	1847	1852	1857	rVV	27029	47403	1.03%	0.376%
21	14.039	1857	1862	1867	rVV3	19478	39470	0.86%	0.313%
22	14.110	1867	1874	1885	rVB6	14182	42071	0.91%	0.334%
23	14.234	1891	1895	1897	rBV4	4388	5496	0.12%	0.044%
24	14.287	1897	1904	1912	rVV	675395	1187565	25.75%	9.421%
25	14.357	1912	1916	1919	rVV2	29765	49053	1.06%	0.389%
26	14.392	1919	1922	1928	rVV5	11044	16719	0.36%	0.133%
27	14.445	1928	1931	1936	rVB6	7048	10231	0.22%	0.081%
28	14.522	1936	1944	1949	rBV3	37265	76223	1.65%	0.605%
29	14.581	1952	1954	1956	rVV3	6699	6577	0.14%	0.052%
30	14.616	1956	1960	1969	rVB10	6473	12863	0.28%	0.102%
31	14.692	1969	1973	1978	rVB7	5372	8626	0.19%	0.068%
32	14.739	1978	1981	1985	rBV5	3304	5636	0.12%	0.045%
33	14.839	1993	1998	1999	rBV5	3067	4645	0.10%	0.037%
34	14.875	1999	2004	2011	rVV7	15233	30493	0.66%	0.242%
35	14.957	2012	2018	2029	rVV3	51980	104370	2.26%	0.828%
36	15.069	2032	2037	2043	rVV6	5768	11310	0.25%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
 Data File : BP020267.D
 Acq On : 09 May 2024 12:57
 Operator : MA/JU
 Sample : P2369-15DL 30X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43N9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

37	15.139	2046	2049	2056	rVB3	9503	13760	0.30%	0.109%
38	15.322	2074	2080	2089	rVB2	33089	61361	1.33%	0.487%
39	15.486	2104	2108	2109	rBV4	5127	5305	0.12%	0.042%
40	15.686	2140	2142	2153	rVB10	3941	8876	0.19%	0.070%
41	15.781	2155	2158	2164	rBV8	3344	5228	0.11%	0.041%
42	15.998	2191	2195	2199	rBV7	3221	5176	0.11%	0.041%
43	16.286	2240	2244	2248	rBV7	5324	7270	0.16%	0.058%
44	16.381	2256	2260	2267	rVB9	5644	11226	0.24%	0.089%
45	16.463	2271	2274	2279	rVB7	4318	8321	0.18%	0.066%
46	16.604	2295	2298	2304	rBV7	4121	7298	0.16%	0.058%
47	16.751	2316	2323	2347	rBV	2561592	4611104	100.00%	36.582%
48	17.116	2378	2385	2399	rBV	929635	1548587	33.58%	12.286%
49	17.228	2399	2404	2414	rVB2	36614	70440	1.53%	0.559%
50	17.551	2457	2459	2461	rBV2	4916	4767	0.10%	0.038%
51	18.080	2545	2549	2555	rVB9	9503	18195	0.39%	0.144%
52	19.633	2809	2813	2820	rBV2	49393	80415	1.74%	0.638%
53	21.627	3145	3152	3160	rBV	787644	1515664	32.87%	12.024%
54	24.992	3715	3724	3739	rVB	503708	1435404	31.13%	11.388%




Sum of corrected areas: 12604867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020267.D
Acq On : 09 May 2024 12:57
Operator : MA/JU
Sample : P2369-15DL 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43N9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

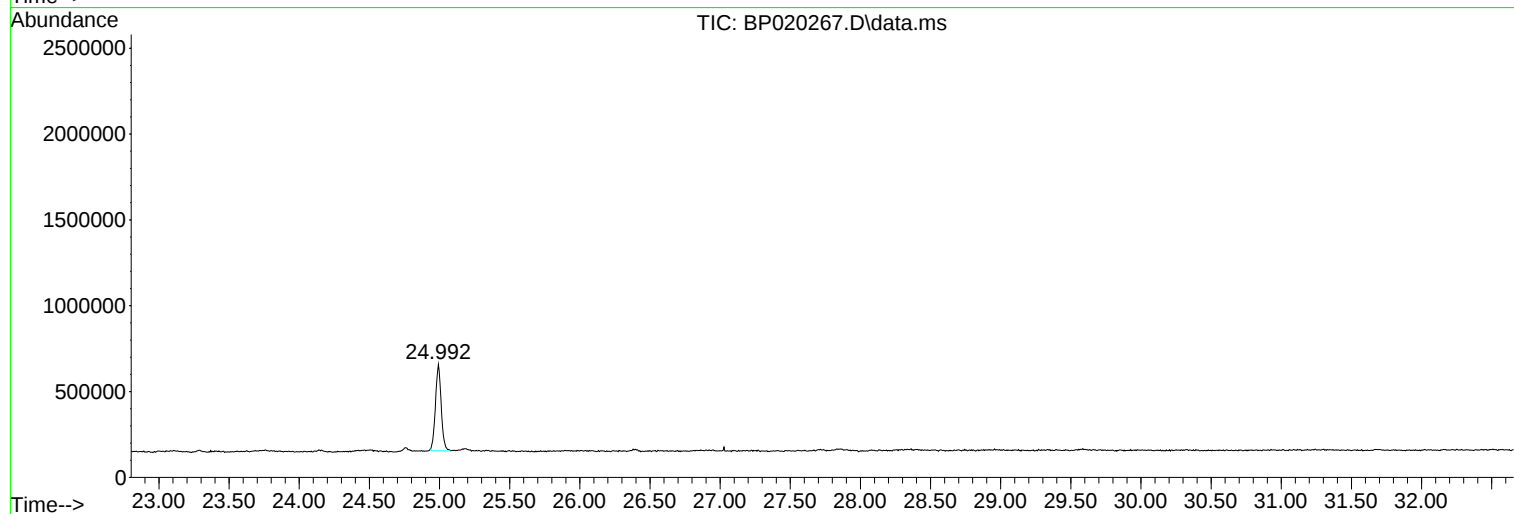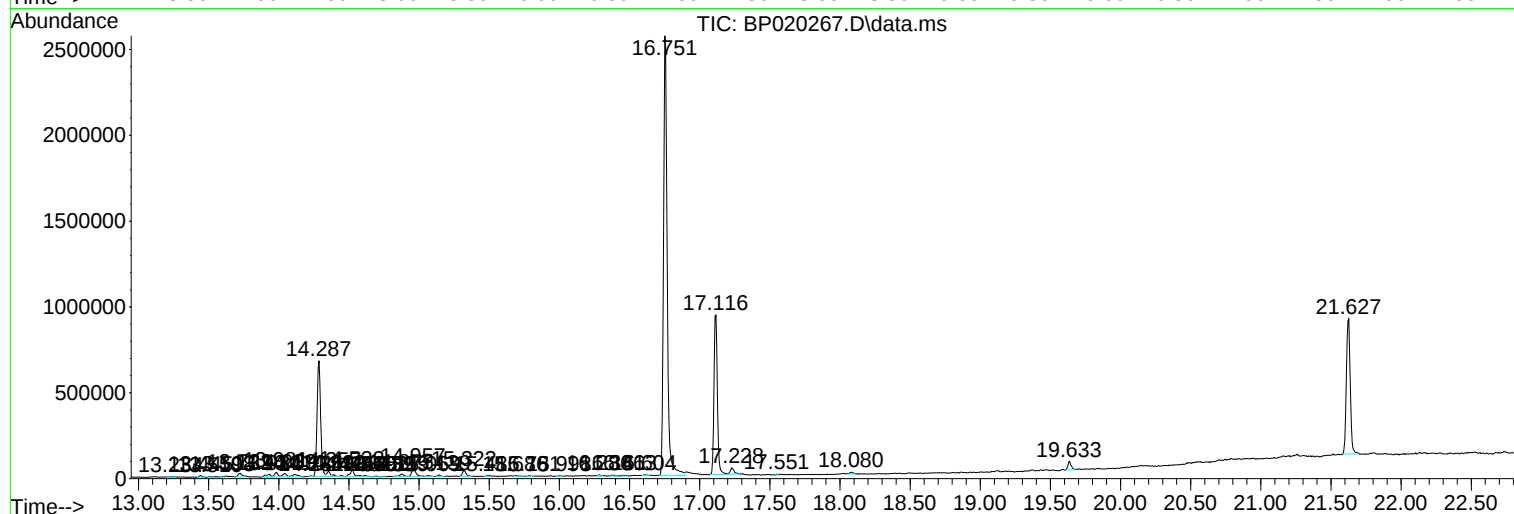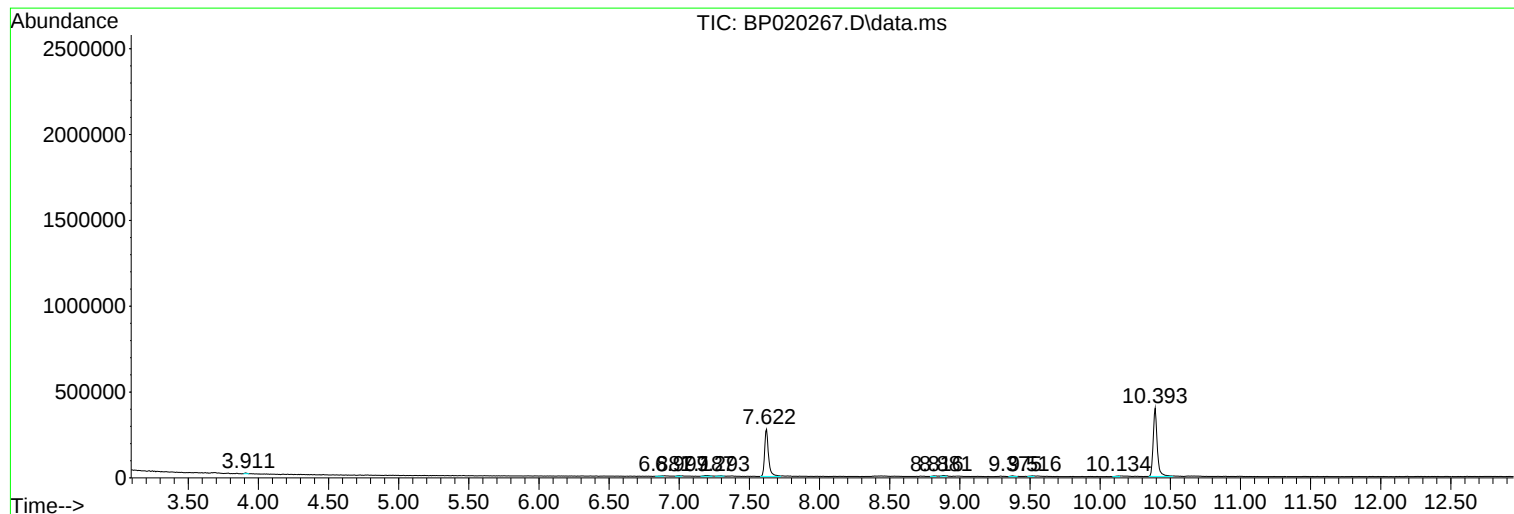

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020267.D
Acq On : 09 May 2024 12:57
Operator : MA/JU
Sample : P2369-15DL 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43N9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050824\
Data File : BP020267.D
Acq On : 09 May 2024 12:57
Operator : MA/JU
Sample : P2369-15DL 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43N9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc