

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG051220\
 Data File : BG045356.D
 Acq On : 13 May 2020 11:00
 Operator : CG/JU
 Sample : PB128795TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB128795TB

Quant Time: May 13 11:44:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 13 11:40:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	63776	20.00	ng	0.00
21) Naphthalene-d8	10.78	136	257284	20.00	ng	0.00
39) Acenaphthene-d10	14.61	164	176079	20.00	ng	0.00
64) Phenanthrene-d10	17.36	188	429771	20.00	ng	0.00
76) Chrysene-d12	21.62	240	467540	20.00	ng	0.00
87) Perylene-d12	24.78	264	496502	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.54	112	398476	103.15	ng	0.00
7) Phenol-d6	7.14	99	568274	99.01	ng	0.00
23) Nitrobenzene-d5	9.13	82	395577	70.15	ng	0.00
42) 2,4,6-Tribromophenol	16.11	330	296693	109.07	ng	0.00
45) 2-Fluorobiphenyl	13.23	172	886517	73.83	ng	0.00
79) Terphenyl-d14	19.98	244	1726219	80.47	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	7.13	77	982	Below Cal	#	4
19) n-Nitroso-di-n-propylamine	9.13	70	51062	12.580	ng	# 80
51) 2,6-Dinitrotoluene	14.61	165	23545	7.342	ng	# 25
57) 2,4-Dinitrotoluene	14.61	165	23545	5.024	ng	# 22
67) 4-Bromophenyl-phenylether	16.11	248	19871	3.584	ng	# 1
74) Di-n-butylphthalate	18.32	149	442	Below Cal	#	76
75) Fluoranthene	19.27	202	59	Below Cal	#	62
77) Benzydine	19.97	184	32297	Below Cal	#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG051220\
Data File : BG045356.D
Acq On : 13 May 2020 11:00
Operator : CG/JU
Sample : PB128795TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB128795TB

Quant Time: May 13 11:44:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG041520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 11:40:01 2020
Response via : Initial Calibration

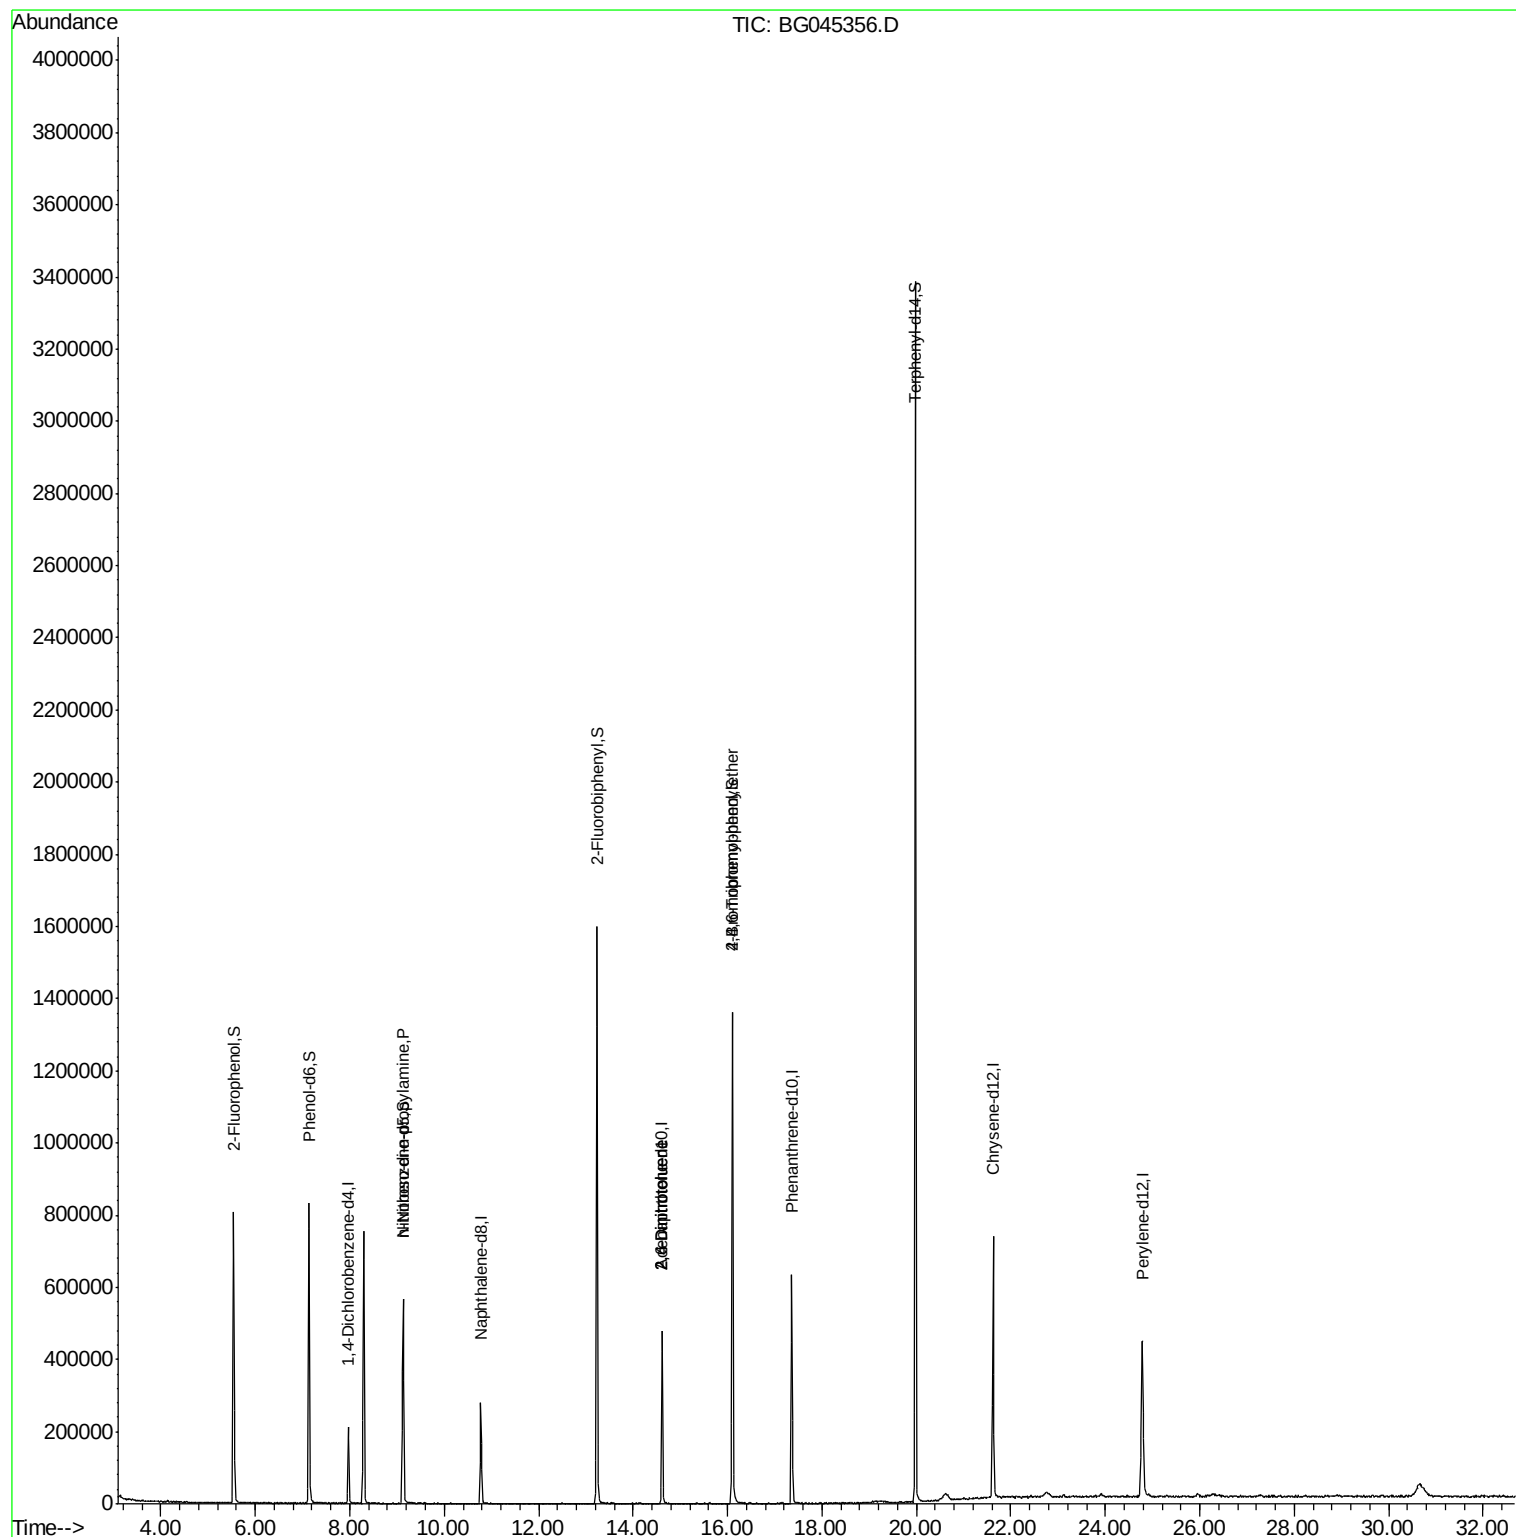

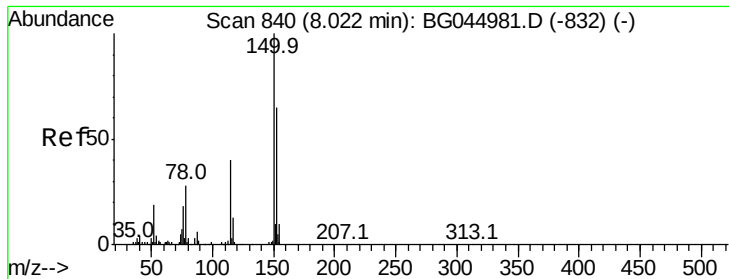


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.97 min Scan# 831
 Delta R.T. -0.00 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00

Instrument :
 BNA_P
 ClientSampleId :
 PB128795TB

Tot Ion:152 Resp: 63776
 Ion Ratio Lower Upper
 152 100
 150 162.8 123.6 185.4
 115 62.5 49.1 73.7

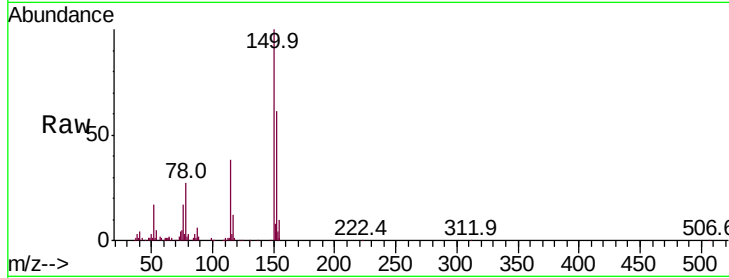


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

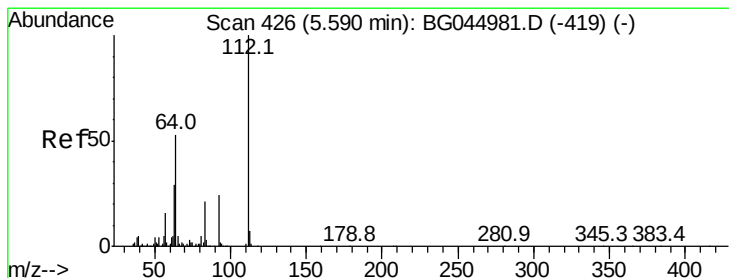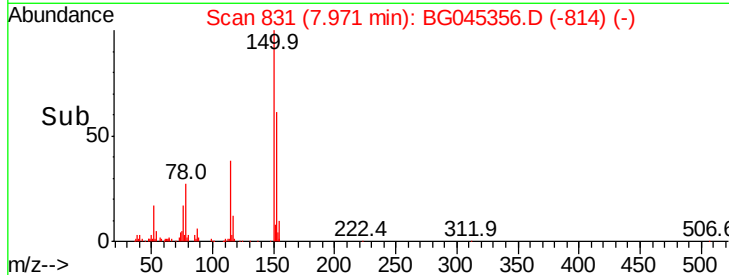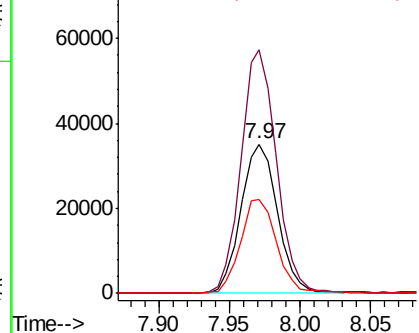



#5


2-Fluorophenol
 Concen: 103.152 ng
 RT: 5.54 min Scan# 417
 Delta R.T. -0.00 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00

Tgt Ion:112 Resp: 398476
 Ion Ratio Lower Upper
 112 100
 64 58.4 42.4 63.6
 63 31.7 23.1 34.7

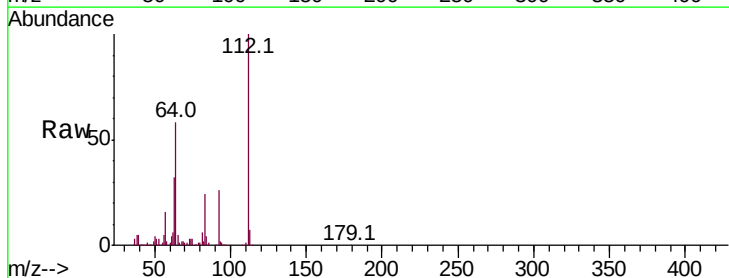

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG0
 Ion 63.00 (62.70 to 63.70): BG0

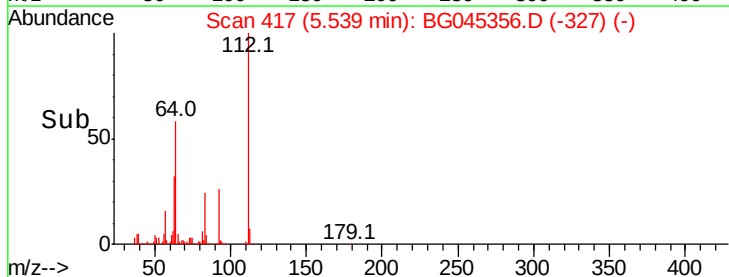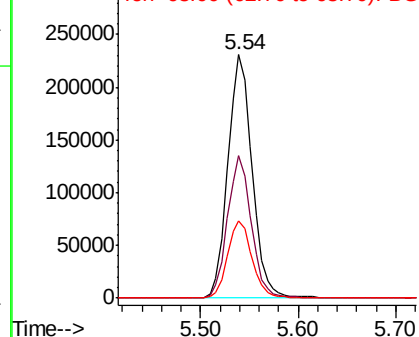

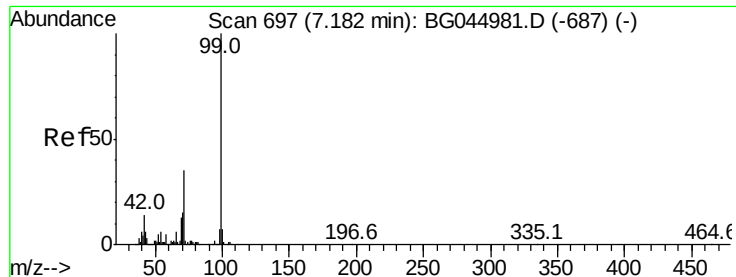

#7

Phenol-d6

Concen: 99.012 ng

RT: 7.14 min Scan# 689

Delta R.T. -0.00 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00

Instrument :

BNA_P

ClientSampleId :

PB128795TB





Tot Ion: 99 Resp: 568274

Ion Ratio Lower Upper

99 100

42 12.3 11.3 16.9

71 35.1 28.3 42.5

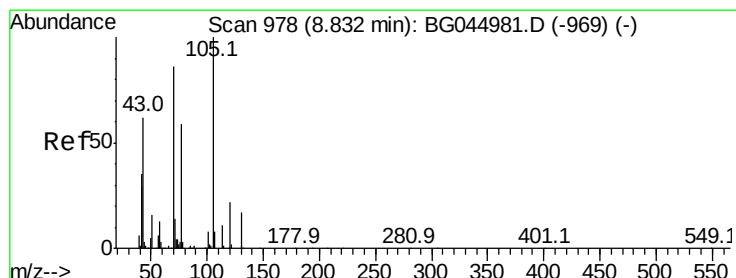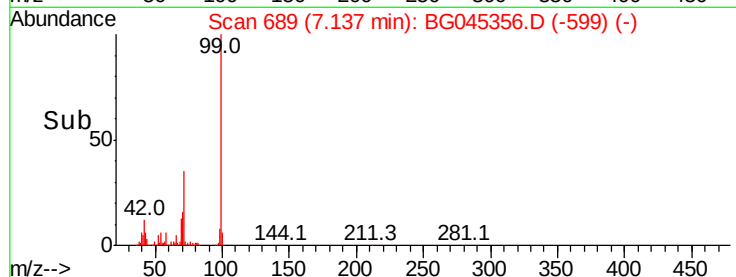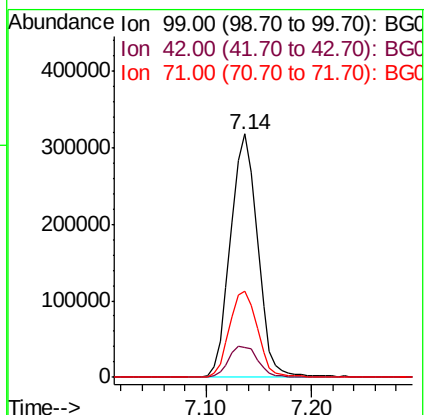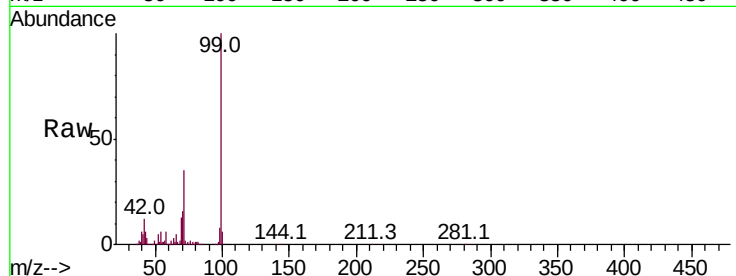

#19

n-Nitroso-di-n-propylamine

Concen: 12.580 ng

RT: 9.13 min Scan# 1028

Delta R.T. 0.35 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00

Tgt Ion: 70 Resp: 51062




Ion Ratio Lower Upper


70 100

42 35.4 33.3 49.9

101 0.0 7.8 11.8#

130 2.4 15.8 23.6#


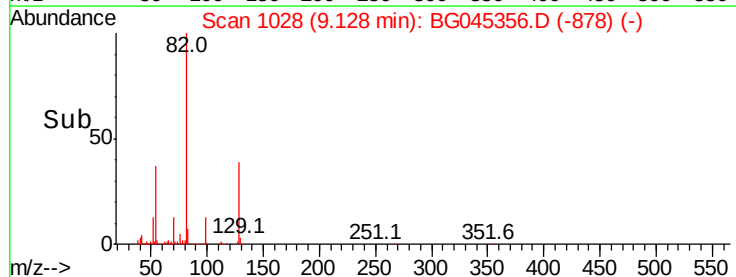
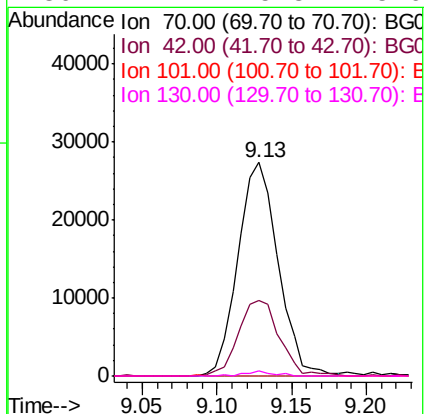
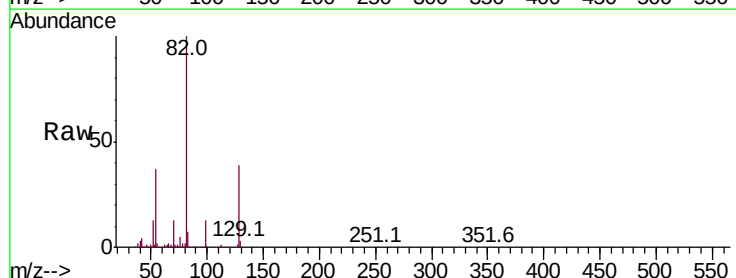


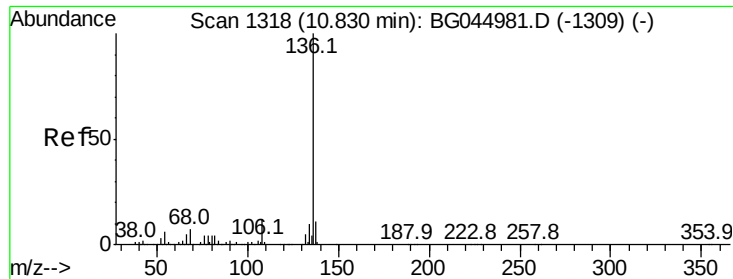

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.78 min Scan# 1309
Delta R.T. -0.00 min
Lab File: BG045356.D
Acq: 13 May 2020 11:00




Instrument :
BNA_P
ClientSampleId :
PB128795TB


Tot Ion:136	Resp:	257284
Ion Ratio	Lower	Upper
136 100		
137 10.2	8.6	13.0
54 6.4	4.8	7.2
68 5.6	5.2	7.8

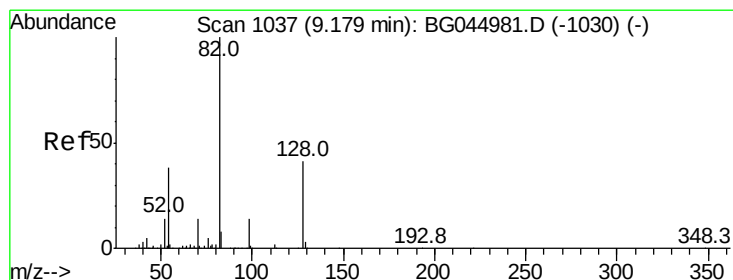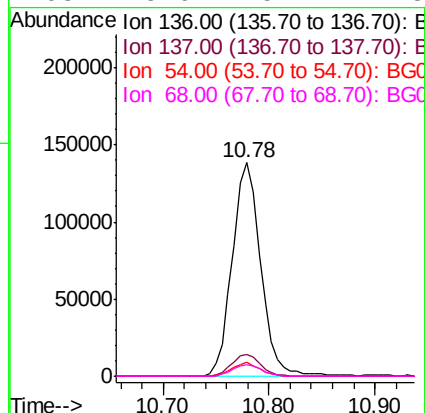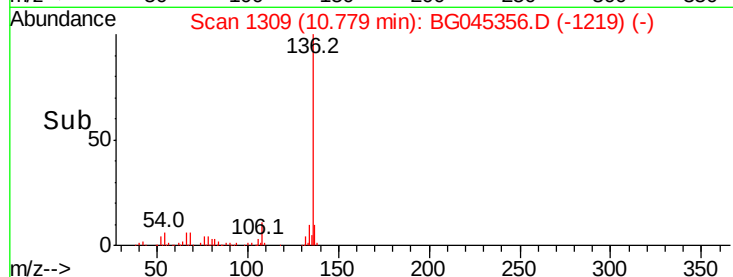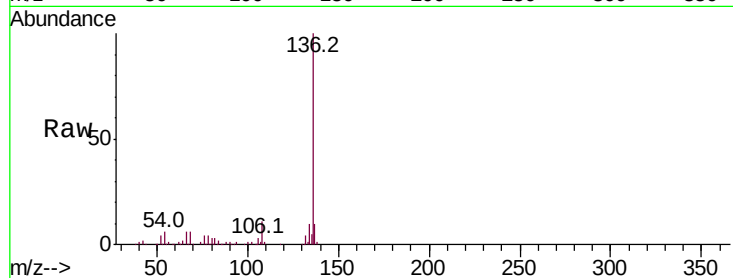

#23
Nitrobenzene-d5
Concen: 70.155 ng
RT: 9.13 min Scan# 1028
Delta R.T. -0.00 min
Lab File: BG045356.D
Acq: 13 May 2020 11:00

Tgt Ion: 82	Resp: 395577
Ion Ratio	Lower Upper
82 100	
128 39.5	33.0 49.4
54 37.4	30.4 45.6

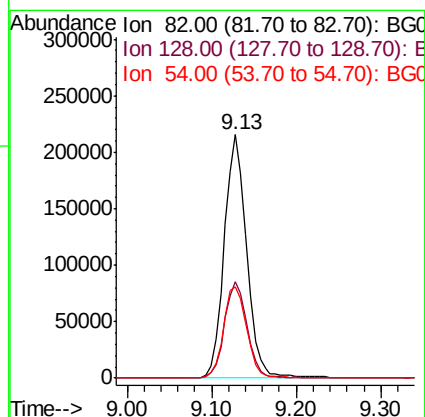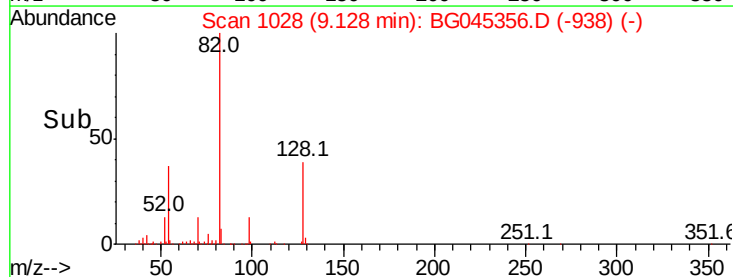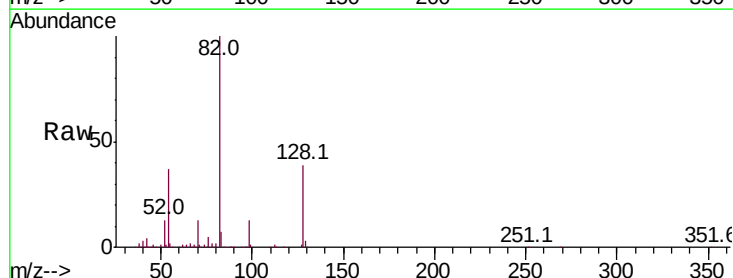

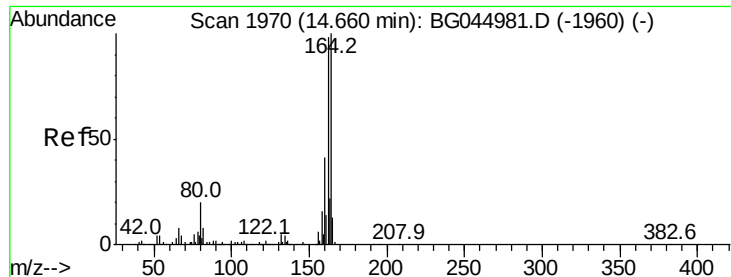

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.61 min Scan# 1962

Delta R.T. -0.00 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00

Instrument :

BNA_P

ClientSampleId :

PB128795TB


Tot Ion:164 Resp: 176079

Ion	Ratio	Lower	Upper
164	100		
162	99.2	78.7	118.1
160	42.3	32.8	49.2

164 100

162 99.2 78.7 118.1

160 42.3 32.8 49.2



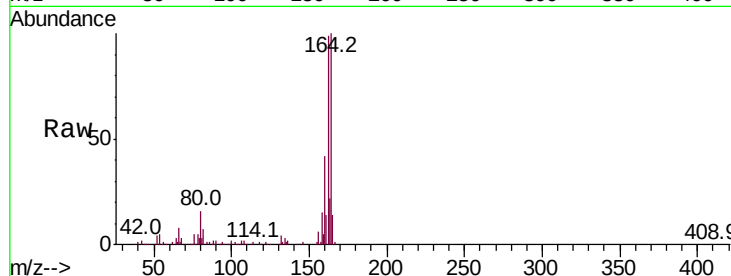


Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

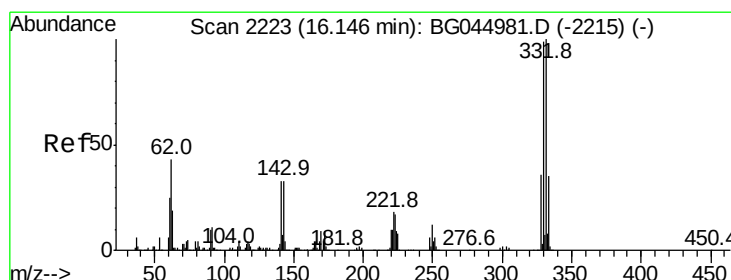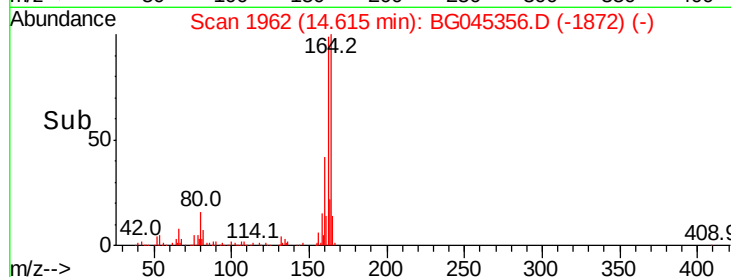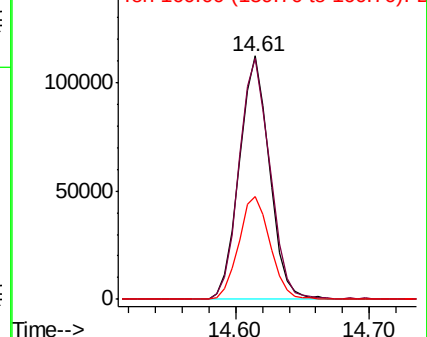

#42

2,4,6-Tribromophenol

Concen: 109.071 ng

RT: 16.11 min Scan# 2216

Delta R.T. -0.00 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00


Tgt Ion:330 Resp: 296693

Ion	Ratio	Lower	Upper
330	100		
332	96.4	79.1	118.7
141	34.8	27.1	40.7

330 100

332 96.4 79.1 118.7

141 34.8 27.1 40.7


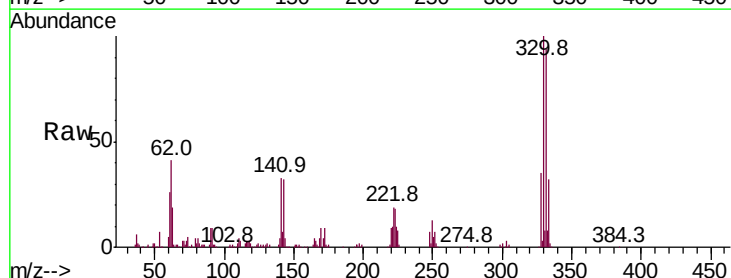



Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



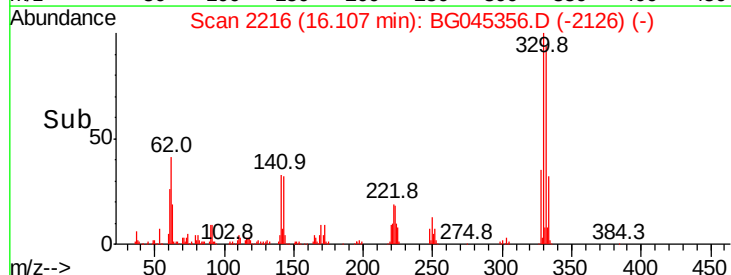
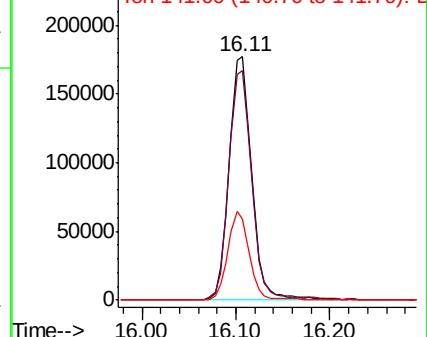


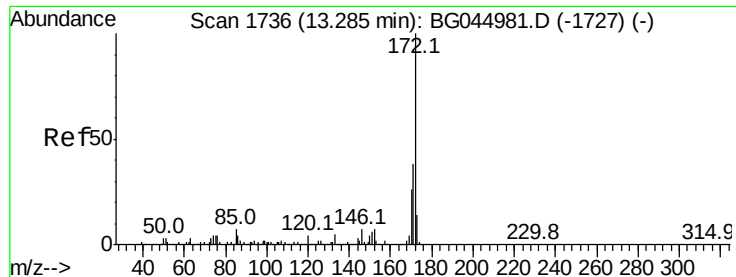

#45
 2-Fluorobiphenyl
 Concen: 73.826 ng
 RT: 13.23 min Scan# 1727
 Delta R.T. -0.00 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00




Instrument :
 BNA_P
 ClientSampleId :
 PB128795TB


Tot Ion:	172	Resp:	886517
Ion	Ratio	Lower	Upper
172	100		
171	36.9	30.6	46.0
170	23.8	20.5	30.7

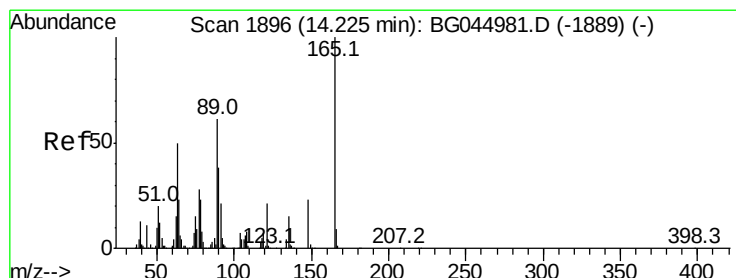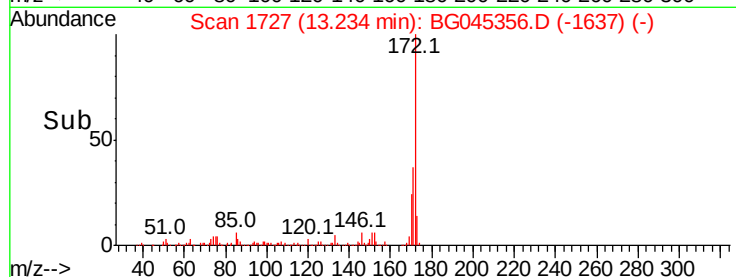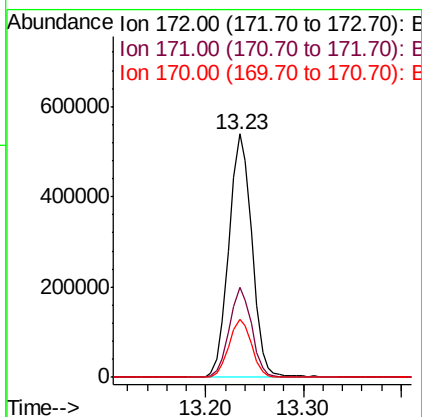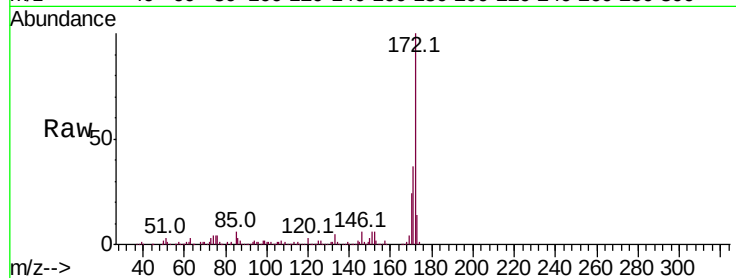

#51
 2,6-Dinitrotoluene
 Concen: 7.342 ng
 RT: 14.61 min Scan# 1962
 Delta R.T. 0.43 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00

Tgt Ion:	165	Resp:	23545
Ion	Ratio	Lower	Upper
165	100		
63	0.0	40.4	60.6#
89	2.0	49.1	73.7#


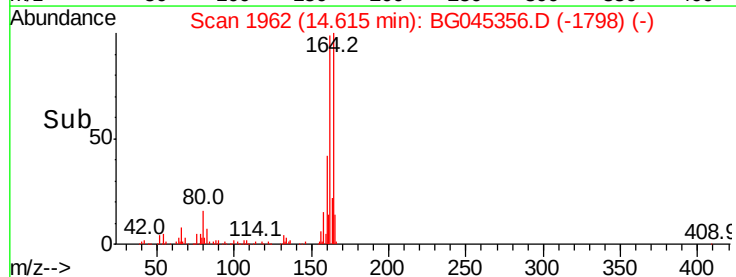
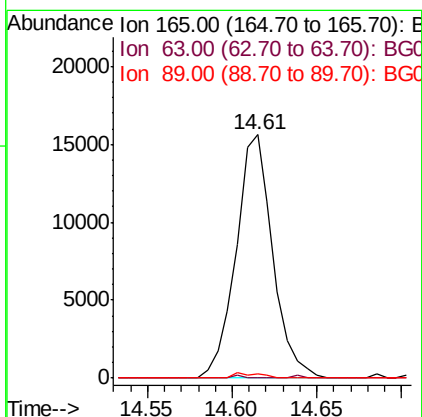
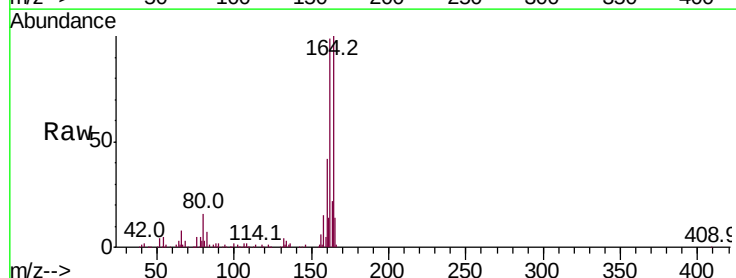


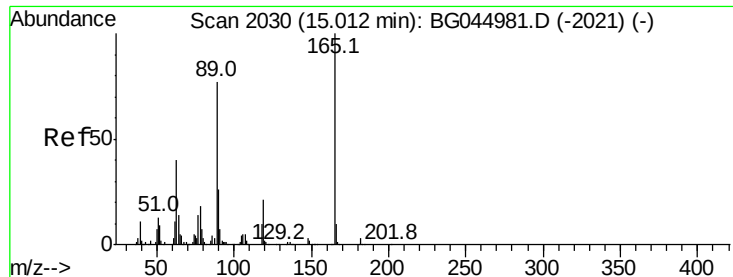

#57
 2,4-Dinitrotoluene
 Concen: 5.024 ng
 RT: 14.61 min Scan# 1962
 Delta R.T. -0.36 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00




Instrument :
 BNA_P
 ClientSampleId :
 PB128795TB


Tot Ion:165 Resp: 23545
 Ion Ratio Lower Upper
 165 100
 63 0.0 32.2 48.2#
 89 2.0 61.7 92.5#
 182 0.0 2.0 3.0#

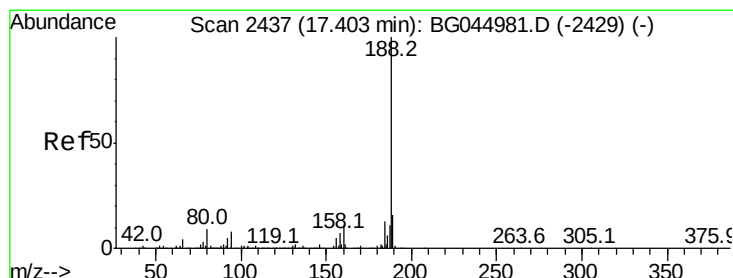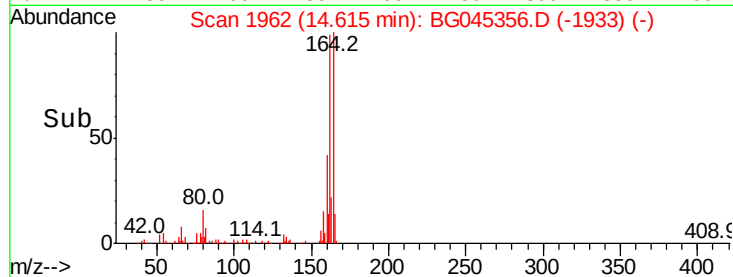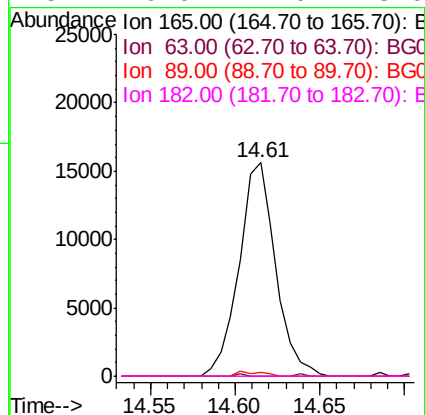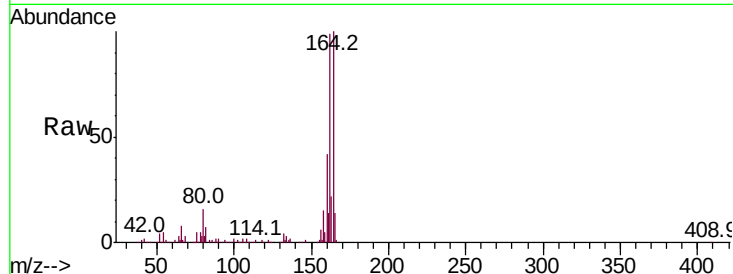

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.36 min Scan# 2429
 Delta R.T. -0.01 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00

Tgt Ion:188 Resp: 429771
 Ion Ratio Lower Upper
 188 100
 94 7.9 6.2 9.4
 80 7.6 7.0 10.6

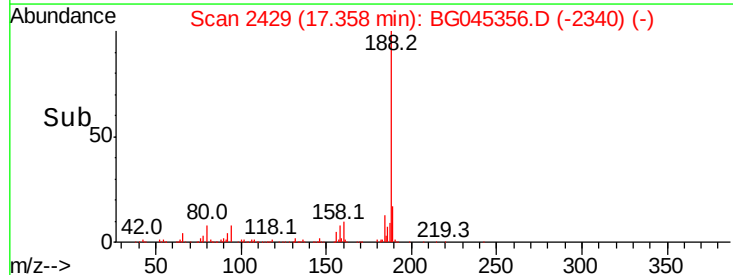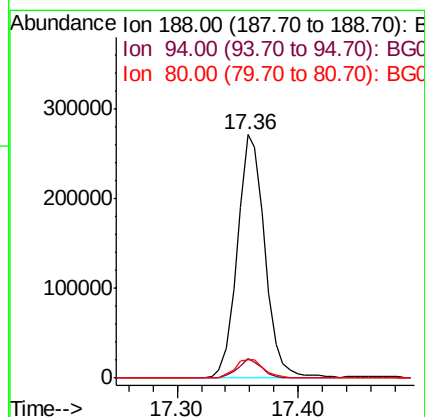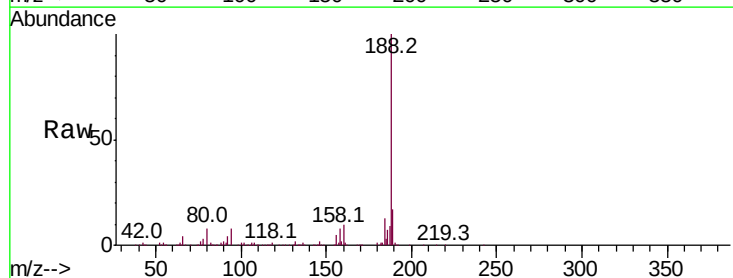


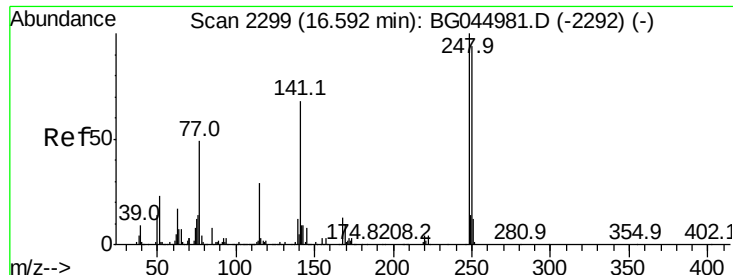




#67
 4-Bromophenyl-phenylether
 Concen: 3.584 ng
 RT: 16.11 min Scan# 2216
 Delta R.T. -0.45 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00

Instrument :
 BNA_P
 ClientSampleId :
 PB128795TB

Tot Ion:248 Resp: 19871
 Ion Ratio Lower Upper
 248 100
 250 182.7 75.4 113.2#
 141 470.3 54.4 81.6#

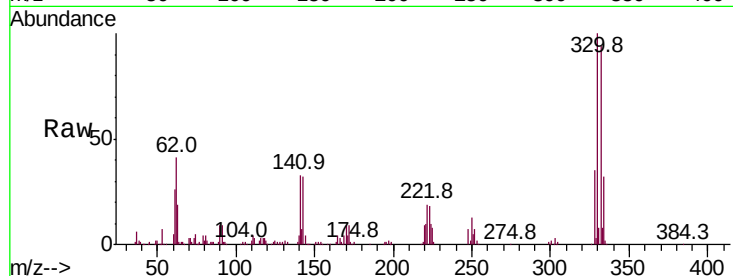


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

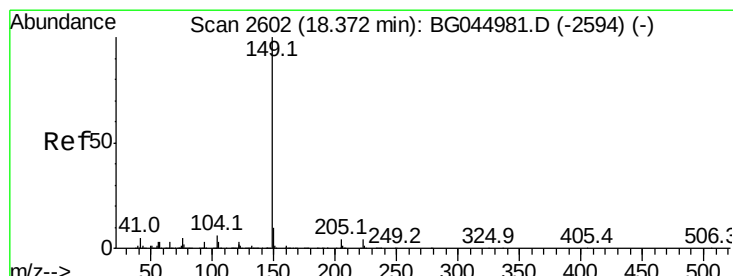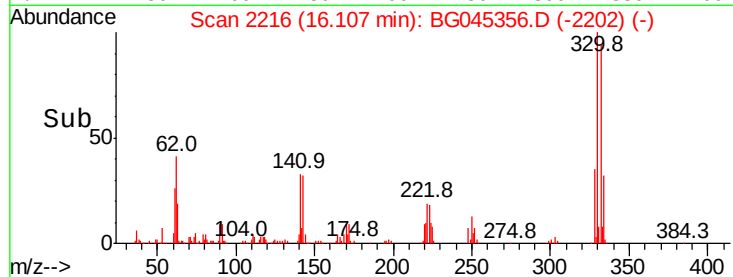
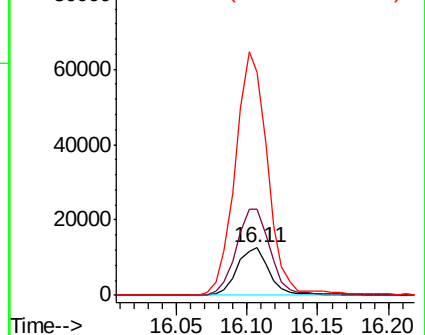



#74
 Di-n-butylphthalate
 Concen: Below Cal
 RT: 18.32 min Scan# 2593
 Delta R.T. -0.01 min
 Lab File: BG045356.D
 Acq: 13 May 2020 11:00

Tgt Ion:149 Resp: 442
 Ion Ratio Lower Upper
 149 100
 150 0.0 8.2 12.2#
 104 0.0 4.8 7.2#

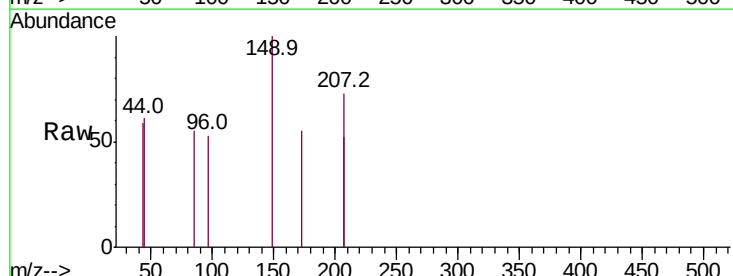

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 104.00 (103.70 to 104.70): E

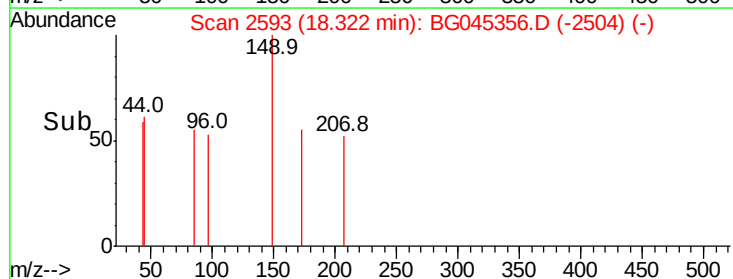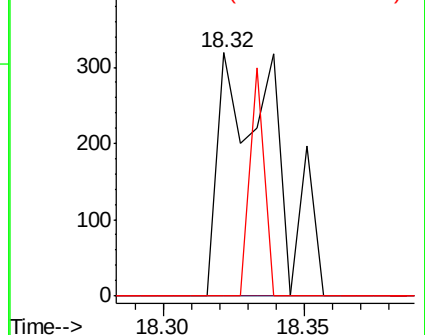

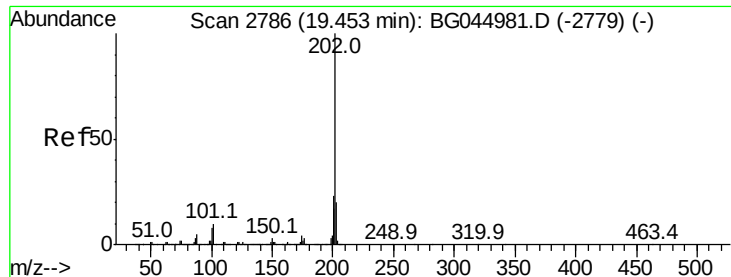

#75

Fluoranthene

Concen: Below Cal

RT: 19.27 min Scan# 2754

Delta R.T. -0.15 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00

Instrument :

BNA_P

ClientSampled :

PB128795TB


Tot Ion:202 Resp: 59

Ion Ratio Lower Upper

202 100

101 0.0 0.0 29.6




203 0.0 0.0 39.7

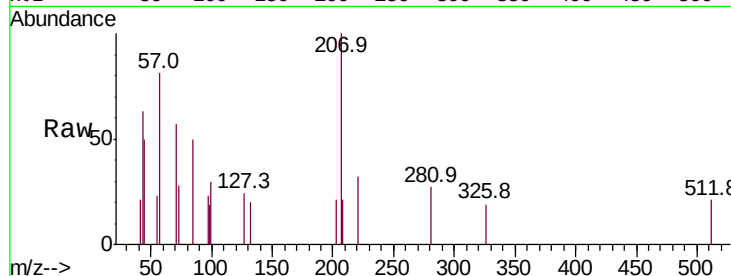

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

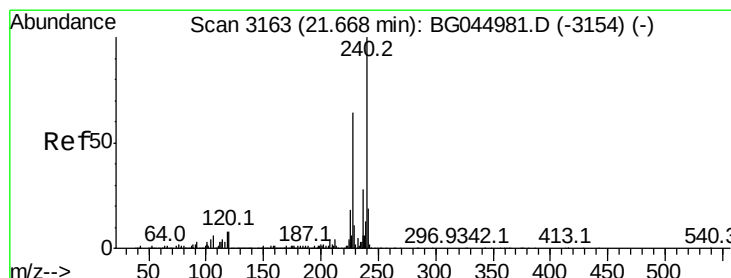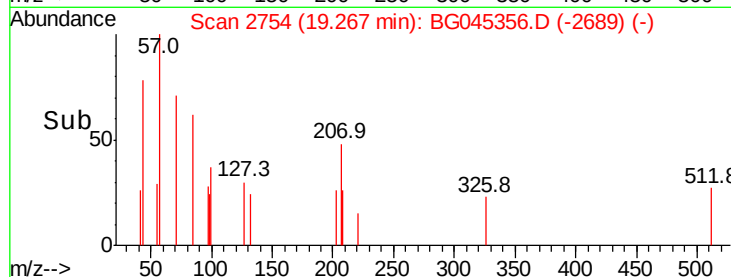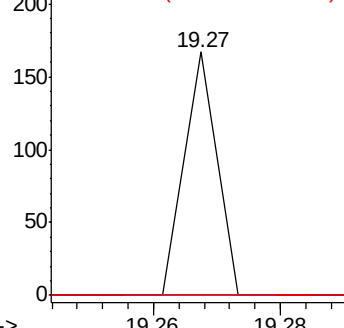

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.62 min Scan# 3155

Delta R.T. -0.00 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00


Tgt Ion:240 Resp: 467540

Ion Ratio Lower Upper

240 100

120 7.3 6.6 10.0



236 26.6 22.2 33.2

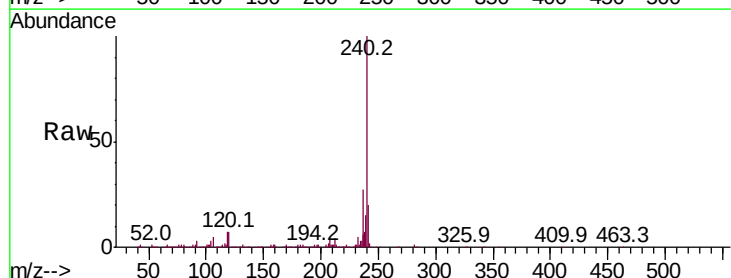


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

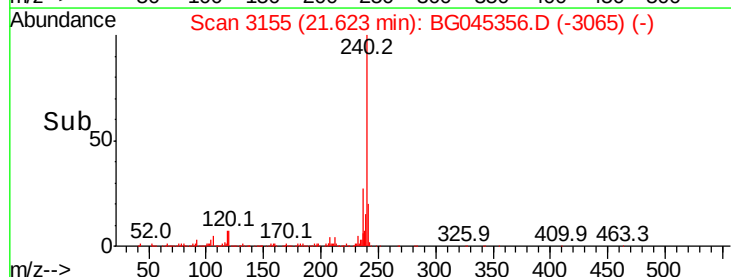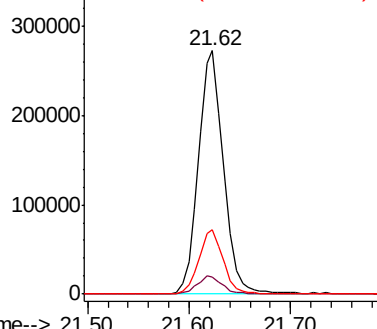

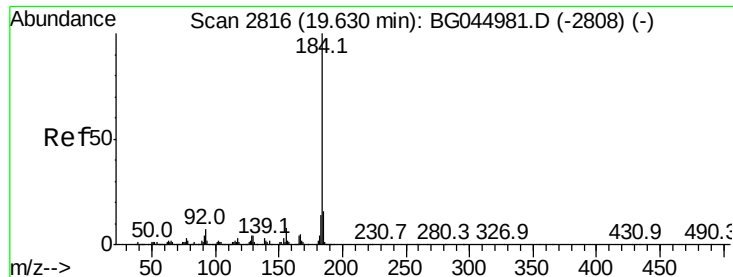

#77

Benzidine

Concen: Below Cal

RT: 19.97 min Scan# 2874

Delta R.T. 0.38 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00

Instrument :

BNA_P

ClientSampleId :

PB128795TB


Tot Ion:184 Resp: 32297

Ion Ratio Lower Upper




184 100

185 15.1 12.6 19.0

183 7.2 11.3 16.9#

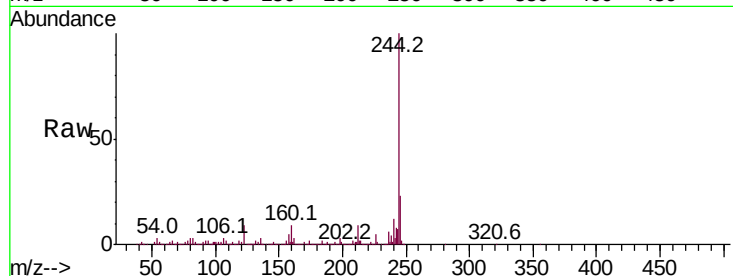

Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E

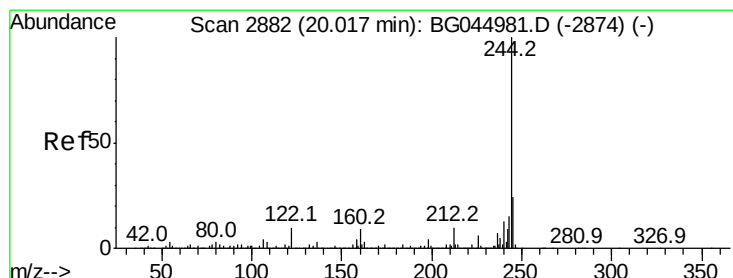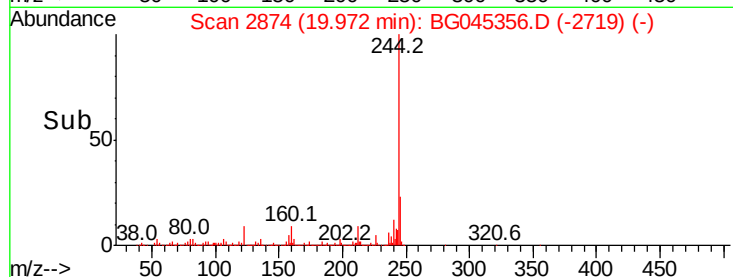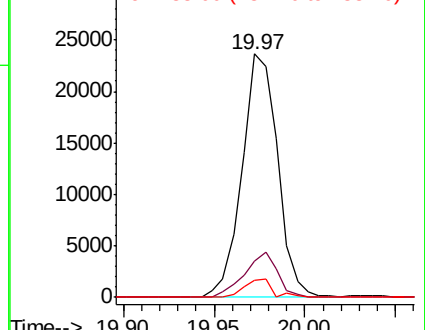

#79

Terphenyl-d14

Concen: 80.472 ng

RT: 19.98 min Scan# 2875

Delta R.T. -0.00 min

Lab File: BG045356.D

Acq: 13 May 2020 11:00


Tgt Ion:244 Resp: 1726219

Ion Ratio Lower Upper



244 100


212 9.0 7.9 11.9

122 8.7 7.7 11.5

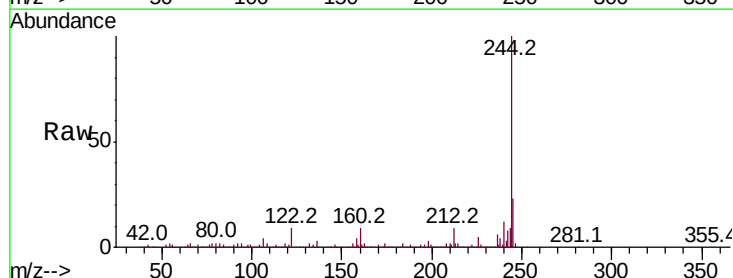

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

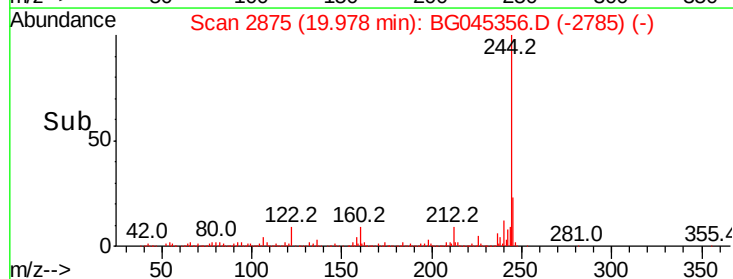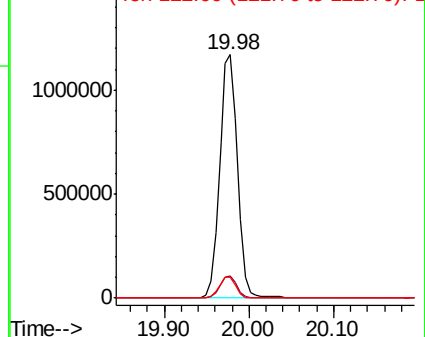

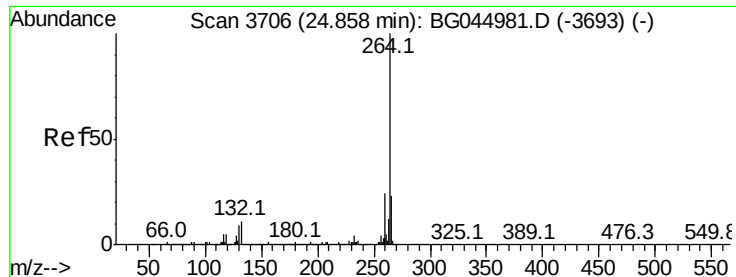

#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.78 min Scan# 3692
Delta R.T. -0.01 min
Lab File: BG045356.D
Acq: 13 May 2020 11:00

Instrument :
BNA_P
ClientSampleId :
PB128795TB

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.6	19.2	28.8
265	21.7	19.0	28.4

