

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002263.D
 Acq On : 12 May 2020 22:01
 Operator : CG/JU
 Sample : PB128669BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 13 03:05:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 12 18:30:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	286561	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1185411	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	674412	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	1234975	20.00	ng/ul	0.00
78) Chrysene-d12	21.10	240	939434	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1003901	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	45389	6.35	ng/uL	0.00
5) Phenol-d5	6.79	99	209861	8.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	509398	33.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	535910	27.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	363736	18.61	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	321584	36.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	344881	36.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	579552	30.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	54724	2.44	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1797967	35.70	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2264440	37.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	52235	5.98	ng/ul	-0.01
58) Fluorene-d10	15.26	176	1532748	36.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	194127	32.48	ng/ul	0.00
71) Anthracene-d10	17.11	188	2223718	40.42	ng/ul	0.00
79) Pyrene-d10	19.35	212	2159857	39.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	2061679	39.66	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.72	163	110526	2.157	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP051220\
Data File : BP002263.D
Acq On : 12 May 2020 22:01
Operator : CG/JU
Sample : PB128669BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 13 03:05:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 12 18:30:49 2020
Response via : Initial Calibration

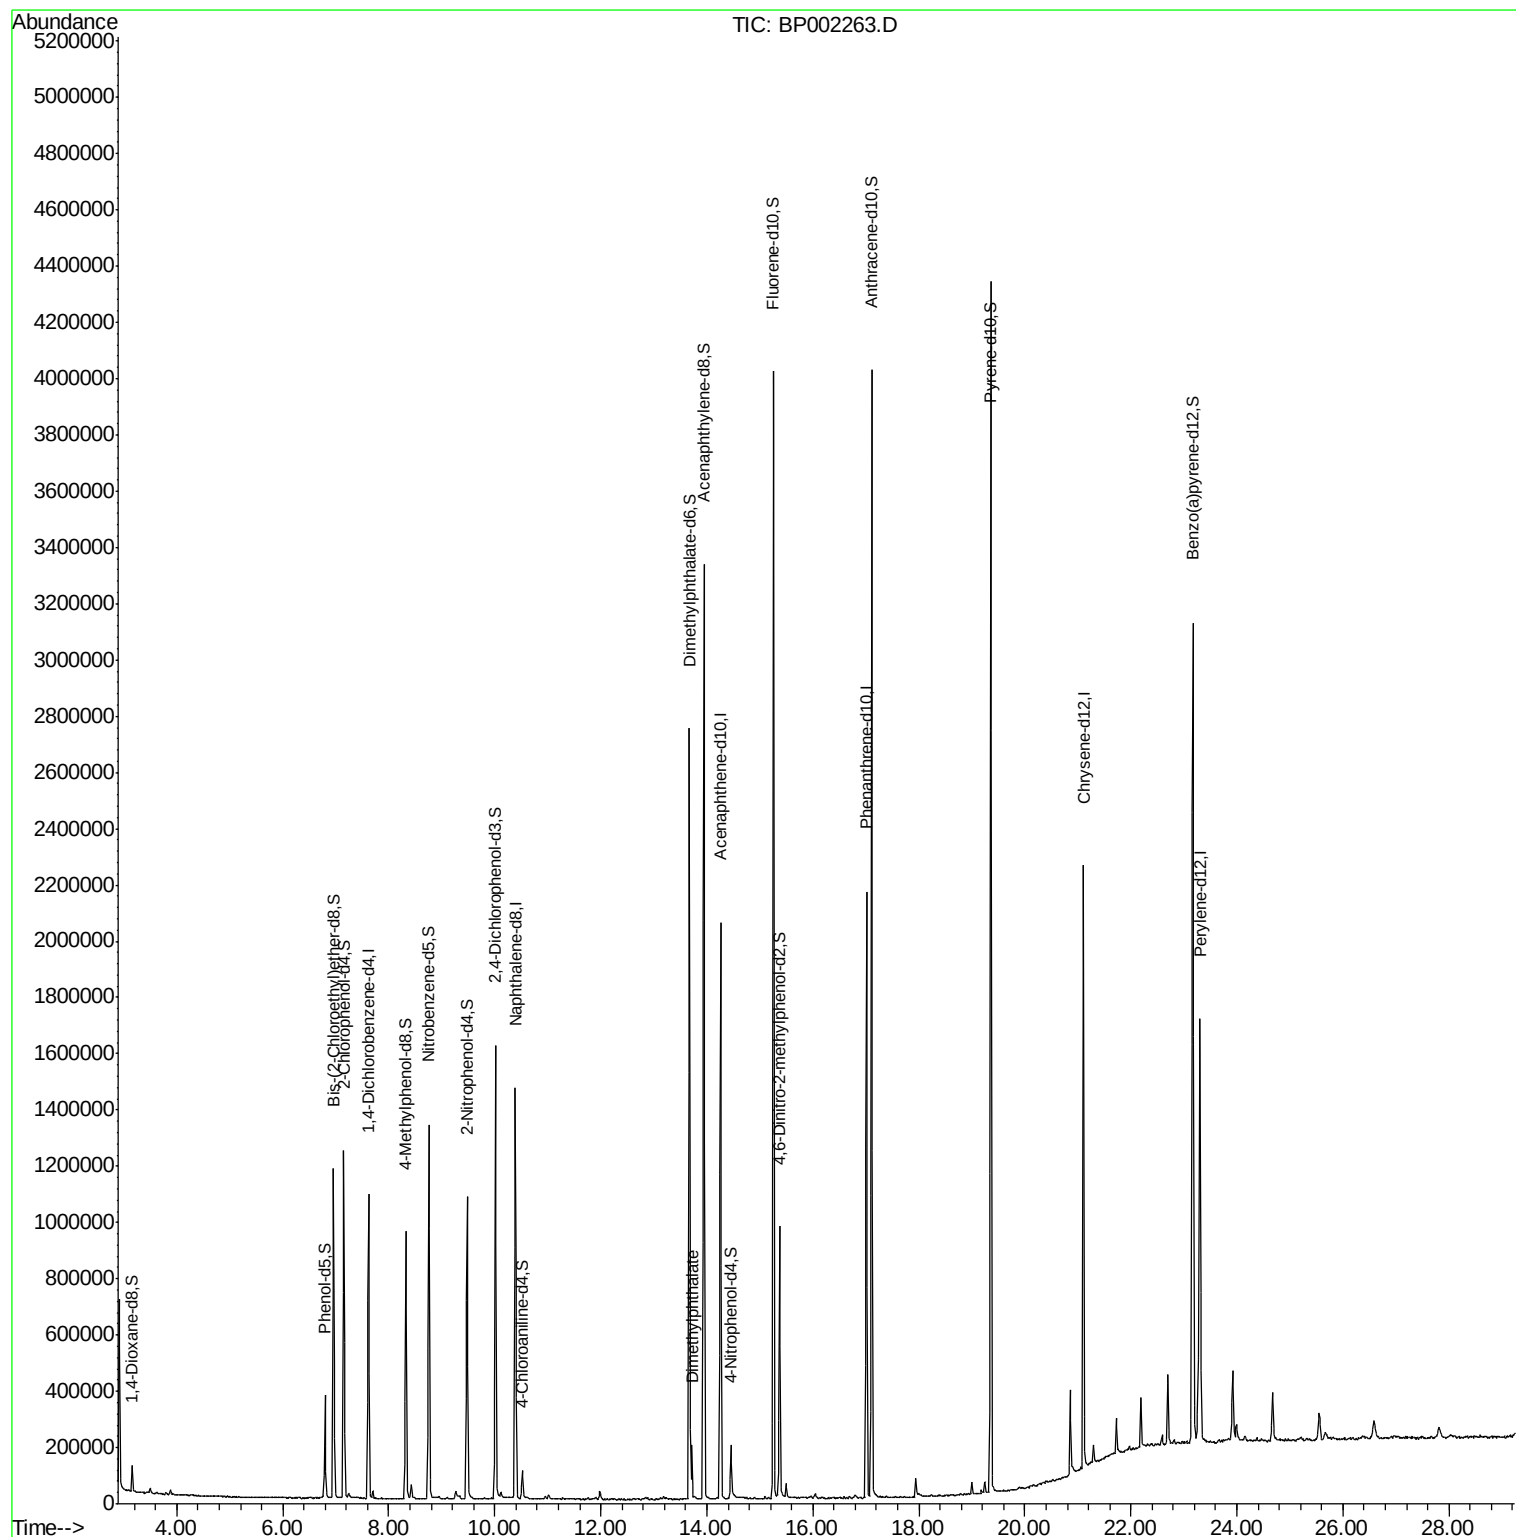


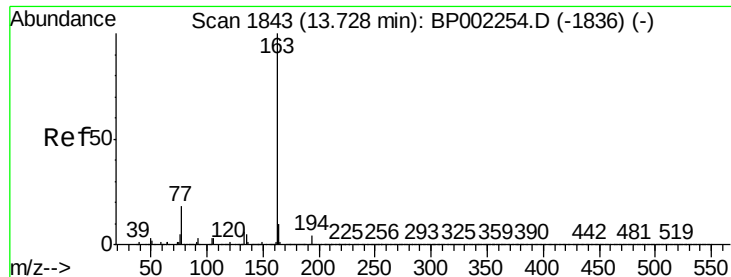

#45
 Dimethylphthalate
 Concen: 2.157 ng/ul
 RT: 13.72 min Scan# 1841
 Delta R.T. -0.01 min
 Lab File: BP002263.D
 Acq: 12 May 2020 22:01

Instrument :
 BNA_P
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.4	5.0
164	10.4	7.8	11.6

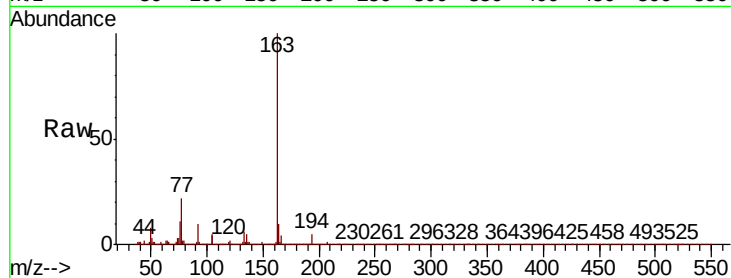

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

