

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002269.D
 Acq On : 13 May 2020 01:24
 Operator : CG/JU
 Sample : L2570-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 13 03:06:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 12 18:30:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	258333	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1045451	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	563285	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1042034	20.00	ng/ul	0.00
78) Chrysene-d12	21.10	240	941404	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	1046652	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	38960	6.04	ng/uL	0.00
5) Phenol-d5	6.79	99	226505	10.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.96	67	502214	36.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	545299	31.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	380044	21.57	ng/ul	-0.01
19) Nitrobenzene-d5	8.75	128	305949	39.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	332990	40.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	581232	34.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	34346	1.73	ng/ul	0.00
44) Dimethylphthalate-d6	13.68	166	1618091	38.47	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2103550	41.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	58306	8.00	ng/ul	-0.01
58) Fluorene-d10	15.25	176	1399985	39.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	185087	36.70	ng/ul	-0.01
71) Anthracene-d10	17.10	188	1971811	42.48	ng/ul	0.00
79) Pyrene-d10	19.35	212	2053500	37.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	2198906	40.57	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.72	163	229469	5.361	ng/ul	99
65) N-Nitrosodiphenylamine	15.52	169	46675	1.566	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP051220\
Data File : BP002269.D
Acq On : 13 May 2020 01:24
Operator : CG/JU
Sample : L2570-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 13 03:06:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 12 18:30:49 2020
Response via : Initial Calibration

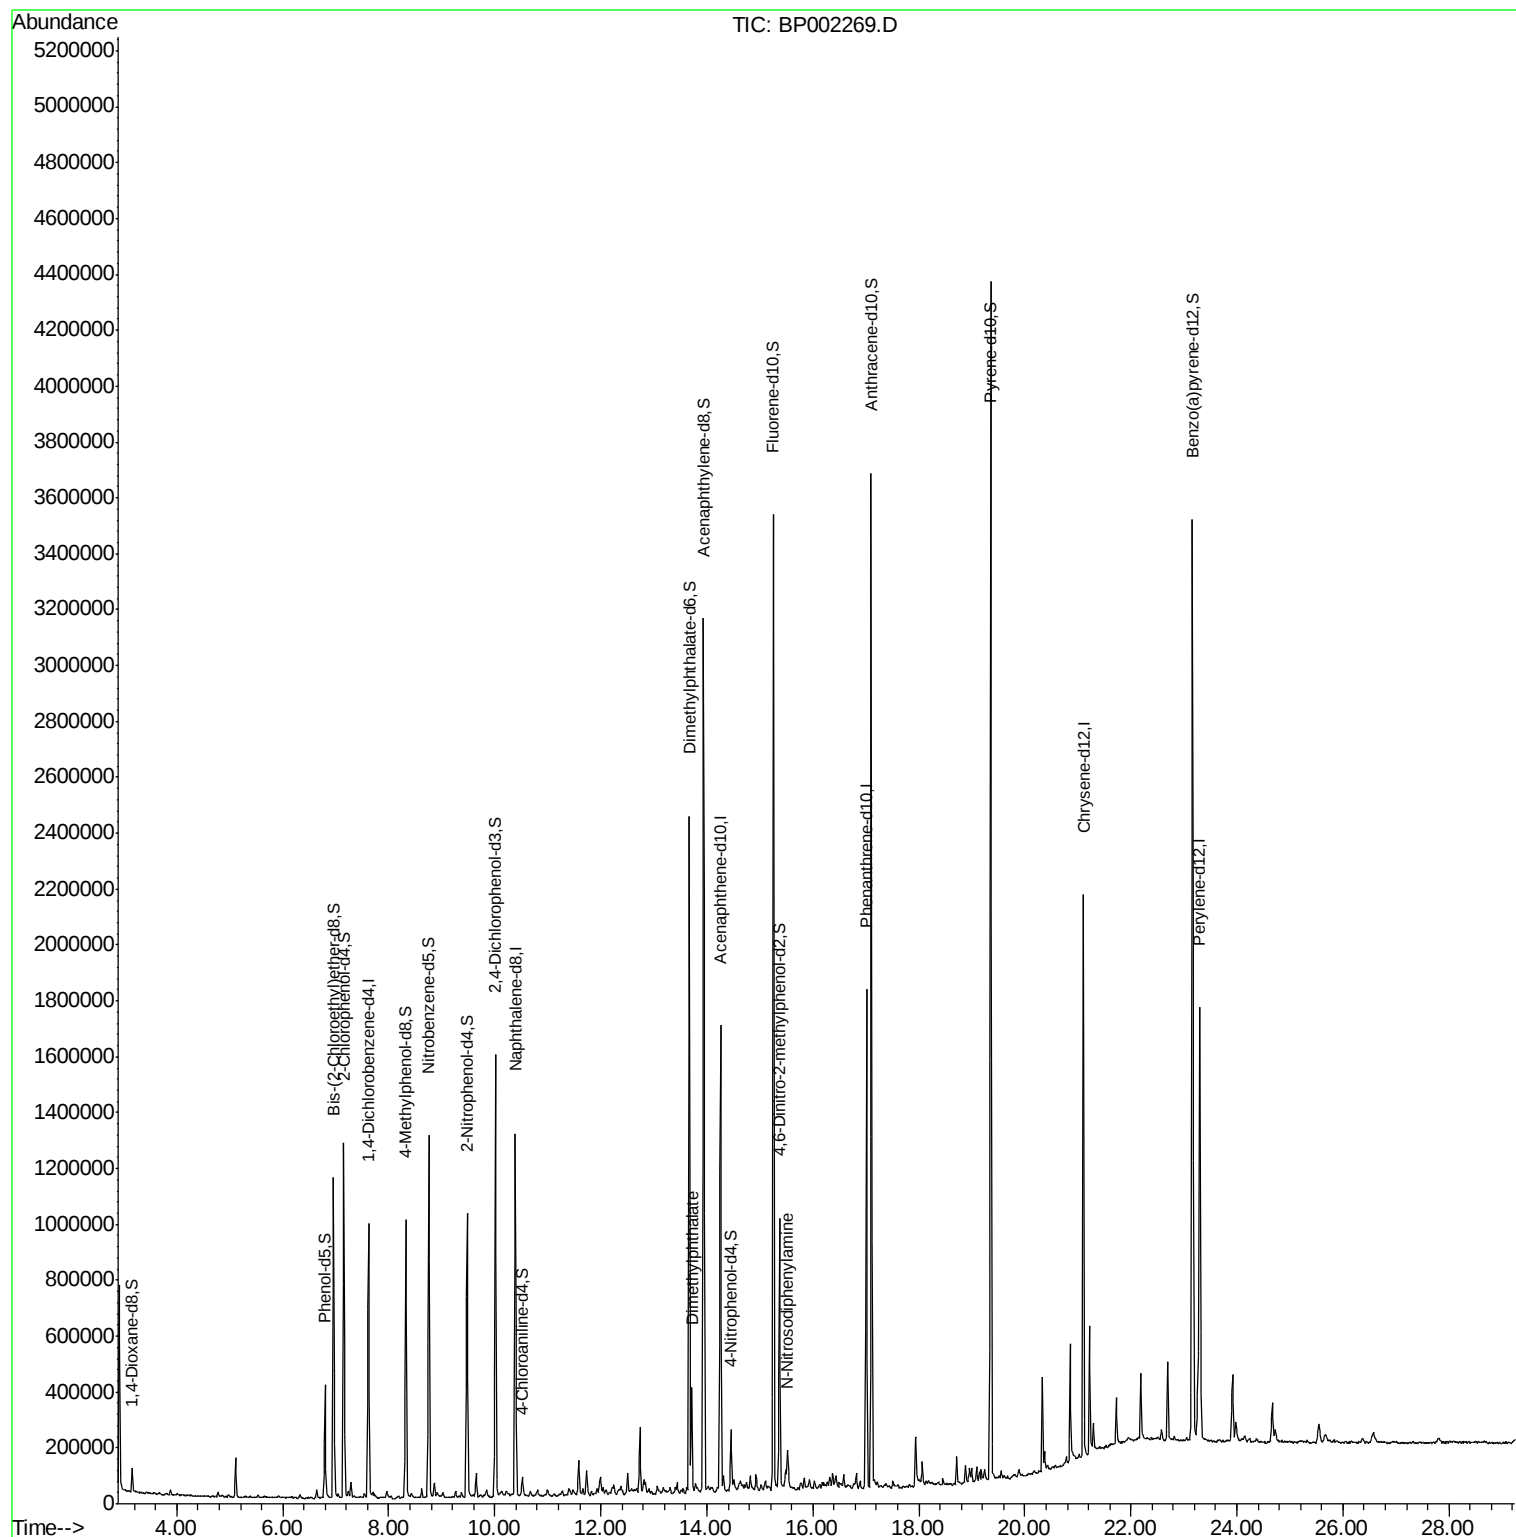

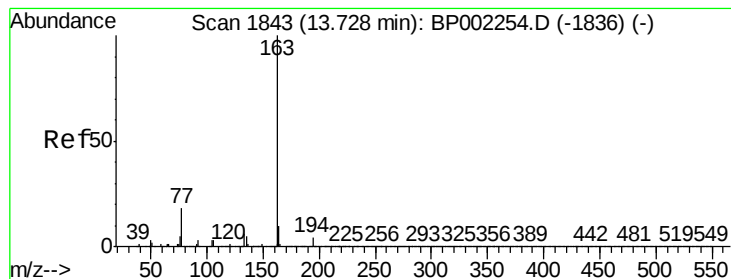

#45

Dimethylphthalate

Concen: 5.361 ng/ul

RT: 13.72 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BP002269.D

Acq: 13 May 2020 01:24

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 229469

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0




164 10.4 7.8 11.6

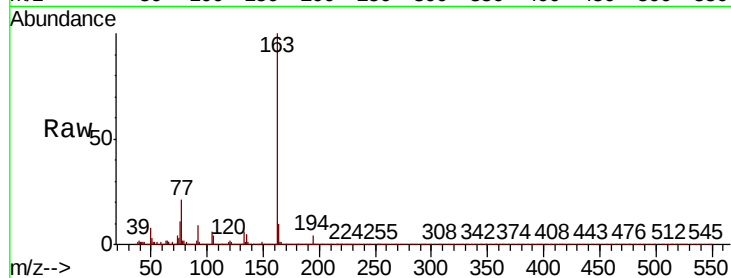

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

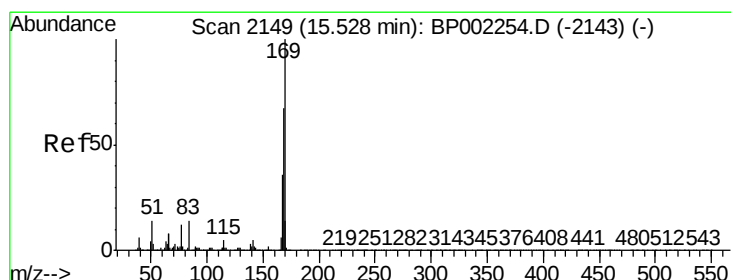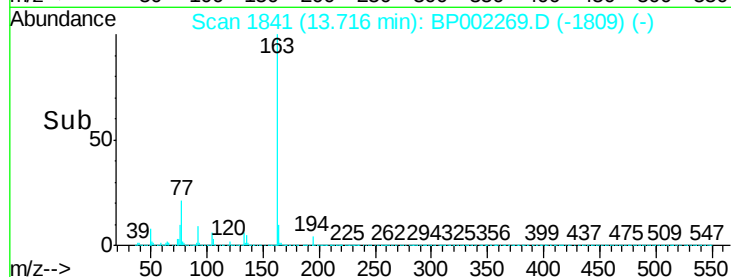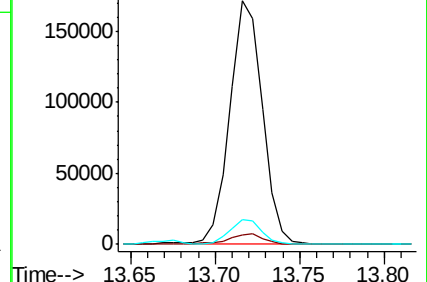

#65

N-Nitrosodiphenylamine

Concen: 1.566 ng/ul

RT: 15.52 min Scan# 2148

Delta R.T. -0.01 min

Lab File: BP002269.D

Acq: 13 May 2020 01:24


Tgt Ion:169 Resp: 46675

Ion Ratio Lower Upper

169 100

168 65.8 54.0 81.0

167 36.7 29.1 43.7

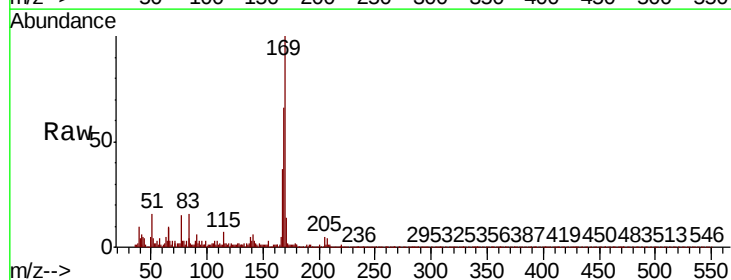

Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

