

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002266.D
 Acq On : 13 May 2020 00:50
 Operator : CG/JU
 Sample : L2488-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BFSN2

Quant Time: May 13 03:06:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 12 18:30:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	257971	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1098664	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	644124	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.01	188	1222478	20.00	ng/ul	0.00
78) Chrysene-d12	21.10	240	865951	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	895456	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	36585	5.68	ng/uL	0.00
5) Phenol-d5	6.79	99	165863	7.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	434029	31.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	451574	25.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	299349	17.02	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	269942	33.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	290075	33.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	490121	27.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	49897	2.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1619807	33.68	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2002977	34.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.46	143	48784	5.85	ng/ul	0.00
58) Fluorene-d10	15.26	176	1426855	35.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	206888	34.96	ng/ul	-0.01
71) Anthracene-d10	17.10	188	2247644	41.28	ng/ul	0.00
79) Pyrene-d10	19.35	212	2163524	42.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	1866994	40.26	ng/ul	-0.01


Target Compounds					Qvalue
45) Dimethylphthalate	13.72	163	88791	1.81 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002266.D
Acq On : 13 May 2020 00:50
Operator : CG/JU
Sample : L2488-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BFSN2

Quant Time: May 13 03:06:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 12 18:30:49 2020
Response via : Initial Calibration

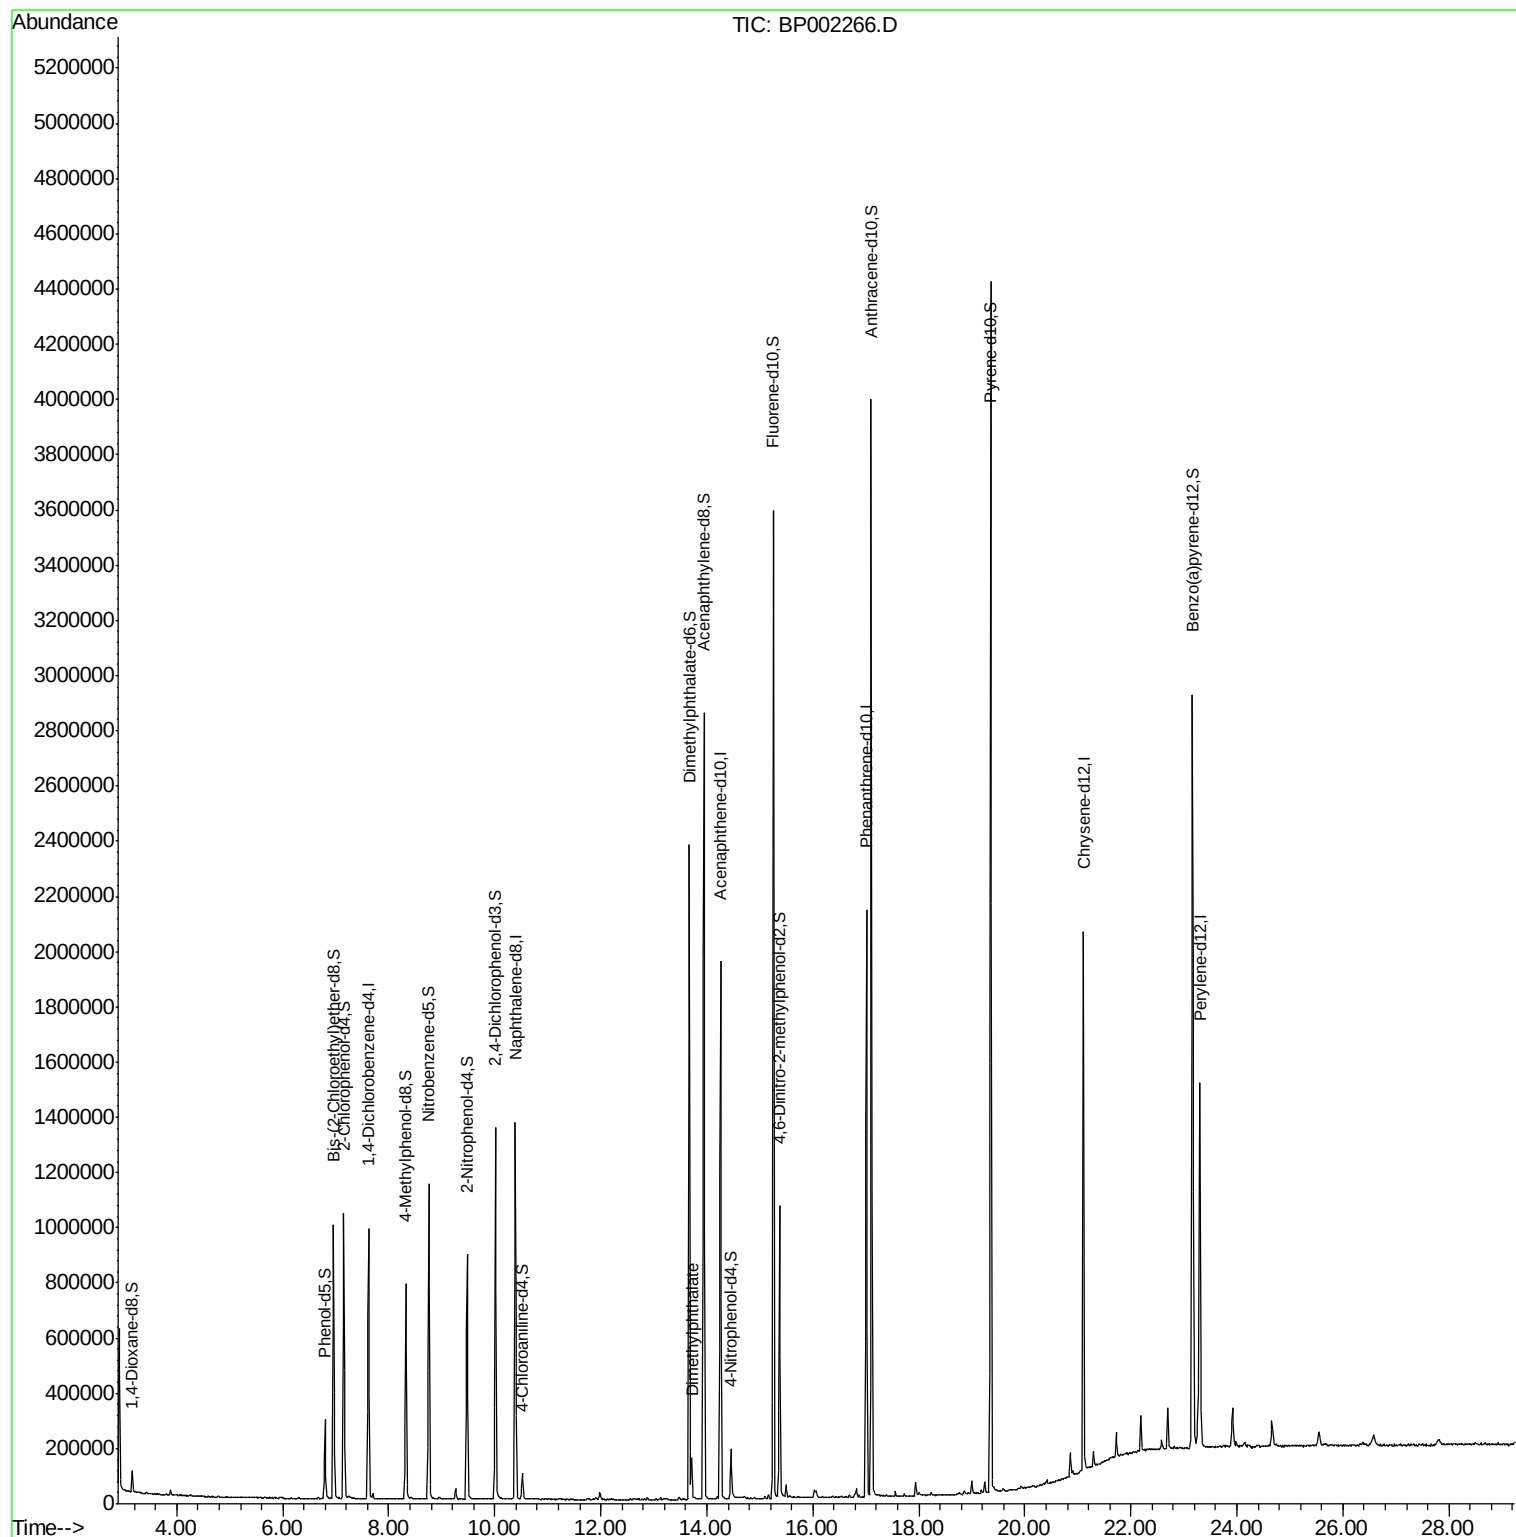

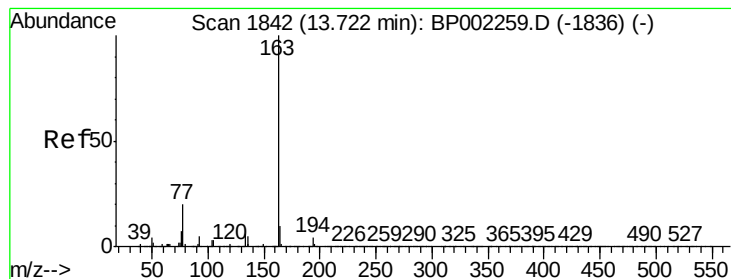

#45

Dimethylphthalate

Concen: 1.81 ng/ul

RT: 13.72 min Scan# 1841

Delta R.T. -0.01 min

Lab File: BP002266.D

Acq: 13 May 2020 00:50

Instrument :

BNA_P

ClientSampleId :

BFSN2

Tgt Ion:163 Resp: 88791

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.0

164 10.7 7.8 11.6

