

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002285.D
 Acq On : 13 May 2020 12:46
 Operator : CG/JU
 Sample : L2568-06DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B99DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP002287.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.917	3	5	12	rVB	199999	217875	3.44%	0.450%
2	3.158	43	46	63	rVB	90672	129024	2.04%	0.267%
3	3.881	164	169	177	rVB	75552	102183	1.61%	0.211%
4	6.140	546	553	557	rVB6	3925	6970	0.11%	0.014%
5	6.793	657	664	675	rBV	90894	161212	2.54%	0.333%
6	6.952	685	691	700	rBV	298188	480114	7.58%	0.992%
7	7.152	716	725	733	rBV	312287	495932	7.83%	1.024%
8	7.511	779	786	787	rBV7	3756	6570	0.10%	0.014%
9	7.611	796	803	814	rBV	1438266	2271738	35.84%	4.693%
10	7.693	814	817	823	rVB	11737	17804	0.28%	0.037%
11	7.987	860	867	873	rVB2	7460	17333	0.27%	0.036%
12	8.264	910	914	918	rBV3	9507	14532	0.23%	0.030%
13	8.316	918	923	935	rVV	247120	400907	6.33%	0.828%
14	8.752	985	997	1009	rBV	327766	566507	8.94%	1.170%
15	8.963	1027	1033	1038	rVB8	6430	11579	0.18%	0.024%
16	9.063	1044	1050	1054	rBV6	6118	10731	0.17%	0.022%
17	9.258	1078	1083	1087	rVB2	6595	9907	0.16%	0.020%
18	9.469	1113	1119	1130	rBV	244028	411006	6.49%	0.849%
19	9.646	1145	1149	1154	rBV5	3969	7249	0.11%	0.015%
20	9.805	1171	1176	1183	rVB5	3331	7739	0.12%	0.016%
21	10.011	1202	1211	1225	rBV	408828	693494	10.94%	1.433%
22	10.387	1266	1275	1282	rBV	2031158	3417924	53.93%	7.060%
23	10.522	1292	1298	1299	rBV3	18270	30148	0.48%	0.062%
24	10.546	1299	1302	1309	rVB	25997	50209	0.79%	0.104%
25	10.858	1351	1355	1362	rVB2	10667	17457	0.28%	0.036%
26	10.963	1367	1373	1379	rBV5	10670	22305	0.35%	0.046%
27	11.299	1425	1430	1435	rBV8	4411	6960	0.11%	0.014%
28	11.487	1456	1462	1469	rBV2	18569	33587	0.53%	0.069%
29	11.752	1499	1507	1512	rBV3	7869	16209	0.26%	0.033%
30	11.946	1535	1540	1543	rBV	14369	22721	0.36%	0.047%
31	12.005	1548	1550	1556	rVB4	5866	9745	0.15%	0.020%
32	12.275	1590	1596	1601	rVB3	12011	18209	0.29%	0.038%
33	12.387	1608	1615	1622	rBV3	6500	15402	0.24%	0.032%
34	12.581	1644	1648	1651	rBV6	5440	6803	0.11%	0.014%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002285.D
 Acq On : 13 May 2020 12:46
 Operator : CG/JU
 Sample : L2568-06DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleID :
 C5B99DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Title : SVOA CALIBRATION

35	12.746	1671	1676	1679	rBV7	6152	11158	0.18%	0.023%
36	13.081	1725	1733	1740	rBV	111886	172976	2.73%	0.357%
37	13.263	1759	1764	1768	rBV3	12349	17654	0.28%	0.036%
38	13.310	1768	1772	1777	rVB3	8708	14359	0.23%	0.030%
39	13.404	1786	1788	1797	rVB8	6240	11613	0.18%	0.024%
40	13.551	1808	1813	1814	rBV4	7046	9082	0.14%	0.019%
41	13.581	1816	1818	1823	rVB6	6757	7333	0.12%	0.015%
42	13.669	1827	1833	1837	rVV	905701	1224354	19.32%	2.529%
43	13.716	1837	1841	1846	rVV	180922	251529	3.97%	0.520%
44	13.763	1846	1849	1855	rVV2	14284	20604	0.33%	0.043%
45	13.940	1872	1879	1891	rBV	1039585	1502782	23.71%	3.104%
46	14.251	1925	1932	1941	rVB2	3165271	4745639	74.88%	9.803%
47	14.351	1944	1949	1955	rVB	24171	34942	0.55%	0.072%
48	14.451	1957	1966	1978	rBV	46543	96159	1.52%	0.199%
49	14.651	1996	2000	2007	rVB	32431	50101	0.79%	0.103%
50	14.804	2018	2026	2030	rBV	54136	87860	1.39%	0.181%
51	14.846	2030	2033	2035	rVV4	14494	21268	0.34%	0.044%
52	14.881	2035	2039	2046	rVB	73547	113201	1.79%	0.234%
53	15.093	2069	2075	2081	rVB5	12503	23071	0.36%	0.048%
54	15.181	2083	2090	2096	rBV10	8867	22699	0.36%	0.047%
55	15.251	2096	2102	2108	rBV	1324813	1882148	29.70%	3.888%
56	15.310	2108	2112	2117	rVV3	38232	69950	1.10%	0.144%
57	15.369	2117	2122	2132	rVB	240322	380522	6.00%	0.786%
58	15.493	2140	2143	2146	rVB2	6569	7192	0.11%	0.015%
59	15.610	2158	2163	2166	rBV5	12693	18184	0.29%	0.038%
60	15.845	2196	2203	2206	rBV5	7244	14607	0.23%	0.030%
61	16.016	2229	2232	2236	rBV5	9901	15360	0.24%	0.032%
62	16.069	2237	2241	2246	rVB8	10642	19011	0.30%	0.039%
63	16.198	2257	2263	2264	rBV6	5094	9467	0.15%	0.020%
64	16.287	2273	2278	2284	rBV4	10859	17517	0.28%	0.036%
65	16.363	2287	2291	2295	rVB5	7143	10009	0.16%	0.021%
66	16.581	2325	2328	2332	rVB3	8622	8980	0.14%	0.019%
67	16.663	2332	2342	2357	rBV	4341280	6337717	100.00%	13.092%
68	16.775	2357	2361	2366	rVV3	82087	148307	2.34%	0.306%
69	16.822	2366	2369	2375	rVB	53481	73384	1.16%	0.152%
70	17.004	2394	2400	2406	rBV	3890957	5446996	85.95%	11.252%
71	17.104	2411	2417	2431	rVB	1432468	2007743	31.68%	4.147%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002285.D
 Acq On : 13 May 2020 12:46
 Operator : CG/JU
 Sample : L2568-06DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B99DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Title : SVOA CALIBRATION

72	17.322	2451	2454	2459	rVB6	9264	12179	0.19%	0.025%
73	17.557	2490	2494	2496	rBV3	11185	15903	0.25%	0.033%
74	17.934	2554	2558	2564	rBV4	24718	35508	0.56%	0.073%
75	18.581	2664	2668	2672	rBV7	6195	10801	0.17%	0.022%
76	18.992	2735	2738	2742	rBV	19049	24211	0.38%	0.050%
77	19.239	2777	2780	2789	rVB	15661	23870	0.38%	0.049%
78	19.351	2793	2799	2806	rBV	1646634	2246606	35.45%	4.641%
79	20.851	3051	3054	3059	rBV5	33720	53847	0.85%	0.111%
80	21.098	3091	3096	3110	rBV	3978286	5102802	80.51%	10.541%
81	21.722	3199	3202	3210	rVB4	39051	59886	0.94%	0.124%
82	22.186	3278	3281	3287	rVB2	68034	97390	1.54%	0.201%
83	22.692	3363	3367	3374	rVB	93540	136510	2.15%	0.282%
84	23.157	3440	3446	3457	rVB	807613	1440601	22.73%	2.976%
85	23.298	3460	3470	3482	rVB	2253301	4376827	69.06%	9.041%
86	23.910	3570	3574	3581	rVB	90591	159076	2.51%	0.329%


Sum of corrected areas: 48409580

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002285.D
Acq On : 13 May 2020 12:46
Operator : CG/JU
Sample : L2568-06DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B99DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

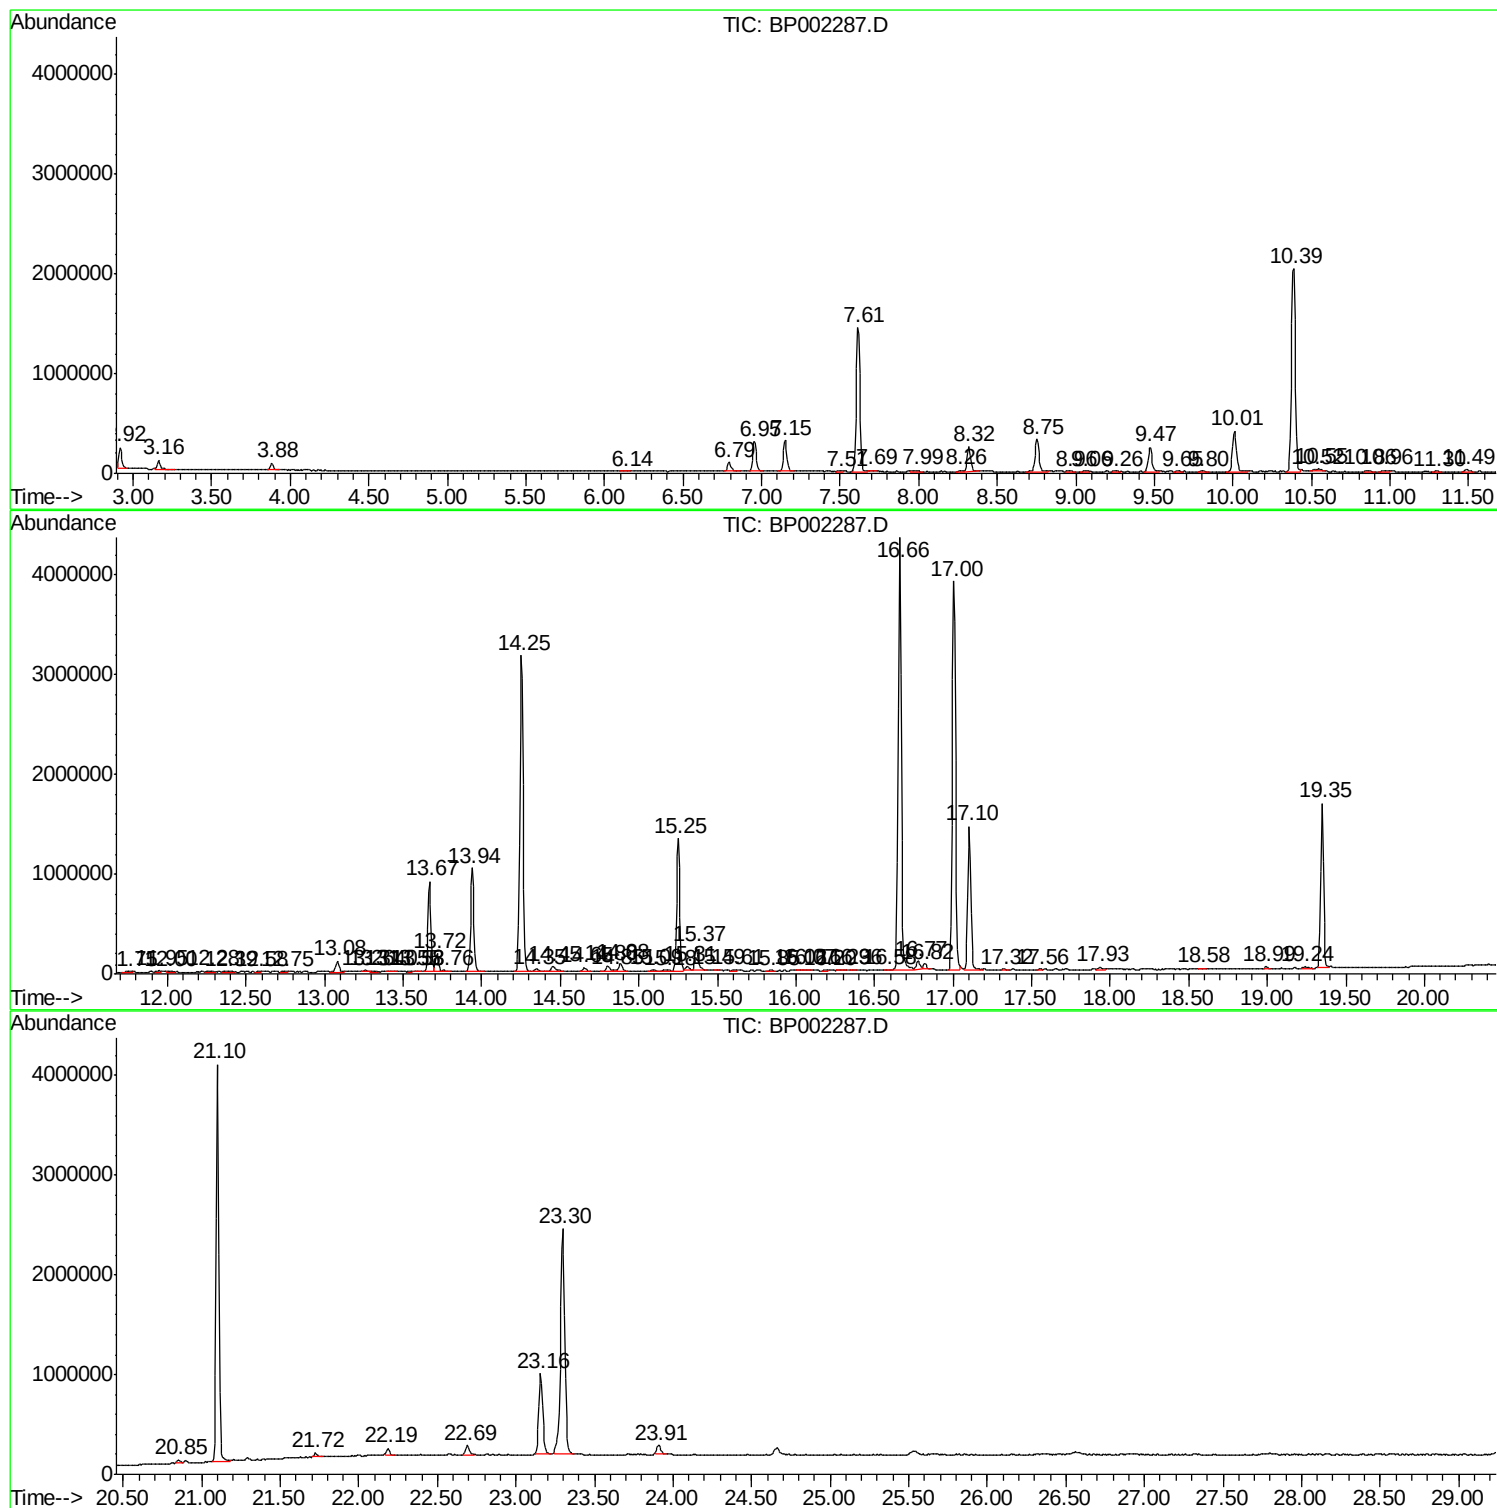

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002285.D
Acq On : 13 May 2020 12:46
Operator : CG/JU
Sample : L2568-06DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B99DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002285.D
Acq On : 13 May 2020 12:46
Operator : CG/JU
Sample : L2568-06DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B99DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc