

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002286.D
 Acq On : 13 May 2020 13:20
 Operator : CG/JU
 Sample : L2568-01DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP002288.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.917	3	5	17	rVB	163844	197485	3.08%	0.412%
2	3.158	42	46	54	rVB	79579	102371	1.59%	0.214%
3	3.881	164	169	174	rVB	56483	75831	1.18%	0.158%
4	6.793	658	664	673	rBV	65796	107743	1.68%	0.225%
5	6.952	685	691	699	rBV	253483	398326	6.21%	0.831%
6	7.152	718	725	734	rBV	245135	392441	6.11%	0.819%
7	7.375	757	763	769	rVB2	37740	84593	1.32%	0.176%
8	7.611	795	803	812	rBV	1351062	2224246	34.65%	4.641%
9	7.693	812	817	823	rVB	52397	75101	1.17%	0.157%
10	7.987	862	867	871	rVV3	10733	16907	0.26%	0.035%
11	8.316	918	923	930	rVV	188351	306911	4.78%	0.640%
12	8.369	930	932	939	rVV3	11376	20625	0.32%	0.043%
13	8.440	939	944	949	rVB6	8792	18928	0.29%	0.039%
14	8.564	960	965	970	rVB9	3638	8903	0.14%	0.019%
15	8.752	986	997	1009	rBV	277015	473153	7.37%	0.987%
16	8.899	1016	1022	1029	rBV	39223	67987	1.06%	0.142%
17	8.958	1029	1032	1041	rVV6	12437	23806	0.37%	0.050%
18	9.063	1045	1050	1058	rVB2	11133	21602	0.34%	0.045%
19	9.334	1092	1096	1101	rVB8	4937	9148	0.14%	0.019%
20	9.411	1104	1109	1113	rBV3	9150	13704	0.21%	0.029%
21	9.469	1113	1119	1128	rVV	206037	337742	5.26%	0.705%
22	9.599	1137	1141	1147	rBV3	10540	18007	0.28%	0.038%
23	9.687	1153	1156	1160	rVB3	6797	9344	0.15%	0.019%
24	9.805	1172	1176	1182	rVB9	6913	14394	0.22%	0.030%
25	10.011	1200	1211	1222	rBV	355769	606246	9.45%	1.265%
26	10.387	1266	1275	1283	rBV	1901883	3224984	50.25%	6.729%
27	10.452	1283	1286	1291	rVV5	17246	31967	0.50%	0.067%
28	10.516	1292	1297	1300	rVV	24199	44675	0.70%	0.093%
29	10.558	1300	1304	1311	rVB3	33874	63972	1.00%	0.133%
30	10.969	1367	1374	1378	rBV4	12269	25004	0.39%	0.052%
31	11.022	1378	1383	1386	rVB5	6348	10733	0.17%	0.022%
32	11.234	1412	1419	1423	rBV9	3812	8030	0.13%	0.017%
33	11.293	1423	1429	1435	rVB10	5901	11713	0.18%	0.024%
34	11.487	1458	1462	1470	rVB5	9507	22496	0.35%	0.047%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002286.D
 Acq On : 13 May 2020 13:20
 Operator : CG/JU
 Sample : L2568-01DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Title : SVOA CALIBRATION

35	11.622	1481	1485	1490	rVB6	4992	8990	0.14%	0.019%
36	11.757	1501	1508	1511	rBV4	6153	13868	0.22%	0.029%
37	11.893	1525	1531	1535	rBV8	5445	12837	0.20%	0.027%
38	11.946	1535	1540	1544	rVV	23482	40598	0.63%	0.085%
39	11.981	1544	1546	1551	rVB5	7220	10709	0.17%	0.022%
40	12.063	1556	1560	1565	rVB8	3679	7846	0.12%	0.016%
41	12.269	1589	1595	1601	rVB8	11361	22448	0.35%	0.047%
42	12.587	1643	1649	1651	rVV7	4946	7968	0.12%	0.017%
43	12.616	1651	1654	1658	rVV4	9053	15286	0.24%	0.032%
44	12.675	1660	1664	1671	rVV6	21506	39052	0.61%	0.081%
45	12.746	1671	1676	1684	rVB5	10652	22363	0.35%	0.047%
46	12.869	1693	1697	1705	rVB5	11794	17531	0.27%	0.037%
47	12.957	1705	1712	1720	rBV2	43861	73716	1.15%	0.154%
48	13.081	1728	1733	1738	rBV	28095	40613	0.63%	0.085%
49	13.175	1743	1749	1759	rBV	41193	74843	1.17%	0.156%
50	13.263	1759	1764	1769	rBV5	28007	49101	0.76%	0.102%
51	13.369	1779	1782	1787	rBV7	5400	8825	0.14%	0.018%
52	13.552	1808	1813	1815	rBV6	9463	13836	0.22%	0.029%
53	13.669	1827	1833	1838	rBV	814220	1092201	17.02%	2.279%
54	13.716	1838	1841	1845	rVV	96565	125973	1.96%	0.263%
55	13.757	1845	1848	1853	rVB3	15114	21819	0.34%	0.046%
56	13.816	1853	1858	1864	rBV9	10439	19710	0.31%	0.041%
57	13.940	1873	1879	1895	rBV	920386	1324424	20.63%	2.763%
58	14.069	1896	1901	1905	rBV8	6849	12827	0.20%	0.027%
59	14.251	1921	1932	1942	rBV	2962571	4515828	70.36%	9.422%
60	14.351	1946	1949	1952	rVB4	6157	8169	0.13%	0.017%
61	14.457	1962	1967	1978	rVB5	42116	89503	1.39%	0.187%
62	14.651	1996	2000	2007	rVB	18499	29508	0.46%	0.062%
63	14.804	2021	2026	2029	rBV	27020	38183	0.59%	0.080%
64	14.840	2029	2032	2035	rVV3	21987	32517	0.51%	0.068%
65	14.881	2035	2039	2050	rVB	110271	171138	2.67%	0.357%
66	15.004	2057	2060	2068	rVB6	14627	31975	0.50%	0.067%
67	15.093	2068	2075	2080	rVB2	37591	53623	0.84%	0.112%
68	15.146	2080	2084	2088	rBV7	5285	11275	0.18%	0.024%
69	15.251	2096	2102	2108	rBV	1210905	1665874	25.95%	3.476%
70	15.304	2108	2111	2117	rVV2	34034	54853	0.85%	0.114%
71	15.369	2117	2122	2123	rVV	227864	302301	4.71%	0.631%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
 Data File : BP002286.D
 Acq On : 13 May 2020 13:20
 Operator : CG/JU
 Sample : L2568-01DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
 Title : SVOA CALIBRATION

72	15.393	2123	2126	2132	rVV	359069	485496	7.56%	1.013%
73	15.463	2133	2138	2143	rVV2	53356	91084	1.42%	0.190%
74	15.522	2144	2148	2152	rVB2	39559	54365	0.85%	0.113%
75	15.604	2160	2162	2167	rVB5	8894	10833	0.17%	0.023%
76	15.693	2173	2177	2178	rBV4	8319	9774	0.15%	0.020%
77	15.840	2199	2202	2206	rVB2	8390	11109	0.17%	0.023%
78	15.922	2214	2216	2222	rVB7	6685	8851	0.14%	0.018%
79	16.134	2246	2252	2257	rVB9	6904	15627	0.24%	0.033%
80	16.193	2257	2262	2266	rBV8	6908	15166	0.24%	0.032%
81	16.293	2274	2279	2283	rBV2	23065	39849	0.62%	0.083%
82	16.363	2288	2291	2294	rVB4	9024	12421	0.19%	0.026%
83	16.663	2335	2342	2357	rBV	4313608	6418450	100.00%	13.392%
84	16.781	2358	2362	2367	rVB3	46398	81475	1.27%	0.170%
85	17.004	2394	2400	2411	rBV	3595617	5237778	81.61%	10.928%
86	17.104	2411	2417	2429	rVB	1289195	1830134	28.51%	3.818%
87	17.934	2554	2558	2560	rBV4	40671	56514	0.88%	0.118%
88	17.992	2566	2568	2573	rVB	18465	20301	0.32%	0.042%
89	18.992	2735	2738	2742	rBV2	18575	24167	0.38%	0.050%
90	19.351	2793	2799	2805	rBV	1555019	2105107	32.80%	4.392%
91	20.851	3050	3054	3059	rBV3	89353	131703	2.05%	0.275%
92	21.098	3091	3096	3111	rVB2	4019657	5136101	80.02%	10.716%
93	21.292	3126	3129	3133	rBV2	33084	36196	0.56%	0.076%
94	21.722	3199	3202	3208	rBV2	54132	68577	1.07%	0.143%
95	22.180	3277	3280	3287	rVB	102261	130989	2.04%	0.273%
96	22.692	3363	3367	3374	rVB	135521	200507	3.12%	0.418%
97	23.157	3440	3446	3457	rVV	778455	1400621	21.82%	2.922%
98	23.298	3459	3470	3489	rVB	2397345	4694664	73.14%	9.795%
99	23.910	3569	3574	3582	rVB	135698	253994	3.96%	0.530%
100	24.657	3697	3701	3709	rVB3	94586	195462	3.05%	0.408%


Sum of corrected areas: 47928564

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002286.D
Acq On : 13 May 2020 13:20
Operator : CG/JU
Sample : L2568-01DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
C5B96DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

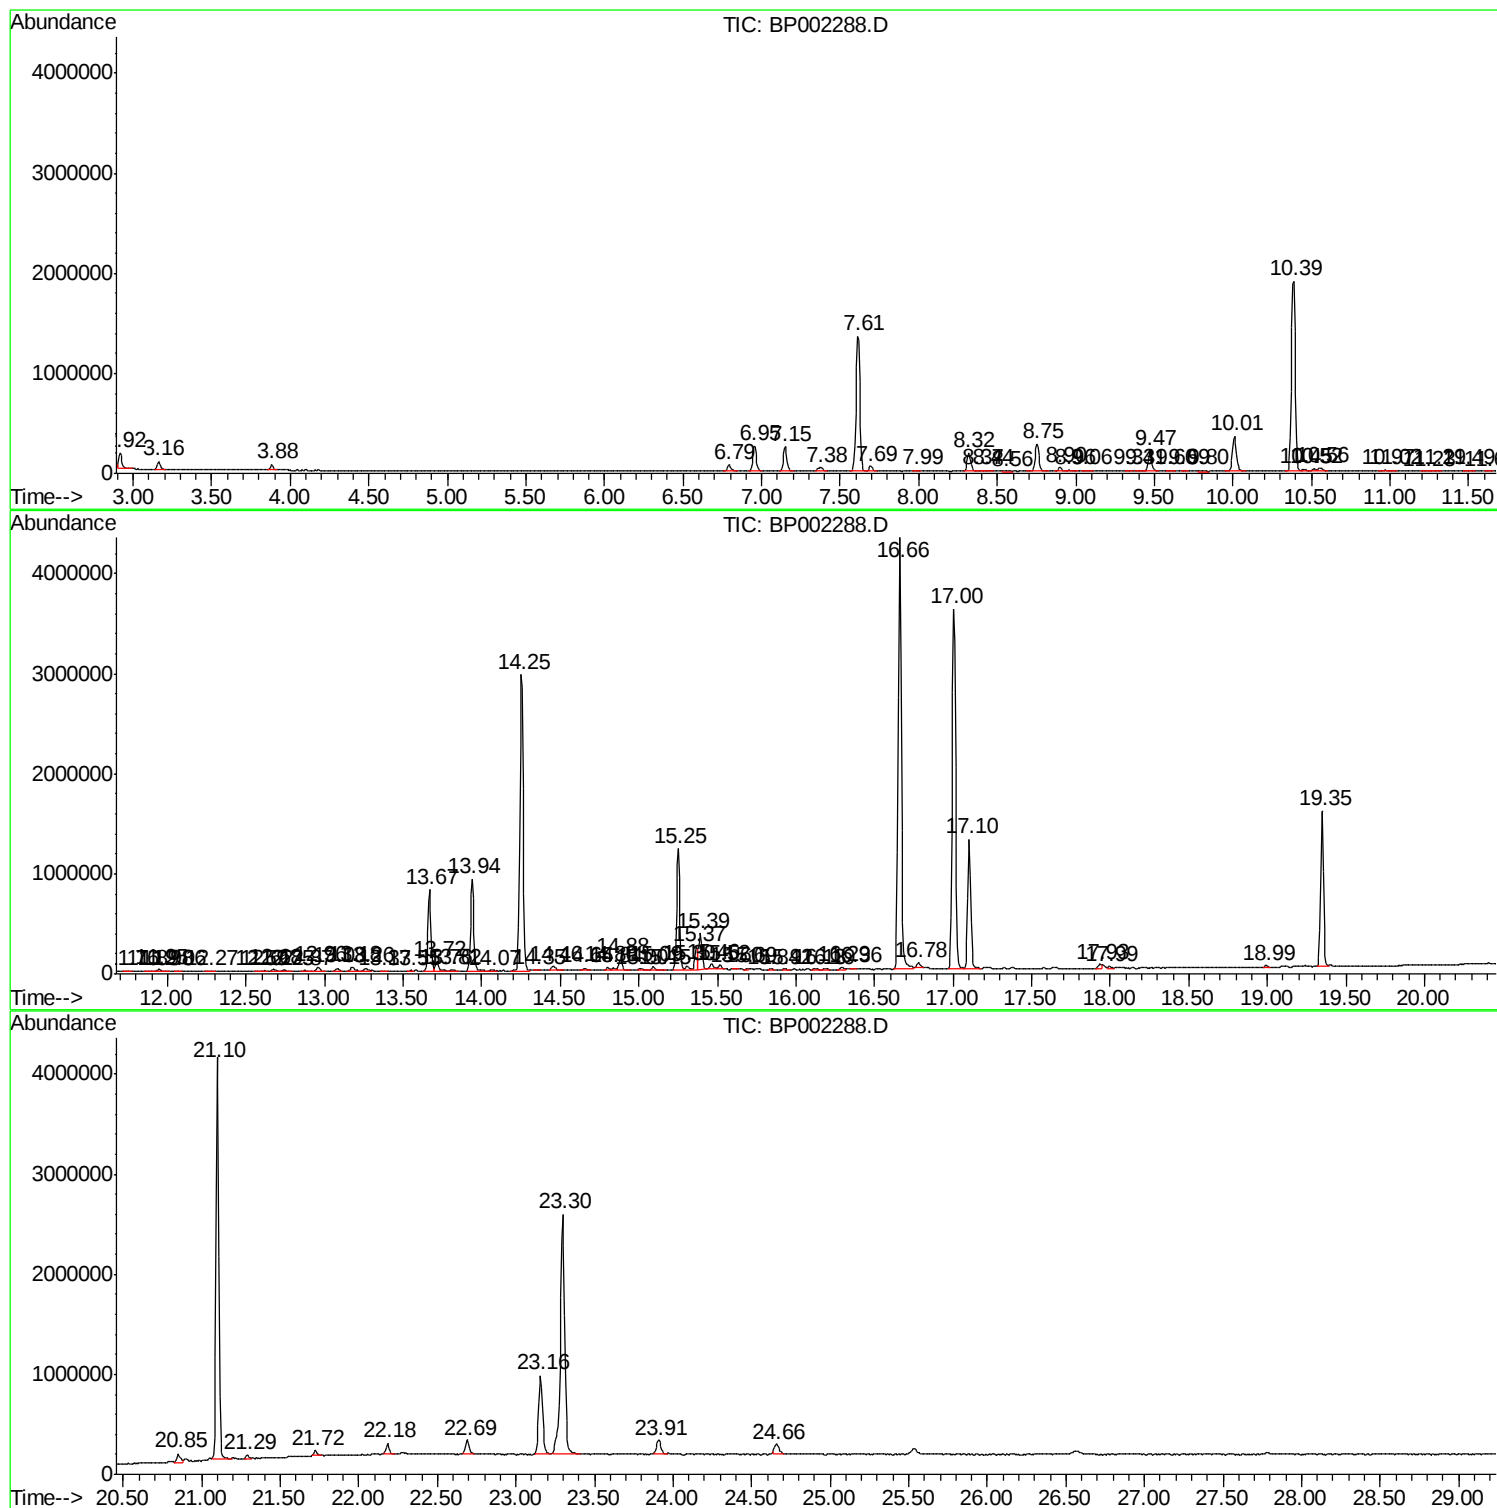

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002286.D
Acq On : 13 May 2020 13:20
Operator : CG/JU
Sample : L2568-01DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B96DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP051220\
Data File : BP002286.D
Acq On : 13 May 2020 13:20
Operator : CG/JU
Sample : L2568-01DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B96DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP051220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc