




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010371.D
 Acq On : 16 May 2022 23:10
 Operator : CG/JU
 Sample : N2831-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J9

Manual IntegrationsAPPROVED

Quant Time: May 17 00:36:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

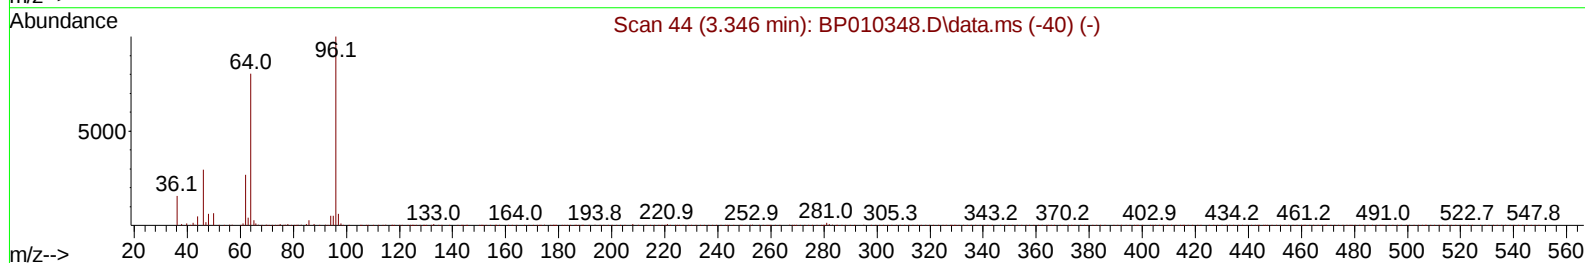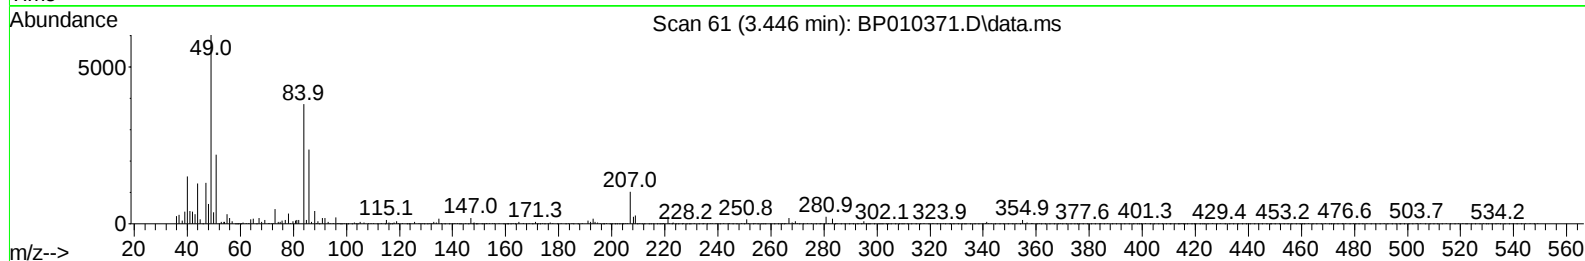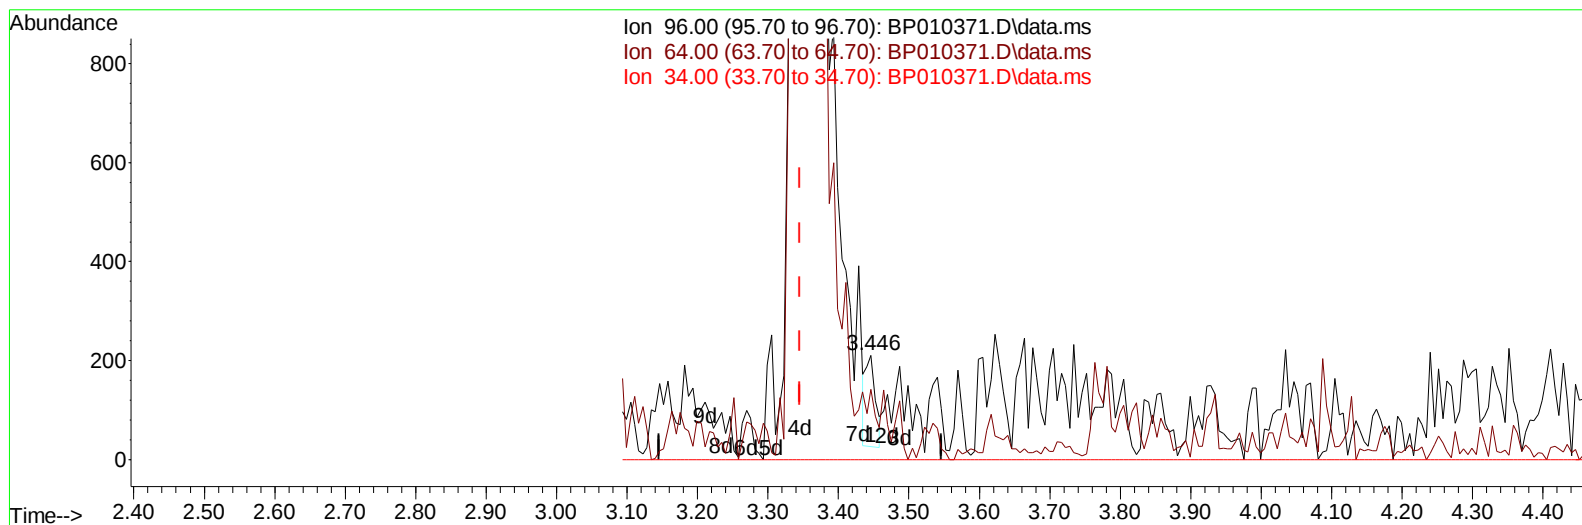

TIC: BP010371.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.446min (+ 0.100) 0.06 ng/uL

response 177

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	60.94
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010371.D
 Acq On : 16 May 2022 23:10
 Operator : CG/JU
 Sample : N2831-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J9

Manual IntegrationsAPPROVED

Quant Time: May 17 00:36:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

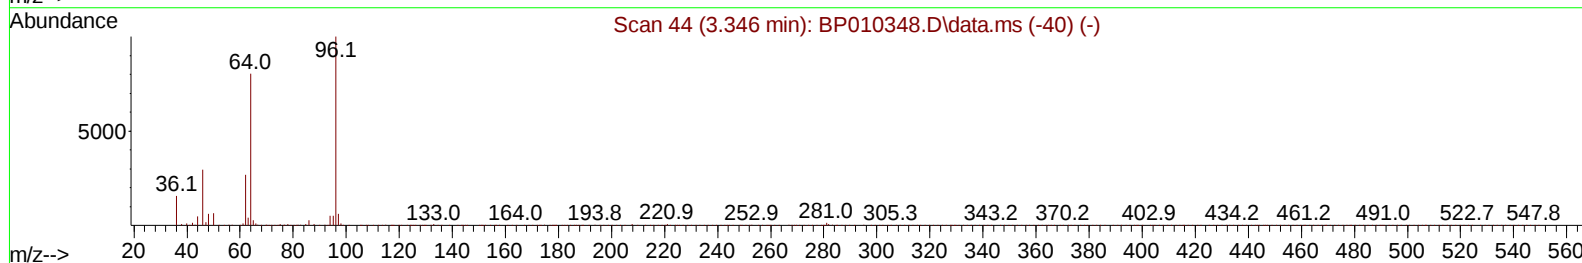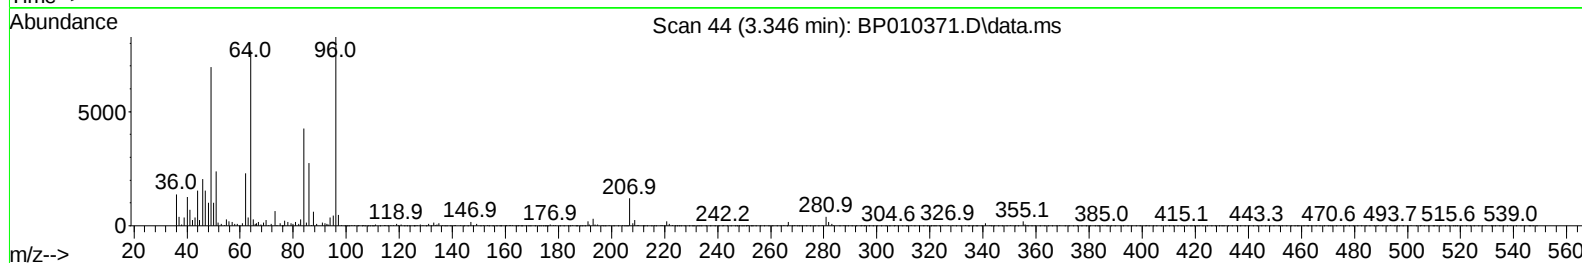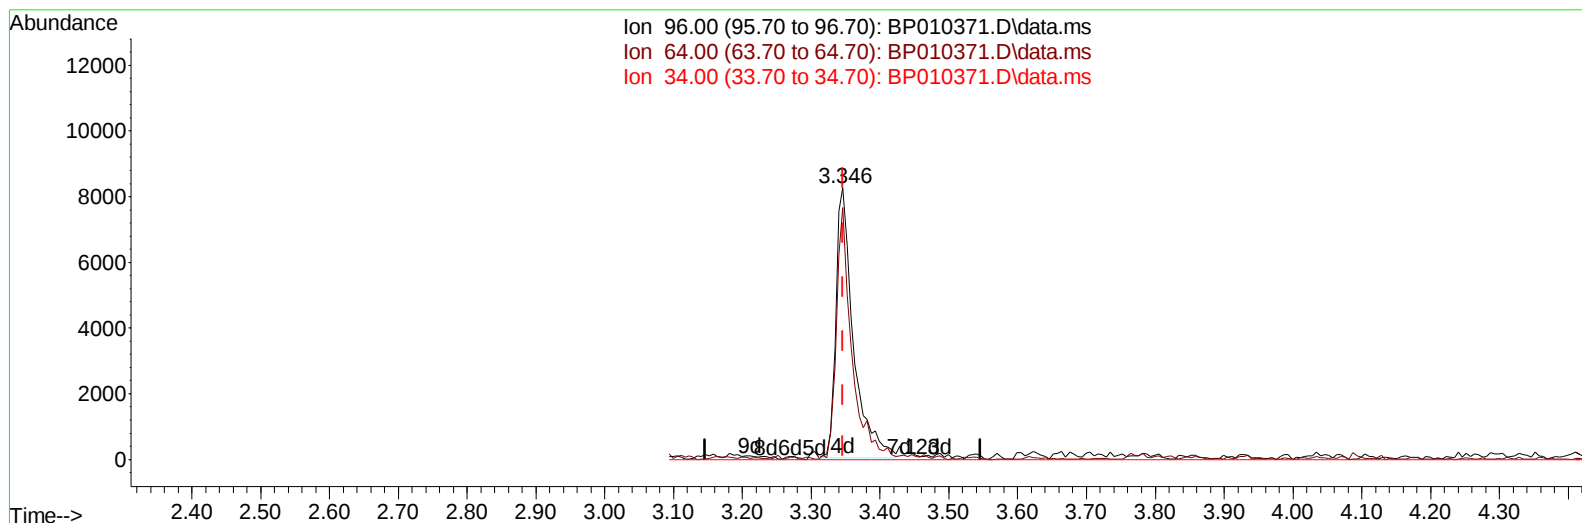

TIC: BP010371.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (+ 0.000) 5.10 ng/uL m

response 14600

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	92.73#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010371.D
Acq On : 16 May 2022 23:10
Operator : CG/JU
Sample : N2831-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J9

Manual IntegrationsAPPROVED

Quant Time: May 17 00:36:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

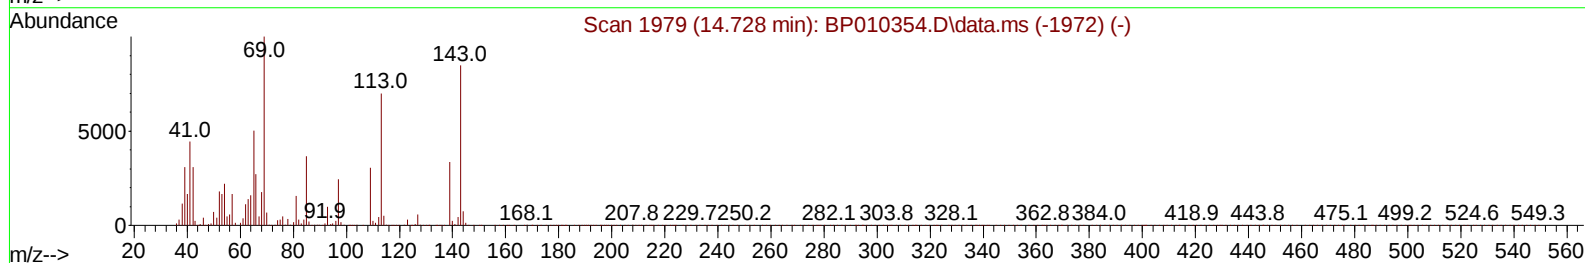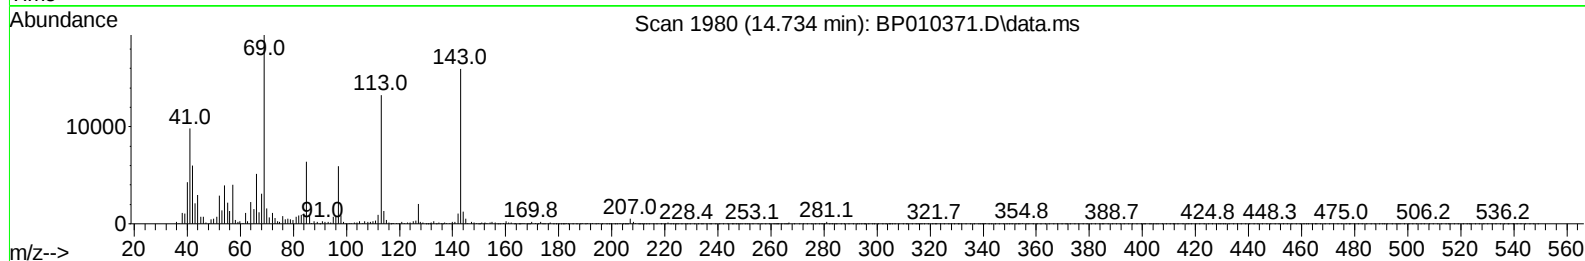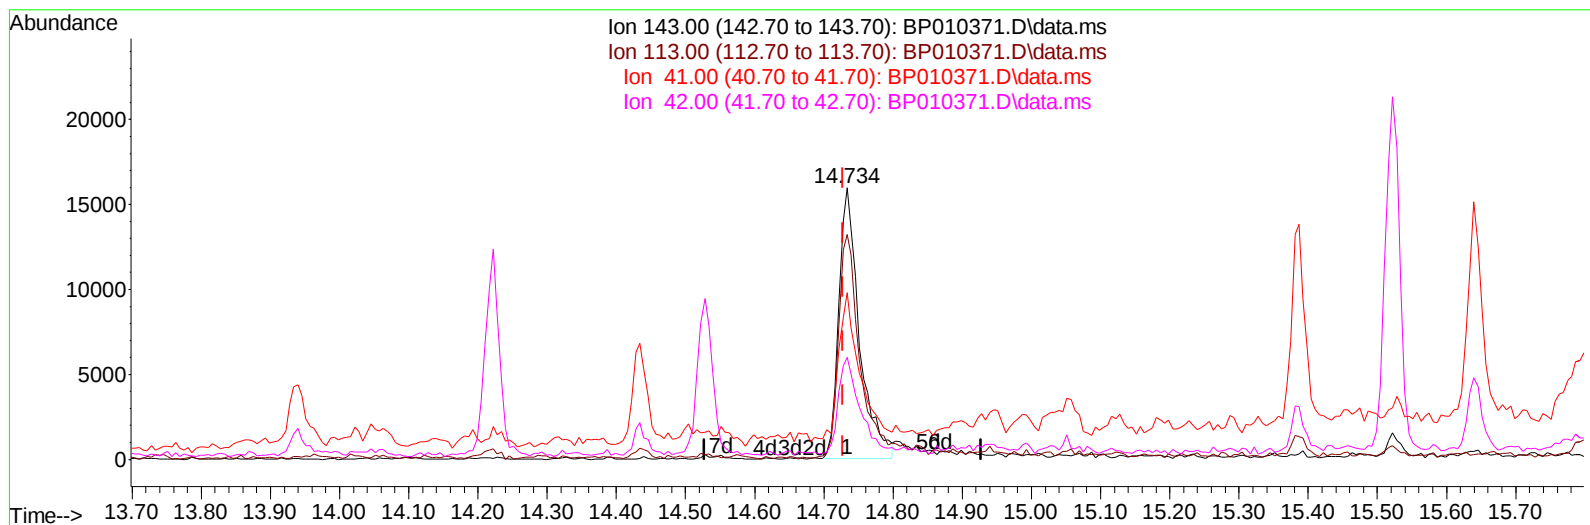

TIC: BP010371.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.006) 6.81 ng/ul

response 33033

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	82.98#
41.00	23.20	61.43#
42.00	18.00	37.70#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010371.D
Acq On : 16 May 2022 23:10
Operator : CG/JU
Sample : N2831-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 00:36:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

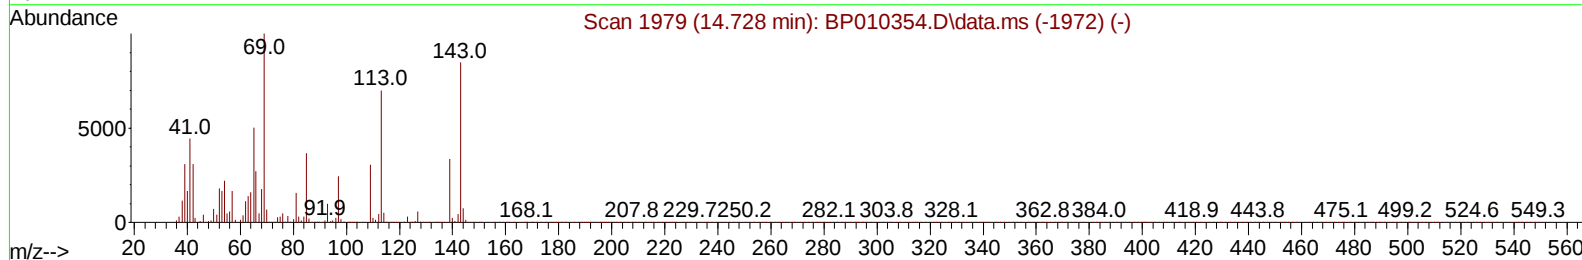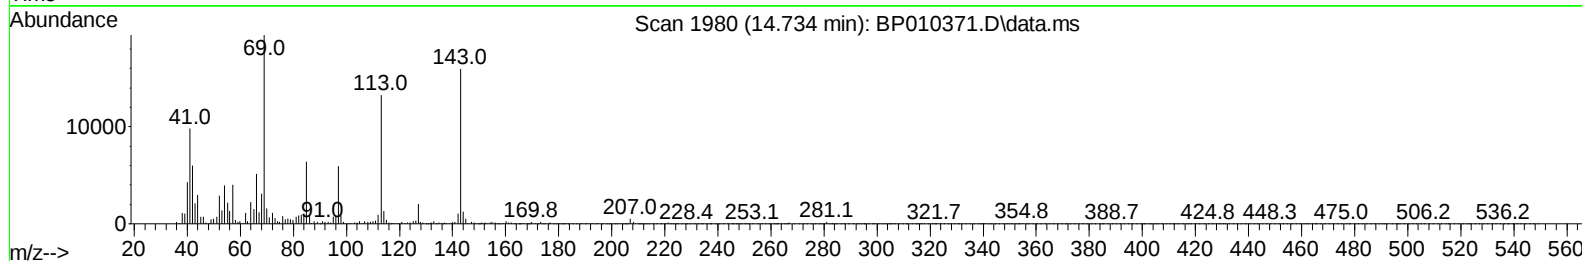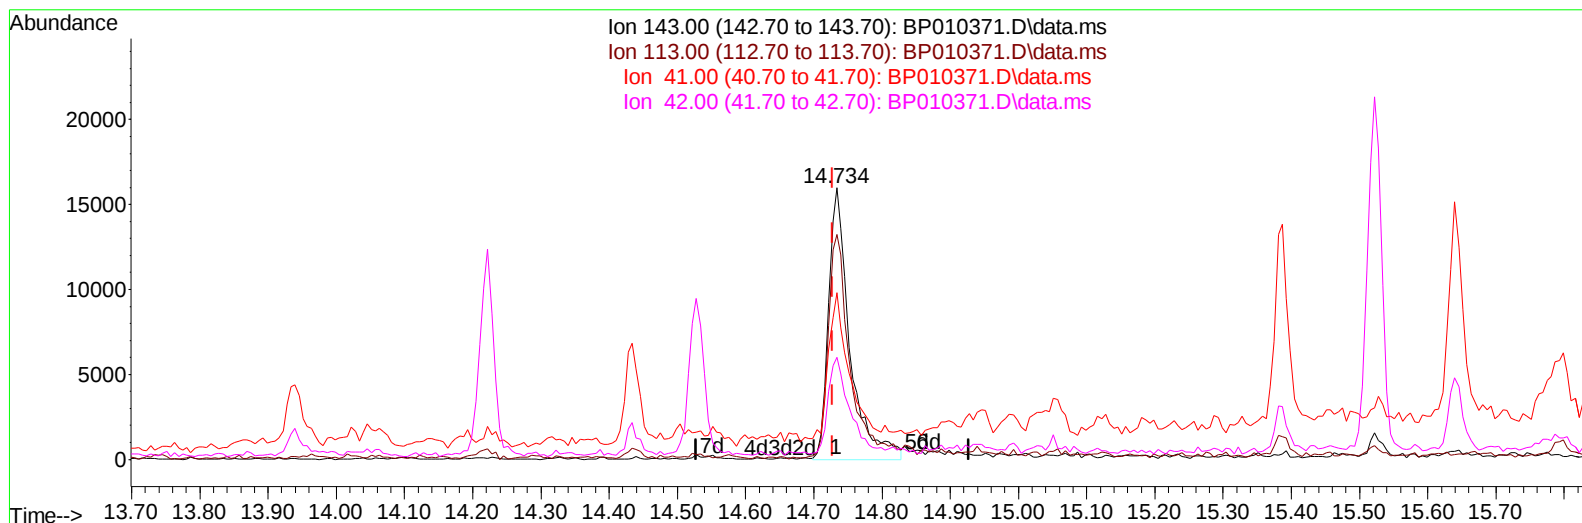

TIC: BP010371.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.006) 7.19 ng/ul m

response 34861

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	82.98#
41.00	23.20	61.43#
42.00	18.00	37.70#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010371.D
 Acq On : 16 May 2022 23:10
 Operator : CG/JU
 Sample : N2831-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 00:36:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	122134	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	529399	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	369735	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	813495	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.363	240	878625	20.000	ng/ul	# 0.00
88) Perylene-d12	23.792	264	864233	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	14600m	5.095	ng/uL	0.00
4) Pyridine-d5	3.770	84	76533	9.407	ng/ul	0.00
7) Phenol-d5	7.064	99	73920	7.211	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	234251	34.012	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	213238	27.185	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	152791	17.539	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	145418	35.492	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	149807	34.501	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	275821	33.595	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	341433	27.969	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	1133836	41.623	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1183545	37.667	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	34861m	7.190	ng/ul	0.00
60) Fluorene-d10	15.522	176	976241	41.193	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	165691	34.826	ng/ul	0.00
73) Anthracene-d10	17.381	188	1662193	45.124	ng/ul	0.00
81) Pyrene-d10	19.616	212	2100950	45.026	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	2018554	46.514	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010371.D
Acq On : 16 May 2022 23:10
Operator : CG/JU
Sample : N2831-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 00:36:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

