




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010372.D
 Acq On : 16 May 2022 23:44
 Operator : CG/JU
 Sample : N2831-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J8

Manual IntegrationsAPPROVED

Quant Time: May 17 00:36:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

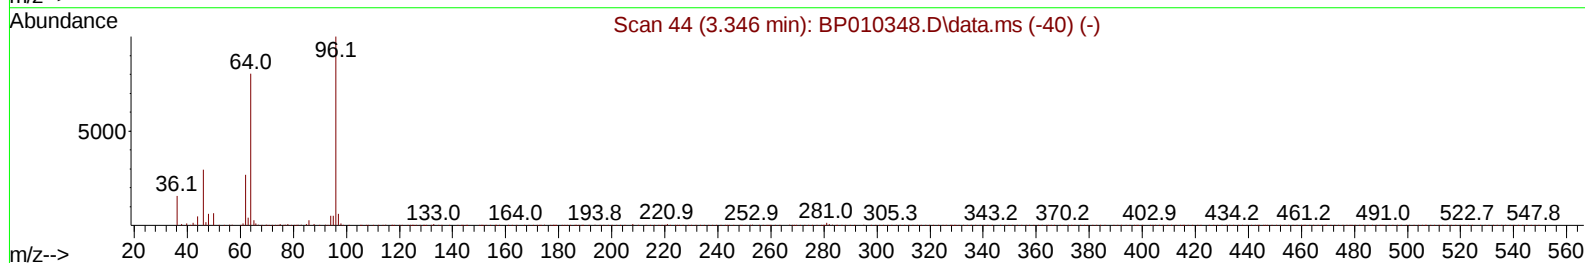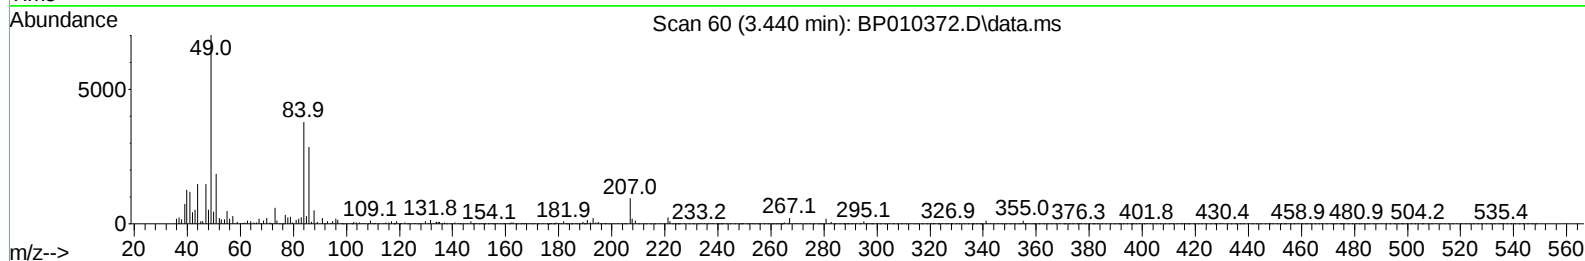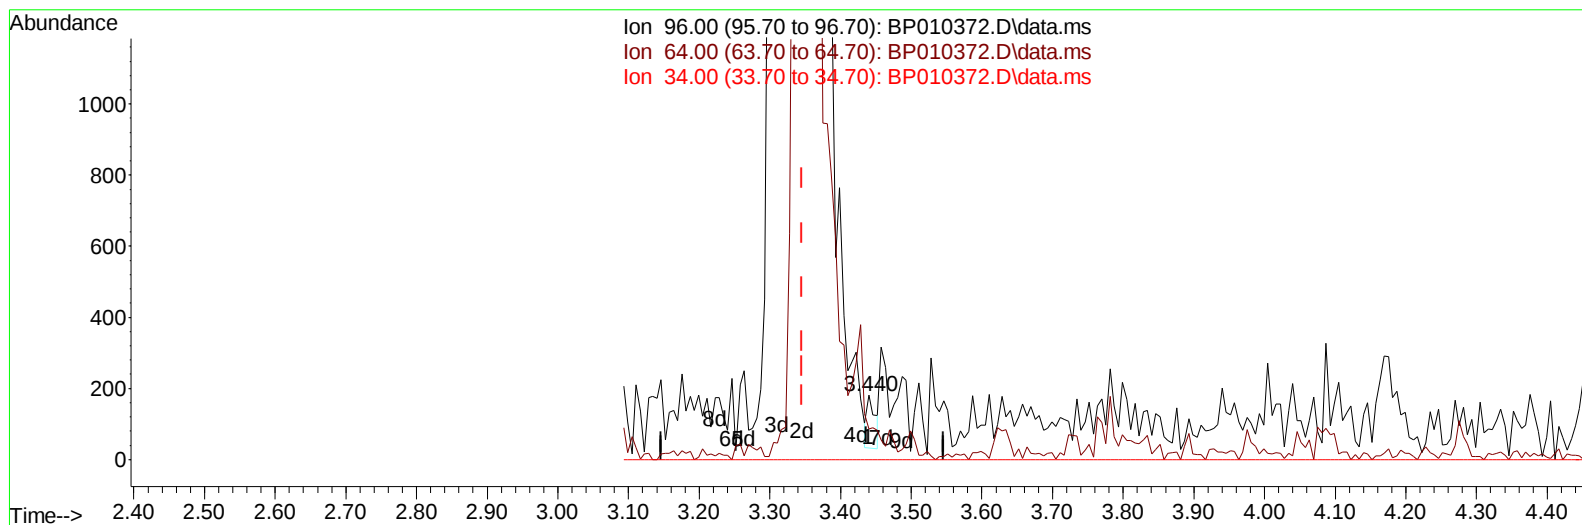

TIC: BP010372.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.440min (+ 0.094) 0.03 ng/uL

response 118

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	47.51
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010372.D
 Acq On : 16 May 2022 23:44
 Operator : CG/JU
 Sample : N2831-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J8

Manual IntegrationsAPPROVED

Quant Time: May 17 00:36:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

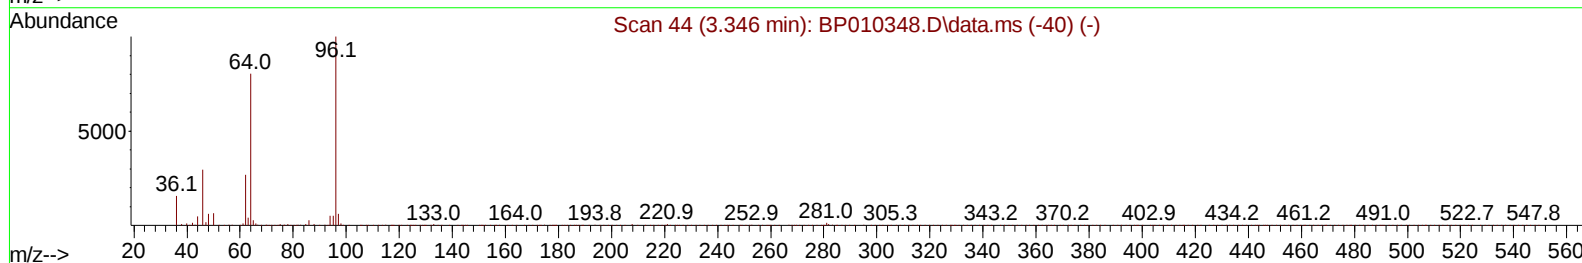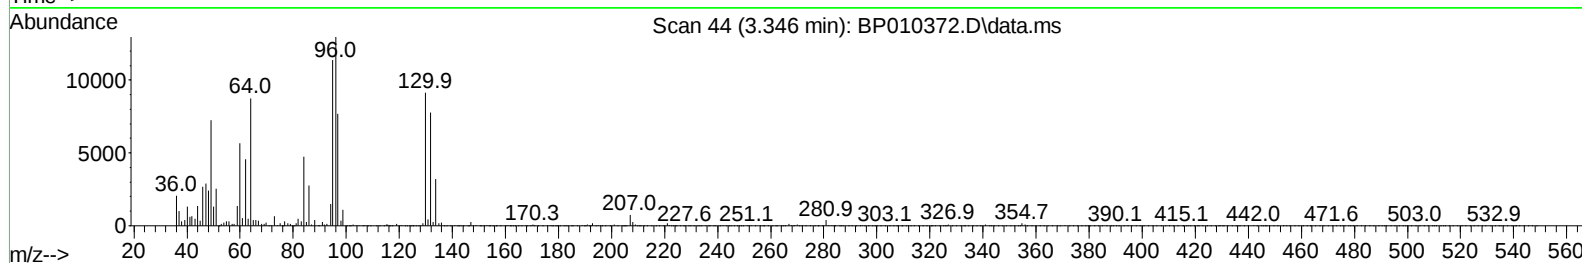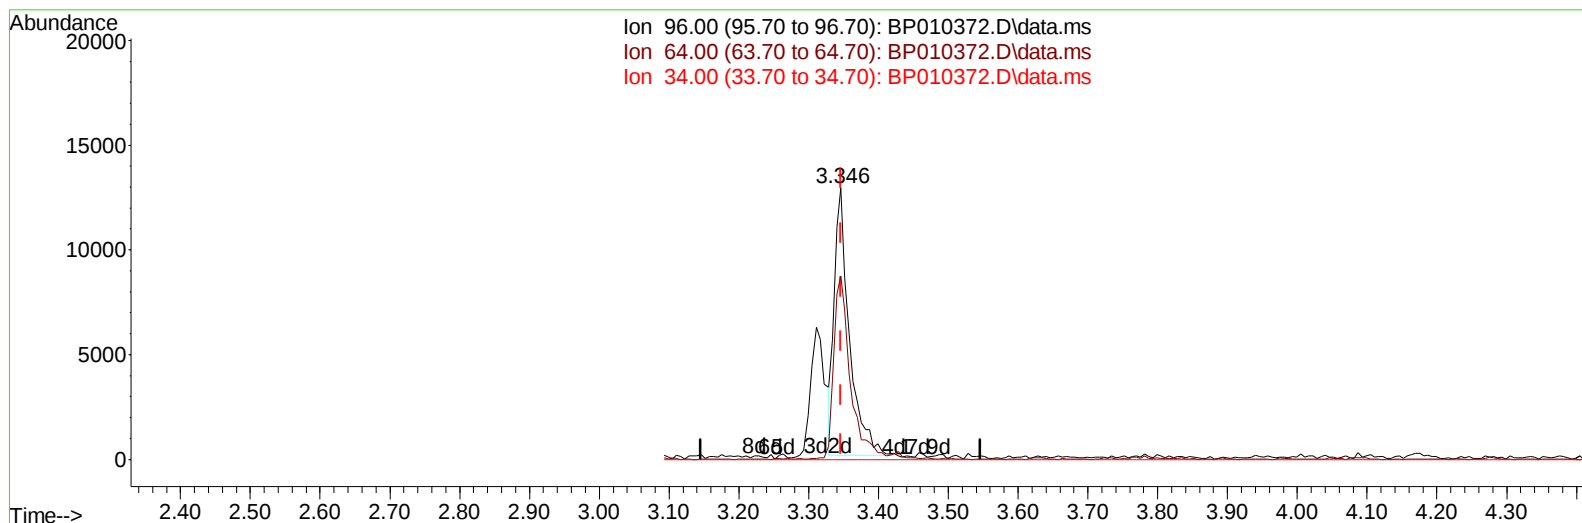

TIC: BP010372.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (-0.000) 5.04 ng/uL m

response 19279

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	67.53#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010372.D
 Acq On : 16 May 2022 23:44
 Operator : CG/JU
 Sample : N2831-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 00:36:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	163170	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	721024	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	494414	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	1081793	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.363	240	1072490	20.000	ng/ul	# 0.00
88) Perylene-d12	23.792	264	975595	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	19279m	5.036	ng/uL	0.00
4) Pyridine-d5	3.775	84	64390	5.924	ng/ul	0.01
7) Phenol-d5	7.063	99	88443	6.458	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	302569	32.883	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	267377	25.514	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	183561	15.772	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	190973	34.223	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	195228	33.013	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	326124	29.165	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	412172	24.791	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	1239406	34.025	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1436285	34.183	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	26654	4.111	ng/ul	0.00
60) Fluorene-d10	15.522	176	1091493	34.442	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	159142	25.154	ng/ul	0.00
73) Anthracene-d10	17.381	188	1712207	34.954	ng/ul	0.00
81) Pyrene-d10	19.616	212	2059697	36.163	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1699302	34.688	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010372.D
Acq On : 16 May 2022 23:44
Operator : CG/JU
Sample : N2831-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 00:36:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

