




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

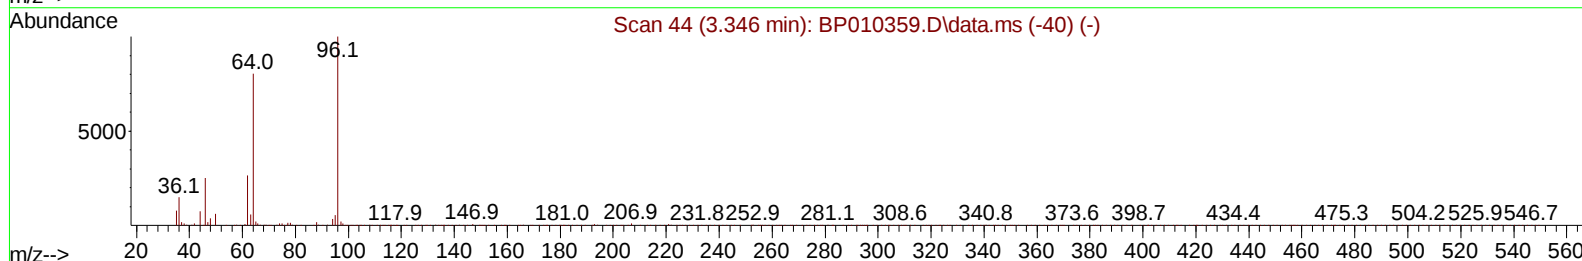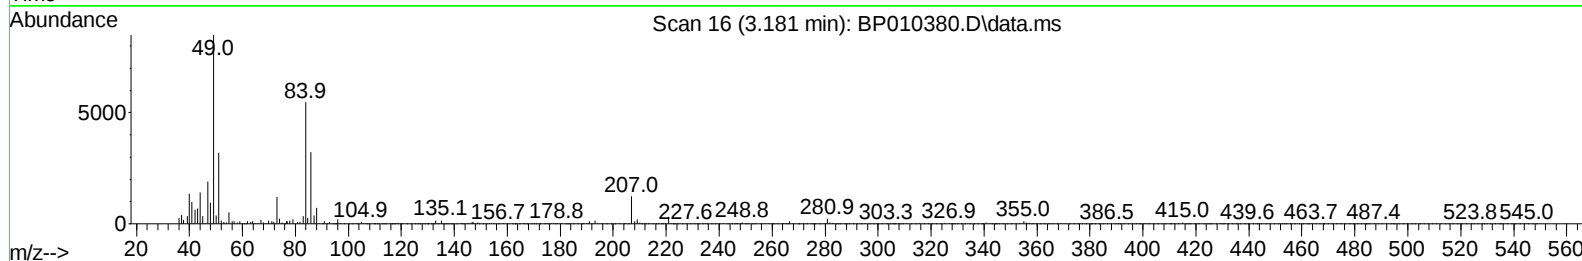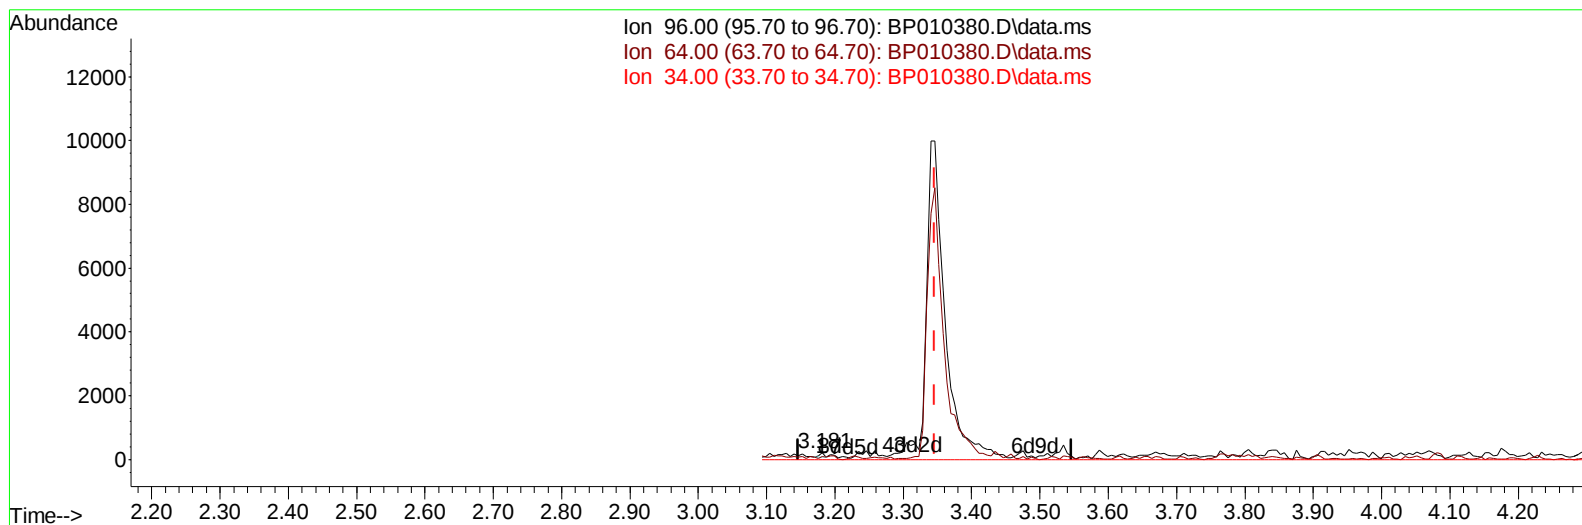

TIC: BP010380.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.181min (-0.165) 0.02 ng/uL

response 70

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	49.04
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

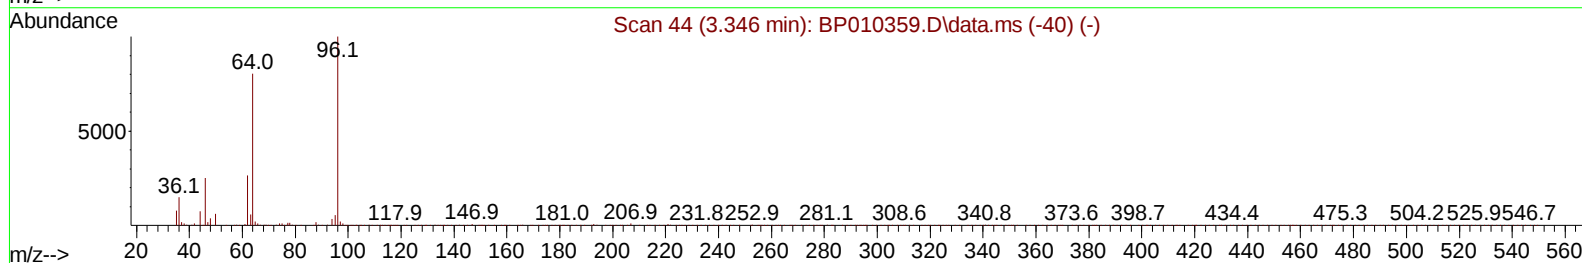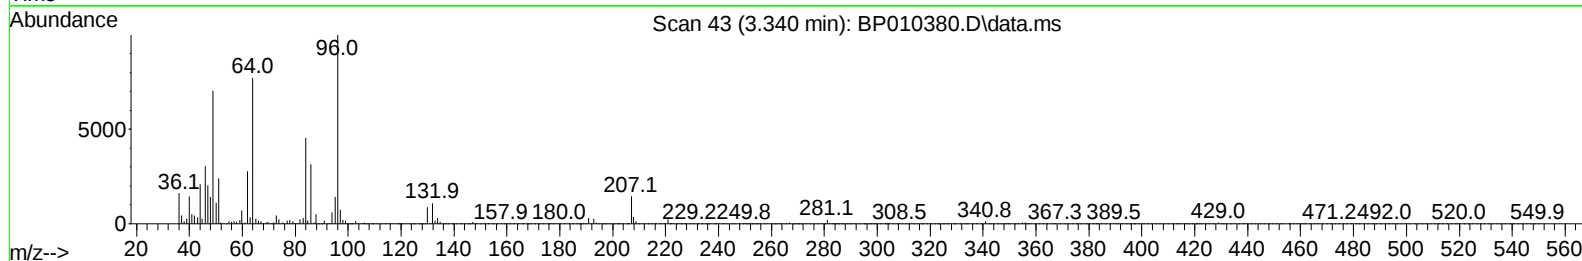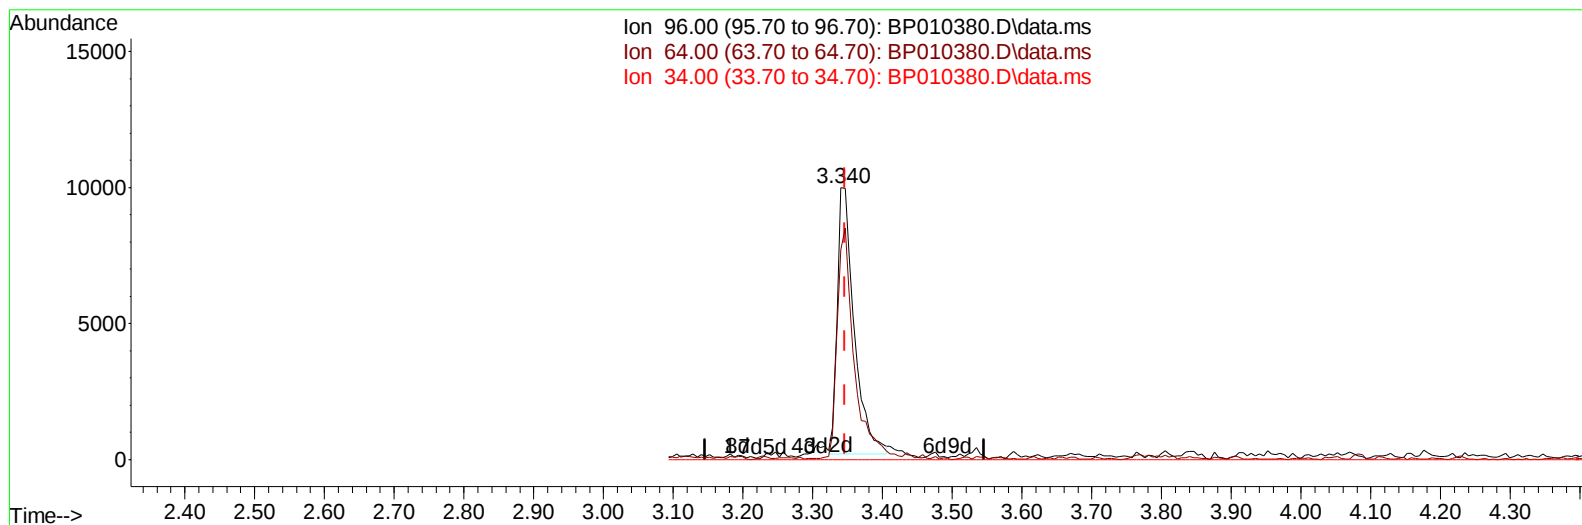

TIC: BP010380.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 4.85 ng/uL m

response 16604

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	77.28#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

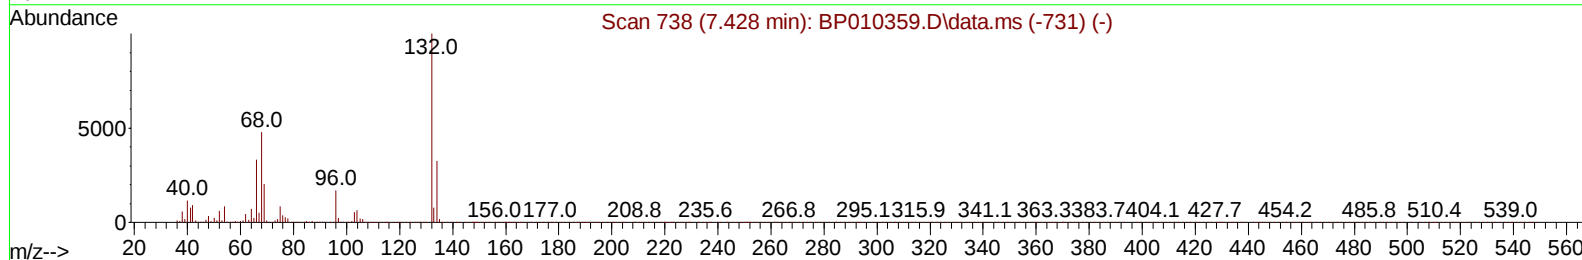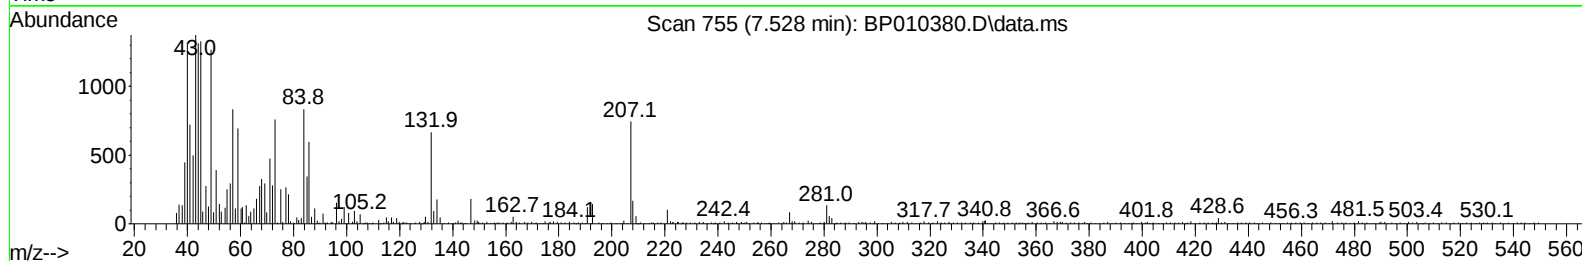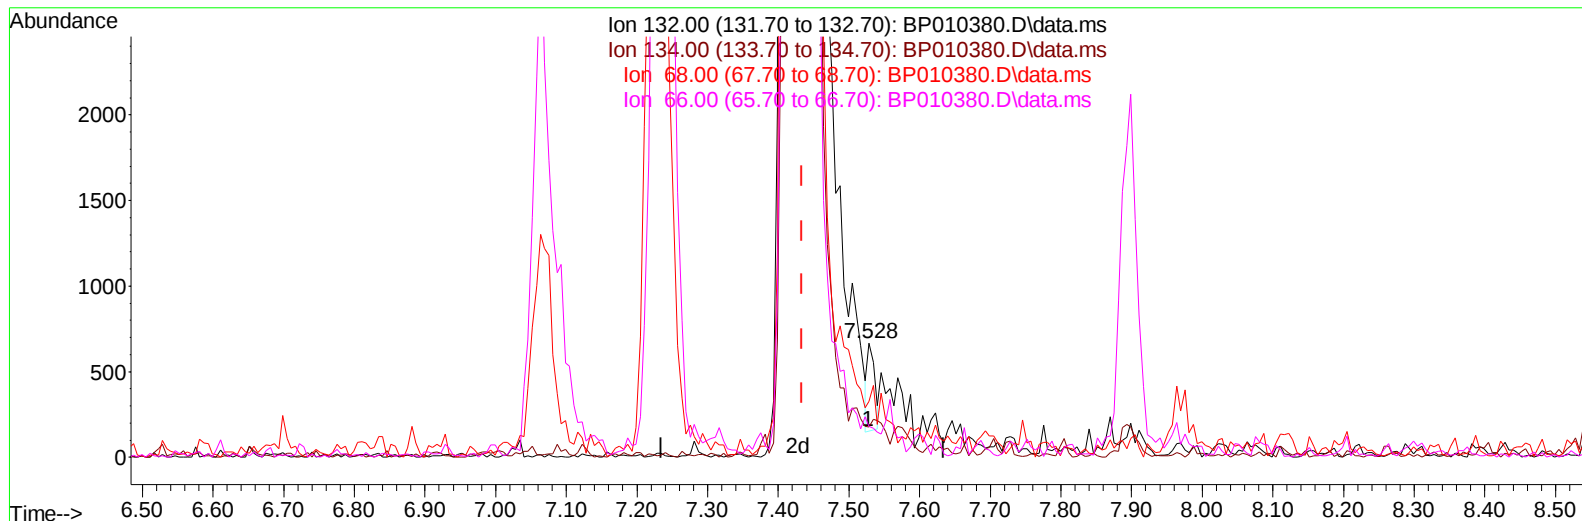

TIC: BP010380.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.528min (+ 0.094) 0.04 ng/u1

response 371

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	26.65
68.00	51.40	49.10
66.00	26.30	26.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

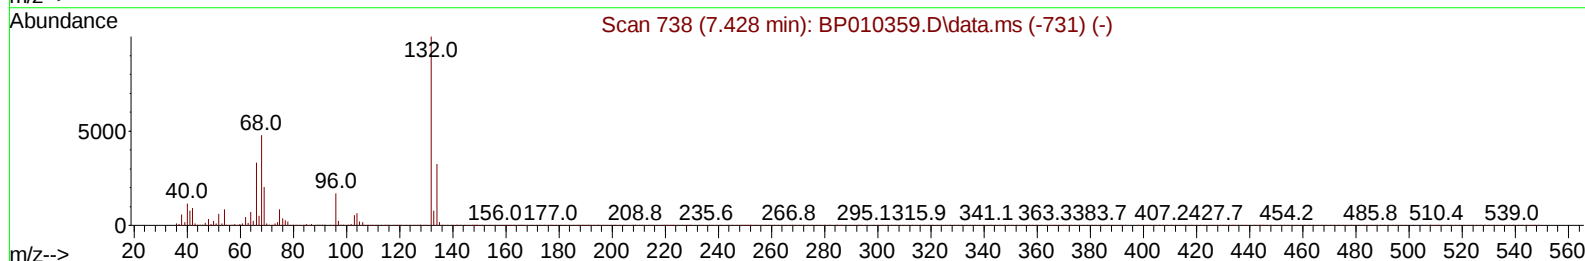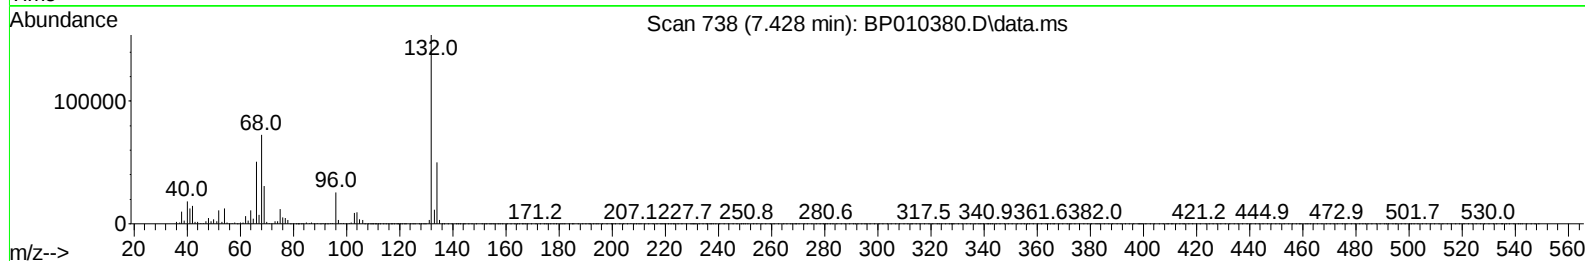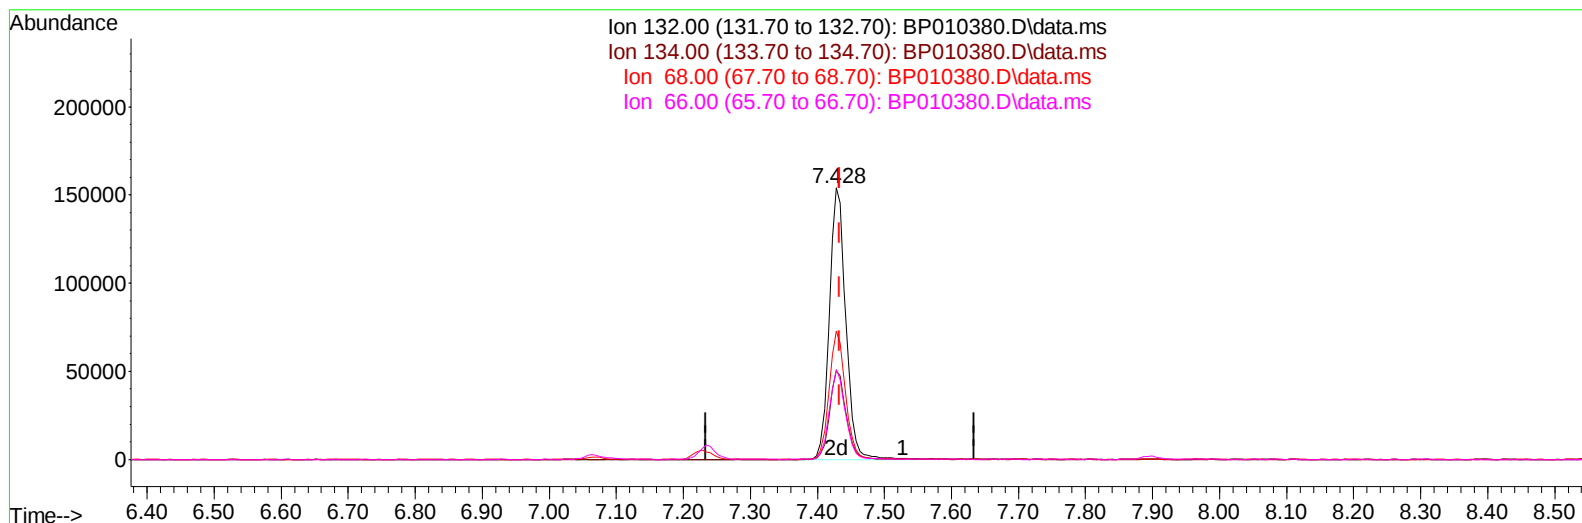

TIC: BP010380.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.428min (-0.006) 28.00 ng/u1 m

response 262391

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	32.67
68.00	51.40	47.23
66.00	26.30	33.03#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

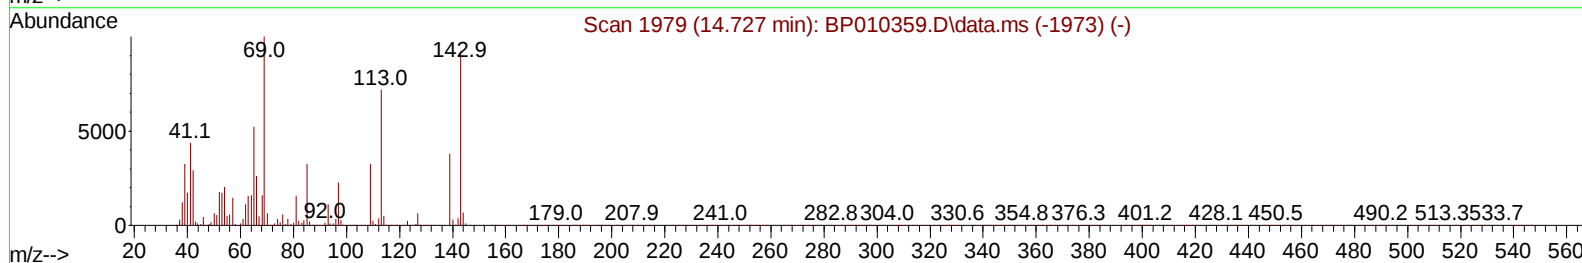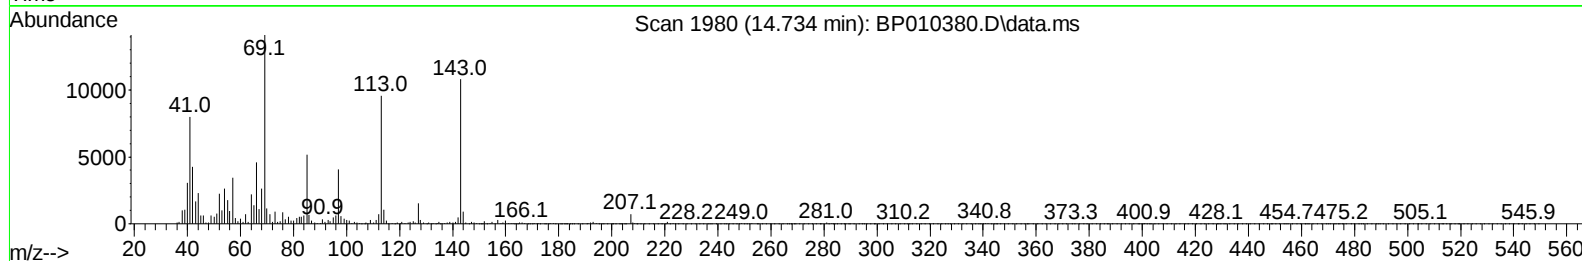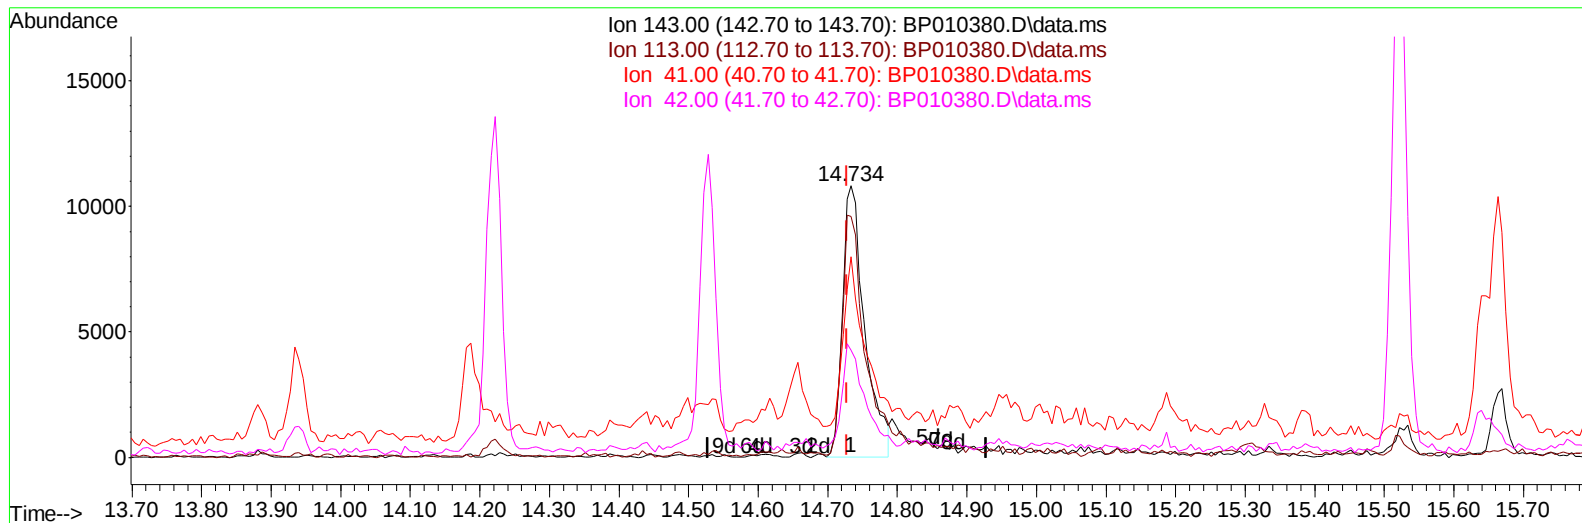

TIC: BP010380.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.006) 4.14 ng/ul

response 23889

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	88.73#
41.00	23.20	73.87#
42.00	18.00	39.60#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

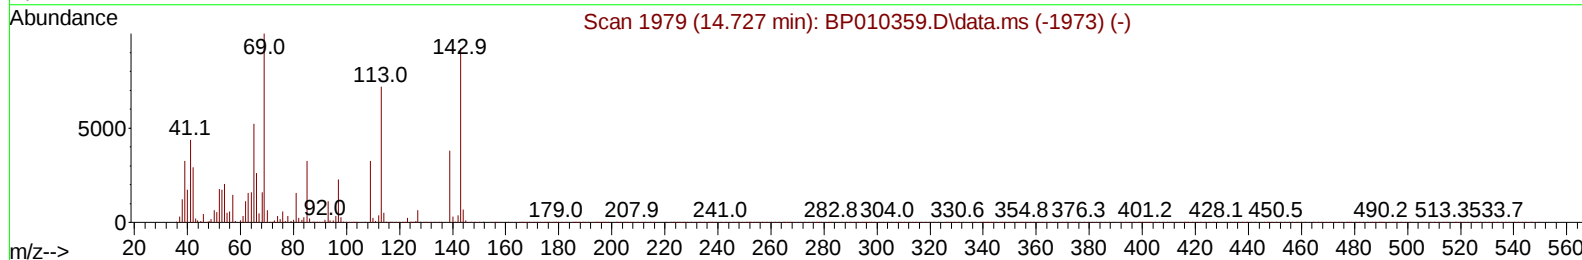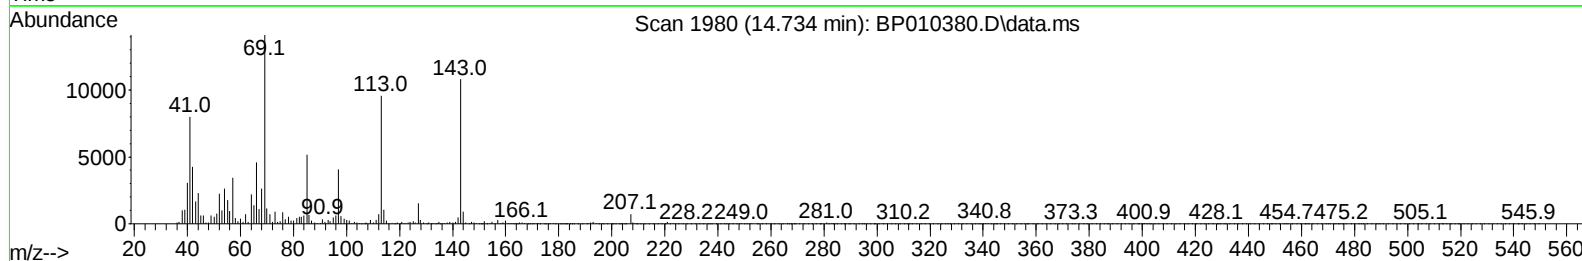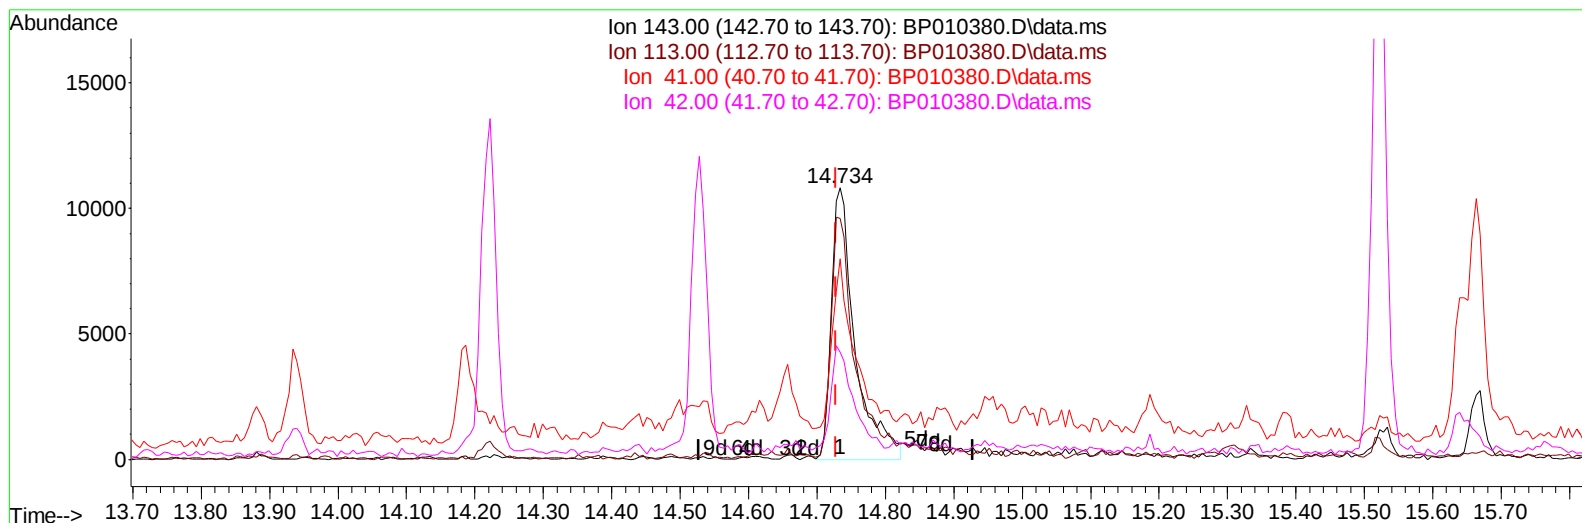

TIC: BP010380.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (+ 0.006) 4.52 ng/ul m

response 26081

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	88.73#
41.00	23.20	73.87#
42.00	18.00	39.60#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010380.D
 Acq On : 17 May 2022 04:48
 Operator : CG/JU
 Sample : N2831-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2K3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 07:07:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	145897	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	622351	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.528	164	440382	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.281	188	998647	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.363	240	1046217	20.000	ng/ul	# 0.00
88) Perylene-d12	23.792	264	957210	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	16604m	4.851	ng/uL	0.00
4) Pyridine-d5	3.770	84	91154	9.379	ng/ul	0.00
7) Phenol-d5	7.064	99	86991	7.104	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	281399	34.203	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	262391m	28.003	ng/ul	0.00
15) 4-Methylphenol-d8	8.611	113	175244	16.840	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	172321	35.777	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	176389	34.556	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	309806	32.098	ng/ul	0.03
31) 4-Chloroaniline-d4	10.834	131	377909	26.333	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	1124895	34.670	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	1328875	35.507	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	26081m	4.516	ng/ul	0.00
60) Fluorene-d10	15.522	176	1021042	36.172	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.640	200	79151	13.552	ng/ul	0.00
73) Anthracene-d10	17.381	188	1636640	36.193	ng/ul	0.00
81) Pyrene-d10	19.616	212	2005278	36.091	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1746300	36.332	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010380.D
Acq On : 17 May 2022 04:48
Operator : CG/JU
Sample : N2831-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2K3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 07:07:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

