

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010360.D
 Acq On : 16 May 2022 16:56
 Operator : CG/JU
 Sample : PB144708BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK708

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	52	rBV	30343	46869	1.19%	0.119%
2	3.764	111	115	136	rBV	385874	790716	20.09%	2.012%
3	4.087	166	170	176	rBV3	8829	13555	0.34%	0.034%
4	7.064	669	676	692	rBV	555971	944818	24.01%	2.405%
5	7.228	697	704	716	rVV	462961	751395	19.10%	1.912%
6	7.428	730	738	748	rBV	577111	956866	24.32%	2.435%
7	7.899	810	818	829	rBV	473175	781241	19.85%	1.988%
8	8.605	931	938	956	rBV	715445	1223839	31.10%	3.115%
9	9.058	1008	1015	1030	rVV	600881	1038616	26.39%	2.643%
10	9.781	1127	1138	1156	rBV	493375	858885	21.83%	2.186%
11	10.322	1222	1230	1245	rBV	682897	1235673	31.40%	3.145%
12	10.699	1286	1294	1307	rBV	680086	1185167	30.12%	3.016%
13	10.834	1310	1317	1339	rBV	674351	1321844	33.59%	3.364%
14	12.304	1561	1567	1575	rBV5	9277	20476	0.52%	0.052%
15	13.940	1838	1845	1860	rBV	1485670	2062793	52.42%	5.250%
16	14.222	1886	1893	1904	rBV	1559754	2269913	57.69%	5.777%
17	14.534	1939	1946	1958	rBV	1089615	1676201	42.60%	4.266%
18	14.728	1973	1979	2003	rBV	453105	951033	24.17%	2.420%
19	15.345	2080	2084	2090	rBV9	2970	5315	0.14%	0.014%
20	15.522	2107	2114	2129	rBV	2008595	2959152	75.20%	7.531%
21	15.645	2129	2135	2151	rVV	637220	982947	24.98%	2.502%
22	15.763	2151	2155	2163	rVB3	25283	46467	1.18%	0.118%
23	16.310	2243	2248	2252	rBV6	8471	12421	0.32%	0.032%
24	16.963	2355	2359	2365	rVV9	4952	8626	0.22%	0.022%
25	17.075	2372	2378	2381	rBV8	3290	6121	0.16%	0.016%
26	17.281	2407	2413	2422	rBV	1419377	2055644	52.24%	5.232%
27	17.381	2424	2430	2445	rVV2	2218874	3263814	82.94%	8.307%
28	19.192	2734	2738	2745	rBV3	30205	41949	1.07%	0.107%
29	19.263	2746	2750	2755	rVV3	21518	34019	0.86%	0.087%
30	19.616	2804	2810	2825	rBV	2894538	3935014	100.00%	10.015%
31	21.369	3102	3108	3121	rBV	1606705	2345786	59.61%	5.970%
32	23.639	3487	3494	3502	rBV2	1638079	3382731	85.96%	8.609%
33	23.798	3514	3521	3534	rVB2	969469	2081001	52.88%	5.296%




Sum of corrected areas: 39290907

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010360.D
Acq On : 16 May 2022 16:56
Operator : CG/JU
Sample : PB144708BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK708

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

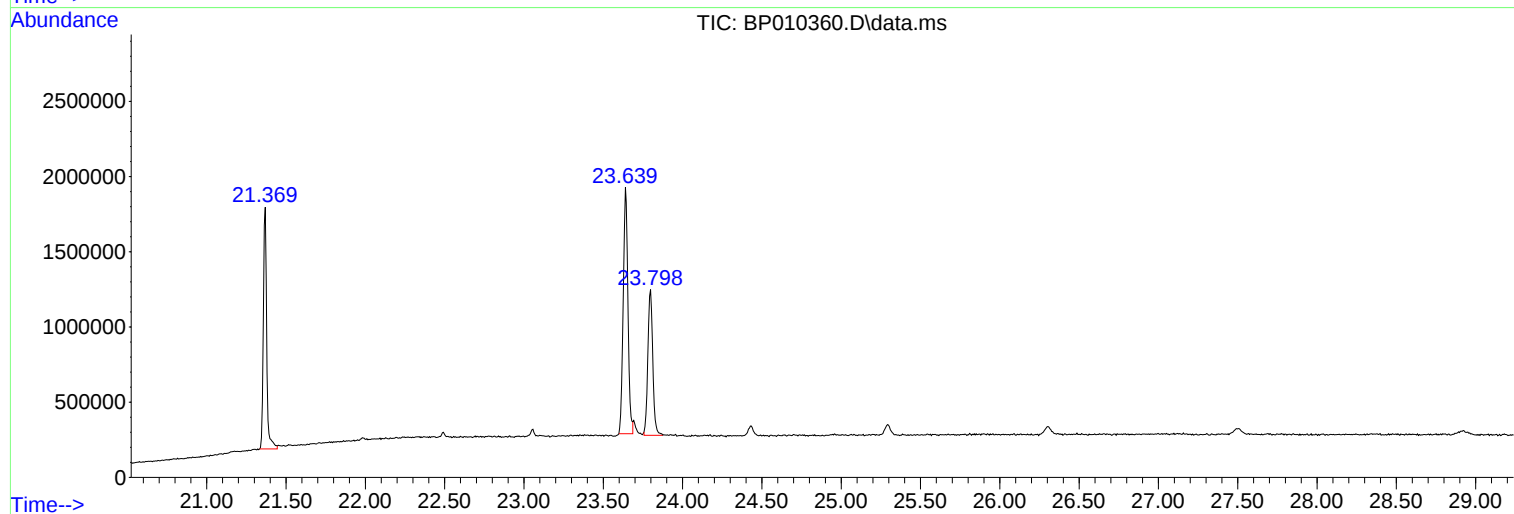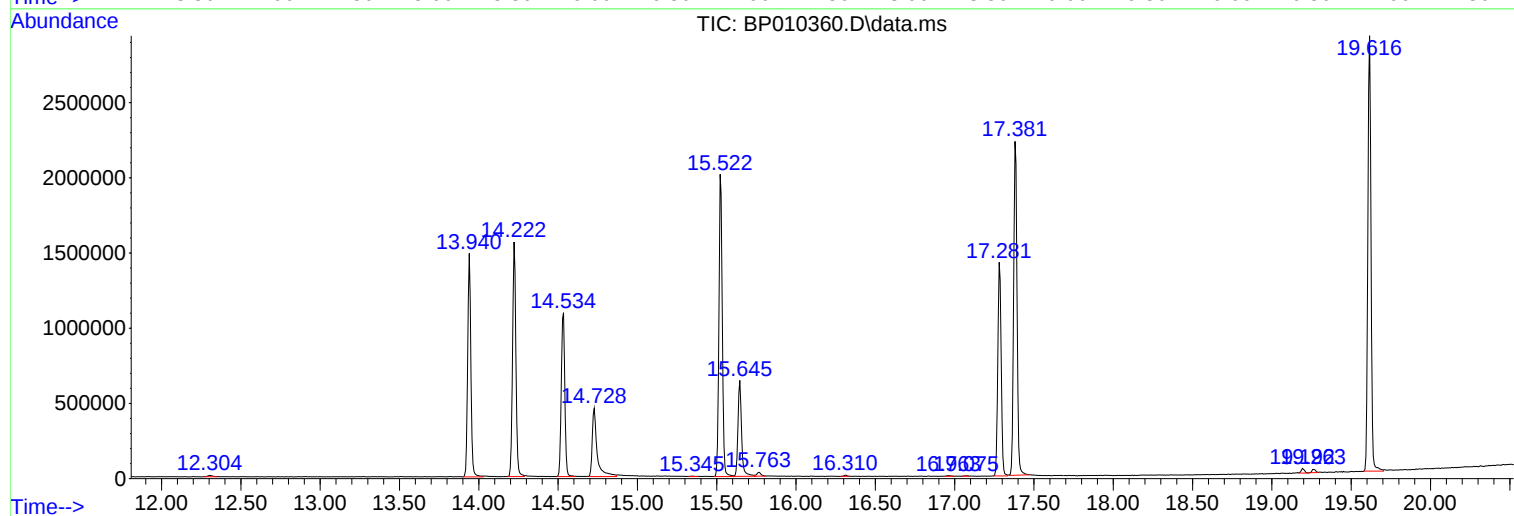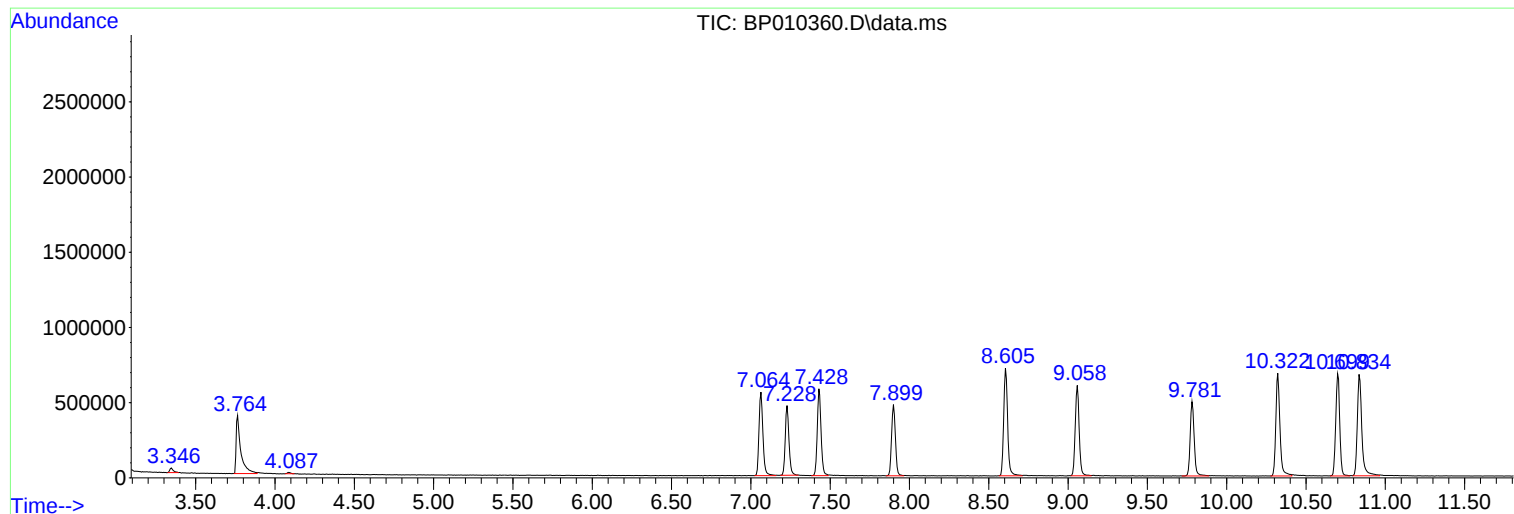

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010360.D
Acq On : 16 May 2022 16:56
Operator : CG/JU
Sample : PB144708BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK708

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010360.D
Acq On : 16 May 2022 16:56
Operator : CG/JU
Sample : PB144708BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK708

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------