

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010372.D
 Acq On : 16 May 2022 23:44
 Operator : CG/JU
 Sample : N2831-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	33	38	59	rVB2	381070	746531	14.24%	1.498%
2	3.775	113	117	133	rBV	93786	205755	3.93%	0.413%
3	4.087	166	170	177	rVB2	13066	20582	0.39%	0.041%
4	4.617	253	260	269	rBV	114338	190665	3.64%	0.383%
5	5.005	322	326	332	rVB2	6440	10469	0.20%	0.021%
6	6.405	556	564	569	rBV10	4163	10132	0.19%	0.020%
7	7.063	668	676	687	rBV	163693	286877	5.47%	0.576%
8	7.228	697	704	716	rBV	643941	1070921	20.43%	2.148%
9	7.310	716	718	723	rVB6	4603	6469	0.12%	0.013%
10	7.428	731	738	752	rBV	633825	1041367	19.87%	2.089%
11	7.522	752	754	762	rVB8	5711	11302	0.22%	0.023%
12	7.899	810	818	827	rBV	614331	1018107	19.43%	2.043%
13	7.969	827	830	836	rVB6	7222	12755	0.24%	0.026%
14	8.605	929	938	951	rBV	508489	864160	16.49%	1.734%
15	9.057	1006	1015	1032	rBV	863165	1496199	28.55%	3.002%
16	9.222	1039	1043	1051	rVB7	13455	22640	0.43%	0.045%
17	9.499	1085	1090	1095	rBV2	11776	19774	0.38%	0.040%
18	9.781	1130	1138	1156	rBV	665557	1176101	22.44%	2.359%
19	10.322	1222	1230	1246	rBV	918660	1614358	30.80%	3.239%
20	10.699	1286	1294	1309	rBV	911396	1552305	29.62%	3.114%
21	10.834	1309	1317	1339	rBV	765663	1445593	27.58%	2.900%
22	11.993	1508	1514	1519	rBV3	7967	14068	0.27%	0.028%
23	12.134	1534	1538	1543	rVB6	5680	11363	0.22%	0.023%
24	12.287	1558	1564	1575	rBV2	15230	32030	0.61%	0.064%
25	13.363	1743	1747	1752	rVB	15381	20274	0.39%	0.041%
26	13.940	1838	1845	1858	rBV	1973268	2777810	53.00%	5.573%
27	14.222	1884	1893	1908	rBV	2177540	3209764	61.25%	6.439%
28	14.322	1908	1910	1918	rVV7	5511	11579	0.22%	0.023%
29	14.398	1918	1923	1927	rVV8	4940	9693	0.18%	0.019%
30	14.440	1927	1930	1933	rVB5	5407	6337	0.12%	0.013%
31	14.528	1938	1945	1960	rBV	1442880	2172308	41.45%	4.358%
32	14.734	1973	1980	1994	rBV2	71765	206781	3.95%	0.415%
33	14.951	2013	2017	2023	rVB8	5421	9601	0.18%	0.019%
34	15.345	2077	2084	2088	rBV10	5280	9912	0.19%	0.020%
35	15.522	2107	2114	2128	rBV	2740264	4115627	78.53%	8.257%
36	15.639	2128	2134	2149	rVV	806326	1226861	23.41%	2.461%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010372.D
 Acq On : 16 May 2022 23:44
 Operator : CG/JU
 Sample : N2831-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YB2J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	15.763	2151	2155	2165	rVB	34416	57058	1.09%	0.114%
38	15.892	2174	2177	2181	rVB6	4396	6709	0.13%	0.013%
39	16.310	2244	2248	2253	rVB3	11269	16435	0.31%	0.033%
40	16.534	2280	2286	2294	rVV3	4357	11931	0.23%	0.024%
41	16.957	2356	2358	2364	rVB6	5406	8458	0.16%	0.017%
42	17.051	2370	2374	2378	rBV7	9389	18878	0.36%	0.038%
43	17.081	2378	2379	2387	rVB7	8072	13605	0.26%	0.027%
44	17.281	2404	2413	2423	rBV	1897243	2665405	50.86%	5.347%
45	17.381	2423	2430	2453	rVB	3035907	4478788	85.46%	8.985%
46	17.563	2459	2461	2466	rBV6	4814	7282	0.14%	0.015%
47	17.945	2524	2526	2530	rVB5	7969	9676	0.18%	0.019%
48	18.169	2560	2564	2565	rBV3	27928	33852	0.65%	0.068%
49	18.186	2565	2567	2573	rVV	41422	58336	1.11%	0.117%
50	18.239	2573	2576	2583	rVB2	24424	32636	0.62%	0.065%
51	19.192	2734	2738	2745	rVB3	37110	51528	0.98%	0.103%
52	19.263	2746	2750	2757	rBV	37137	57556	1.10%	0.115%
53	19.616	2804	2810	2822	rBV	3823956	5240743	100.00%	10.514%
54	21.074	3054	3058	3064	rBV2	102919	179340	3.42%	0.360%
55	21.363	3102	3107	3118	rBV	2041417	2879435	54.94%	5.777%
56	23.639	3486	3494	3509	rVB	2331902	4729500	90.24%	9.488%
57	23.792	3513	3520	3534	rVB2	1257252	2631396	50.21%	5.279%




Sum of corrected areas: 49845617

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010372.D
Acq On : 16 May 2022 23:44
Operator : CG/JU
Sample : N2831-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

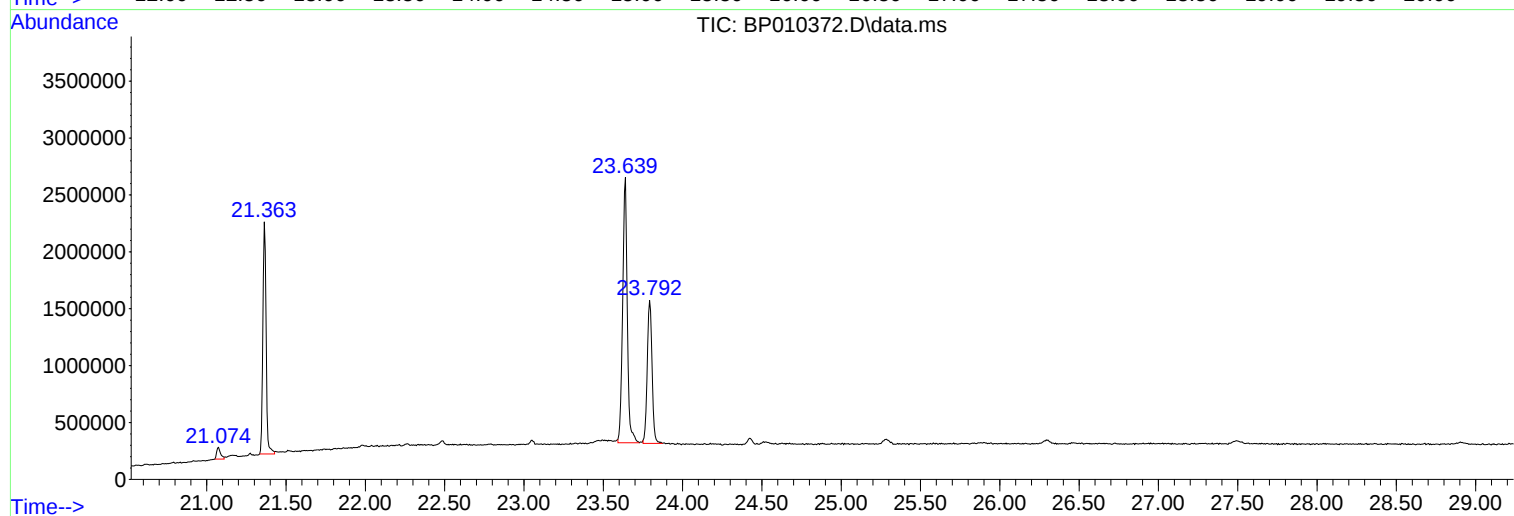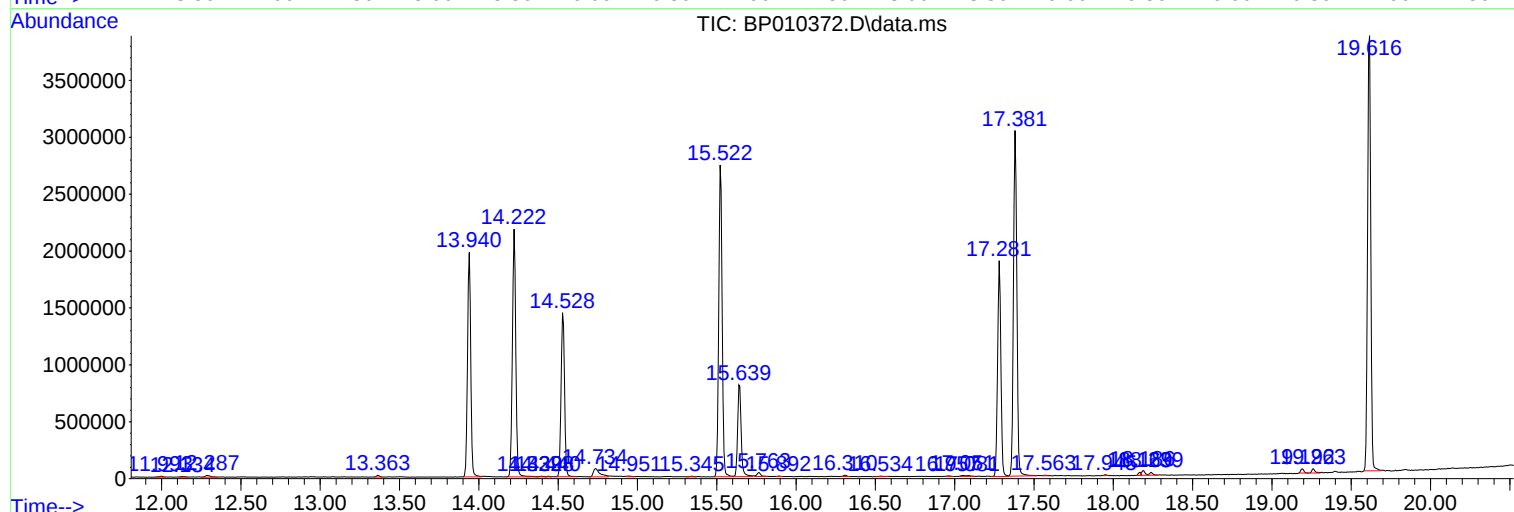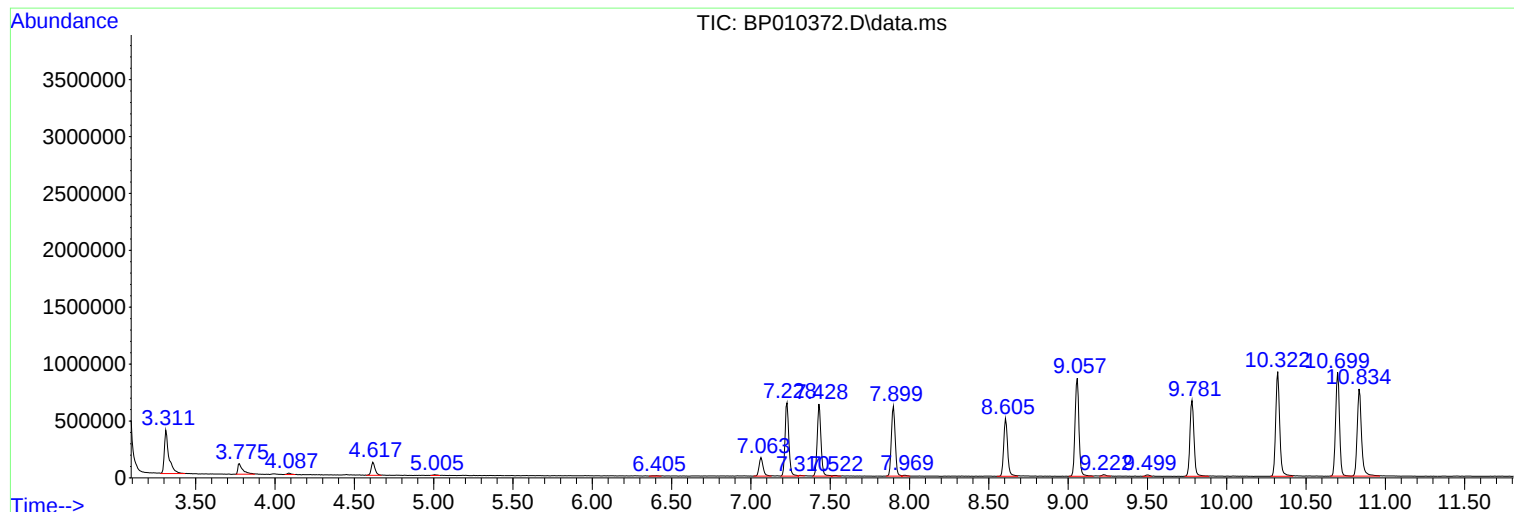

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010372.D
Acq On : 16 May 2022 23:44
Operator : CG/JU
Sample : N2831-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010372.D
Acq On : 16 May 2022 23:44
Operator : CG/JU
Sample : N2831-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YB2J8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------