

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010373.D
 Acq On : 17 May 2022 00:18
 Operator : CG/JU
 Sample : N2801-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	49	rVB3	12600	16776	0.36%	0.038%
2	3.775	113	117	131	rBV	89362	195646	4.22%	0.445%
3	3.993	151	154	160	rVB5	8249	12137	0.26%	0.028%
4	4.087	167	170	173	rBV3	10403	13028	0.28%	0.030%
5	5.011	323	327	329	rBV3	5869	7922	0.17%	0.018%
6	5.410	392	395	400	rVB2	10014	16571	0.36%	0.038%
7	5.910	474	480	485	rBV5	8554	14054	0.30%	0.032%
8	6.387	555	561	568	rVB2	18439	29873	0.64%	0.068%
9	6.881	640	645	655	rBV	27263	48016	1.04%	0.109%
10	7.063	670	676	686	rBV2	133102	231449	4.99%	0.526%
11	7.228	696	704	710	rBV	528184	865569	18.67%	1.967%
12	7.287	710	714	722	rVB	141799	233063	5.03%	0.530%
13	7.428	731	738	751	rBV	519951	865332	18.66%	1.966%
14	7.799	798	801	808	rVV5	4858	8880	0.19%	0.020%
15	7.899	811	818	827	rVV	554170	912128	19.67%	2.073%
16	7.963	827	829	833	rVV5	6733	10843	0.23%	0.025%
17	8.016	833	838	844	rVB6	10734	20508	0.44%	0.047%
18	8.187	862	867	878	rBV7	4078	6728	0.15%	0.015%
19	8.275	877	882	888	rBV2	18260	33887	0.73%	0.077%
20	8.393	897	902	906	rBV3	14625	20734	0.45%	0.047%
21	8.546	923	928	931	rBV7	5636	10038	0.22%	0.023%
22	8.604	931	938	951	rVV	428223	732328	15.79%	1.664%
23	8.710	951	956	963	rVB2	15946	30675	0.66%	0.070%
24	9.010	1002	1007	1009	rBV2	22824	35870	0.77%	0.082%
25	9.057	1009	1015	1028	rVB	702626	1274759	27.49%	2.897%
26	9.346	1060	1064	1071	rVB6	6126	10523	0.23%	0.024%
27	9.504	1087	1091	1092	rBV4	5474	7445	0.16%	0.017%
28	9.528	1092	1095	1100	rVB2	11535	18687	0.40%	0.042%
29	9.710	1121	1126	1129	rVB7	3462	4932	0.11%	0.011%
30	9.781	1129	1138	1152	rBV	560514	982292	21.19%	2.232%
31	10.034	1177	1181	1182	rBV3	5391	5988	0.13%	0.014%
32	10.098	1187	1192	1199	rVV	28396	50394	1.09%	0.115%
33	10.198	1202	1209	1213	rVB8	4266	7547	0.16%	0.017%
34	10.322	1222	1230	1241	rBV	747555	1331345	28.71%	3.025%
35	10.404	1242	1244	1252	rVB7	11183	18301	0.39%	0.042%
36	10.698	1286	1294	1301	rBV	830905	1374502	29.64%	3.123%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010373.D
 Acq On : 17 May 2022 00:18
 Operator : CG/JU
 Sample : N2801-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	10.834	1309	1317	1329	rBV	590690	1119343	24.14%	2.544%
38	11.322	1396	1400	1404	rBV7	5387	9778	0.21%	0.022%
39	11.510	1427	1432	1434	rBV6	3225	5036	0.11%	0.011%
40	11.740	1467	1471	1474	rBV5	4032	5512	0.12%	0.013%
41	12.010	1514	1517	1523	rVV8	3045	6018	0.13%	0.014%
42	12.093	1523	1531	1535	rVV7	13083	27926	0.60%	0.063%
43	12.128	1535	1537	1543	rVB7	5808	7678	0.17%	0.017%
44	12.292	1556	1565	1566	rBV3	13640	23370	0.50%	0.053%
45	12.328	1566	1571	1576	rVB	33427	54142	1.17%	0.123%
46	12.428	1584	1588	1595	rVB7	6533	11667	0.25%	0.027%
47	12.528	1601	1605	1610	rBV5	5970	9407	0.20%	0.021%
48	12.575	1610	1613	1619	rVB7	5984	10167	0.22%	0.023%
49	12.816	1648	1654	1658	rBV7	4287	8346	0.18%	0.019%
50	12.998	1679	1685	1694	rBV4	12535	25370	0.55%	0.058%
51	13.081	1694	1699	1705	rVB10	4160	7480	0.16%	0.017%
52	13.263	1725	1730	1736	rBV8	4977	9464	0.20%	0.022%
53	13.363	1740	1747	1752	rVB4	16075	25563	0.55%	0.058%
54	13.498	1764	1770	1778	rVB5	22755	41103	0.89%	0.093%
55	13.669	1791	1799	1802	rBV5	11181	17734	0.38%	0.040%
56	13.704	1802	1805	1812	rVB7	8976	15112	0.33%	0.034%
57	13.939	1834	1845	1857	rBV	1683515	2378698	51.30%	5.405%
58	14.222	1883	1893	1908	rBV	1824625	2658044	57.33%	6.040%
59	14.357	1911	1916	1920	rVB7	6503	11331	0.24%	0.026%
60	14.434	1926	1929	1937	rVB9	6134	11159	0.24%	0.025%
61	14.528	1937	1945	1961	rBV	1304326	1971339	42.52%	4.480%
62	14.734	1973	1980	1992	rBV2	65912	168668	3.64%	0.383%
63	14.957	2011	2018	2035	rBV	356132	555106	11.97%	1.261%
64	15.163	2050	2053	2057	rVB6	4568	6375	0.14%	0.014%
65	15.339	2080	2083	2088	rBV5	4543	8182	0.18%	0.019%
66	15.522	2107	2114	2128	rBV	2408933	3444484	74.29%	7.827%
67	15.639	2128	2134	2148	rVV	668361	1033875	22.30%	2.349%
68	15.763	2151	2155	2164	rVB2	29829	49717	1.07%	0.113%
69	16.310	2243	2248	2255	rVB7	11719	20063	0.43%	0.046%
70	16.769	2322	2326	2328	rBV4	4130	4775	0.10%	0.011%
71	16.963	2355	2359	2363	rVB7	4670	7692	0.17%	0.017%
72	17.280	2406	2413	2423	rBV	1660000	2407130	51.92%	5.470%
73	17.380	2424	2430	2444	rVV2	2678796	3867004	83.40%	8.788%
74	17.951	2522	2527	2530	rBV7	5426	10266	0.22%	0.023%
75	18.169	2559	2564	2570	rBV3	33960	57586	1.24%	0.131%
76	18.233	2573	2575	2582	rVB4	7790	14044	0.30%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010373.D
 Acq On : 17 May 2022 00:18
 Operator : CG/JU
 Sample : N2801-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	18.451	2607	2612	2616	rBV8	6391	11863	0.26%	0.027%
78	19.192	2733	2738	2743	rBV3	35511	52098	1.12%	0.118%
79	19.263	2746	2750	2757	rVV	29275	44792	0.97%	0.102%
80	19.616	2803	2810	2822	rBV	3334247	4636624	100.00%	10.537%
81	21.069	3053	3057	3066	rBV	240317	415396	8.96%	0.944%
82	21.363	3102	3107	3119	rBV	2007400	2708317	58.41%	6.155%
83	23.639	3486	3494	3500	rBV2	2050278	4110457	88.65%	9.341%
84	23.792	3513	3520	3532	rVB	1193758	2441249	52.65%	5.548%




Sum of corrected areas: 44005320

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010373.D
Acq On : 17 May 2022 00:18
Operator : CG/JU
Sample : N2801-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

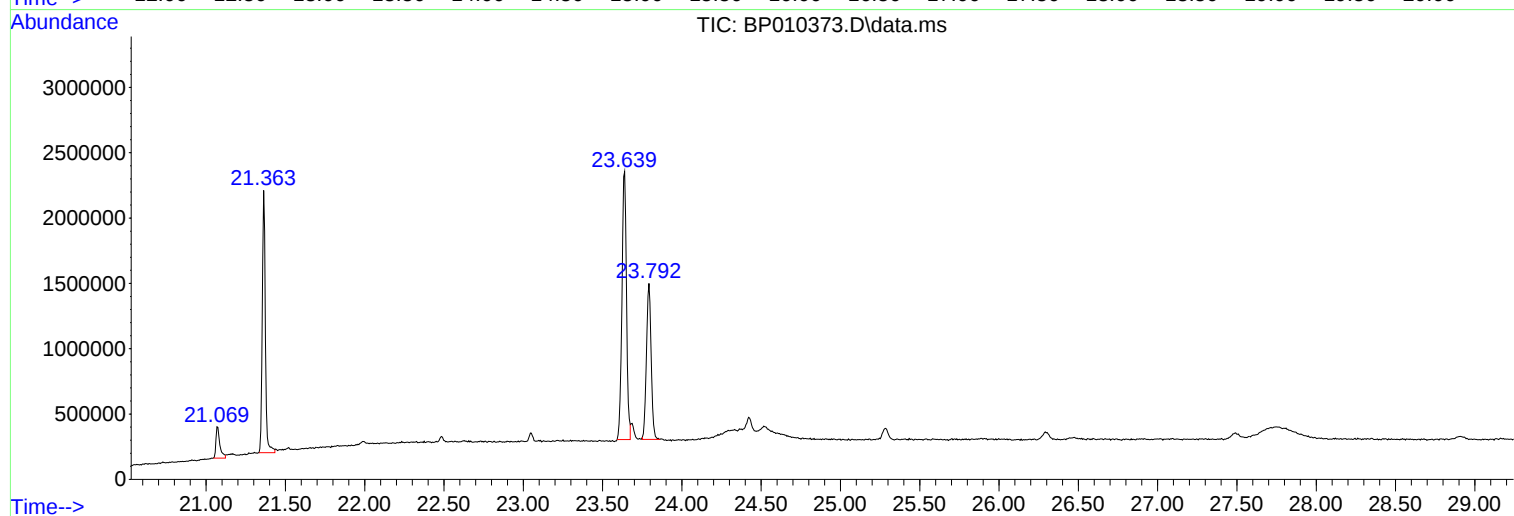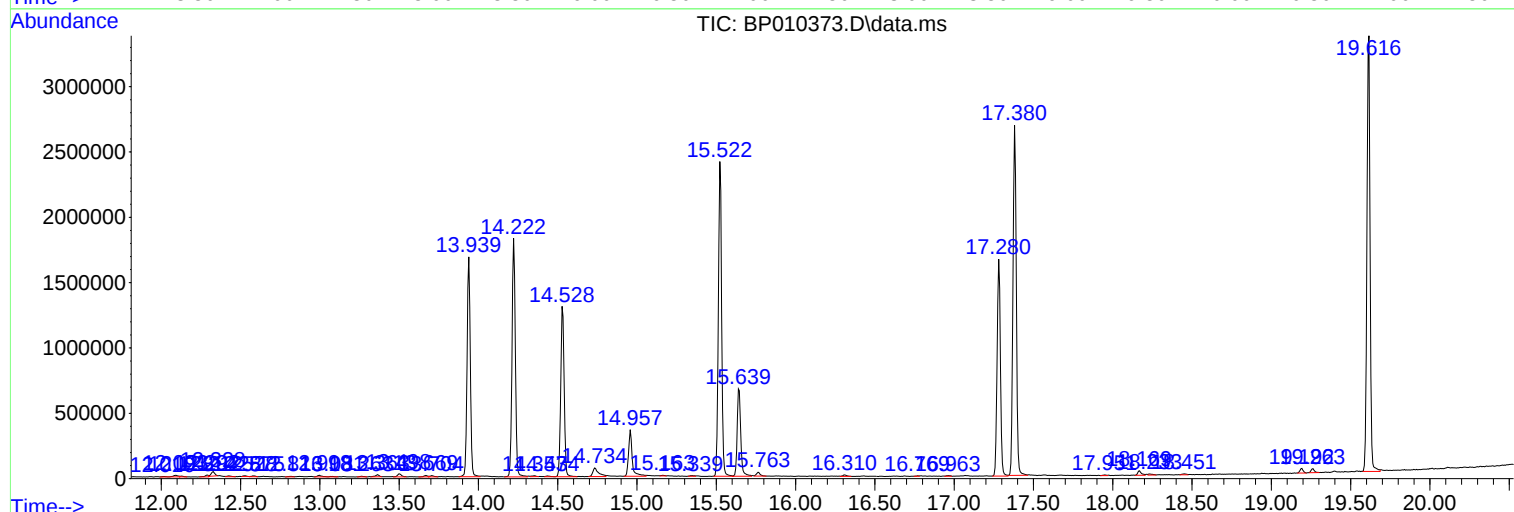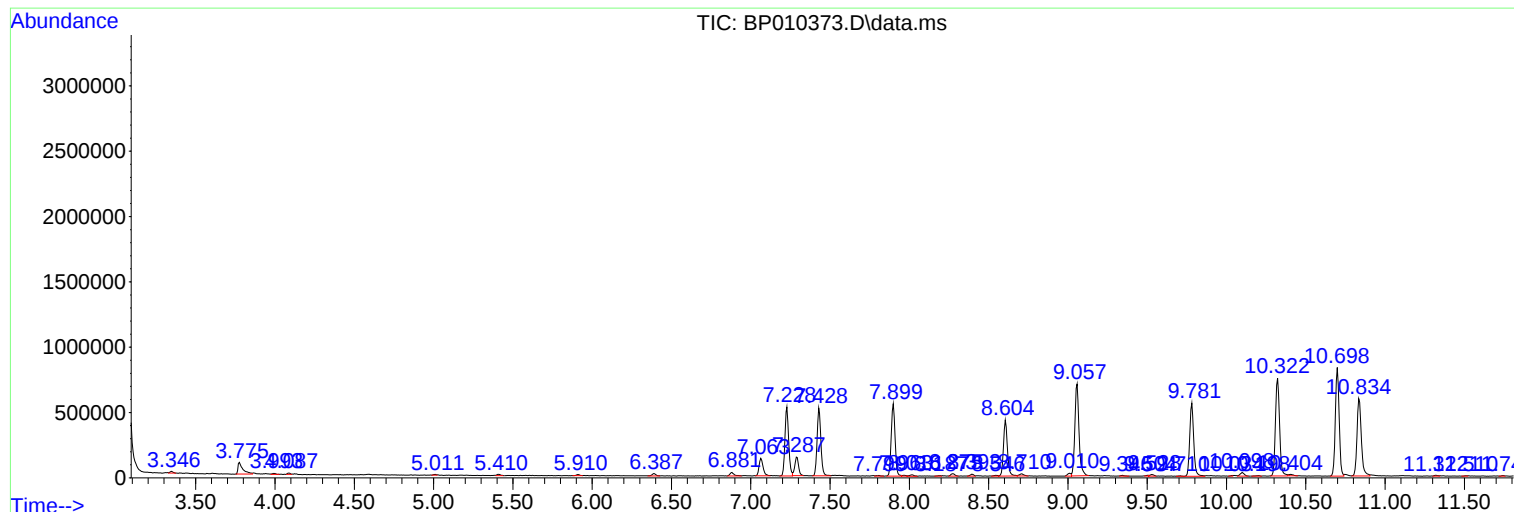

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010373.D
Acq On : 17 May 2022 00:18
Operator : CG/JU
Sample : N2801-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010373.D
Acq On : 17 May 2022 00:18
Operator : CG/JU
Sample : N2801-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc