

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
 Data File : BP010385.D
 Acq On : 17 May 2022 09:02
 Operator : CG/JU
 Sample : PB144810BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	52	rBV	54447	82133	1.21%	0.122%
2	3.764	111	115	145	rBV	731241	1500475	22.09%	2.236%
3	4.087	168	170	174	rVB3	8998	9853	0.15%	0.015%
4	7.063	669	676	695	rBV	1076264	1844522	27.16%	2.749%
5	7.228	698	704	719	rVV	860532	1421202	20.92%	2.118%
6	7.434	730	739	752	rBV	1118213	1840319	27.09%	2.743%
7	7.899	810	818	830	rBV	684709	1164084	17.14%	1.735%
8	8.610	930	939	959	rBV	1393387	2383187	35.09%	3.552%
9	9.063	1008	1016	1032	rBV	1183591	1971526	29.03%	2.939%
10	9.787	1130	1139	1153	rBV	968364	1657100	24.40%	2.470%
11	10.328	1223	1231	1248	rBV	1319443	2377806	35.01%	3.544%
12	10.704	1287	1295	1310	rBV	1033027	1759737	25.91%	2.623%
13	10.840	1310	1318	1346	rVV	1314165	2461969	36.25%	3.670%
14	12.299	1559	1566	1575	rBV	22698	43999	0.65%	0.066%
15	13.945	1838	1846	1860	rBV	2576519	3682958	54.22%	5.489%
16	14.045	1860	1863	1871	rVB9	4919	12081	0.18%	0.018%
17	14.228	1883	1894	1911	rBV	2760735	4169967	61.39%	6.215%
18	14.540	1938	1947	1958	rBV	1575316	2424746	35.70%	3.614%
19	14.734	1973	1980	2002	rBV	1099761	1854669	27.31%	2.764%
20	14.957	2015	2018	2023	rVB7	6111	11771	0.17%	0.018%
21	15.198	2056	2059	2066	rVB8	5195	9705	0.14%	0.014%
22	15.534	2109	2116	2129	rBV	3656430	5233984	77.06%	7.801%
23	15.651	2130	2136	2150	rVV	1107747	1599422	23.55%	2.384%
24	15.775	2152	2157	2162	rVB	43352	66648	0.98%	0.099%
25	16.104	2207	2213	2215	rBV7	4185	7055	0.10%	0.011%
26	16.316	2244	2249	2255	rBV3	13475	21323	0.31%	0.032%
27	16.975	2355	2361	2364	rVB7	7734	10962	0.16%	0.016%
28	17.081	2373	2379	2384	rBV4	4670	9184	0.14%	0.014%
29	17.292	2407	2415	2425	rBV	2072971	2926577	43.09%	4.362%
30	17.392	2425	2432	2448	rVV	3962957	5708870	84.05%	8.509%
31	18.192	2563	2568	2573	rBV8	5047	9049	0.13%	0.013%
32	19.198	2734	2739	2744	rBV2	52872	75256	1.11%	0.112%
33	19.269	2747	2751	2757	rVV2	46190	65976	0.97%	0.098%
34	19.322	2757	2760	2768	rVB4	23949	33623	0.50%	0.050%
35	19.551	2796	2799	2804	rVB2	31618	34860	0.51%	0.052%
36	19.622	2805	2811	2826	rBV	5011535	6792260	100.00%	10.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010385.D
Acq On : 17 May 2022 09:02
Operator : CG/JU
Sample : PB144810BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION

37	21.375	3104	3109	3122	rBV	2265995	3125147	46.01%	4.658%
38	23.657	3488	3497	3504	rBV2	2772017	5929510	87.30%	8.838%
39	23.810	3516	3523	3533	rVB2	1354784	2758747	40.62%	4.112%




Sum of corrected areas: 67092262

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010385.D
Acq On : 17 May 2022 09:02
Operator : CG/JU
Sample : PB144810BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

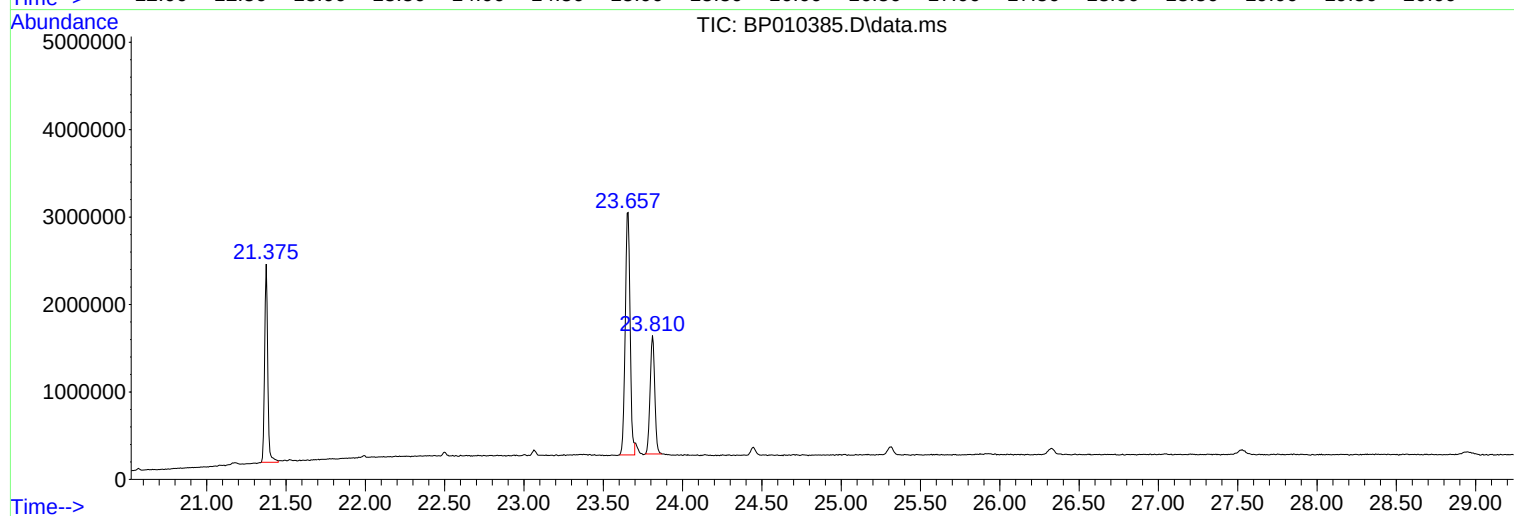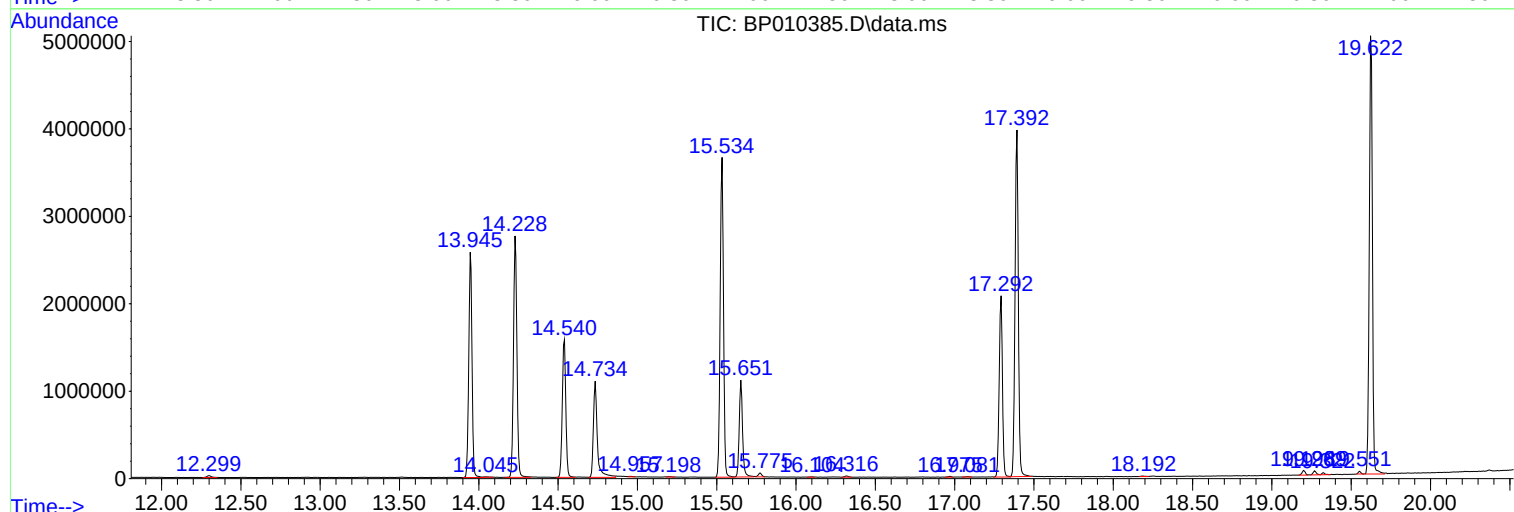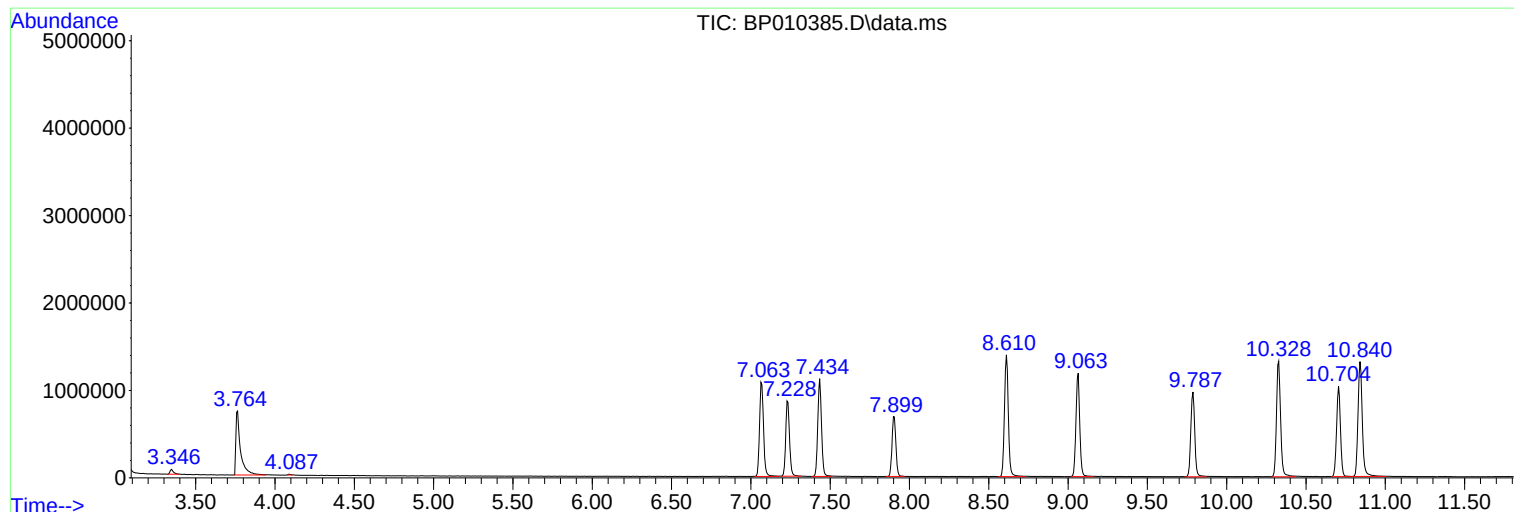

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010385.D
Acq On : 17 May 2022 09:02
Operator : CG/JU
Sample : PB144810BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051622\
Data File : BP010385.D
Acq On : 17 May 2022 09:02
Operator : CG/JU
Sample : PB144810BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc