
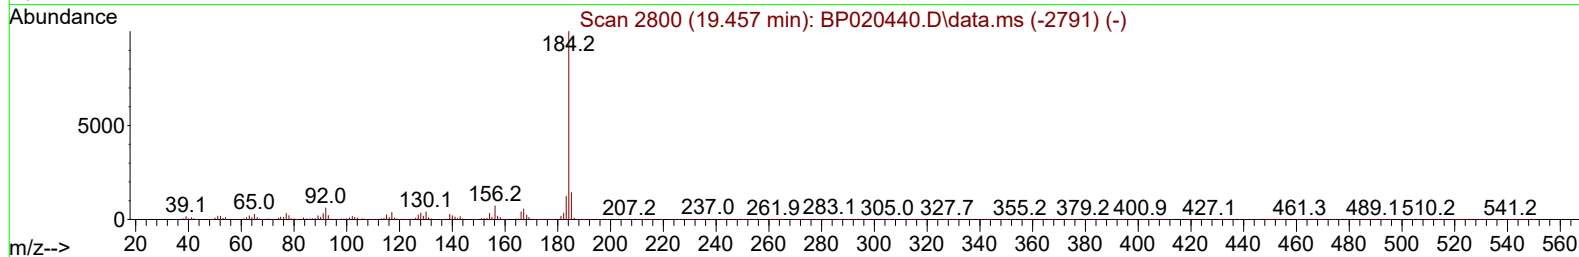
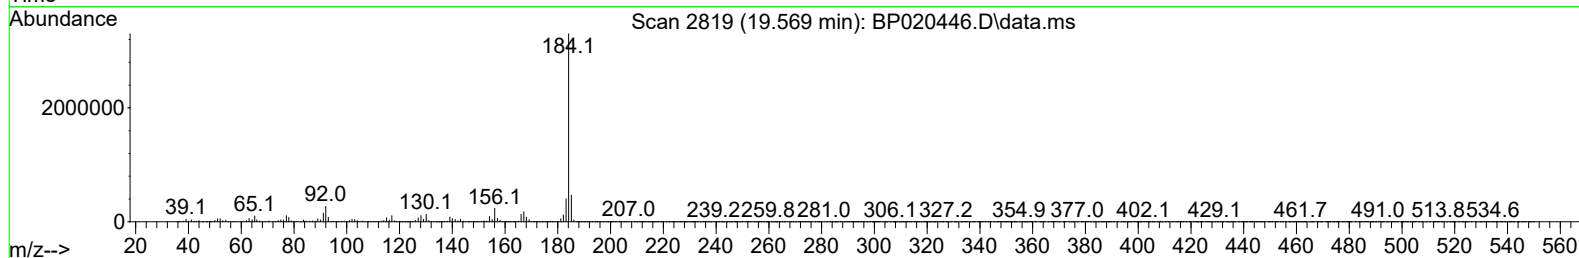


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020446.D
Acq On : 24 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 13:11:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

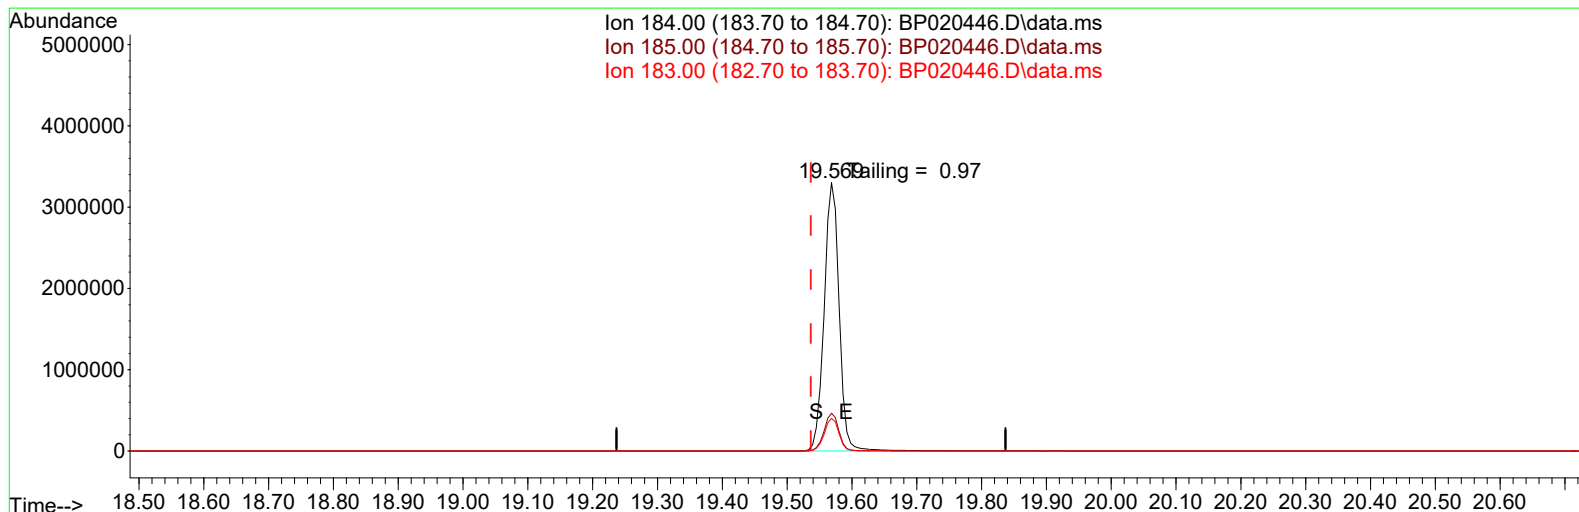

TIC: BP020446.D\data.ms

(77) Benzidine




19.569min (+ 0.032) 2172389.60 ng

response 5318904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.10
183.00	12.20	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020446.D
Acq On : 24 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 13:11:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

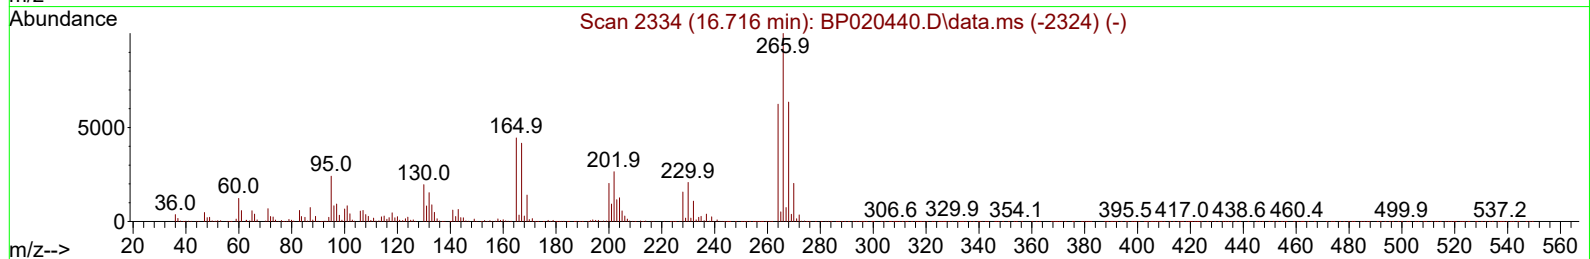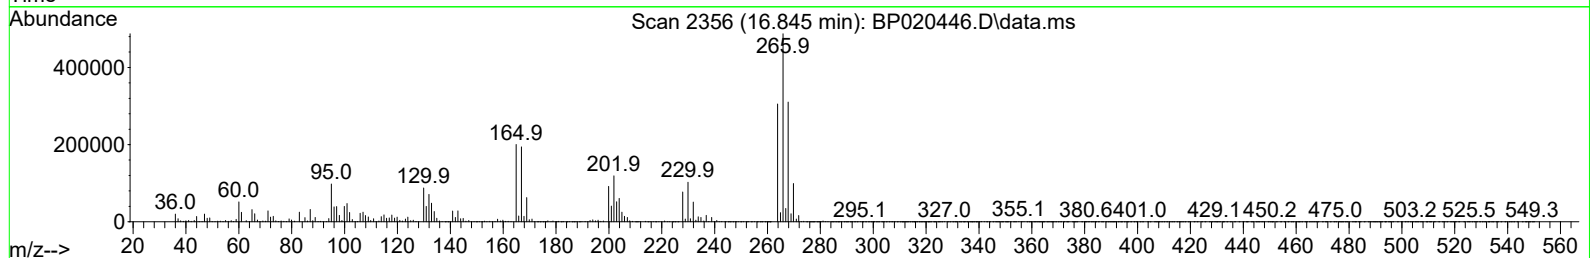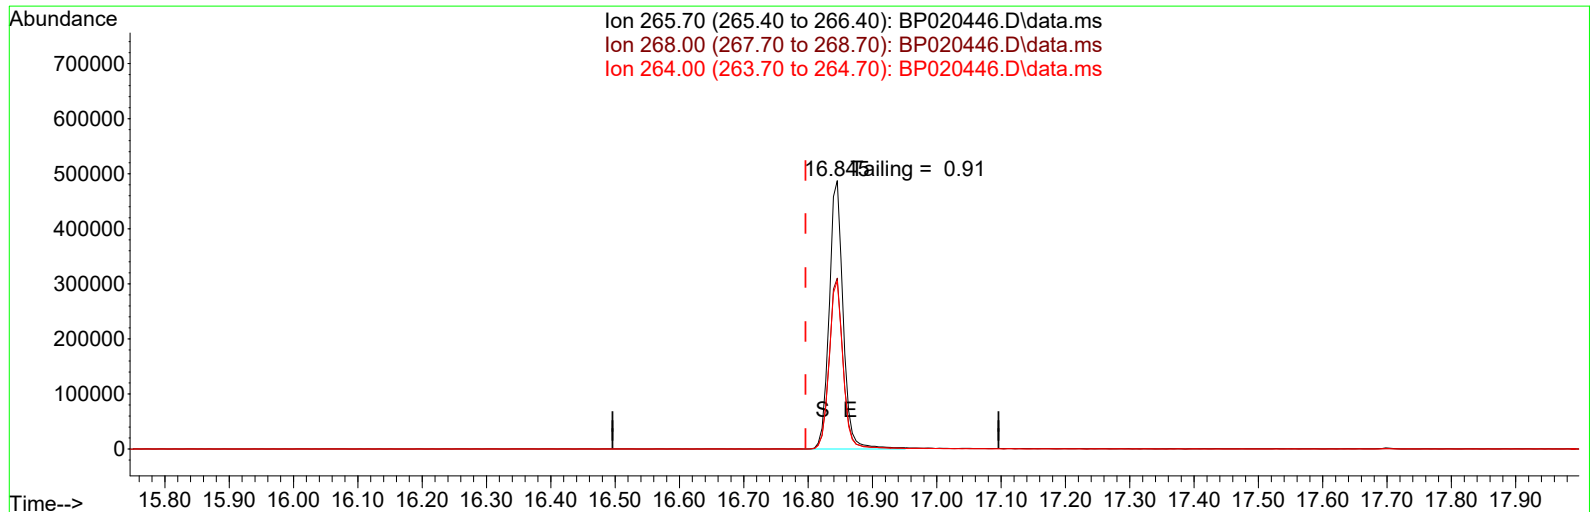

TIC: BP020446.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.049) 1189615.68 ng

response 737284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.69
264.00	62.40	62.65
0.00	0.00	0.00