

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
 Data File : BP020456.D
 Acq On : 24 May 2024 17:26
 Operator : MA/JU
 Sample : PB160983BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB160983BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP020456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	5	10	14	rBV	241630	278333	1.43%	0.295%
2	5.381	399	407	425	rBV	6339698	9335052	47.86%	9.908%
3	6.934	662	671	681	rBV	6137396	9913146	50.83%	10.521%
4	7.769	804	813	823	rBV	1311062	2096155	10.75%	2.225%
5	8.916	1000	1008	1021	rBV	4025446	6240587	32.00%	6.623%
6	10.540	1274	1284	1293	rBV	1590428	3051551	15.65%	3.239%
7	13.010	1695	1704	1712	rBV	8734341	14871035	76.25%	15.783%
8	14.392	1932	1939	1947	rBV	2926759	4216207	21.62%	4.475%
9	15.910	2189	2197	2214	rBV	7011641	10275948	52.69%	10.906%
10	17.204	2410	2417	2428	rBV	3149588	5091613	26.11%	5.404%
11	17.681	2491	2498	2508	rBV2	88142	271485	1.39%	0.288%
12	18.580	2641	2651	2666	rBV2	66132	239919	1.23%	0.255%
13	19.957	2879	2885	2889	rBV	16039761	19503709	100.00%	20.700%
14	21.663	3168	3175	3183	rBV2	2861197	4548125	23.32%	4.827%
15	25.039	3739	3749	3765	rVB	1611998	4287614	21.98%	4.551%




Sum of corrected areas: 94220479

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020456.D
Acq On : 24 May 2024 17:26
Operator : MA/JU
Sample : PB160983BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB160983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

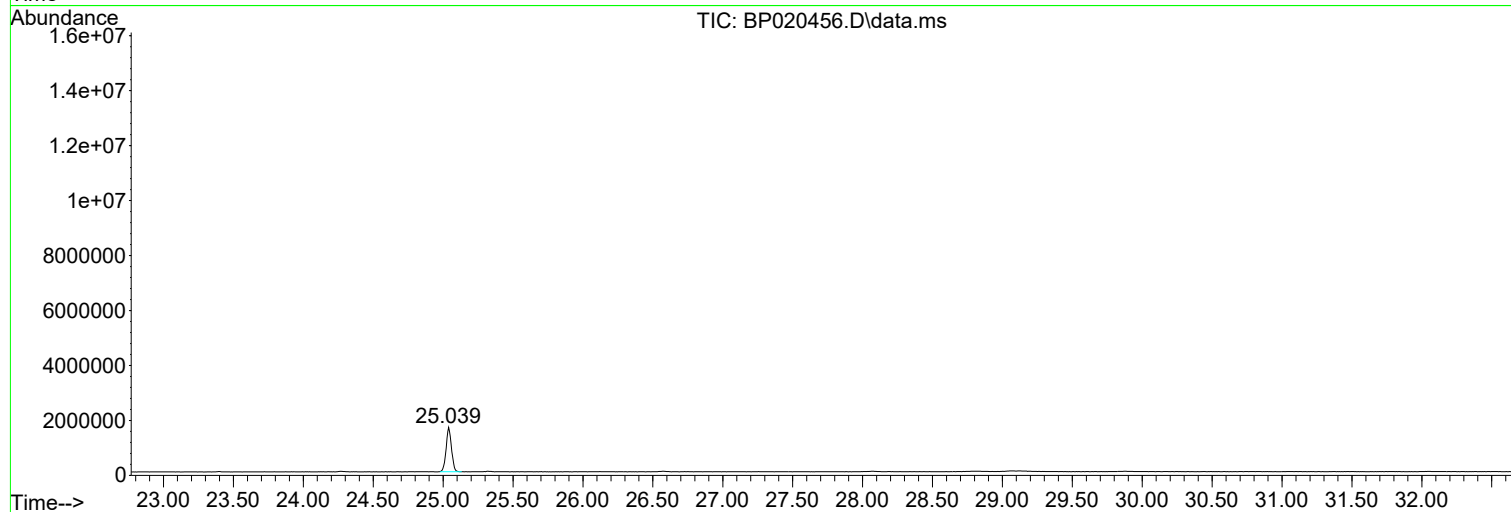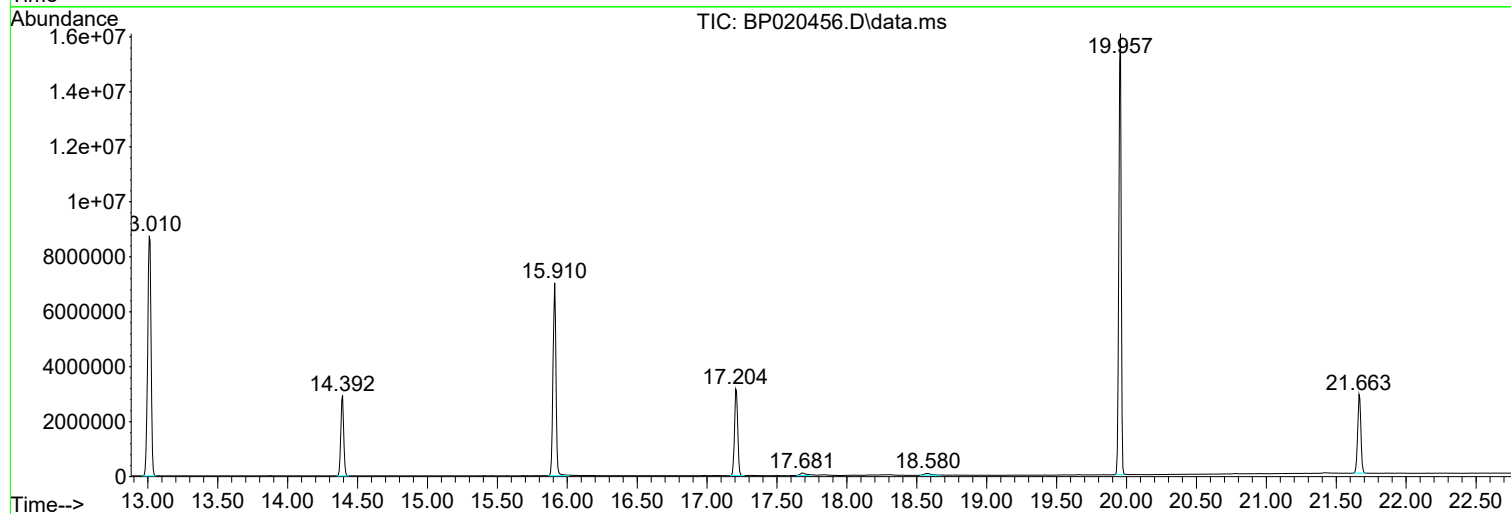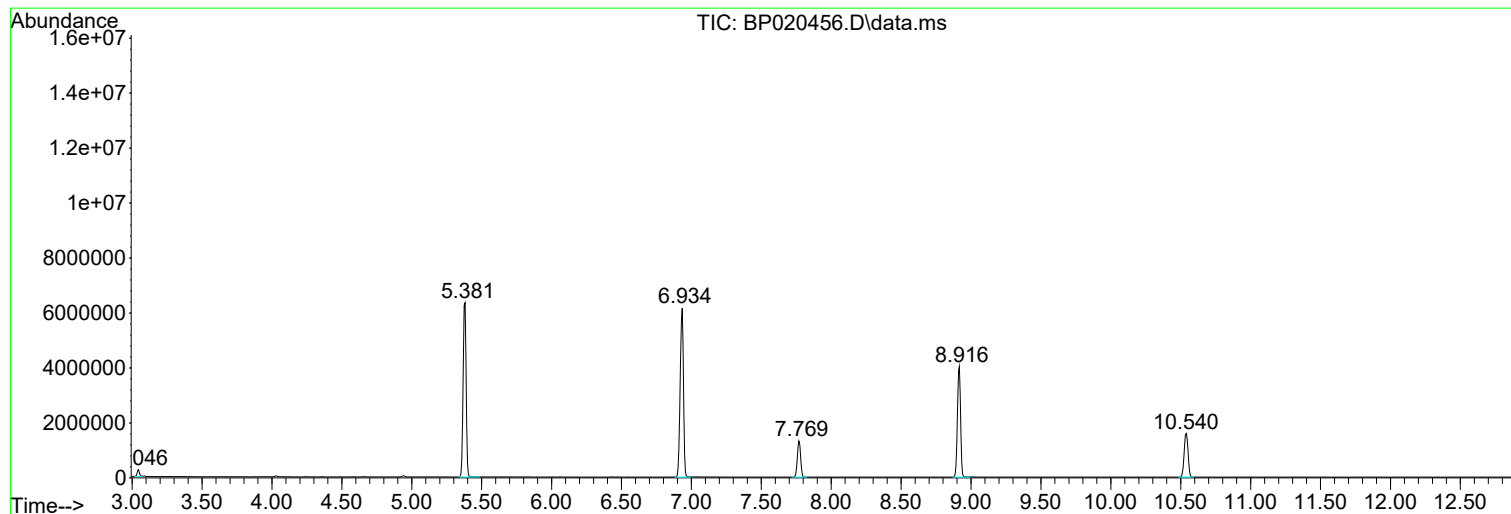

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020456.D
Acq On : 24 May 2024 17:26
Operator : MA/JU
Sample : PB160983BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB160983BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.046	2.66 ng	278333	1,4-Dichlorobenzene-d4	7.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	32
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	32
5			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	17

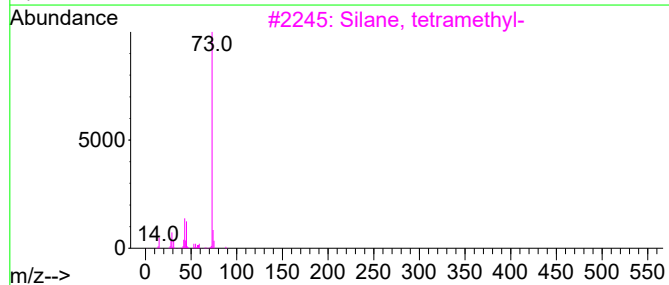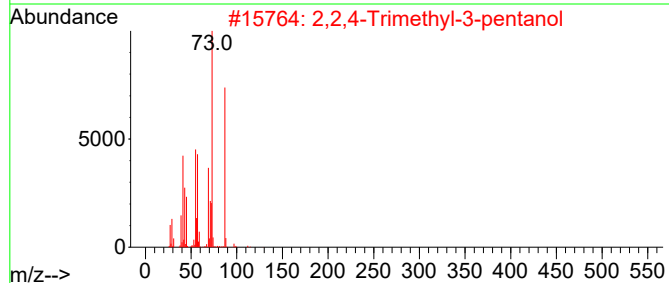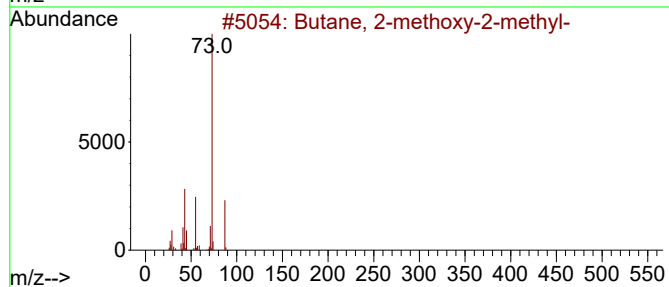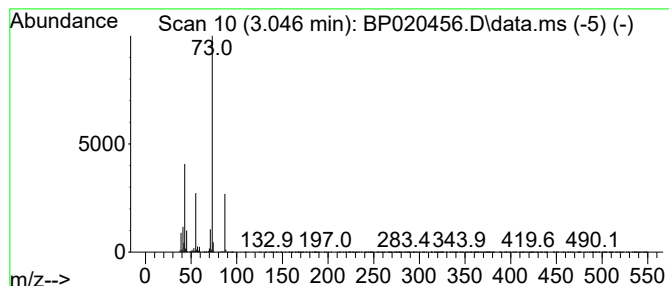

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020456.D
Acq On : 24 May 2024 17:26
Operator : MA/JU
Sample : PB160983BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB160983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.046	2.7	ng	278333	1	7.769	2096160	20.0