
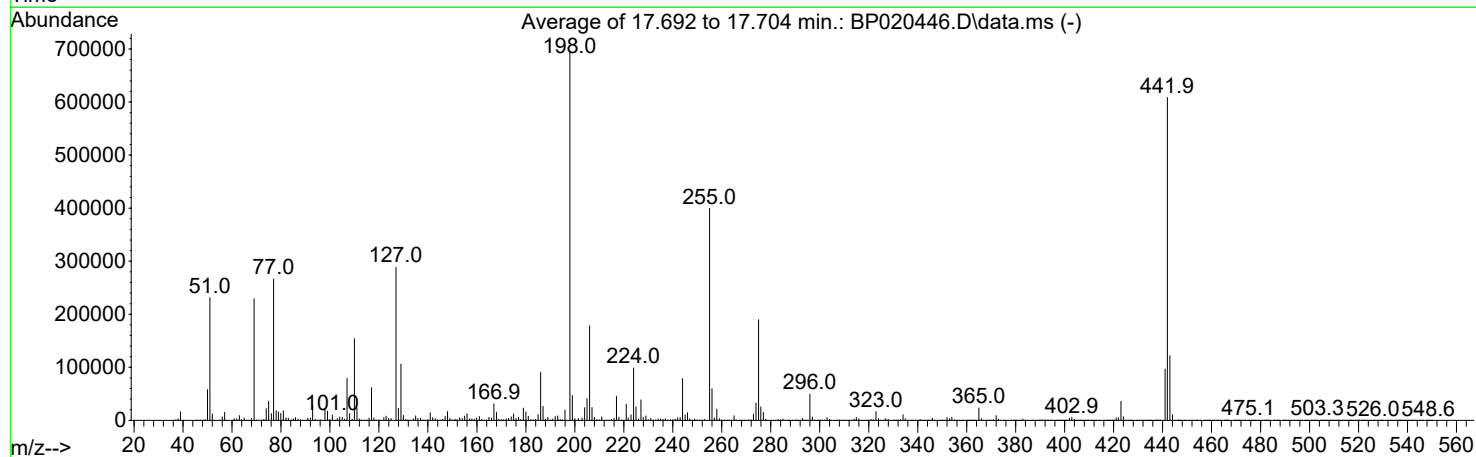


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020446.D
Acq On : 24 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat May 25 02:22:23 2024

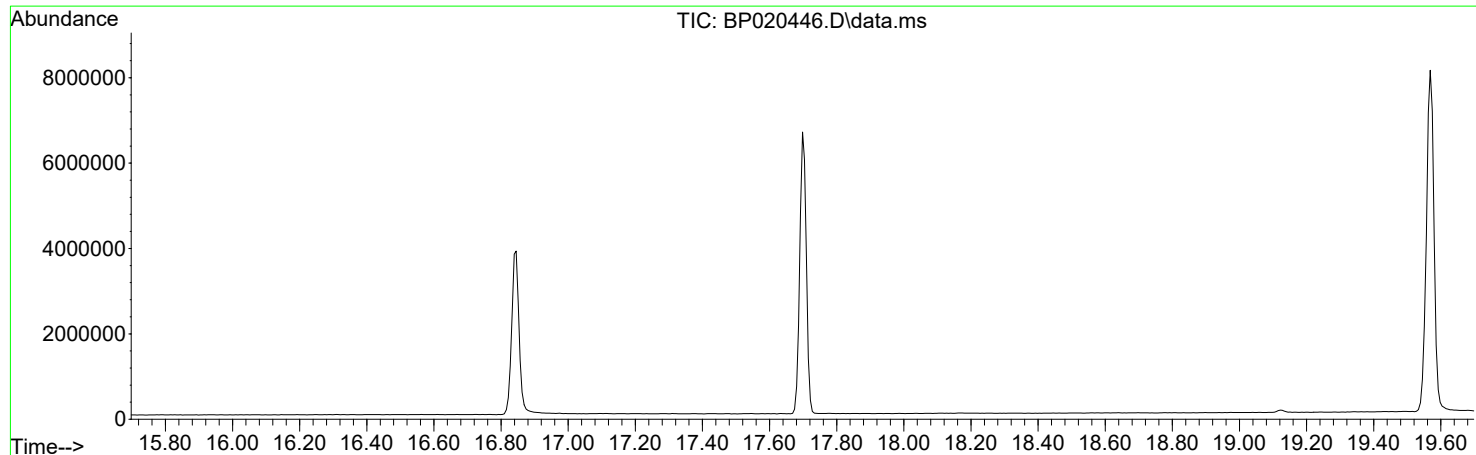

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	231435	PASS
68	69	0.00	2	1.7	3857	PASS
69	198	0.00	100	33.1	229211	PASS
70	69	0.00	2	0.4	940	PASS
127	198	10	80	41.6	288757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	693345	PASS
199	198	5	9	6.7	46792	PASS
275	198	10	60	27.4	189675	PASS
365	198	1	100	3.3	23107	PASS
441	198	0.01	100	14.0	96732	PASS
442	442	100	100	100.0	608465	PASS
443	442	15	24	20.0	121900	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/24/2024	BNA_P	<u>BP020446.D</u>
Compound Name	Response	Retention Time
DDT	2206482	20.863
DDD	28729	20.451
DDE	1426	19.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30155	2236637	1.35

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020446.D
Acq On : 24 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 24 13:11:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

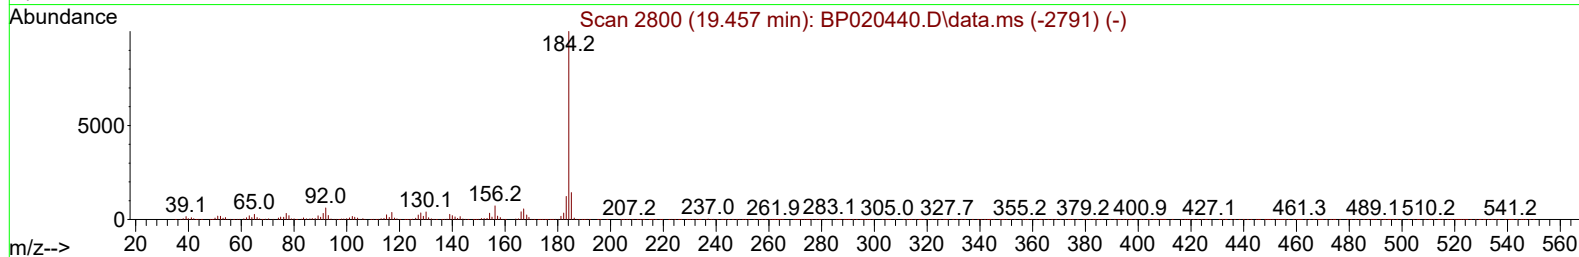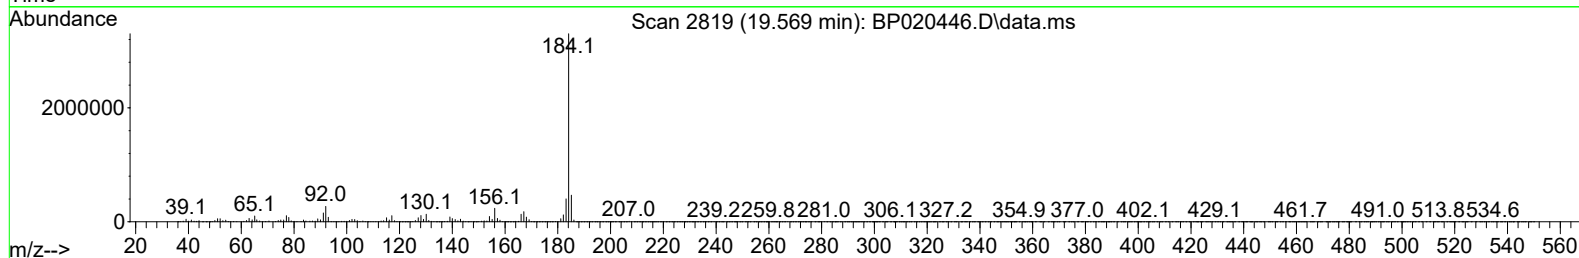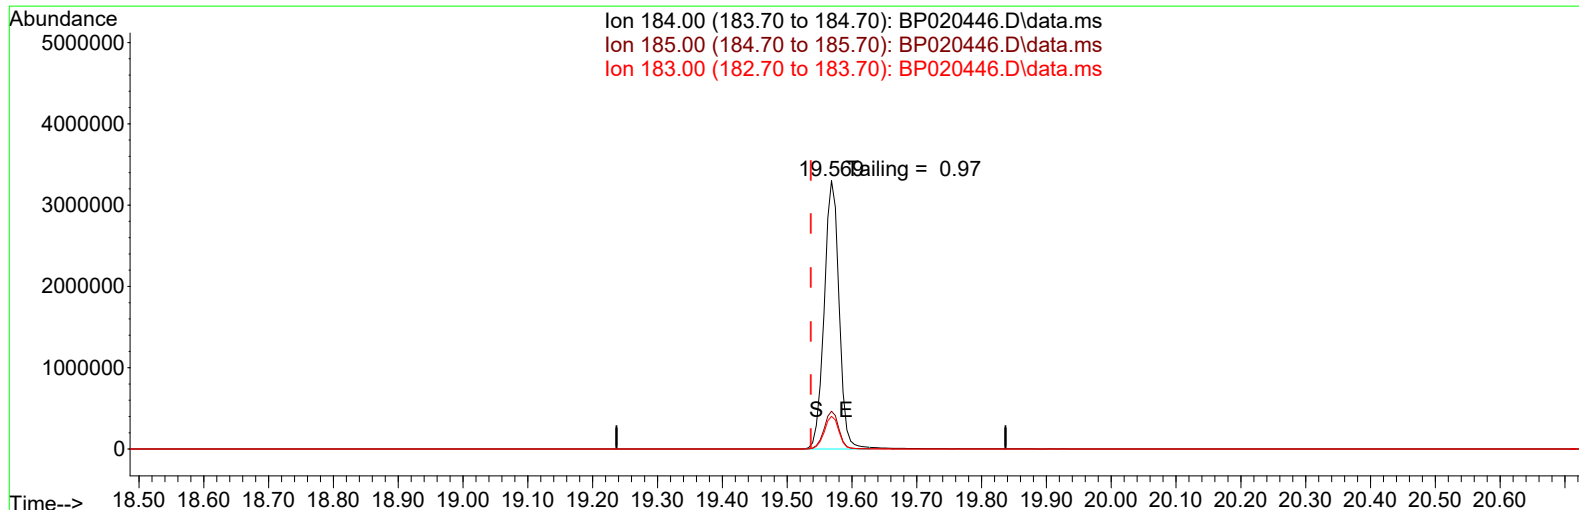

TIC: BP020446.D\data.ms

(77) Benzidine

19.569min (+ 0.032) 2172389.60 ng




response 5318904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.10
183.00	12.20	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052424\
Data File : BP020446.D
Acq On : 24 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 24 13:11:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

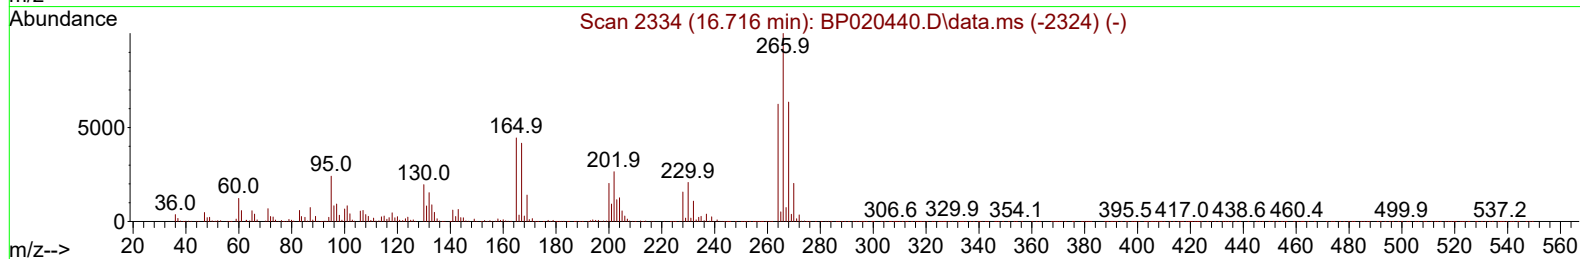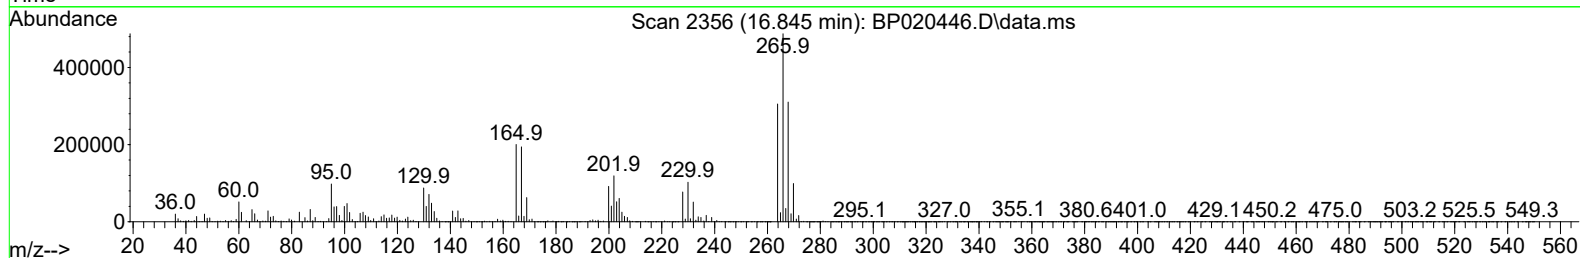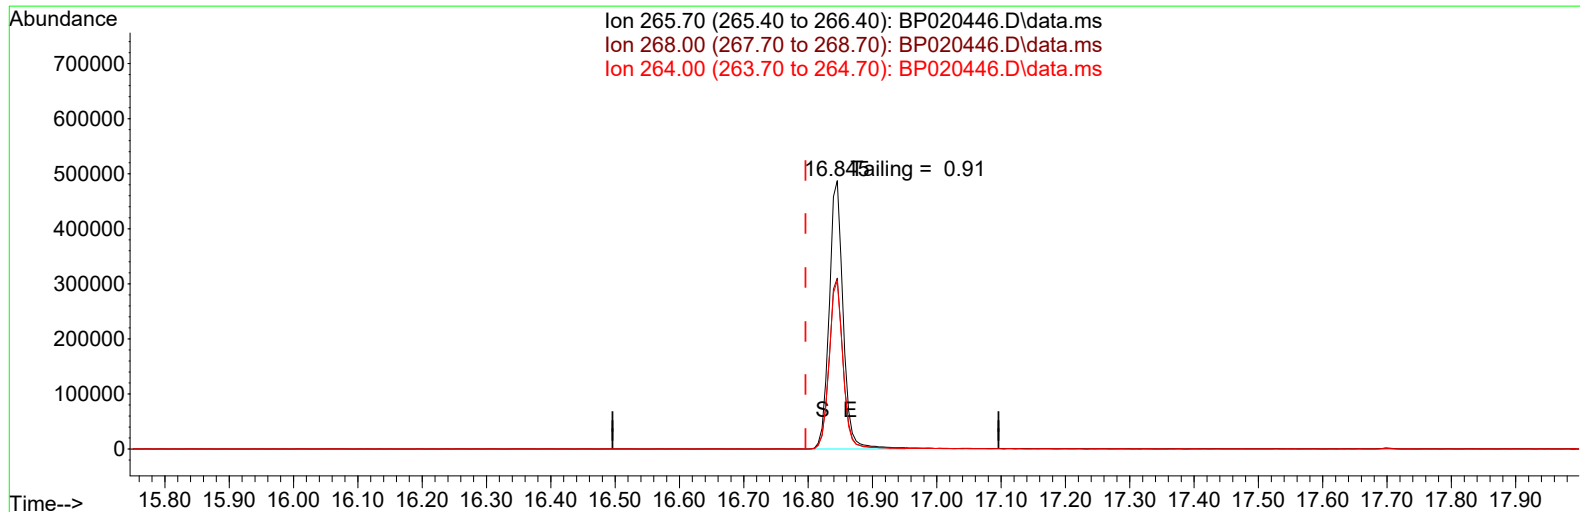

TIC: BP020446.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.049) 1189615.68 ng

response 737284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.69
264.00	62.40	62.65
0.00	0.00	0.00